

LB11537

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092Reviewed by : AK Instrument ID : Konelab

7/14/2021 12:47

Test: ^{Detective} Total CN ^{mark}

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	94.544	0.0	0.076	
ICB1	0.845	0.0	0.002	
CCV1	245.935	0.0	0.196	
CCB1	-0.163	0.0	0.001	
PB137681BL	-0.078	0.0	0.001	
M3012-02	1.364	0.0	0.002	
M3012-02DUP	0.255	0.0	0.001	
M3012-05	-0.764	0.0	0.000	
M3013-02	-0.340	0.0	0.001	
M3026-03	-0.396	0.0	0.001	
M3026-06	-0.476	0.0	0.001	
M3026-09	-0.332	0.0	0.001	
M3026-12	-0.519	0.0	0.001	
CCV2	252.947	0.0	0.202	
CCB2	-1.146	0.0	0.000	

N	15
Mean	39.445
SD	88.6694
CV%	224.79

Aquakem v. 7.2AQ1

Results from time period:

Wed Jul 14 11:50:00 2021

Wed Jul 14 12:22:41 2021

Sample Id	Sam/Ctr/c/	Test short nan	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Reactive CN	P	-0.5911	µg/l	7/14/2021 11:50:00	
5.0PPBCN	A	Reactive CN	P	4.4972	µg/l	7/14/2021 11:50:01	
10PPBCN	A	Reactive CN	P	10.3906	µg/l	7/14/2021 11:50:02	
50PPBCN	A	Reactive CN	P	49.4435	µg/l	7/14/2021 11:50:03	
100PPBCN	A	Reactive CN	P	98.8239	µg/l	7/14/2021 11:50:04	
250PPBCN	A	Reactive CN	P	254.2956	µg/l	7/14/2021 11:50:05	
500PPBCN	A	Reactive CN	P	498.1403	µg/l	7/14/2021 11:50:06	
ICV1	S	Reactive CN	P	94.5439	µg/l	7/14/2021 12:16:23	
ICB1	S	Reactive CN	P	0.8446	µg/l	7/14/2021 12:16:26	
CCV1	S	Reactive CN	P	245.935	µg/l	7/14/2021 12:16:27	
CCB1	S	Reactive CN	P	-0.1626	µg/l	7/14/2021 12:16:29	
PB137681BL	S	Reactive CN	P	-0.0784	µg/l	7/14/2021 12:16:31	
M3012-02	S	Reactive CN	P	1.3643	µg/l	7/14/2021 12:16:32	
M3012-02DUP	S	Reactive CN	P	0.255	µg/l	7/14/2021 12:16:33	
M3012-05	S	Reactive CN	P	-0.7642	µg/l	7/14/2021 12:22:34	
M3013-02	S	Reactive CN	P	-0.3402	µg/l	7/14/2021 12:22:35	
M3026-03	S	Reactive CN	P	-0.3958	µg/l	7/14/2021 12:22:36	
M3026-06	S	Reactive CN	P	-0.4759	µg/l	7/14/2021 12:22:37	
M3026-09	S	Reactive CN	P	-0.3324	µg/l	7/14/2021 12:22:38	
M3026-12	S	Reactive CN	P	-0.519	µg/l	7/14/2021 12:22:39	
CCV2	S	Reactive CN	P	252.9471	µg/l	7/14/2021 12:22:40	
CCB2	S	Reactive CN	P	-1.1465	µg/l	7/14/2021 12:22:41	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : AB

Instrument ID : Konelab

7/14/2021 11:50


Test Total CN

Accepted 7/14/2021 11:50

Factor 1258
Bias 0.001

Coeff. of det. 0.999882

Errors

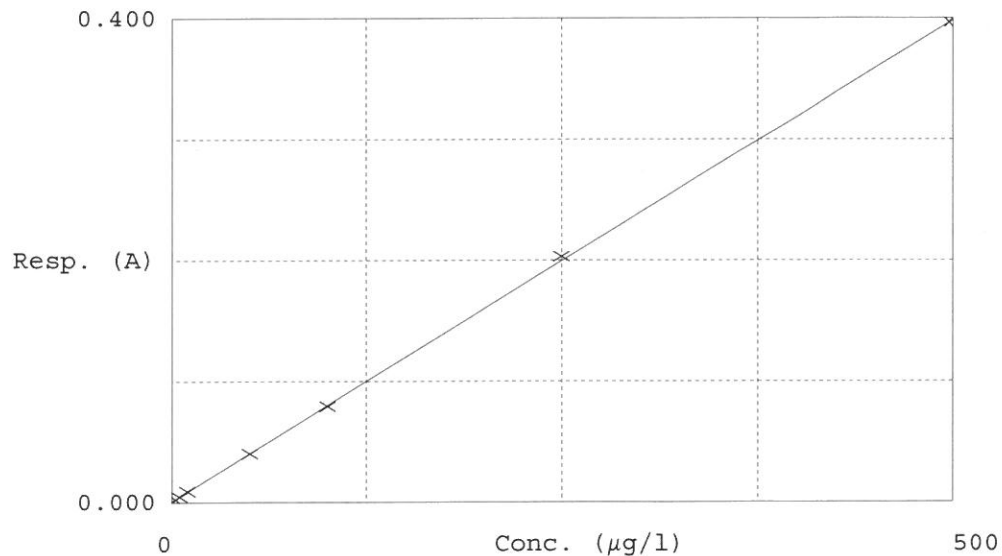

					Relative
Calibrator	Response	Calc. con.	Conc.	Errors	Errors
1	0.0PPBCN	0.001	-0.5911	0.0000	-10
2	5.0PPBCN	0.005	4.4972	5.0000	8.9
3	10PPBCN	0.009	10.3906	10.0000	-1.1
4	50PPBCN	0.040	49.4435	50.0000	-1.2
5	100PPBCN	0.080	98.8239	100.0000	1.8
6	250PPBCN	0.203	254.2956	250.0000	0.4
7	500PPBCN	0.397	498.1403	500.0000	

AB
7/14/21