


LB115365

7470A

INSTRUMENT ID: CV2

Linear

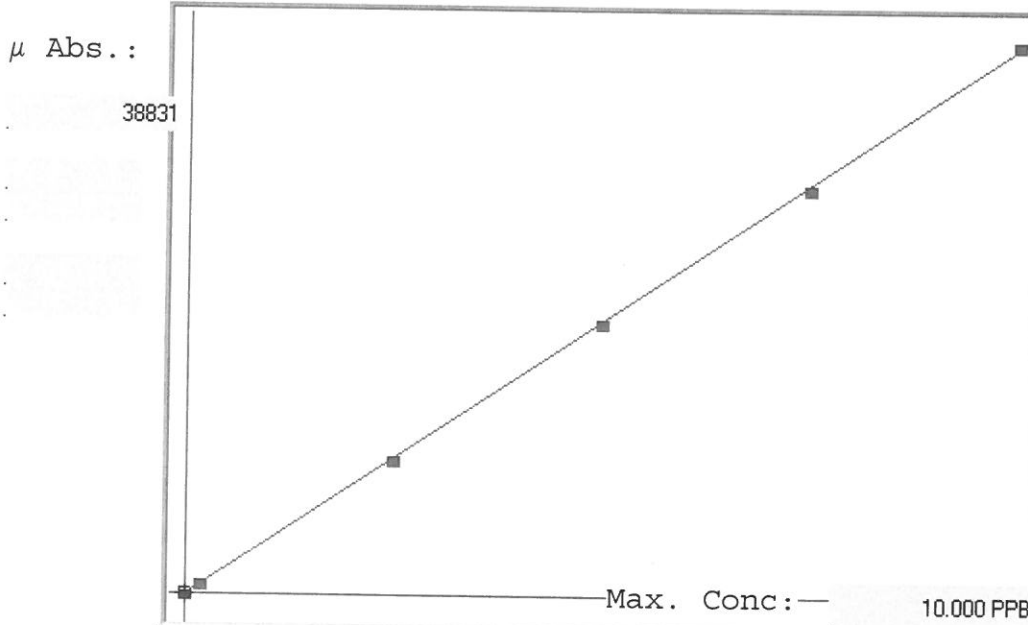

A= 0.0000e+000

B= 2.5867e-004

C= 2.2418e-002

Rho= 0.9999327

Accept=Accepted

td ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	
0.0	0.000	0.024	0.024	7	0.000	7					900
0.2	0.200	0.215	0.015	746	0.0 %	746					8
0.5	2.500	2.490	-0.010	9538	0.0 %	9538					0
1.0	5.000	4.974	-0.026	19144	0.0 %	19144					-1
1.5	7.500	7.430	-0.070	28636	0.0 %	28636					-1
2.0	10.000	10.067	0.067	38831	0.0 %	38831					1

LB115365 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 15 Jul 2021 09:28:43

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	7	-	0.0000	7470A	PPB	15 Jul 2021 09:35:44	S	Std
0.2 - 1	50.2	746	-	0.2000	7470A	PPB	15 Jul 2021 09:38:01	S	Std
2.5 - 1	52.5	9538	-	2.5000	7470A	PPB	15 Jul 2021 09:40:17	S	Std
5.0 - 1	55	19144	-	5.0000	7470A	PPB	15 Jul 2021 09:42:34	S	Std
7.5 - 1	57.5	28636	-	7.5000	7470A	PPB	15 Jul 2021 09:44:51	S	Std
10.0 - 1	510	38831	-	10.0000	7470A	PPB	15 Jul 2021 09:47:06	S	Std
ICV06 - 1	ICV06	15347	3.9922	-7470A	PPB	15 Jul 2021 09:52:51	U	SMPL	
ICB06 - 1	ICB06	-89	-0.0006	-7470A	PPB	15 Jul 2021 09:55:06	U	SMPL	
CCV67 - 1	CCV67	19021	4.9426	-7470A	PPB	15 Jul 2021 09:57:21	U	SMPL	
CCB67 - 1	CCB67	-92	-0.0014	-7470A	PPB	15 Jul 2021 09:59:35	U	SMPL	
CRA - 1	CRA	720	0.2087	-7470A	PPB	15 Jul 2021 10:01:51	U	SMPL	
HighStd - 1	HighStd	38654	10.0210	-7470A	PPB	15 Jul 2021 10:04:05	U	SMPL	
ChkStd - 1	ChkStd	26939	6.9907	-7470A	PPB	15 Jul 2021 10:06:20	U	SMPL	
PB137712BL - 1	PBW	-172	-0.0221	-7470A	PPB	15 Jul 2021 10:08:37	U	SMPL	
PB137712BS - 1	LCSW	14300	3.7214	-7470A	PPB	15 Jul 2021 10:10:54	U	SMPL	
M2846-03 - 1	DRUM-1	85	0.0444	-7470A	PPB	15 Jul 2021 10:13:10	U	SMPL	
M2846-03DUP - 1	DRUM-1DUP	110	0.0509	-7470A	PPB	15 Jul 2021 10:15:26	U	SMPL	
M2846-03MS - 1	DRUM-1MS	13449	3.5013	-7470A	PPB	15 Jul 2021 10:17:43	U	SMPL	
M2846-03MSD - 1	DRUM-1MSD	13603	3.5411	-7470A	PPB	15 Jul 2021 10:20:00	U	SMPL	
CCV68 - 1	CCV68	19038	4.9469	-7470A	PPB	15 Jul 2021 10:22:15	U	SMPL	
CCB68 - 1	CCB68	-96	-0.0024	-7470A	PPB	15 Jul 2021 10:24:30	U	SMPL	
M2846-03LX5 - 1		36	0.0317	-7470A	PPB	15 Jul 2021 10:26:45	U	SMPL	
M2846-03A - 1		15680	4.0783	-7470A	PPB	15 Jul 2021 10:29:01	U	SMPL	
CCV69 - 1	CCV69	18977	4.9312	-7470A	PPB	15 Jul 2021 10:31:16	U	SMPL	
CCB69 - 1	CCB69	-100	-0.0034	-7470A	PPB	15 Jul 2021 10:33:31	U	SMPL	