


LB115384

245.1

INSTRUMENT ID: CV 1

Linear

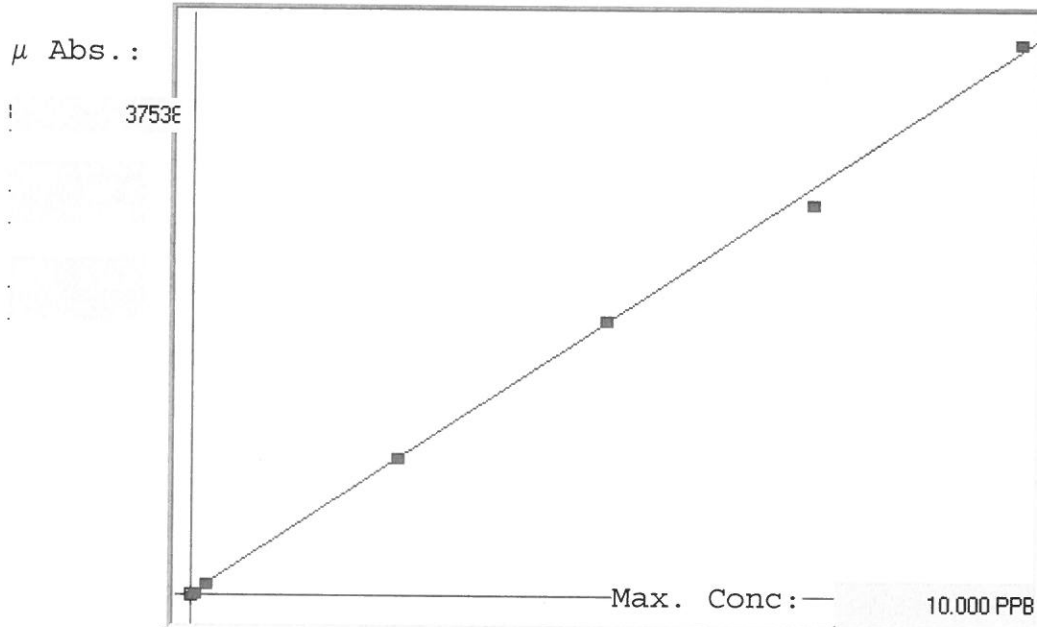

A= 0.0000e+000

B= 2.7088e-004

C= -1.1292e-002

Rho= 0.9993906

Accept=Accepted

td ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0	0.000	-0.001	-0.001	38	0.000	38					10
.05	0.050	0.055	0.005	243	0.0 %	243	0				9
.2	0.200	0.219	0.019	852	0.0 %	852					1
.5	2.500	2.525	0.025	9365	0.0 %	9365					2
.0	5.000	5.086	0.086	18816	0.0 %	18816					-4
.5	7.500	7.209	-0.291	26656	0.0 %	26656					2
0.0	10.000	10.157	0.157	37538	0.0 %	37538					

LB115384 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 16 Jul 2021 12:22:24

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc/Method	Units	Date	Type	Type
0.0 - 1	50	38	-	0.0000245.1	PPB	16 Jul 2021 12:27:21	S	Std
0.05 - 1	50-05	243	-	0.0500245.1	PPB	16 Jul 2021 12:29:38	S	Std
0.2 - 1	50.2	852	-	0.2000245.1	PPB	16 Jul 2021 12:31:55	S	Std
2.5 - 1	52.5	9365	-	2.5000245.1	PPB	16 Jul 2021 12:34:12	S	Std
5.0 - 1	55	18816	-	5.0000245.1	PPB	16 Jul 2021 12:36:28	S	Std
7.5 - 1	57.5	26656	-	7.5000245.1	PPB	16 Jul 2021 12:43:56	S	Std
10.0 - 1	510	37538	-	10.0000245.1	PPB	16 Jul 2021 13:01:39	S	Std
CV09 - 1	ICV09	14977	4.0456	-245.1	PPB	16 Jul 2021 13:04:28	U	SMPL
CB09 - 1	ICB09	-81	-0.0332	-245.1	PPB	16 Jul 2021 13:06:43	U	SMPL
CV79 - 1	CCV79	18816	5.0855	-245.1	PPB	16 Jul 2021 13:08:58	U	SMPL
CB79 - 1	CCB79	-80	-0.0330	-245.1	PPB	16 Jul 2021 13:11:12	U	SMPL
CRA - 1	CRA	211	0.0459	-245.1	PPB	16 Jul 2021 13:13:27	U	SMPL
HighStd - 1	HighStd	36712	9.9331	-245.1	PPB	16 Jul 2021 13:15:42	U	SMPL
ChkStd - 1	ChkStd	25744	6.9621	-245.1	PPB	16 Jul 2021 13:17:57	U	SMPL
B137759BL - 1	PBW	-126	-0.0454	-245.1	PPB	16 Jul 2021 13:20:13	U	SMPL
B137759BS - 1	LCSW	14638	3.9538	-245.1	PPB	16 Jul 2021 13:22:30	U	SMPL
A2940-10 - 1	LOD-MDL-WATER-04-QT3-2021	549	0.1374	-245.1	PPB	16 Jul 2021 13:24:46	U	SMPL
A2940-12 - 1	MDL-WATER-06-QT3-2021	207	0.0448	-245.1	PPB	16 Jul 2021 13:27:02	U	SMPL
A3039-22 - 1	EX-05	218	0.0478	-245.1	PPB	16 Jul 2021 13:29:19	U	SMPL
A3039-22DUP - 1	EX-05DUP	177	0.0367	-245.1	PPB	16 Jul 2021 13:31:36	U	SMPL
A3039-22MS - 1	EX-05MS	15922	4.3016	-245.1	PPB	16 Jul 2021 13:33:51	U	SMPL
CV80 - 1	CCV80	18720	5.0595	-245.1	PPB	16 Jul 2021 13:36:06	U	SMPL
CB80 - 1	CCB80	-80	-0.0330	-245.1	PPB	16 Jul 2021 13:38:22	U	SMPL
A3039-22MSD - 1	EX-05MSD	14752	3.9847	-245.1	PPB	16 Jul 2021 13:40:37	U	SMPL
A3057-01 - 1	EQ-TANK-TESTING-TOP	-66	-0.0292	-245.1	PPB	16 Jul 2021 13:42:52	U	SMPL
A3057-02 - 1	EQ-TANK-TESTING-MIDDLE	-16	-0.0156	-245.1	PPB	16 Jul 2021 13:45:07	U	SMPL
A3057-03 - 1	EQ-TANK-TESTING-BOTTOM	-5	-0.0126	-245.1	PPB	16 Jul 2021 13:47:23	U	SMPL
A3039-22LX5 - 1		50	0.0023	-245.1	PPB	16 Jul 2021 13:49:38	U	SMPL
A3039-22A - 1		15893	4.2937	-245.1	PPB	16 Jul 2021 13:51:54	U	SMPL
CV81 - 1	CCV81	18241	4.9298	-245.1	PPB	16 Jul 2021 13:54:10	U	SMPL
CB81 - 1	CCB81	-59	-0.0273	-245.1	PPB	16 Jul 2021 13:56:27	U	SMPL