


Clear table

Instrument ID: IC-2										Analyst : AP		Method: 300.0 / 9056A	
ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time	Initial wt/ Final Vol	Analyst		
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2021-07-09_	7/9/21 9:42		AP/MA		
STD2	0.4290	0.6630	0.6670	2.2450	0.5810	0.8760	3.5010	_2021-07-09_	7/9/21 10:10		AP/MA		
STD3	0.7920	1.2070	1.2030	4.0520	1.0180	2.0320	6.0650	_2021-07-09_	7/9/21 10:39		AP/MA		
STD4	1.0300	1.4850	1.4820	4.9290	1.2380	2.5490	7.3860	_2021-07-09_	7/9/21 11:07		AP/MA		
STD5	1.9480	2.9110	2.9160	9.6610	2.3920	5.0590	14.3460	_2021-07-09_	7/9/21 11:36		AP/MA		
STD6	3.9460	6.0160	6.0140	19.9940	4.9470	10.0720	29.9440	_2021-07-09_	7/9/21 12:05		AP/MA		
STD7	5.0550	7.5180	7.5190	25.1190	6.3240	12.4110	37.7580	_2021-07-09_	7/9/21 12:33		AP/MA		
ICV	1.9440	2.9090	2.9370	9.6930	2.3900	4.9880	14.3530	_2021-07-09_	7/9/21 13:05		AP/MA		
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2021-07-09_	7/9/21 13:34		AP/MA		
CCV	2.1190	2.9360	2.9490	9.7340	2.4150	4.9940	14.4550	_2021-07-16_	7/16/21 9:09		AP/MA		
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2021-07-16_	7/16/21 9:42		AP/MA		
LB115386BLW	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2021-07-16_	7/16/21 10:10		AP/MA		
LB115386BSW	2.0420	2.8870	2.9160	9.5930	2.3740	5.1860	14.2510	_2021-07-16_	7/16/21 10:39		AP/MA		
M3086-01	0.0000	0.0000	0.1970	0.0000	0.4240	0.0000	0.9880	_2021-07-16_	7/16/21 11:57		AP/MA		
M3086-02	0.0000	0.1580	0.1520	0.0000	0.4350	0.0000	1.0200	_2021-07-16_	7/16/21 12:26		AP/MA		
M3086-03	0.1700	0.0000	0.0000	0.0000	0.2660	0.0000	0.9570	_2021-07-16_	7/16/21 12:54		AP/MA		
M3086-03MS	2.2420	3.0080	3.0070	9.8860	2.5920	4.8830	14.7360	_2021-07-16_	7/16/21 13:23		AP/MA		
M3086-03MSD	2.0620	2.8450	2.8450	9.3220	2.4430	4.7000	13.8810	_2021-07-16_	7/16/21 13:52		AP/MA		
CCV	2.0460	2.9230	2.9230	9.7270	2.4050	5.3130	14.3960	_2021-07-16_	7/16/21 14:20		AP/MA		
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2021-07-16_	7/16/21 14:49		AP/MA		

CALIBRATION OF COMPONENT F-

Method: AnionsIC2-070921.mtw
 Equation: $Q = 0.0750899 \cdot A + 2.06898$
 RSD: 2.325 %
 Correlation coefficient: 0.999705

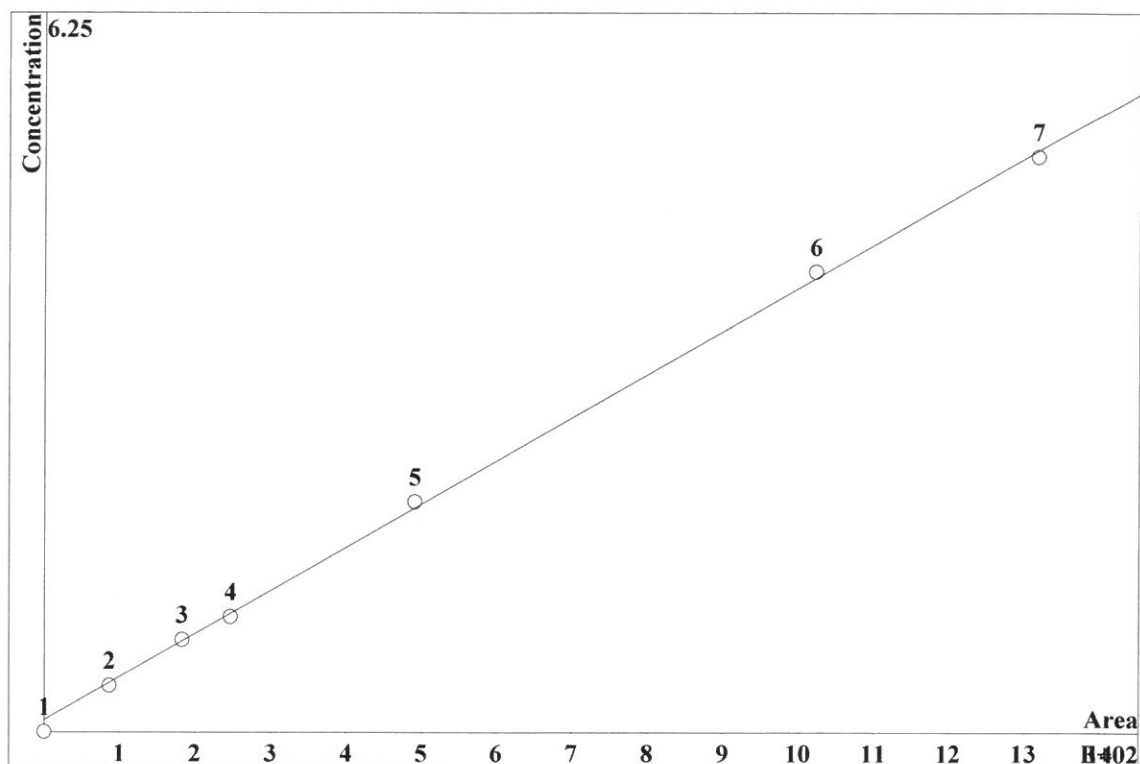

K3 = 0 K2 = 0 K1 = 0.0750899 K0 = 2.06898

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	2.336	86.64	0.4	20	5.75		
3	5.02	183.5	0.8	20	5.75		
4	6.724	246.8	1	20	5.75		
5	14.65	491.4	2	20	5.75		
6	31.01	1023	4	20	5.75		
7	38.73	1319	5	20	5.75		

CALIBRATION OF COMPONENT CL-

Method: AnionsIC2-070921.mtw
 Equation: $Q = 0.114962 \cdot A + 2.44005$
 RSD: 1.709 %
 Correlation coefficient: 0.999841



K3 = 0 K2 = 0 K1 = 0.114962 K0 = 2.44005

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	6.27	94.1	0.6	20	8.834		
3	12.68	188.7	1.2	20	8.834		
4	15.95	237.1	1.5	20	8.834		
5	33.19	485.2	3	20	8.834		
6	71.27	1025	6	20	8.834		
7	88.63	1287	7.5	20	8.834		

CALIBRATION OF COMPONENT NO2

Method: AnionsIC2-070921.mtw
 Equation: $Q = 0.051109 \cdot A + 2.59501$
 RSD: 1.685 %
 Correlation coefficient: 0.999845

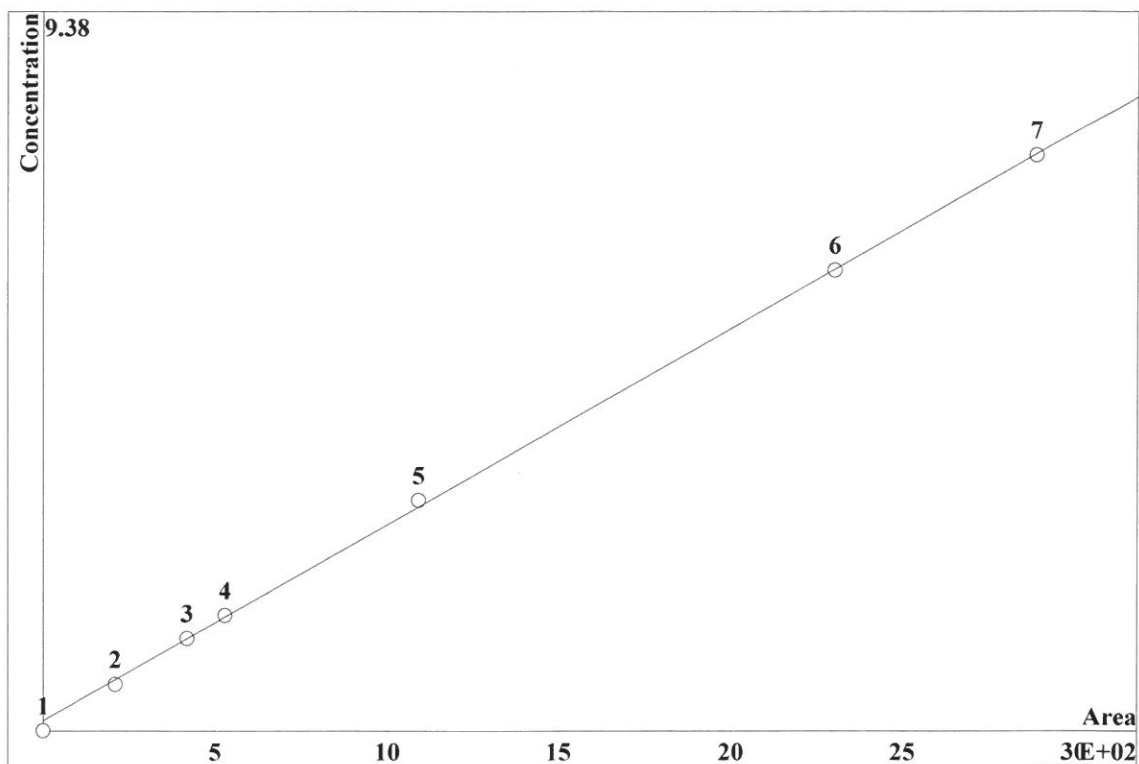

K3 = 0 K2 = 0 K1 = 0.051109 K0 = 2.59501

Base: Area

Ref.channel: ch1

ISTD:

Formula: Linear


Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	11.22	210.2	0.6	20	10.64		
3	22.26	419.9	1.2	20	10.64		
4	28.16	529.1	1.5	20	10.64		
5	57.52	1090	3	20	10.64		
6	115.2	2303	6	20	10.64		
7	142.6	2891	7.5	20	10.64		

±□:□

CALIBRATION OF COMPONENT BR-

Method: AnionsIC2-070921.mtw
 Equation: $Q = 0.254436 \cdot A + 9.45477$
 RSD: 2.017 %
 Correlation coefficient: 0.999778

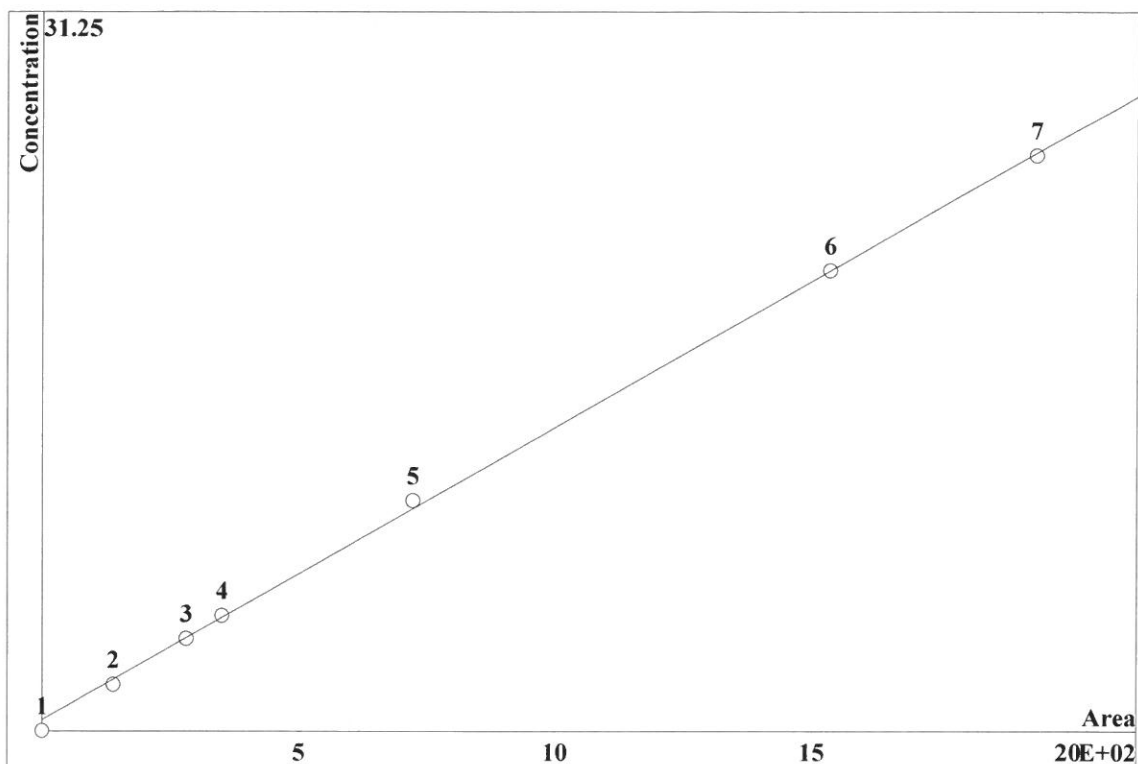

K3 = 0 K2 = 0 K1 = 0.254436 K0 = 9.45477

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	6.921	139.3	2	20			14
3	14.18	281.4	4	20			14
4	17.89	350.3	5	20			14
5	37.58	722.2	10	20			14
6	81.68	1534	20	20			14
7	102.3	1937	25	20			14

CALIBRATION OF COMPONENT NO3

Method: AnionsIC2-070921.mtw
 Equation: $Q = 0.0438083 \cdot A + 2.94619$
 RSD: 2.995 %
 Correlation coefficient: 0.999511

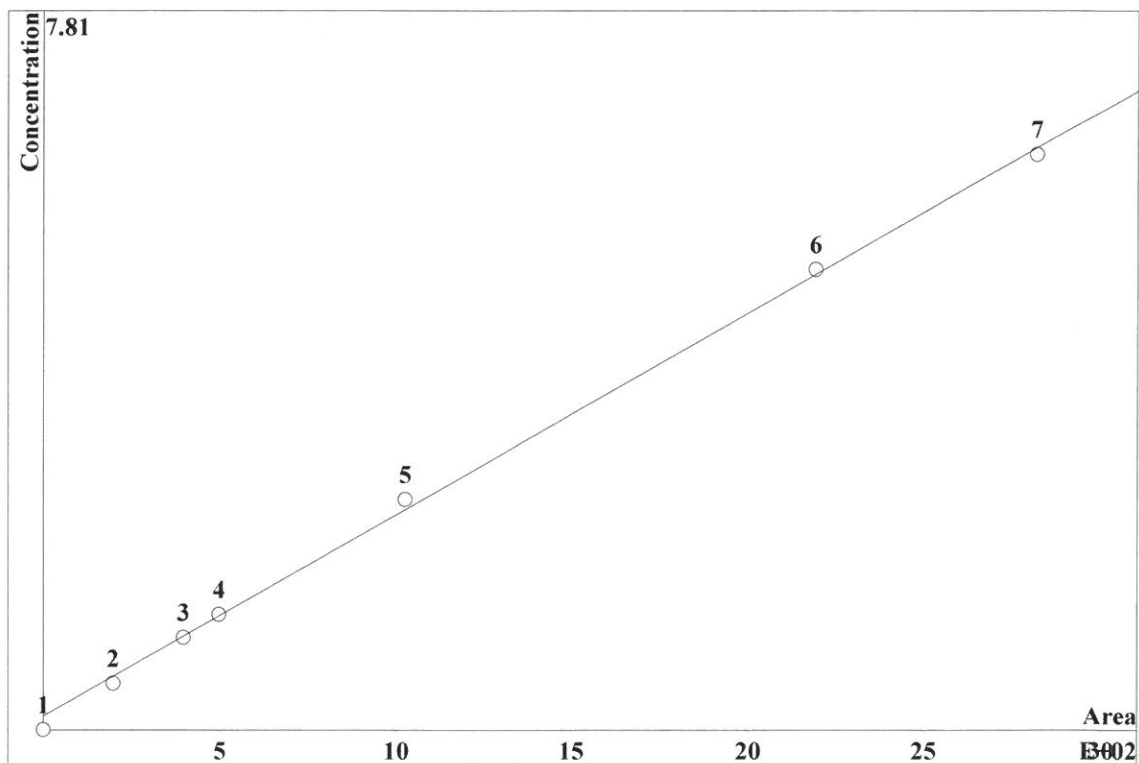


K3 = 0 K2 = 0 K1 = 0.0438083 K0 = 2.94619
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	8.418	198.1	0.5	20	16.28		
3	17.08	397.4	1	20	16.28		
4	21.57	497.9	1.25	20	16.28		
5	44.85	1025	2.5	20	16.28		
6	97.19	2191	5	20	16.28		
7	122.3	2820	6.25	20	16.28		

CALIBRATION OF COMPONENT HPO4

Method: AnionsIC2-070921.mtw
 Equation: $Q = 0.0885729 \cdot A - 11.3055$
 RSD: 1.708 %
 Correlation coefficient: 0.999841

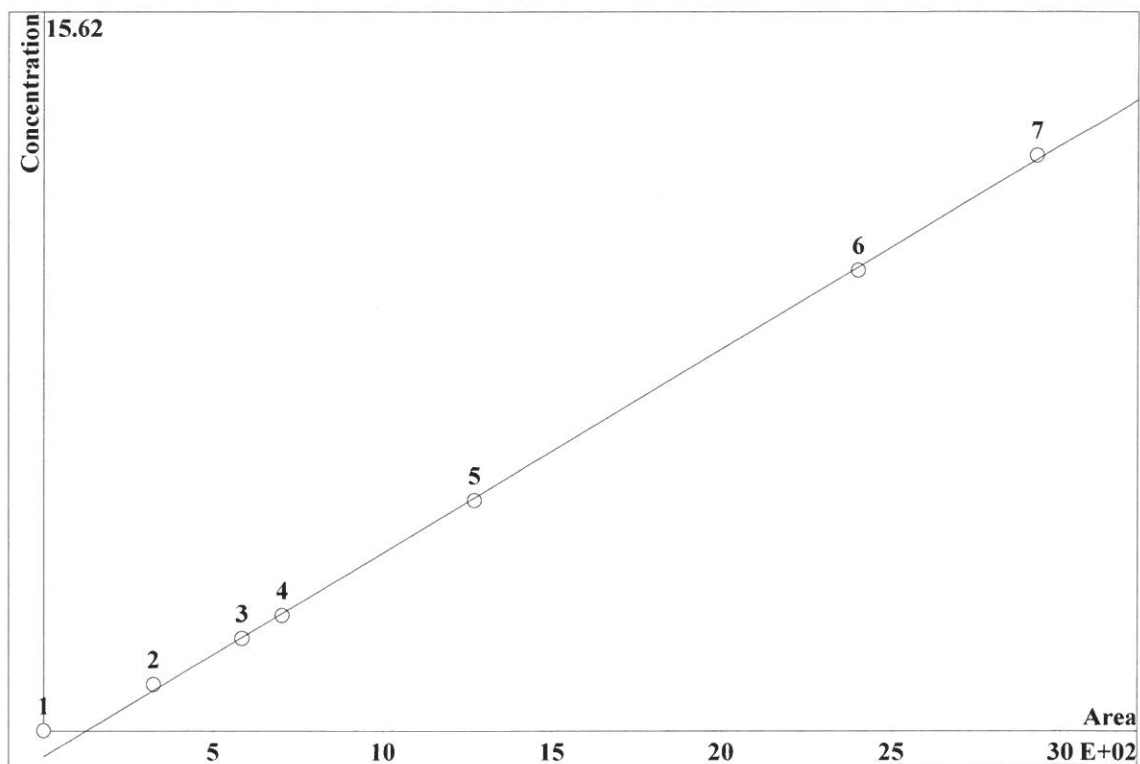

K3 = 0 K2 = 0 K1 = 0.0885729 K0 = -11.3055

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	8.78	325.5	1	20	21.2		
3	16.61	586.6	2	20	21.2		
4	20.09	703.3	2.5	20	21.2		
5	37.65	1270	5	20	21.2		
6	74.91	2402	10	20	21.2		
7	91.49	2930	12.5	20	21.2		

CALIBRATION OF COMPONENT SO4

Method: AnionsIC2-070921.mtw
 Equation: $Q = 0.143844 \cdot A + 17.5564$
 RSD: 2.650 %
 Correlation coefficient: 0.999617

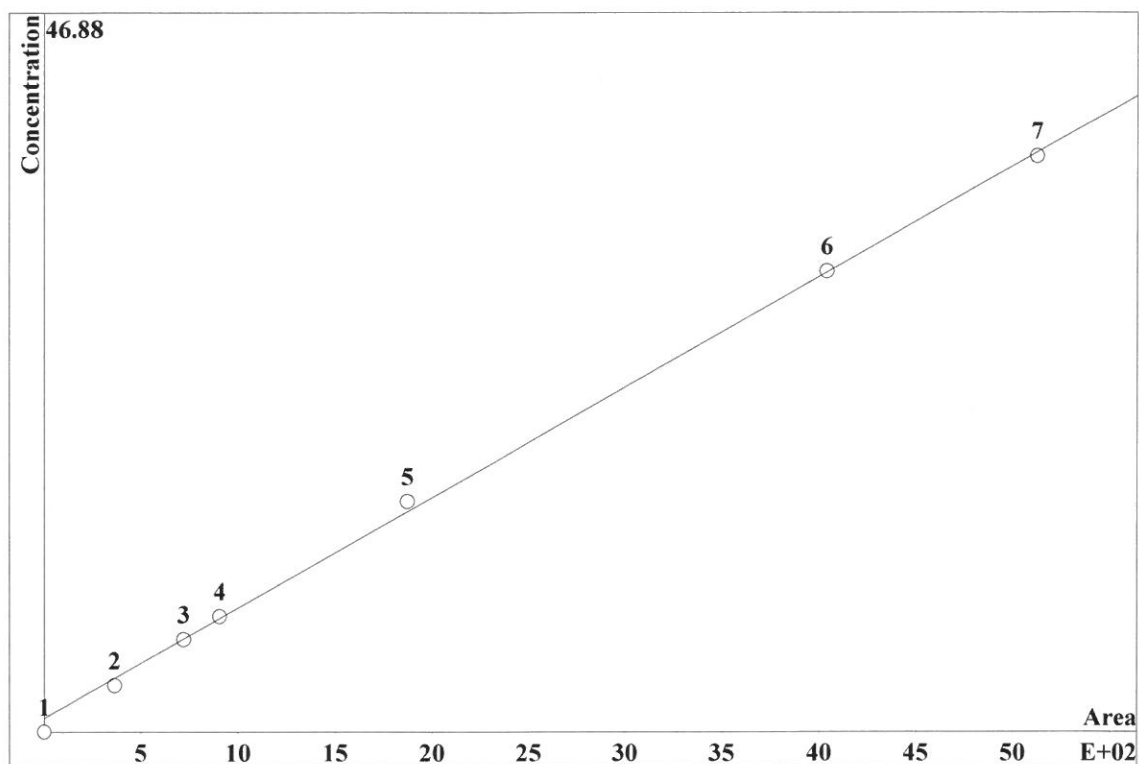

K3 = 0 K2 = 0 K1 = 0.143844 K0 = 17.5564

Base: Area

Ref.channel: ch1

ISTD:

Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	12.45	364.7	3	20	24.73		
3	24.99	721.2	6	20	24.73		
4	31.58	904.9	7.5	20	24.73		
5	66.09	1873	15	20	24.73		
6	145.1	4041	30	20	24.73		
7	182.6	5128	37.5	20	24.73		

æ#□

Clear table

Instrument ID: IC-2 Analyst: AP Method: 300 / 9056A

ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time	Initial wt/ Final Vol	Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-07-09_	7/9/21 9:42		AP/MA
STD2	0.4290	0.6630	0.6670	2.2450	0.5810	0.8760	3.5010	2021-07-09_	7/9/21 10:10		AP/MA
STD3	0.7920	1.2070	1.2030	4.0520	1.0180	2.0320	6.0650	2021-07-09_	7/9/21 10:39		AP/MA
STD4	1.0300	1.4850	1.4820	4.9290	1.2380	2.5490	7.3860	2021-07-09_	7/9/21 11:07		AP/MA
STD5	1.9480	2.9110	2.9160	9.6610	2.3920	5.0590	14.3460	2021-07-09_	7/9/21 11:36		AP/MA
STD6	3.9460	6.0160	6.0140	19.9940	4.9470	10.0720	29.9440	2021-07-09_	7/9/21 12:05		AP/MA
STD7	5.0550	7.5180	7.5190	25.1190	6.3240	12.4110	37.7580	2021-07-09_	7/9/21 12:33		AP/MA

ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.5000

ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4
STD1							
STD2	7.2500	10.5000	11.1667	12.2500	16.2000	-12.4000	16.7000
STD3	-1.0000	0.5833	0.2500	1.3000	1.8000	1.6000	1.0833
STD4	3.0000	-1.0000	-1.2000	-1.4200	-0.9600	1.9600	-1.5200
STD5	-2.6000	-2.9667	-2.8000	-3.3900	-4.3200	1.1800	-4.3600
STD6	-1.3500	0.2667	0.2333	-0.0300	-1.0600	0.7200	-0.1867
STD7	1.1000	0.2400	0.2533	0.4760	1.1840	-0.7120	0.6880

Report date: 7/12/2021 3:22:09 PM
Printed by: wet


Ident: STD1
Analysis from: 7/9/2021 9:42:11 AM
File: _2021-07-09_

Last save: 7/12/2021 3:21:23 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27529

Last save: 7/9/2021 12:31:

SAMPLE:
: AM/AP
Vial number: 2
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

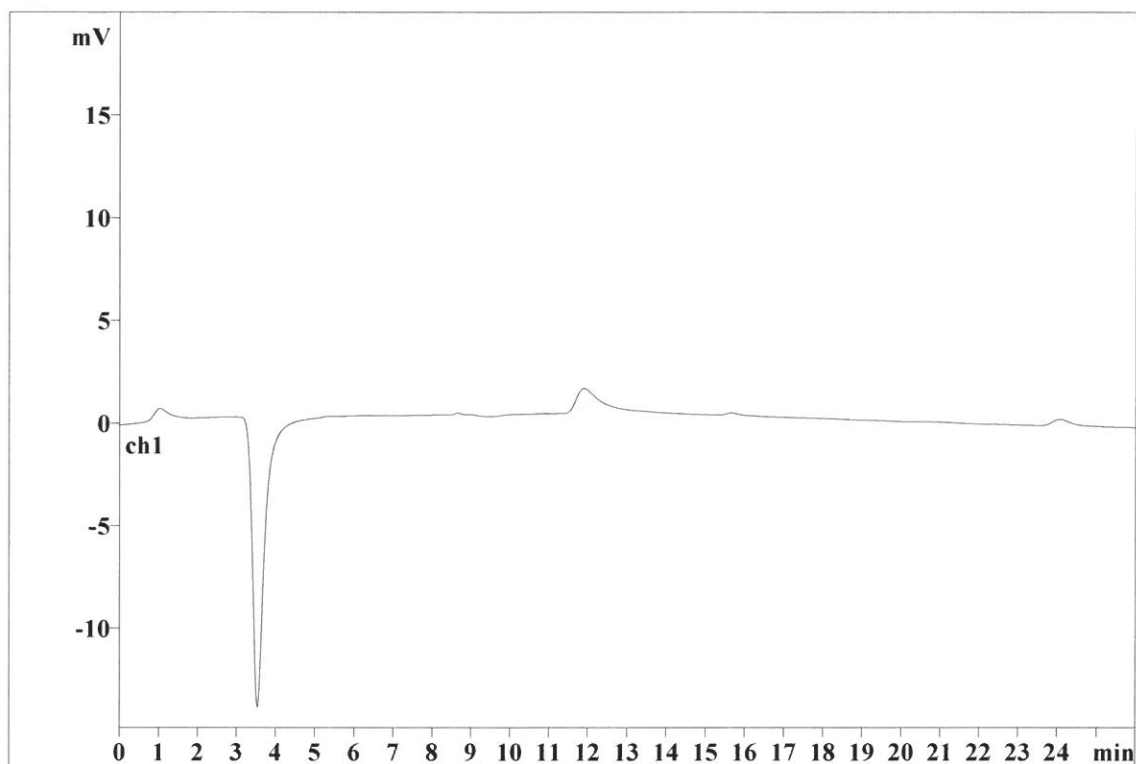

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 7/12/2021 3:22:24 PM
Printed by: wet


Ident: STD2
Analysis from: 7/9/2021 10:10:47 AM
File: _2021-07-09_

Last save: 7/12/2021 3:21:23 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27530

Last save: 7/9/2021 12:31:

SAMPLE:
: AM/AP
Vial number: 3
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

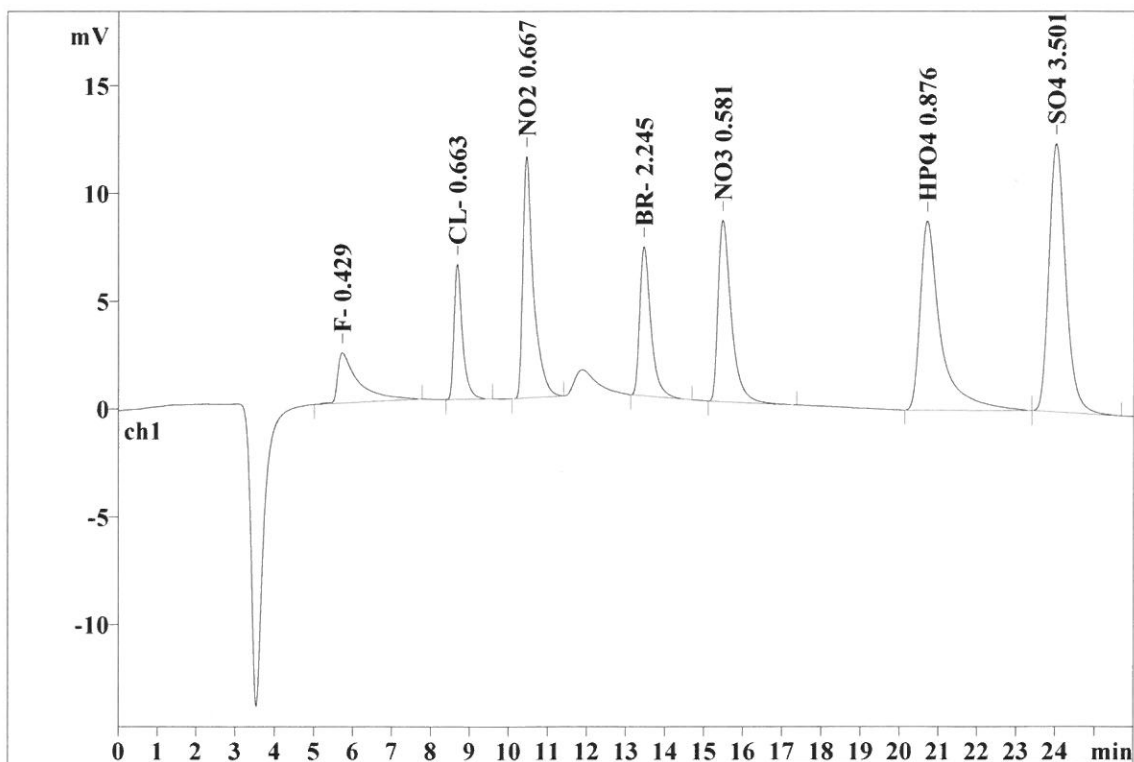

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.72	0.459	2.33	4.14	86.639	6.11
2	8.66	0.212	6.27	11.12	94.105	6.63
3	10.45	0.257	11.21	19.89	210.169	14.82
4	13.45	0.294	6.92	12.27	139.302	9.82
5	15.48	0.342	8.42	14.93	198.098	13.96
6	20.71	0.480	8.78	15.57	325.546	22.95
7	24.02	0.438	12.45	22.08	364.708	25.71
7	26.00	0.355	56.39	99.99	1418.567	100.00

This report has been created by IC Net
METROHM LTD

Report date: 7/12/2021 3:22:35 PM
Printed by: wet


Ident: STD3
Analysis from: 7/9/2021 10:39:23 AM
File: _2021-07-09_

Last save: 7/12/2021 3:21:23 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27531

Last save: 7/9/2021 12:31:

SAMPLE:
: AM/AP
Vial number: 4
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.72	0.442	5.02	4.45	183.476	6.60
2	8.66	0.211	12.68	11.24	188.743	6.79
3	10.43	0.260	22.26	19.73	419.875	15.11
4	13.40	0.288	14.18	12.57	281.364	10.13
5	15.40	0.338	17.08	15.14	397.403	14.30
6	20.70	0.461	16.61	14.72	586.574	21.11
7	24.02	0.431	24.99	22.15	721.152	25.95
7	26.00	0.347	112.82	99.99	2778.588	100.00

This report has been created by IC Net
METROHM LTD

Report date: 7/12/2021 3:22:45 PM
Printed by: wet


Ident: STD4
Analysis from: 7/9/2021 11:07:59 AM
File: _2021-07-09_

Last save: 7/12/2021 3:21:23 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27532

Last save: 7/9/2021 12:31:

SAMPLE:
: AM/AP
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

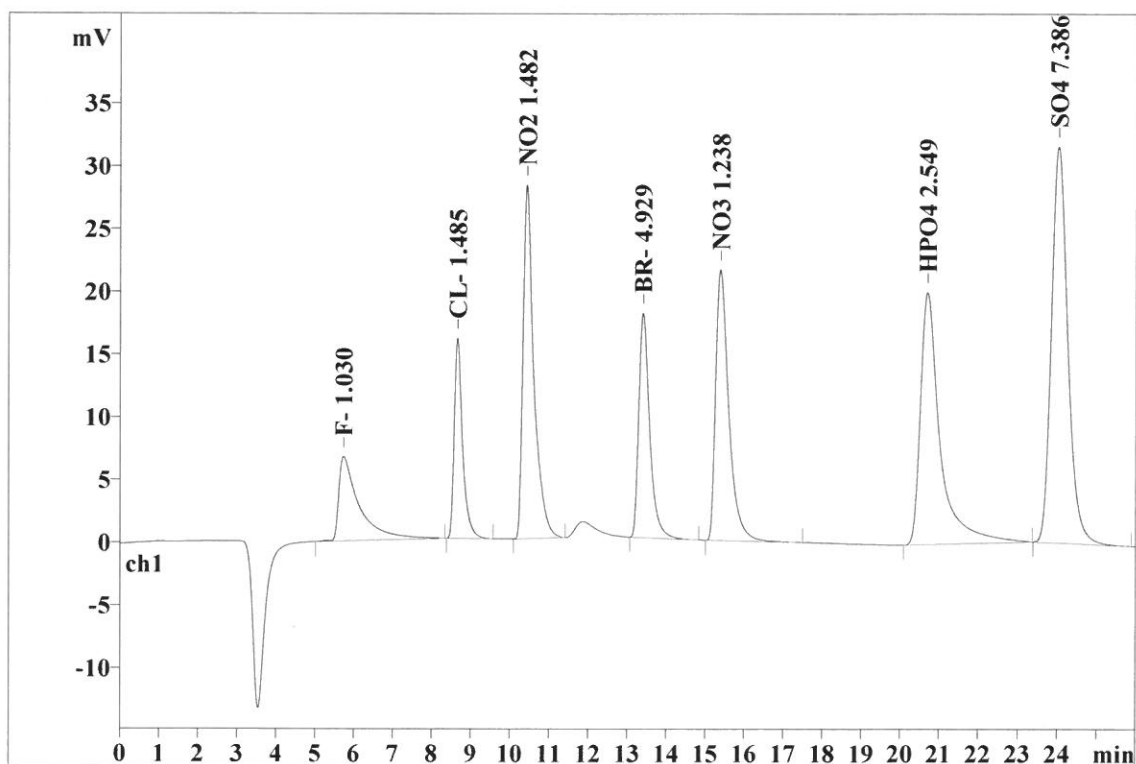

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.73	0.463	6.72	4.74	246.804	7.11
2	8.64	0.212	15.95	11.23	237.133	6.84
3	10.41	0.259	28.16	19.84	529.064	15.25
4	13.39	0.287	17.89	12.60	350.308	10.10
5	15.38	0.336	21.57	15.19	497.876	14.35
6	20.69	0.457	20.09	14.15	703.257	20.27
7	24.02	0.429	31.58	22.24	904.879	26.08
7	26.00	0.349	141.96	100.00	3469.319	100.00

This report has been created by IC Net
METROHM LTD

Report date: 7/12/2021 3:22:51 PM
Printed by: wet


Ident: STD5
Analysis from: 7/9/2021 11:36:37 AM
File: _2021-07-09_

Last save: 7/12/2021 3:21:23 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27533

Last save: 7/9/2021 12:31:

SAMPLE:
: AM/AP
Vial number: 6
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.71	0.419	14.65	5.02	491.359	7.06
2	8.62	0.207	33.19	11.38	485.218	6.98
3	10.38	0.260	57.52	19.73	1090.401	15.67
4	13.34	0.280	37.57	12.89	722.244	10.38
5	15.30	0.332	44.85	15.38	1024.583	14.73
6	20.68	0.444	37.65	12.91	1270.020	18.26
7	24.02	0.423	66.09	22.67	1872.658	26.92
7	26.00	0.338	291.51	100.00	6956.483	100.00

This report has been created by IC Net
METROHM LTD

Report date: 7/12/2021 3:22:58 PM
Printed by: wet


Ident: STD6
Analysis from: 7/9/2021 12:05:13 PM
File: _2021-07-09_

Last save: 7/12/2021 3:21:23 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27534

Last save: 7/9/2021 12:31:

SAMPLE:
: AM/AP
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

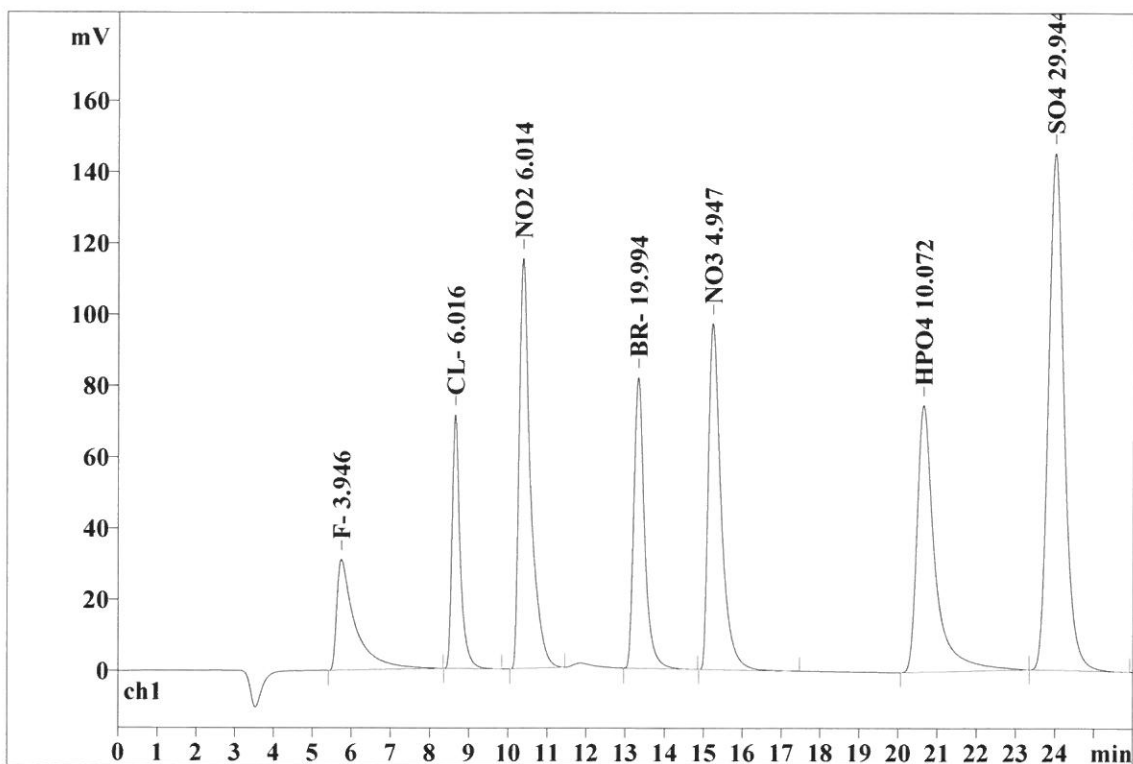

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.74	0.420	31.01	5.03	1023.332	7.05
2	8.63	0.203	71.27	11.56	1025.455	7.06
3	10.36	0.278	115.20	18.69	2302.532	15.86
4	13.31	0.273	81.68	13.25	1534.445	10.57
5	15.22	0.326	97.19	15.77	2191.307	15.09
6	20.63	0.428	74.91	12.15	2401.858	16.54
7	23.98	0.416	145.08	23.54	4041.385	27.83
7	26.00	0.335	616.34	100.00	14520.314	100.00

This report has been created by IC Net
METROHM LTD

Report date: 7/12/2021 3:23:05 PM
Printed by: wet


Ident: STD7
Analysis from: 7/9/2021 12:33:49 PM
File: _2021-07-09_

Last save: 7/12/2021 3:21:23 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27535

Last save: 7/9/2021 12:31:

SAMPLE:
: AM/AP
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

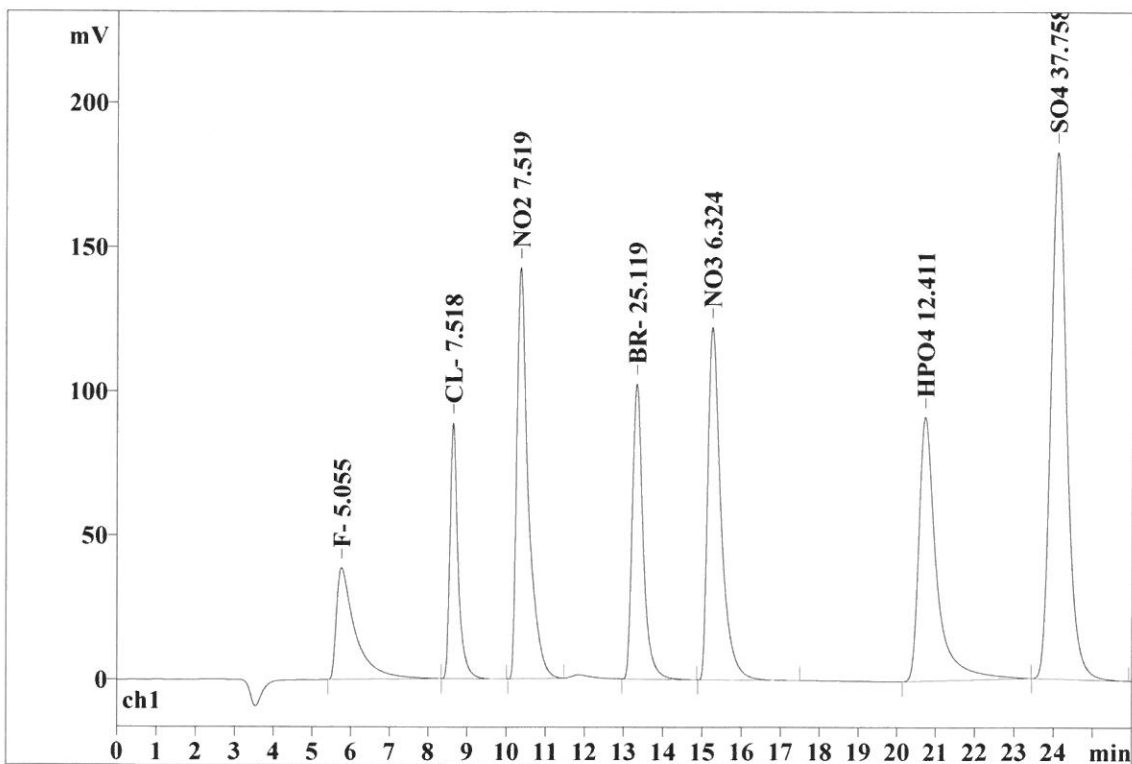

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.75	0.452	38.73	5.04	1318.856	7.20
2	8.62	0.204	88.63	11.53	1286.609	7.03
3	10.34	0.281	142.57	18.55	2891.454	15.79
4	13.32	0.275	102.34	13.31	1937.333	10.58
5	15.24	0.333	122.27	15.91	2820.037	15.40
6	20.71	0.429	91.49	11.90	2930.072	16.00
7	24.08	0.420	182.57	23.75	5127.796	28.00
7	26.00	0.342	768.59	100.00	18312.159	100.00

This report has been created by IC Net
METROHM LTD

Report date: 7/12/2021 3:23:12 PM
Printed by: wet


Ident: ICV
Analysis from: 7/9/2021 1:05:41 PM
File: _2021-07-09_

Last save: 7/9/2021 1:31:41 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27536

Last save: 7/9/2021 12:59:

SAMPLE:
: AM/AP
Vial number: 9
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

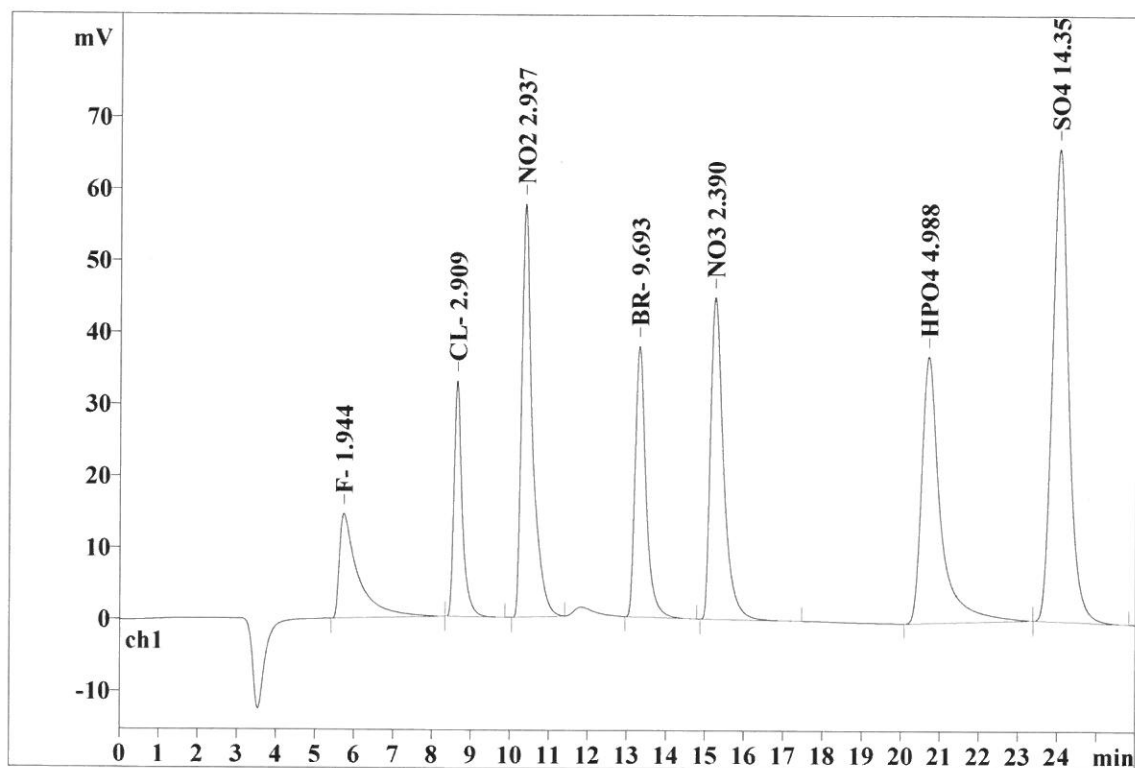

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.72	0.423	14.56	5.01	490.144	7.05
2	8.62	0.208	32.84	11.31	484.812	6.98
3	10.36	0.261	57.55	19.81	1098.352	15.80
4	13.29	0.280	37.73	12.99	724.773	10.43
5	15.23	0.331	44.83	15.43	1024.024	14.73
6	20.68	0.445	37.09	12.77	1254.043	18.04
7	24.02	0.425	65.85	22.67	1873.591	26.96
7	26.00	0.339	290.45	100.00	6949.740	100.00

This report has been created by IC Net
METROHM LTD

Report date: 7/12/2021 3:23:24 PM
Printed by: wet


Ident: ICB
Analysis from: 7/9/2021 1:34:44 PM
File: _2021-07-09_

Last save: 7/9/2021 2:00:44 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27537

Last save: 7/9/2021 12:59:

SAMPLE:
: AP/MA
Vial number: 10
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

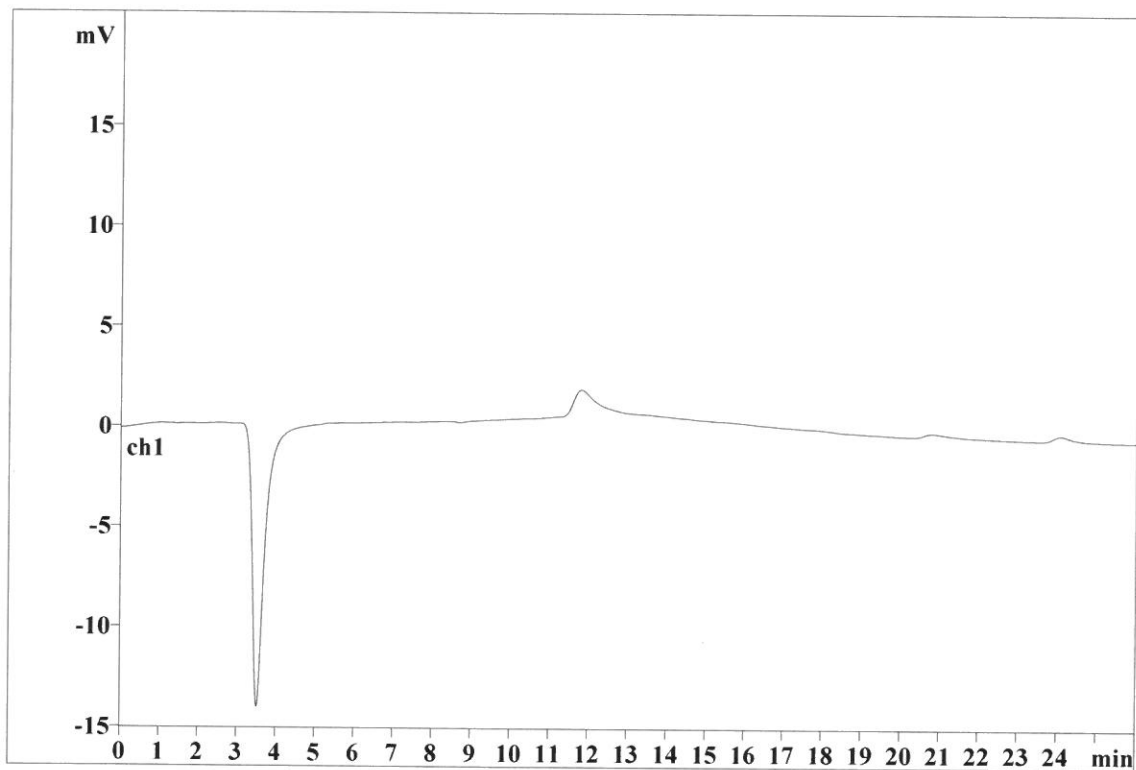

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 7/16/2021 3:15:33 PM
Printed by: wet


Ident: CCV
Analysis from: 7/16/2021 9:09:41 AM
File: _2021-07-16_

Last save: 7/16/2021 9:39:39 AM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27608

Last save: 7/12/2021 3:21:

SAMPLE:
: AP/MA
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.69	0.467	14.63	5.00	536.881	7.63
2	8.55	0.213	32.75	11.20	489.536	6.96
3	10.28	0.267	57.52	19.67	1103.357	15.68
4	13.21	0.280	37.93	12.97	727.986	10.35
5	15.14	0.333	44.99	15.39	1035.106	14.71
6	20.26	0.447	36.91	12.63	1255.245	17.84
7	23.36	0.416	67.65	23.14	1887.700	26.83
7	26.00	0.346	292.37	100.00	7035.810	100.00

This report has been created by IC Net
METROHM LTD

Report date: 7/16/2021 3:15:41 PM
Printed by: wet


Ident: CCB
Analysis from: 7/16/2021 9:42:20 AM
File: _2021-07-16_

Last save: 7/16/2021 10:08:20 AM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27609

Last save: 7/12/2021 3:21:

SAMPLE:
: AP/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 7/16/2021 3:16:23 PM
Printed by: wet


Ident: LB115386BLW
Analysis from: 7/16/2021 10:10:56 AM
File: _2021-07-16_

Last save: 7/16/2021 12:39:39 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27610

Last save: 7/12/2021 3:21:

SAMPLE:
: AP/MA
Vial number: 13
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 7/16/2021 3:16:30 PM
Printed by: wet


Ident: LB115386BSW
Analysis from: 7/16/2021 10:39:31 AM
File: _2021-07-16_

Last save: 7/16/2021 12:39:39 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27611

Last save: 7/12/2021 3:21:

SAMPLE:
: AP/MA
Vial number: 14
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.68	0.438	14.97	5.07	516.317	7.40
2	8.52	0.209	32.82	11.12	480.997	6.89
3	10.24	0.261	58.06	19.67	1090.503	15.62
4	13.12	0.275	38.20	12.94	716.919	10.27
5	15.02	0.326	45.39	15.37	1016.573	14.57
6	20.28	0.442	38.53	13.05	1298.765	18.61
7	23.41	0.414	67.24	22.78	1859.397	26.64
7	26.00	0.338	295.20	100.00	6979.470	100.00

This report has been created by IC Net
METROHM LTD

Report date: 7/16/2021 3:16:36 PM
Printed by: wet


Ident: M3086-01
Analysis from: 7/16/2021 11:57:48 AM
File: _2021-07-16_

Last save: 7/16/2021 12:39:57 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27614

Last save: 7/12/2021 3:21:

SAMPLE:
: AP/MA
Vial number: 15
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	0.00	0.000	0.00	0.00	0.000	0.00
3	10.26	0.252	1.41	19.03	26.358	15.69
4	0.00	0.000	0.00	0.00	0.000	0.00
5	15.09	0.329	5.55	74.76	126.377	75.20
6	0.00	0.000	0.00	0.00	0.000	0.00
7	23.50	0.470	0.46	6.15	15.312	9.11
7	26.00	0.150	7.42	99.94	168.047	100.00

This report has been created by IC Net
METROHM LTD

Report date: 7/16/2021 3:16:43 PM
Printed by: wet


Ident: M3086-02
Analysis from: 7/16/2021 12:26:24 PM
File: _2021-07-16_

Last save: 7/16/2021 1:25:12 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27615

Last save: 7/12/2021 3:21:

SAMPLE:
: AP/MA
Vial number: 16
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	8.50	0.196	0.45	6.18	6.184	3.73
3	10.24	0.259	0.37	5.07	8.648	5.22
4	0.00	0.000	0.00	0.00	0.000	0.00
5	15.05	0.327	5.81	80.10	131.118	79.11
6	0.00	0.000	0.00	0.00	0.000	0.00
7	23.47	0.462	0.62	8.56	19.796	11.94
7	26.00	0.178	7.24	99.91	165.746	100.00

This report has been created by IC Net
METROHM LTD

Report date: 7/16/2021 3:16:49 PM
Printed by: wet


Ident: M3086-03
Analysis from: 7/16/2021 12:54:59 PM
File: _2021-07-16_

Last save: 7/16/2021 1:25:32 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27616

Last save: 7/12/2021 3:21:

SAMPLE:
: AP/MA
Vial number: 17
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.65	0.438	0.60	18.38	17.593	21.29
2	0.00	0.000	0.00	0.00	0.000	0.00
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	15.06	0.333	2.36	71.74	54.030	65.38
6	0.00	0.000	0.00	0.00	0.000	0.00
7	23.49	0.482	0.32	9.78	11.012	13.33
7	26.00	0.179	3.28	99.91	82.636	100.00

This report has been created by IC Net
METROHM LTD

Report date: 7/16/2021 3:16:56 PM
Printed by: wet


Ident: M3086-03MS
Analysis from: 7/16/2021 1:23:35 PM
File: _2021-07-16_

Last save: 7/16/2021 2:47:46 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27617

Last save: 7/12/2021 3:21:

SAMPLE:
: AP/MA
Vial number: 18
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.69	0.469	15.80	5.15	569.585	7.90
2	8.49	0.208	34.37	11.19	502.005	6.96
3	10.19	0.260	59.91	19.51	1125.833	15.61
4	13.04	0.270	40.12	13.07	739.909	10.26
5	14.90	0.320	50.68	16.51	1116.035	15.48
6	20.30	0.441	36.51	11.89	1230.143	17.06
7	23.43	0.414	69.67	22.69	1926.860	26.72
7	26.00	0.340	307.07	100.00	7210.370	100.00

This report has been created by IC Net
METROHM LTD

Report date: 7/16/2021 3:17:03 PM
Printed by: wet


Ident: M3086-03MSD
Analysis from: 7/16/2021 1:52:10 PM
File: _2021-07-16_

Last save: 7/16/2021 2:48:35 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27618

Last save: 7/12/2021 3:21:

SAMPLE:
: AP/MA
Vial number: 19
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.66	0.432	15.25	5.25	521.774	7.68
2	8.47	0.208	32.41	11.15	473.668	6.97
3	10.17	0.260	56.46	19.43	1062.377	15.63
4	13.00	0.269	37.84	13.02	695.597	10.23
5	14.86	0.319	47.79	16.45	1048.146	15.42
6	20.28	0.438	35.48	12.21	1188.843	17.49
7	23.41	0.413	65.37	22.50	1807.919	26.59
7	26.00	0.334	290.59	100.00	6798.323	100.00

This report has been created by IC Net
METROHM LTD

Report date: 7/16/2021 3:17:10 PM
Printed by: wet


Ident: CCV
Analysis from: 7/16/2021 2:20:49 PM
File: _2021-07-16_

Last save: 7/16/2021 2:47:21 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27619

Last save: 7/12/2021 3:21:

SAMPLE:
: AP/MA
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.66	0.439	14.95	4.99	517.315	7.32
2	8.47	0.207	33.42	11.14	487.287	6.90
3	10.16	0.262	57.73	19.25	1093.196	15.48
4	12.98	0.270	39.41	13.14	727.409	10.30
5	14.84	0.319	47.02	15.68	1030.726	14.59
6	20.28	0.441	39.31	13.11	1327.384	18.79
7	23.41	0.413	68.04	22.69	1879.573	26.61
7	26.00	0.336	299.89	100.00	7062.889	100.00

This report has been created by IC Net
METROHM LTD

Report date: 7/16/2021 3:17:19 PM
Printed by: wet


Ident: CCB
Analysis from: 7/16/2021 2:49:24 PM
File: _2021-07-16_

Last save: 7/16/2021 3:15:24 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27620

Last save: 7/12/2021 3:21:

SAMPLE:
: AP/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD