


LB115401

7471B

INSTRUMENT ID: CV2

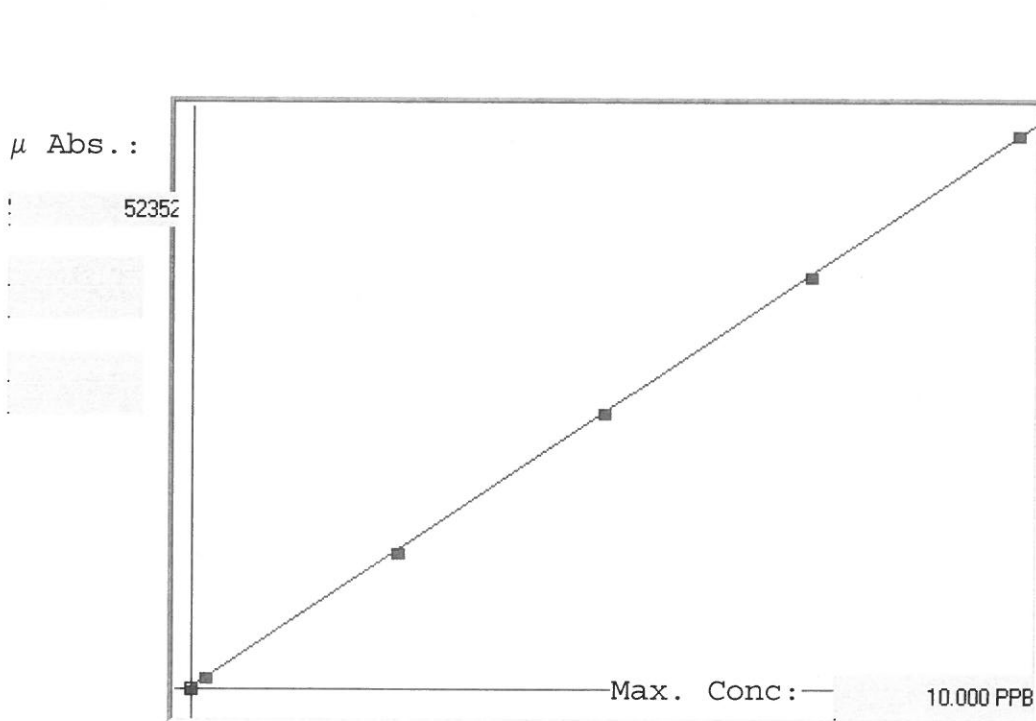

Linear

A= 0.0000e+000

B= 1.9186e-004

C= -1.6590e-002

Rho= 0.9999786

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.017	0.017	176	0.000	176					1
0.2	0.200	0.216	0.016	1212	0.0 %	1212					8
2.5	2.500	2.463	-0.037	12925	0.0 %	12925					-1
5.0	5.000	5.005	0.005	26171	0.0 %	26171					0
7.5	7.500	7.472	-0.028	39030	0.0 %	39030					0
10.0	10.000	10.028	0.028	52352	0.0 %	52352					0

LB115401 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 16 Jul 2021 16:01:46

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	SV	176	-	0.0000	7471B	PPB	16 Jul 2021 16:03:09	S	Std
0.2 - 1	SV2	1212	-	0.2000	7471B	PPB	16 Jul 2021 16:05:26	S	Std
2.5 - 1	SV2.5	12925	-	2.5000	7471B	PPB	16 Jul 2021 16:07:43	S	Std
5.0 - 1	SV5	26171	-	5.0000	7471B	PPB	16 Jul 2021 16:10:00	S	Std
7.5 - 1	SV7.5	39030	-	7.5000	7471B	PPB	16 Jul 2021 16:12:16	S	Std
10.0 - 1	SV10	52352	-	10.0000	7471B	PPB	16 Jul 2021 16:14:32	S	Std
ICV10 - 1	ICV10	21962	4.1970	-	7471B	PPB	16 Jul 2021 16:17:17	U	SMPL
ICB10 - 1	ICB10	145	0.0112	-	7471B	PPB	16 Jul 2021 16:19:32	U	SMPL
CCV84 - 1	CCV84	26205	5.0110	-	7471B	PPB	16 Jul 2021 16:21:48	U	SMPL
CCB84 - 1	CCB84	155	0.0131	-	7471B	PPB	16 Jul 2021 16:24:04	U	SMPL
CRA - 1	CRA	1176	0.2090	-	7471B	PPB	16 Jul 2021 16:26:19	U	SMPL
HighStd - 1	HighStd	51943	9.9491	-	7471B	PPB	16 Jul 2021 16:28:34	U	SMPL
ChkStd - 1	ChkStd	36494	6.9851	-	7471B	PPB	16 Jul 2021 16:30:49	U	SMPL
PB137766BL - 1	PBS	6	-0.0154	-	7471B	PPB	16 Jul 2021 16:33:06	U	SMPL
PB137766BS - 1	LCSS	22958	4.3881	-	7471B	PPB	16 Jul 2021 16:35:24	U	SMPL
M3051-01 - 1	41260	537	0.0864	-	7471B	PPB	16 Jul 2021 16:37:40	U	SMPL
M3051-08 - 1	41213	2439	0.4514	-	7471B	PPB	16 Jul 2021 16:39:57	U	SMPL
M3056-01 - 1	RO-VNJ-239	3425	0.6405	-	7471B	PPB	16 Jul 2021 16:42:14	U	SMPL
M3065-01 - 1	TR-04-071521	1822	0.3330	-	7471B	PPB	16 Jul 2021 16:49:30	U	SMPL
M3065-01DUP - 1	TR-04-071521DUP	1704	0.3103	-	7471B	PPB	16 Jul 2021 16:51:45	U	SMPL
CCV85 - 1	CCV85	25503	4.8764	-	7471B	PPB	16 Jul 2021 16:54:00	U	SMPL
CCB85 - 1	CCB85	156	0.0133	-	7471B	PPB	16 Jul 2021 16:56:15	U	SMPL
M3065-01MS - 1	TR-04-071521MS	22718	4.3420	-	7471B	PPB	16 Jul 2021 16:58:30	U	SMPL
M3065-01MSD - 1	TR-04-071521MSD	22302	4.2622	-	7471B	PPB	16 Jul 2021 17:00:45	U	SMPL
M3065-01LX5 - 1		474	0.0744	-	7471B	PPB	16 Jul 2021 17:03:00	U	SMPL
M3065-01A - 1		22308	4.2634	-	7471B	PPB	16 Jul 2021 17:05:16	U	SMPL
CCV86 - 1	CCV86	25409	4.8583	-	7471B	PPB	16 Jul 2021 17:07:31	U	SMPL
CCB86 - 1	CCB86	169	0.0158	-	7471B	PPB	16 Jul 2021 17:09:48	U	SMPL