

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : PS

Instrument ID : Konelab

7/19/2021 11:53

Test: ~~Total~~ CN *Reactive* *hml*

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	94.914	0.0	0.075	
ICB1	0.283	0.0	0.001	
CCV1	248.899	0.0	0.196	
CCB1	0.222	0.0	0.001	
PB137744BL	0.223	0.0	0.001	
M3038-13	0.001	0.0	0.001	
M3038-13DUP	0.083	0.0	0.001	
M3038-14	0.144	0.0	0.001	
M3038-15	-0.014	0.0	0.001	
M3038-16	0.307	0.0	0.001	
M3038-17	0.257	0.0	0.001	
M3039-15	0.234	0.0	0.001	
M3039-16	0.261	0.0	0.001	
M3039-17	0.286	0.0	0.001	
CCV2	249.348	0.0	0.196	
CCB2	0.491	0.0	0.001	
M3039-18	0.150	0.0	0.001	
M3039-19	0.242	0.0	0.001	
M3039-20	0.329	0.0	0.001	
M3039-21	0.354	0.0	0.001	
M3061-01	0.337	0.0	0.001	
PB137745BL	0.523	0.0	0.001	
M3061-02	0.424	0.0	0.001	
M3061-02DUP	0.311	0.0	0.001	
CCV3	254.722	0.0	0.200	
CCB3	-2.448	0.0	-0.001	

N	26
Mean	32.726
SD	82.5054
CV%	252.11

Aquakem v. 7.2AQ1

Results from time period:

Mon Jul 19 11:33:58 2021

Mon Jul 19 11:47:51 2021

Sample Id	Sam/Ctr/c/	Test short nam	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	-0.1948	µg/l	7/19/2021 9:26:26	
5.OPPBCN	A	Reactive CN	P	4.1785	µg/l	7/19/2021 9:26:27	
10PPBCN	A	Reactive CN	P	9.5691	µg/l	7/19/2021 9:26:28	
50PPBCN	A	Reactive CN	P	49.0295	µg/l	7/19/2021 9:26:29	
100PPBCN	A	Reactive CN	P	99.4789	µg/l	7/19/2021 9:26:30	
250PPBCN	A	Reactive CN	P	255.4415	µg/l	7/19/2021 9:26:31	
500PPBCN	A	Reactive CN	P	497.4973	µg/l	7/19/2021 9:26:32	
ICV1	S	Reactive CN	P	94.9141	µg/l	7/19/2021 11:33:59	
ICB1	S	Reactive CN	P	0.2831	µg/l	7/19/2021 11:34:00	
CCV1	S	Reactive CN	P	248.8987	µg/l	7/19/2021 11:34:03	
CCB1	S	Reactive CN	P	0.2216	µg/l	7/19/2021 11:34:05	
PB137744BL	S	Reactive CN	P	0.223	µg/l	7/19/2021 11:34:06	
M3038-13	S	Reactive CN	P	0.0012	µg/l	7/19/2021 11:34:07	
M3038-13DUPS		Reactive CN	P	0.083	µg/l	7/19/2021 11:34:08	
M3038-14	S	Reactive CN	P	0.144	µg/l	7/19/2021 11:41:33	
M3038-15	S	Reactive CN	P	-0.0135	µg/l	7/19/2021 11:41:34	
M3038-16	S	Reactive CN	P	0.3068	µg/l	7/19/2021 11:41:35	
M3038-17	S	Reactive CN	P	0.2567	µg/l	7/19/2021 11:41:36	
M3039-15	S	Reactive CN	P	0.234	µg/l	7/19/2021 11:41:37	
M3039-16	S	Reactive CN	P	0.2613	µg/l	7/19/2021 11:41:38	
M3039-17	S	Reactive CN	P	0.2861	µg/l	7/19/2021 11:41:39	
CCV2	S	Reactive CN	P	249.3481	µg/l	7/19/2021 11:41:40	
CCB2	S	Reactive CN	P	0.4915	µg/l	7/19/2021 11:41:41	
M3039-18	S	Reactive CN	P	0.1496	µg/l	7/19/2021 11:41:42	
M3039-19	S	Reactive CN	P	0.2416	µg/l	7/19/2021 11:41:43	
M3039-20	S	Reactive CN	P	0.3295	µg/l	7/19/2021 11:47:44	
M3039-21	S	Reactive CN	P	0.354	µg/l	7/19/2021 11:47:45	
M3061-01	S	Reactive CN	P	0.3365	µg/l	7/19/2021 11:47:46	
PB137745BL	S	Reactive CN	P	0.5233	µg/l	7/19/2021 11:47:47	
M3061-02	S	Reactive CN	P	0.4241	µg/l	7/19/2021 11:47:48	
M3061-02DUPS		Reactive CN	P	0.3107	µg/l	7/19/2021 11:47:49	
CCV3	S	Reactive CN	P	254.722	µg/l	7/19/2021 11:47:50	
CCB3	S	Reactive CN	P	-2.4476	µg/l	7/19/2021 11:47:51	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : Instrument ID : Konelab

7/19/2021 9:27


Test Total CN

Accepted 7/19/2021 9:27

Factor 1276
Bias 0.001

Coeff. of det. 0.999815

Errors

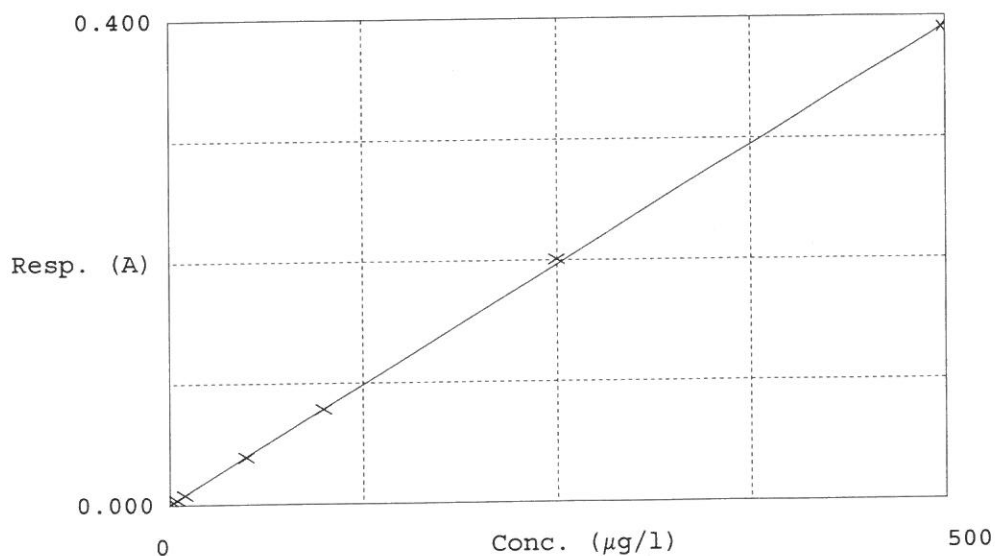

					Relative
					Errors
Calibrator	Response	Calc. con.	Conc.		
1	0.0PPBCN	0.001	-0.1948	0.0000	-16.4
2	5.0PPBCN	0.004	4.1785	5.0000	-2.3
3	10PPBCN	0.008	9.5691	10.0000	-1.9
4	50PPBCN	0.039	49.0295	50.0000	-0.5
5	100PPBCN	0.079	99.4789	100.0000	2.2
6	250PPBCN	0.201	255.4415	250.0000	-0.5
7	500PPBCN	0.390	497.4973	500.0000	