


LB115459

7470A

INSTRUMENT ID: CV1

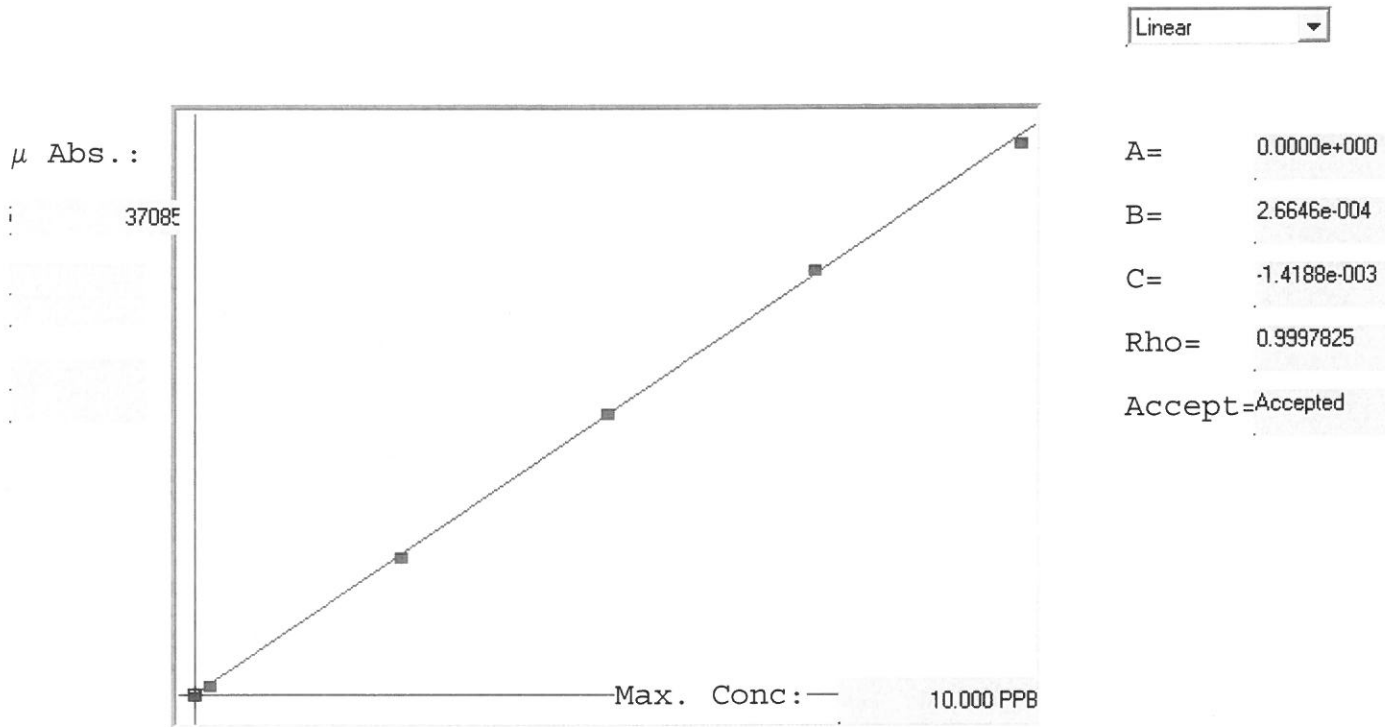

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	0/00
0.0	0.000	-0.021	-0.021	-74	0.000	-74					-6
0.2	0.200	0.188	-0.012	710	0.0 %	710					-1
2.5	2.500	2.468	-0.032	9267	0.0 %	9267					-1
5.0	5.000	5.058	0.058	18987	0.0 %	18987					2
7.5	7.500	7.627	0.127	28630	0.0 %	28630					-1
10.0	10.000	9.880	-0.120	37085	0.0 %	37085					

LB115459 INSTRUMENT ID :CV1

Method: 7470A

Operator: Admin

Date of Analysis: 21 Jul 2021 15:09:40

Sample ID	Extended ID	μ Abs.	Conc.	Std CondMethod	Units	Date	Type	Type
0.0 - 1	50	-74	-	0.00007470A	PPB	21 Jul 2021 15:27:19	S	Std
0.2 - 1	50.2	710	-	0.20007470A	PPB	21 Jul 2021 15:29:36	S	Std
2.5 - 1	52.5	9267	-	2.50007470A	PPB	21 Jul 2021 15:31:53	S	Std
5.0 - 1	55	18987	-	5.00007470A	PPB	21 Jul 2021 15:34:09	S	Std
7.5 - 1	57.5	28630	-	7.50007470A	PPB	21 Jul 2021 15:36:26	S	Std
10.0 - 1	510	37085	-	10.00007470A	PPB	21 Jul 2021 15:38:42	S	Std
ICV14 - 1	ICV14	14572	3.8814	-7470A	PPB	21 Jul 2021 15:41:35	U	SMPL
ICB14 - 1	ICB14	-66	-0.0190	-7470A	PPB	21 Jul 2021 15:43:50	U	SMPL
CCV01 - 1	CCV01	18995	5.0600	-7470A	PPB	21 Jul 2021 15:46:05	U	SMPL
CCB01 - 1	CCB01	-64	-0.0185	-7470A	PPB	21 Jul 2021 15:48:19	U	SMPL
CRA - 1	CRA	716	0.1894	-7470A	PPB	21 Jul 2021 15:50:34	U	SMPL
HighStd - 1	HighStd	37314	9.9413	-7470A	PPB	21 Jul 2021 15:52:49	U	SMPL
ChkStd - 1	ChkStd	26347	7.0190	-7470A	PPB	21 Jul 2021 15:55:04	U	SMPL
PB137855BL - 1	PBW	-151	-0.0417	-7470A	PPB	21 Jul 2021 15:57:19	U	SMPL
PB137855BS - 1	LCSW	12778	3.4034	-7470A	PPB	21 Jul 2021 15:59:35	U	SMPL
M3114-06 - 1	20210516-FIELD-BLANK-2	-97	-0.0273	-7470A	PPB	21 Jul 2021 16:01:51	U	SMPL
M3120-02 - 1	TT-RW6B-IDWGW-20210719	-34	-0.0105	-7470A	PPB	21 Jul 2021 16:04:07	U	SMPL
M3120-03 - 1	TT-RW6A-IDWGW-20210720	-13	-0.0049	-7470A	PPB	21 Jul 2021 16:06:24	U	SMPL
M3120-03DUP - 1	TT-RW6A-IDWGW-20210720DUP	-5	-0.0028	-7470A	PPB	21 Jul 2021 16:08:41	U	SMPL
M3120-03MS - 1	TT-RW6A-IDWGW-20210720MS	13115	3.4932	-7470A	PPB	21 Jul 2021 16:13:25	U	SMPL
CCV02 - 1	CCV02	18863	5.0248	-7470A	PPB	21 Jul 2021 16:15:39	U	SMPL
CCB02 - 1	CCB02	-78	-0.0222	-7470A	PPB	21 Jul 2021 16:17:55	U	SMPL
M3120-03MSD - 1	TT-RW6A-IDWGW-20210720MSD	13707	3.6510	-7470A	PPB	21 Jul 2021 16:20:10	U	SMPL
M3120-03LX5 - 1		-109	-0.0305	-7470A	PPB	21 Jul 2021 16:22:25	U	SMPL
M3120-03A - 1		14636	3.8985	-7470A	PPB	21 Jul 2021 16:24:40	U	SMPL
CCV03 - 1	CCV03	19193	5.1128	-7470A	PPB	21 Jul 2021 16:26:55	U	SMPL
CCB03 - 1	CCB03	-83	-0.0235	-7470A	PPB	21 Jul 2021 16:29:11	U	SMPL