


LB 115473

7471B

INSTRUMENT ID: CV2

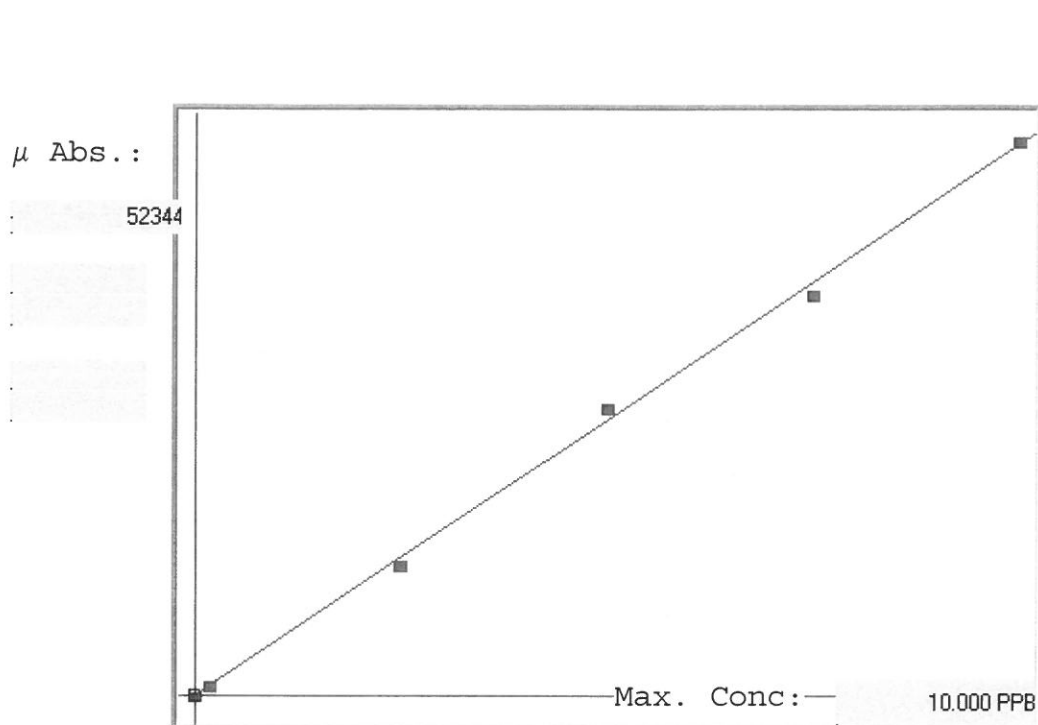

Linear

A= 0.0000e+000

B= 1.9194e-004

C= 6.5127e-003

Rho= 0.9993674

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.021	0.021	73	0.000	73					0
0.2	0.200	0.200	0.000	1009	0.0 %	1009					-4
2.5	2.500	2.404	-0.096	12493	0.0 %	12493					4
5.0	5.000	5.224	0.224	27182	0.0 %	27182					-3
7.5	7.500	7.298	-0.202	37988	0.0 %	37988					1
10.0	10.000	10.053	0.053	52344	0.0 %	52344					

LB115473 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 22 Jul 2021 09:13:28

Sample ID	Extended ID	µ Abs	Conc	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	73	-	0.0000	7471B	PPB	22 Jul 2021 09:22:55	S	Std
0.2 - 1	50.2	1009	-	0.2000	7471B	PPB	22 Jul 2021 09:25:12	S	Std
2.5 - 1	52.5	12493	-	2.5000	7471B	PPB	22 Jul 2021 09:27:29	S	Std
5.0 - 1	55	27182	-	5.0000	7471B	PPB	22 Jul 2021 09:29:45	S	Std
7.5 - 1	57.5	37988	-	7.5000	7471B	PPB	22 Jul 2021 09:32:02	S	Std
10.0 - 1	59.0	52344	-	10.0000	7471B	PPB	22 Jul 2021 09:37:01	S	Std
ICV15 - 1	ICV15	20401	3.9222	-	7471B	PPB	22 Jul 2021 09:42:42	U	SMPL
ICB15 - 1	ICB15	-71	-0.0071	-	7471B	PPB	22 Jul 2021 09:44:56	U	SMPL
CCV04 - 1	CCV04	27582	5.3005	-	7471B	PPB	22 Jul 2021 09:47:11	U	SMPL
CCB04 - 1	CCB04	-85	-0.0098	-	7471B	PPB	22 Jul 2021 09:49:26	U	SMPL
CRA - 1	CRA	965	0.1917	-	7471B	PPB	22 Jul 2021 09:51:41	U	SMPL
HighStd - 1	HighStd	53010	10.1811	-	7471B	PPB	22 Jul 2021 09:53:55	U	SMPL
ChkStd - 1	ChkStd	35887	6.8946	-	7471B	PPB	22 Jul 2021 09:56:10	U	SMPL
PB137856BL - 1	PBS	-146	-0.0215	-	7471B	PPB	22 Jul 2021 09:58:27	U	SMPL
PB137856BS - 1	LCSS	20718	3.9831	-	7471B	PPB	22 Jul 2021 10:00:44	U	SMPL
M3098-01 - 1	F0604S	5302	1.0242	-	7471B	PPB	22 Jul 2021 10:03:00	U	SMPL
M3114-01 - 1	20210541-COM-14	27780	5.3385	-	7471B	PPB	22 Jul 2021 10:05:16	U	SMPL
M3114-02 - 1	20210550-COM-23	23538	4.5243	-	7471B	PPB	22 Jul 2021 10:07:33	U	SMPL
M3114-03 - 1	20210559-COM-32	24656	4.7389	-	7471B	PPB	22 Jul 2021 10:09:49	U	SMPL
M3114-04 - 1	20210585-COM-8	21586	4.1497	-	7471B	PPB	22 Jul 2021 10:12:06	U	SMPL
CCV05 - 1	CCV05	26075	5.0113	-	7471B	PPB	22 Jul 2021 10:14:21	U	SMPL
CCB05 - 1	CCB05	-96	-0.0119	-	7471B	PPB	22 Jul 2021 10:16:36	U	SMPL
M3114-05 - 1	20210594-AMENDED-COM-8	27921	5.3656	-	7471B	PPB	22 Jul 2021 10:18:51	U	SMPL
M3114-05DUP - 1	20210594-AMENDED-COM-8DUP	24995	4.8040	-	7471B	PPB	22 Jul 2021 10:21:06	U	SMPL
M3114-05MS - 1	20210594-AMENDED-COM-8MS	48069	9.2328	-	7471B	PPB	22 Jul 2021 10:25:59	U	SMPL
M3114-05MSD - 1	20210594-AMENDED-COM-8MSD	49966	9.5969	-	7471B	PPB	22 Jul 2021 10:30:51	U	SMPL
M3117-01 - 1	NJ-CLEAN-1	1085	0.2148	-	7471B	PPB	22 Jul 2021 10:33:07	U	SMPL
M3117-02 - 1	NJ-CLEAN-2	933	0.1856	-	7471B	PPB	22 Jul 2021 10:35:24	U	SMPL
M3117-03 - 1	NJ-CLEAN-3	1502	0.2948	-	7471B	PPB	22 Jul 2021 10:37:41	U	SMPL
M3117-04 - 1	NJ-CLEAN-4	913	0.1818	-	7471B	PPB	22 Jul 2021 10:39:58	U	SMPL
M3117-05 - 1	NJ-CLEAN-5	1577	0.3092	-	7471B	PPB	22 Jul 2021 10:42:15	U	SMPL
M3117-06 - 1	NJ-CLEAN-6	845	0.1687	-	7471B	PPB	22 Jul 2021 10:44:30	U	SMPL
CCV06 - 1	CCV06	26634	5.1186	-	7471B	PPB	22 Jul 2021 10:46:46	U	SMPL
CCB06 - 1	CCB06	-79	-0.0087	-	7471B	PPB	22 Jul 2021 10:49:01	U	SMPL
M3117-07 - 1	NJ-CLEAN-7	1116	0.2207	-	7471B	PPB	22 Jul 2021 10:51:16	U	SMPL
M3117-08 - 1	NJ-CLEAN-8	784	0.1570	-	7471B	PPB	22 Jul 2021 10:53:32	U	SMPL
M3117-09 - 1	NJ-CLEAN-9	1479	0.2904	-	7471B	PPB	22 Jul 2021 10:55:47	U	SMPL
M3118-01 - 1	20210546-COM-19	10650	2.0506	-	7471B	PPB	22 Jul 2021 10:58:02	U	SMPL
M3118-02 - 1	20210563-COM-36	4088	0.7912	-	7471B	PPB	22 Jul 2021 11:00:18	U	SMPL
M3118-03 - 1	20210579-COM-2	12294	2.3662	-	7471B	PPB	22 Jul 2021 11:02:35	U	SMPL
M3118-04 - 1	20210588-AMENDED-COM-2	6672	1.2871	-	7471B	PPB	22 Jul 2021 11:04:51	U	SMPL
M3128-01 - 1	ETGI-358	223712	42.9453	-	7471B	PPB	22 Jul 2021 11:07:08	U	SMPL
M3114-05LX5 - 1		4811	0.9299	-	7471B	PPB	22 Jul 2021 11:09:25	U	SMPL
M3114-05A - 1		45593	8.7575	-	7471B	PPB	22 Jul 2021 11:11:43	U	SMPL
CCV07 - 1	CCV07	25974	4.9919	-	7471B	PPB	22 Jul 2021 11:13:58	U	SMPL
CCB07 - 1	CCB07	-80	-0.0088	-	7471B	PPB	22 Jul 2021 11:16:15	U	SMPL
M3128-01DLX10 - 1		23625	4.5410	-	7471B	PPB	22 Jul 2021 11:18:30	U	SMPL
CCV08 - 1	CCV08	26804	5.1512	-	7471B	PPB	22 Jul 2021 11:20:45	U	SMPL
CCB08 - 1	CCB08	-85	-0.0098	-	7471B	PPB	22 Jul 2021 11:23:01	U	SMPL