


LB115503

245.1

INSTRUMENT ID: CV1

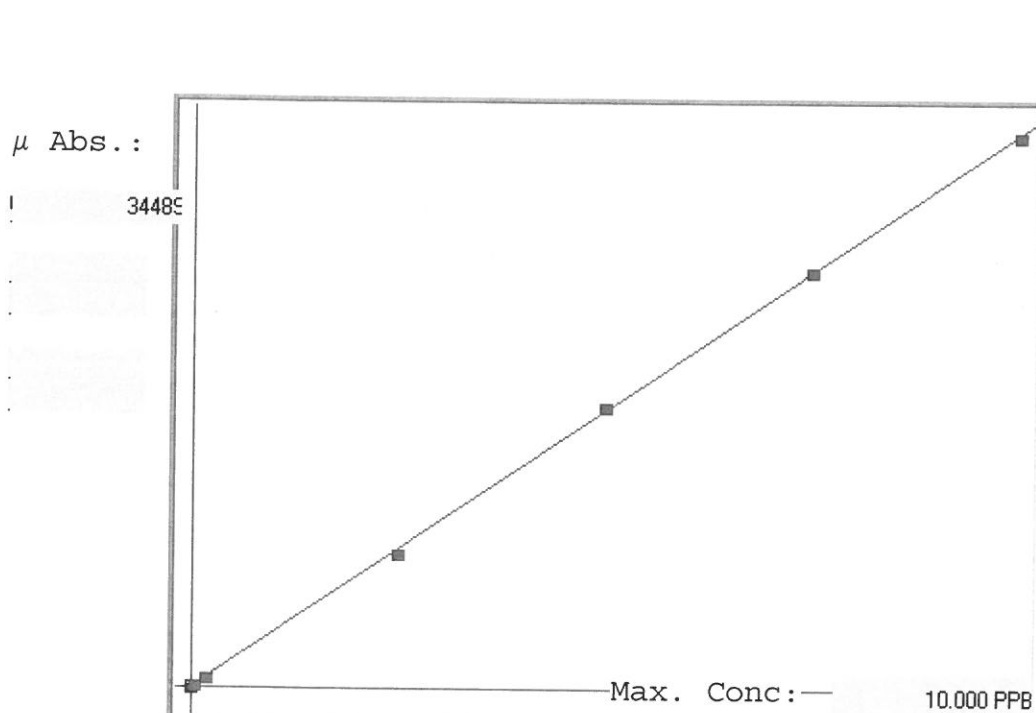

Linear

A= 0.0000e+000

B= 2.8883e-004

C= -3.5339e-003

Rho= 0.9999381

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	0/0/0
0.0	0.000	0.004	0.004	25	0.000	25					
0.05	0.050	0.049	-0.001	183	0.0 %	183	0				-2
0.2	0.200	0.197	-0.003	695	0.0 %	695					-2
2.5	2.500	2.441	-0.059	8465	0.0 %	8465					-2
5.0	5.000	5.079	0.079	17597	0.0 %	17597					2
7.5	7.500	7.522	0.022	26054	0.0 %	26054					0
10.0	10.000	9.958	-0.042	34489	0.0 %	34489					0

LB115503 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 23 Jul 2021 13:46:32

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	25	-	0.0000	245.1	PPB	23 Jul 2021 13:53:21	S	Std
0.05 - 1	50.05	183	-	0.0500	245.1	PPB	23 Jul 2021 13:55:37	S	Std
0.2 - 1	50.2	695	-	0.2000	245.1	PPB	23 Jul 2021 13:57:55	S	Std
2.5 - 1	52.5	8465	-	2.5000	245.1	PPB	23 Jul 2021 14:00:11	S	Std
5.0 - 1	55	17597	-	5.0000	245.1	PPB	23 Jul 2021 14:02:28	S	Std
7.5 - 1	57.5	26054	-	7.5000	245.1	PPB	23 Jul 2021 14:04:43	S	Std
10.0 - 1	510	34489	-	10.0000	245.1	PPB	23 Jul 2021 14:23:41	S	Std
ICV18 - 1	ICV18	13928	4.0193	-245.1		PPB	23 Jul 2021 14:26:26	U	SMPL
ICB18 - 1	ICB18	-75	-0.0252	-245.1		PPB	23 Jul 2021 14:28:41	U	SMPL
CCV17 - 1	CCV17	17963	5.1847	-245.1		PPB	23 Jul 2021 14:30:56	U	SMPL
CCB17 - 1	CCB17	-69	-0.0235	-245.1		PPB	23 Jul 2021 14:33:11	U	SMPL
CRA - 1	CRA	169	0.0453	-245.1		PPB	23 Jul 2021 14:35:25	U	SMPL
HighStd - 1	HighStd	34329	9.9116	-245.1		PPB	23 Jul 2021 14:37:40	U	SMPL
ChkStd - 1	ChkStd	25279	7.2977	-245.1		PPB	23 Jul 2021 14:39:55	U	SMPL
PB137920BL - 1	PBW	-21	-0.0096	-245.1		PPB	23 Jul 2021 14:45:02	U	SMPL
PB137920BS - 1	LCSW	13750	3.9678	-245.1		PPB	23 Jul 2021 14:47:18	U	SMPL
M3110-01 - 1	MANHOLE	87	0.0216	-245.1		PPB	23 Jul 2021 14:51:50	U	SMPL
M3132-01 - 1	55-ST-32	27	0.0043	-245.1		PPB	23 Jul 2021 14:54:07	U	SMPL
M3132-01DUP - 1	55-ST-32DUP	36	0.0069	-245.1		PPB	23 Jul 2021 14:56:24	U	SMPL
M3132-01MS - 1	55-ST-32MS	15206	4.3884	-245.1		PPB	23 Jul 2021 14:58:39	U	SMPL
CCV18 - 1	CCV18	17865	5.1564	-245.1		PPB	23 Jul 2021 15:00:54	U	SMPL
CCB18 - 1	CCB18	-72	-0.0243	-245.1		PPB	23 Jul 2021 15:03:09	U	SMPL
M3132-01MSD - 1	55-ST-32MSD	14856	4.2873	-245.1		PPB	23 Jul 2021 15:05:24	U	SMPL
M3035-05 - 1	PT-HG-WS	5569	1.6049	-245.1		PPB	23 Jul 2021 15:07:39	U	SMPL
M3132-01LX5 - 1		-25	-0.0108	-245.1		PPB	23 Jul 2021 15:12:10	U	SMPL
M3132-01A - 1		14936	4.3104	-245.1		PPB	23 Jul 2021 15:14:26	U	SMPL
CCV19 - 1	CCV19	18085	5.2199	-245.1		PPB	23 Jul 2021 15:16:42	U	SMPL
CCB19 - 1	CCB19	-52	-0.0186	-245.1		PPB	23 Jul 2021 15:18:58	U	SMPL