


Clear table

Instrument ID: IC-2 Analyst: AP Method: 300.0 / 9056A

ident	concentratio tion F-	concentratio n CL-	concentratio on NO2	concentratio on BR-	concentratio on NO3	concentratio on HPO4	concentratio on SO4	file name	date time	Initial wt/ Final Vol	Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-07-09_	7/9/21 9:42		AP/MA
STD2	0.4290	0.6630	0.6670	2.2450	0.5810	0.8760	3.5010	2021-07-09_	7/9/21 10:10		AP/MA
STD3	0.7920	1.2070	1.2030	4.0520	1.0180	2.0320	6.0650	2021-07-09_	7/9/21 10:39		AP/MA
STD4	1.0300	1.4850	1.4820	4.9290	1.2380	2.5490	7.3860	2021-07-09_	7/9/21 11:07		AP/MA
STD5	1.9480	2.9110	2.9160	9.6610	2.3920	5.0590	14.3460	2021-07-09_	7/9/21 11:36		AP/MA
STD6	3.9460	6.0160	6.0140	19.9940	4.9470	10.0720	29.9440	2021-07-09_	7/9/21 12:05		AP/MA
STD7	5.0550	7.5180	7.5190	25.1190	6.3240	12.4110	37.7580	2021-07-09_	7/9/21 12:33		AP/MA
ICV	1.9440	2.9090	2.9370	9.6930	2.3900	4.9880	14.3530	2021-07-09_	7/9/21 13:05		AP/MA
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-07-09_	7/9/21 13:34		AP/MA
CCV	2.0970	2.9670	2.8630	9.7670	2.4110	4.8130	14.4390	2021-07-23_	7/23/21 9:18		AP/MA
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-07-23_	7/23/21 10:10		AP/MA
LB115504BLS	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-07-23_	7/23/21 10:39	5.00G/100n	AP/MA
LB115504BSS	2.1170	3.0040	2.9170	9.8430	2.4360	4.9730	14.5980	2021-07-23_	7/23/21 11:07	5.00G/100n	AP/MA
M3151-01	0.3160	0.7910	0.0000	0.0000	0.1670	0.0000	1.4660	2021-07-23_	7/23/21 11:55	5.06g/100n	AP/MA
M3151-02	0.2440	0.9480	0.0000	0.0000	0.0000	-0.4960	1.7580	2021-07-23_	7/23/21 12:42	5.25g/100r	AP/MA
M3151-03	0.2740	0.7550	0.0000	0.0000	0.0000	0.0000	1.9270	2021-07-23_	7/23/21 13:11	5.21g/100r	AP/MA
M3151-03MS	2.4080	3.7050	2.9790	9.9320	2.4650	5.5650	15.8500	2021-07-23_	7/23/21 13:39	5.20g/100r	AP/MA
M3151-03MSD	2.3340	3.6910	2.9800	9.9470	2.4680	5.8170	15.8420	2021-07-23_	7/23/21 14:08	5.22g/100r	AP/MA
CCV	2.1180	3.0500	3.0000	10.0780	2.4950	5.5420	14.9240	2021-07-23_	7/23/21 14:37		AP/MA
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-07-23_	7/23/21 15:44		AP/MA

CALIBRATION OF COMPONENT F-

Method: AnionsIC2-070921.mtw
 Equation: $Q = 0.0750899 \cdot A + 2.06898$
 RSD: 2.325 %
 Correlation coefficient: 0.999705

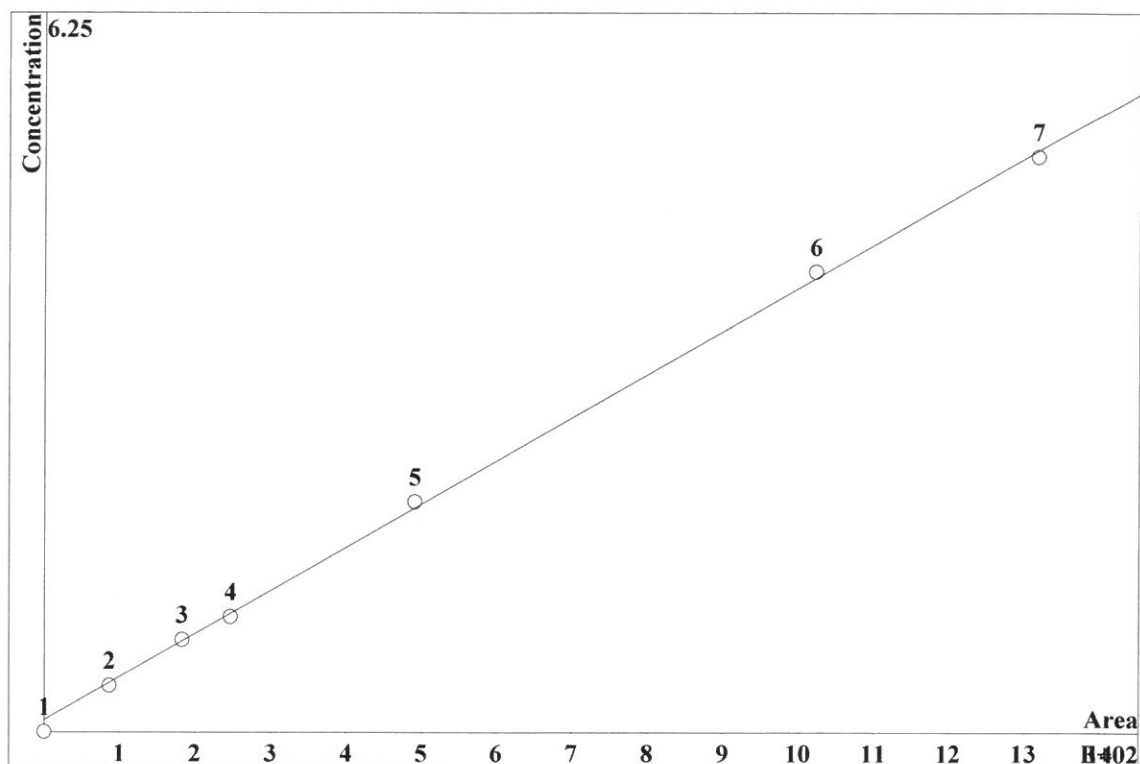

K3 = 0 K2 = 0 K1 = 0.0750899 K0 = 2.06898

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	2.336	86.64	0.4	20	5.75		
3	5.02	183.5	0.8	20	5.75		
4	6.724	246.8	1	20	5.75		
5	14.65	491.4	2	20	5.75		
6	31.01	1023	4	20	5.75		
7	38.73	1319	5	20	5.75		

CALIBRATION OF COMPONENT CL-

Method: AnionsIC2-070921.mtw
 Equation: $Q = 0.114962 \cdot A + 2.44005$
 RSD: 1.709 %
 Correlation coefficient: 0.999841

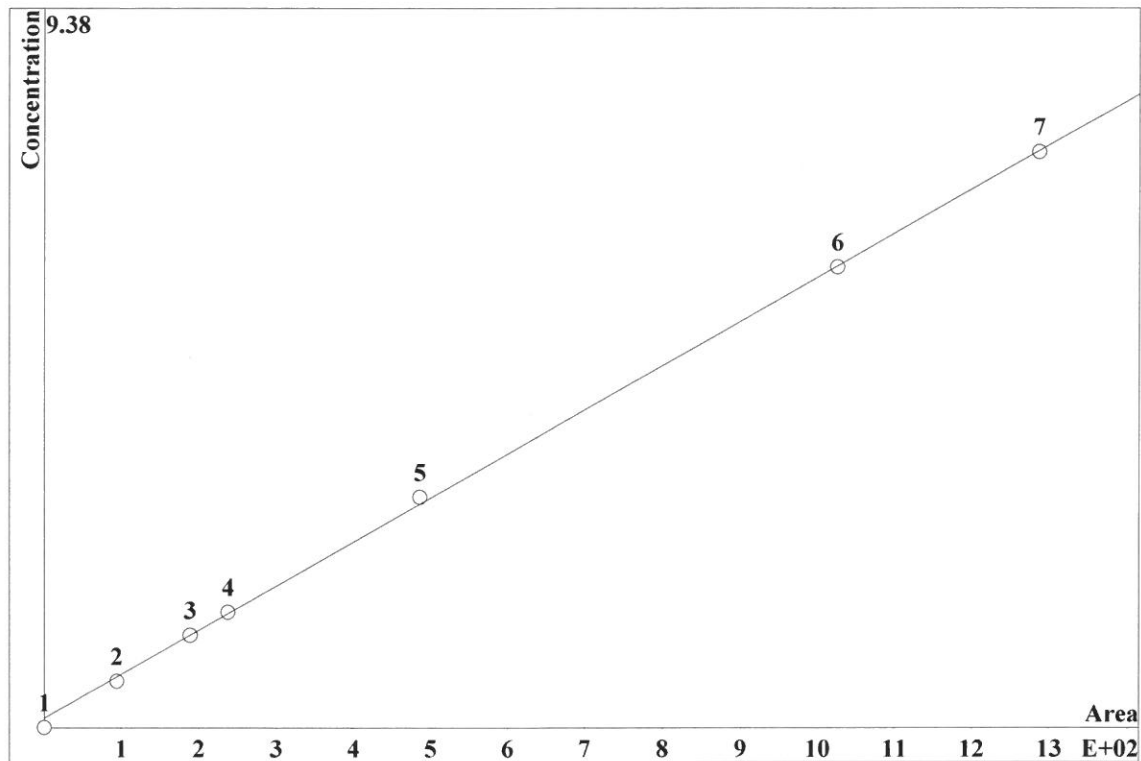

K3 = 0 K2 = 0 K1 = 0.114962 K0 = 2.44005

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	6.27	94.1	0.6	20	8.834		
3	12.68	188.7	1.2	20	8.834		
4	15.95	237.1	1.5	20	8.834		
5	33.19	485.2	3	20	8.834		
6	71.27	1025	6	20	8.834		
7	88.63	1287	7.5	20	8.834		

CALIBRATION OF COMPONENT NO2

Method: AnionsIC2-070921.mtw
 Equation: $Q = 0.051109 \cdot A + 2.59501$
 RSD: 1.685 %
 Correlation coefficient: 0.999845

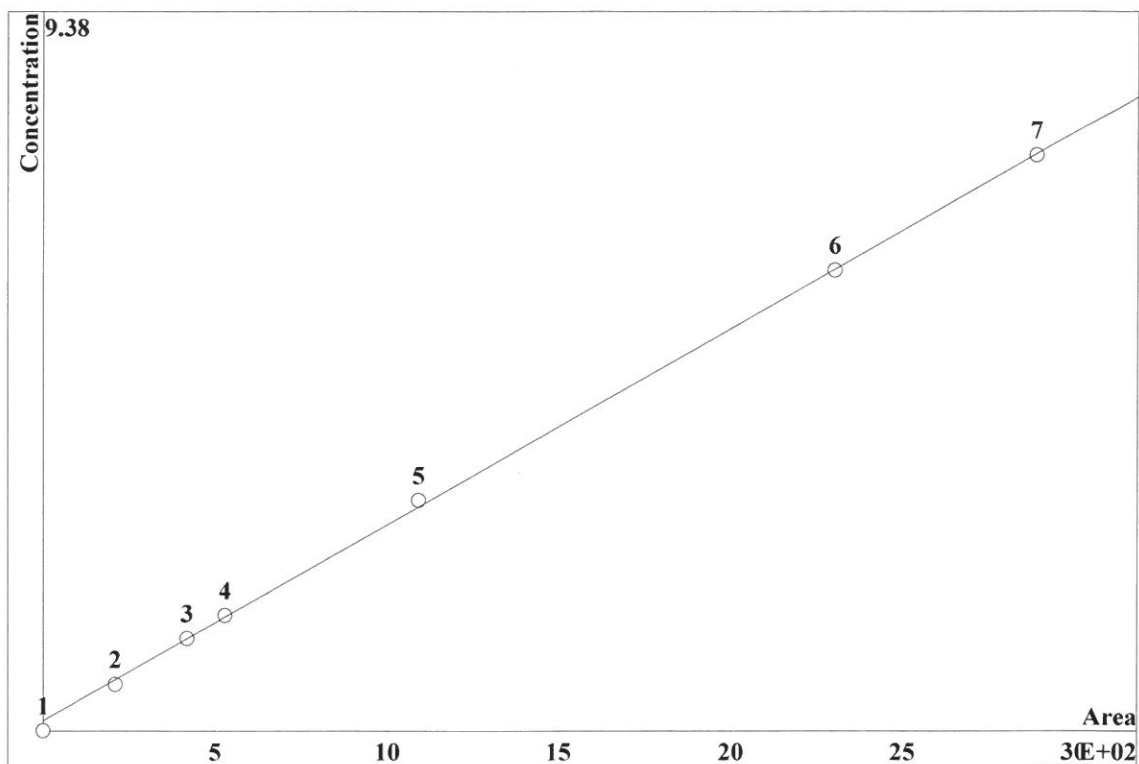

K3 = 0 K2 = 0 K1 = 0.051109 K0 = 2.59501

Base: Area

Ref.channel: ch1

ISTD:

Formula: Linear


Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	11.22	210.2	0.6	20	10.64		
3	22.26	419.9	1.2	20	10.64		
4	28.16	529.1	1.5	20	10.64		
5	57.52	1090	3	20	10.64		
6	115.2	2303	6	20	10.64		
7	142.6	2891	7.5	20	10.64		

±□:□

CALIBRATION OF COMPONENT BR-

Method: AnionsIC2-070921.mtw
 Equation: $Q = 0.254436 \cdot A + 9.45477$
 RSD: 2.017 %
 Correlation coefficient: 0.999778

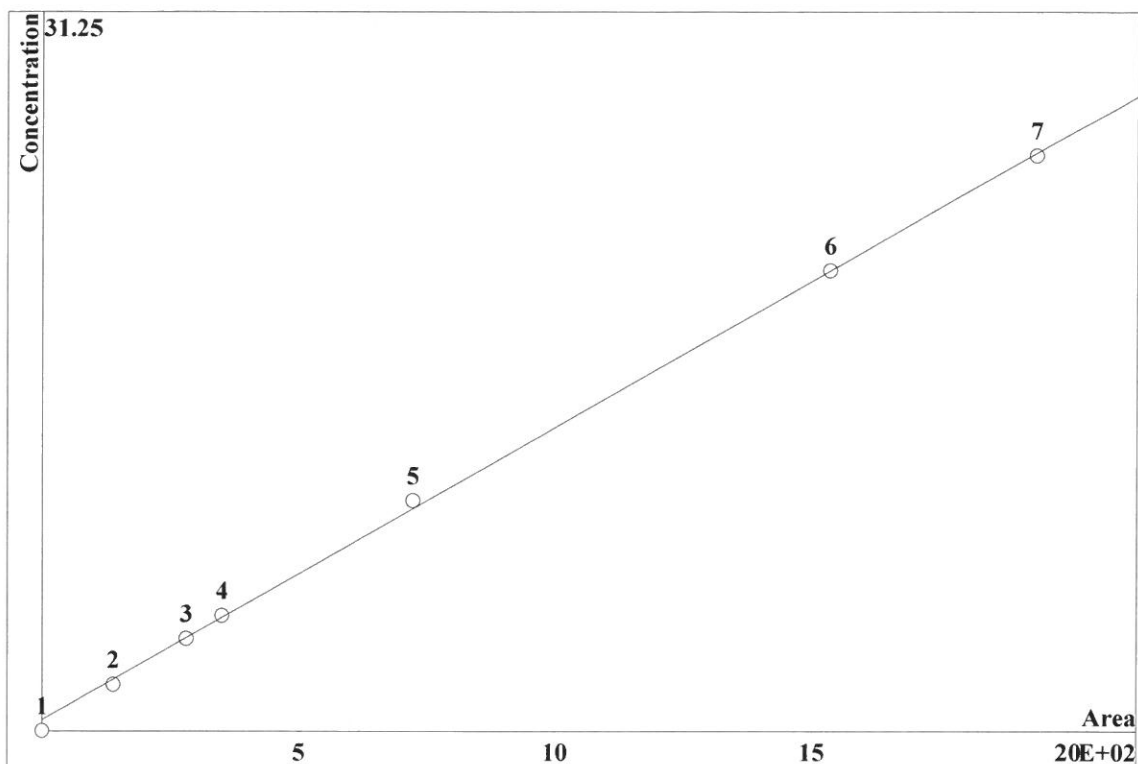

K3 = 0 K2 = 0 K1 = 0.254436 K0 = 9.45477

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	6.921	139.3	139.3	2	20		14
3	14.18	281.4	281.4	4	20		14
4	17.89	350.3	350.3	5	20		14
5	37.58	722.2	722.2	10	20		14
6	81.68	1534	1534	20	20		14
7	102.3	1937	1937	25	20		14

CALIBRATION OF COMPONENT NO3

Method: AnionsIC2-070921.mtw
 Equation: $Q = 0.0438083 \cdot A + 2.94619$
 RSD: 2.995 %
 Correlation coefficient: 0.999511

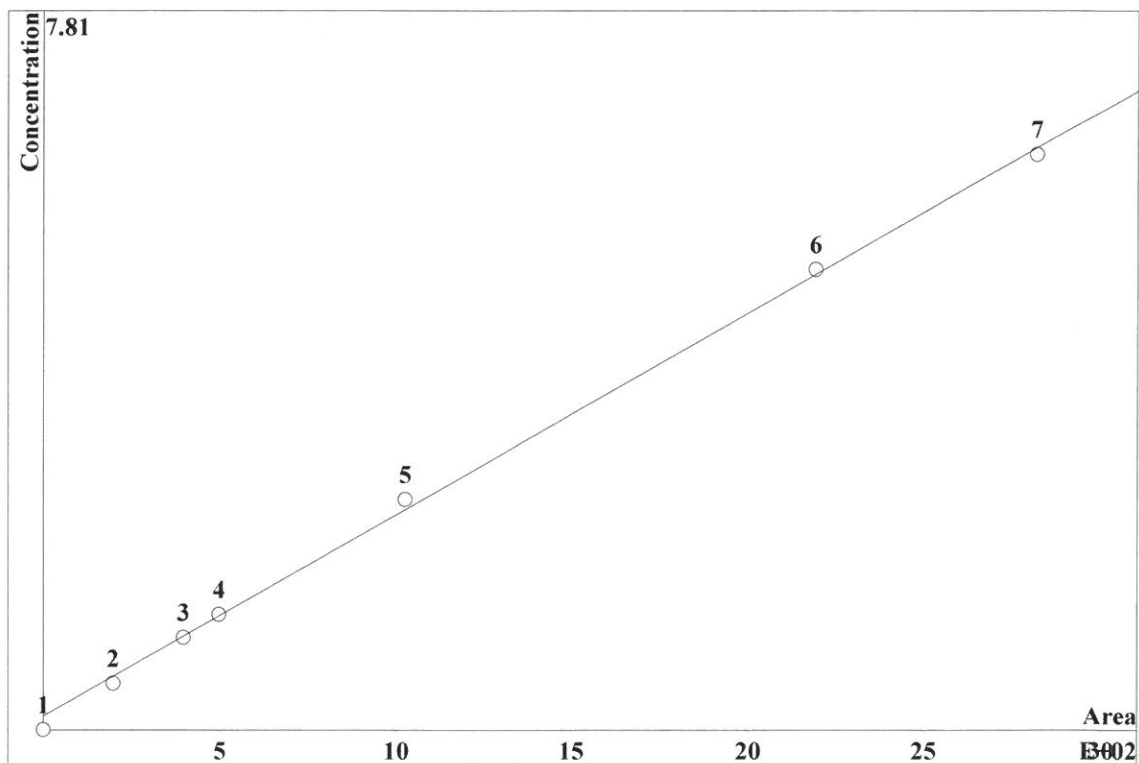


K3 = 0 K2 = 0 K1 = 0.0438083 K0 = 2.94619
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	8.418	198.1	0.5	20	16.28		
3	17.08	397.4	1	20	16.28		
4	21.57	497.9	1.25	20	16.28		
5	44.85	1025	2.5	20	16.28		
6	97.19	2191	5	20	16.28		
7	122.3	2820	6.25	20	16.28		

CALIBRATION OF COMPONENT HPO4

Method: AnionsIC2-070921.mtw
 Equation: $Q = 0.0885729 \cdot A - 11.3055$
 RSD: 1.708 %
 Correlation coefficient: 0.999841

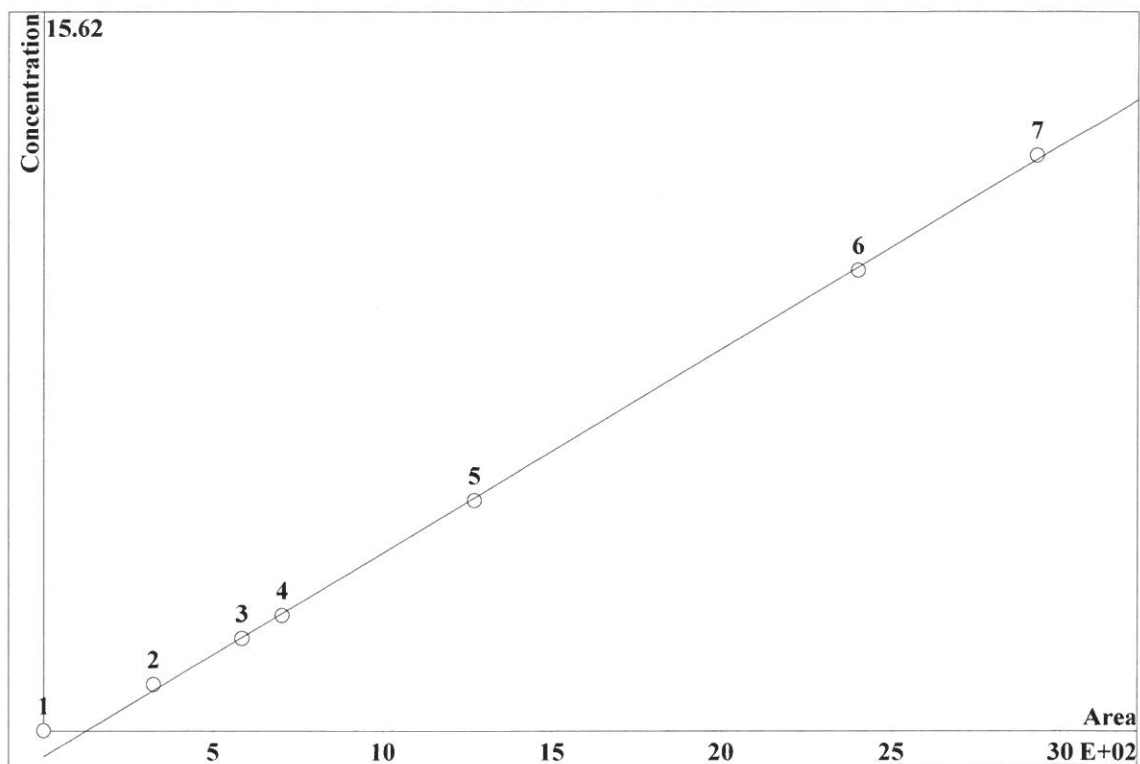

K3 = 0 K2 = 0 K1 = 0.0885729 K0 = -11.3055

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	8.78	325.5	1	20	21.2		
3	16.61	586.6	2	20	21.2		
4	20.09	703.3	2.5	20	21.2		
5	37.65	1270	5	20	21.2		
6	74.91	2402	10	20	21.2		
7	91.49	2930	12.5	20	21.2		

CALIBRATION OF COMPONENT SO4

Method: AnionsIC2-070921.mtw
 Equation: $Q = 0.143844 \cdot A + 17.5564$
 RSD: 2.650 %
 Correlation coefficient: 0.999617

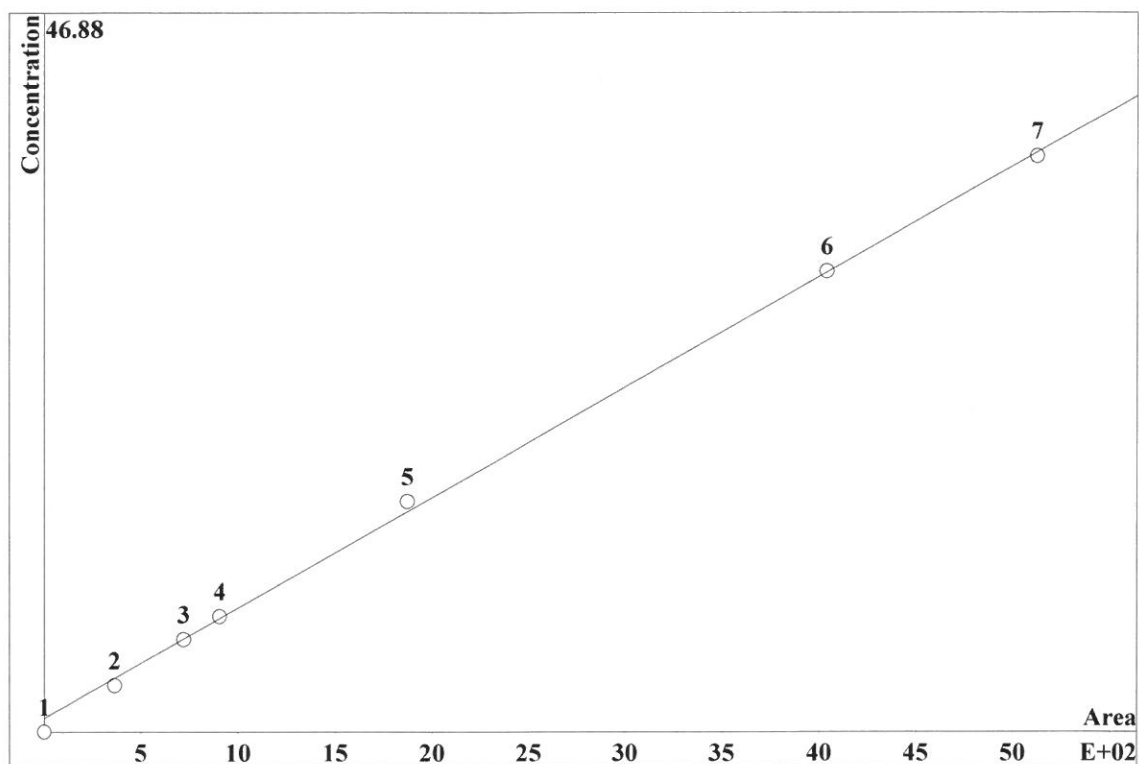

K3 = 0 K2 = 0 K1 = 0.143844 K0 = 17.5564

Base: Area

Ref.channel: ch1

ISTD:

Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	12.45	364.7	3	20	24.73		
3	24.99	721.2	6	20	24.73		
4	31.58	904.9	7.5	20	24.73		
5	66.09	1873	15	20	24.73		
6	145.1	4041	30	20	24.73		
7	182.6	5128	37.5	20	24.73		

æ#□

Clear table

Instrument ID: IC-2 Analyst: AP Method: 300 / 9056A

ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time	Initial wt/ Final Vol	Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-07-09_	7/9/21 9:42		AP/MA
STD2	0.4290	0.6630	0.6670	2.2450	0.5810	0.8760	3.5010	2021-07-09_	7/9/21 10:10		AP/MA
STD3	0.7920	1.2070	1.2030	4.0520	1.0180	2.0320	6.0650	2021-07-09_	7/9/21 10:39		AP/MA
STD4	1.0300	1.4850	1.4820	4.9290	1.2380	2.5490	7.3860	2021-07-09_	7/9/21 11:07		AP/MA
STD5	1.9480	2.9110	2.9160	9.6610	2.3920	5.0590	14.3460	2021-07-09_	7/9/21 11:36		AP/MA
STD6	3.9460	6.0160	6.0140	19.9940	4.9470	10.0720	29.9440	2021-07-09_	7/9/21 12:05		AP/MA
STD7	5.0550	7.5180	7.5190	25.1190	6.3240	12.4110	37.7580	2021-07-09_	7/9/21 12:33		AP/MA

ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.5000

ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4
STD1							
STD2	7.2500	10.5000	11.1667	12.2500	16.2000	-12.4000	16.7000
STD3	-1.0000	0.5833	0.2500	1.3000	1.8000	1.6000	1.0833
STD4	3.0000	-1.0000	-1.2000	-1.4200	-0.9600	1.9600	-1.5200
STD5	-2.6000	-2.9667	-2.8000	-3.3900	-4.3200	1.1800	-4.3600
STD6	-1.3500	0.2667	0.2333	-0.0300	-1.0600	0.7200	-0.1867
STD7	1.1000	0.2400	0.2533	0.4760	1.1840	-0.7120	0.6880

Report date: 7/12/2021 3:22:09 PM
Printed by: wet


Ident: STD1
Analysis from: 7/9/2021 9:42:11 AM
File: _2021-07-09_

Last save: 7/12/2021 3:21:23 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27529

Last save: 7/9/2021 12:31:

SAMPLE:
: AM/AP
Vial number: 2
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

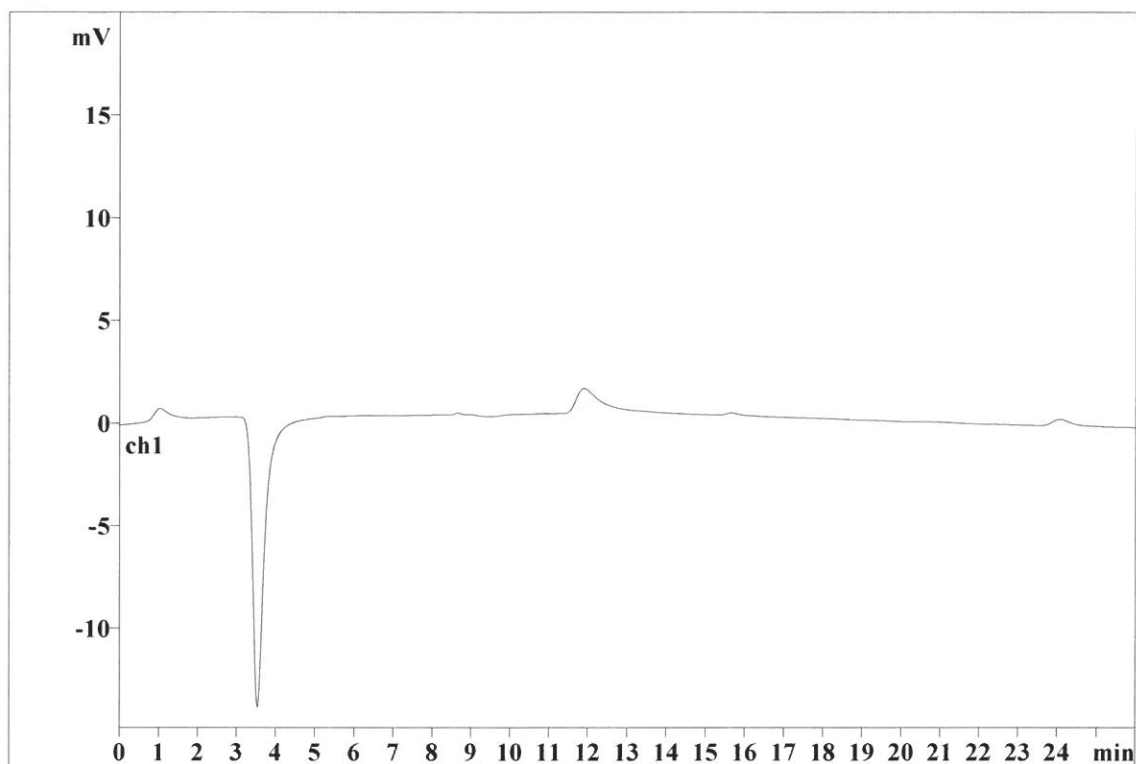

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 7/12/2021 3:22:24 PM
Printed by: wet


Ident: STD2
Analysis from: 7/9/2021 10:10:47 AM
File: _2021-07-09_

Last save: 7/12/2021 3:21:23 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27530

Last save: 7/9/2021 12:31:

SAMPLE:
: AM/AP
Vial number: 3
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

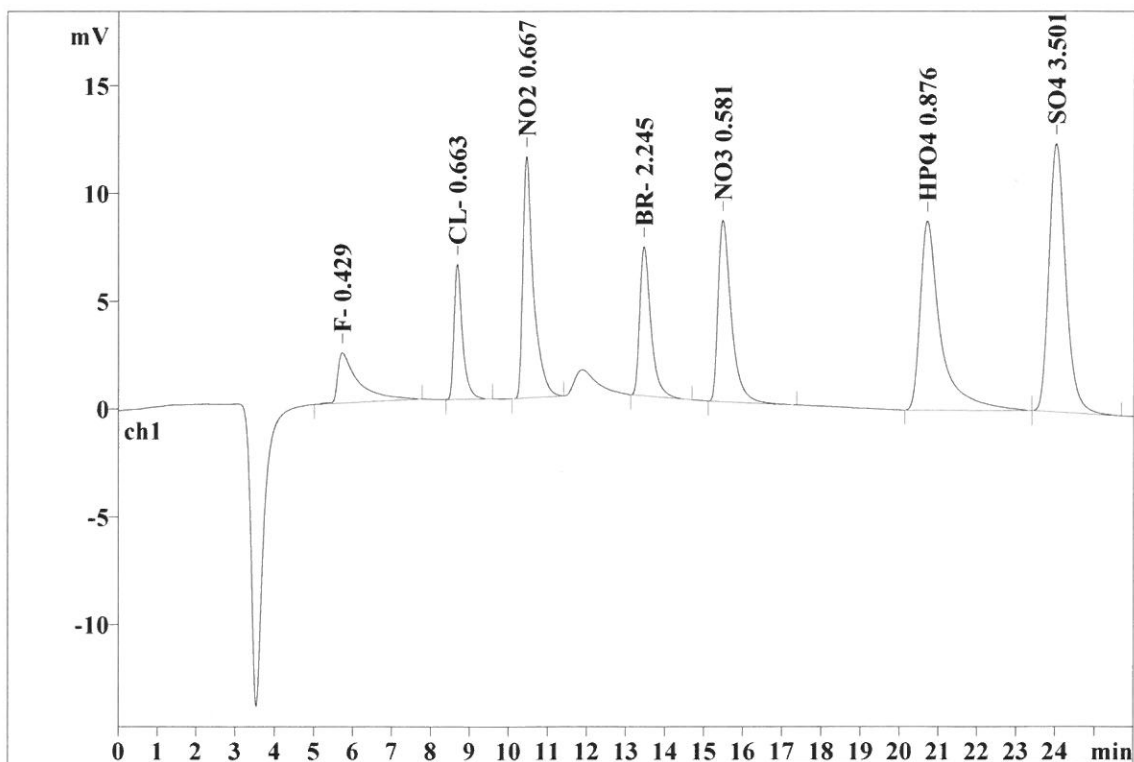

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.72	0.459	2.33	4.14	86.639	6.11
2	8.66	0.212	6.27	11.12	94.105	6.63
3	10.45	0.257	11.21	19.89	210.169	14.82
4	13.45	0.294	6.92	12.27	139.302	9.82
5	15.48	0.342	8.42	14.93	198.098	13.96
6	20.71	0.480	8.78	15.57	325.546	22.95
7	24.02	0.438	12.45	22.08	364.708	25.71
7	26.00	0.355	56.39	99.99	1418.567	100.00

This report has been created by IC Net
METROHM LTD

Report date: 7/12/2021 3:22:35 PM
Printed by: wet


Ident: STD3
Analysis from: 7/9/2021 10:39:23 AM
File: _2021-07-09_

Last save: 7/12/2021 3:21:23 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27531

Last save: 7/9/2021 12:31:

SAMPLE:
: AM/AP
Vial number: 4
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

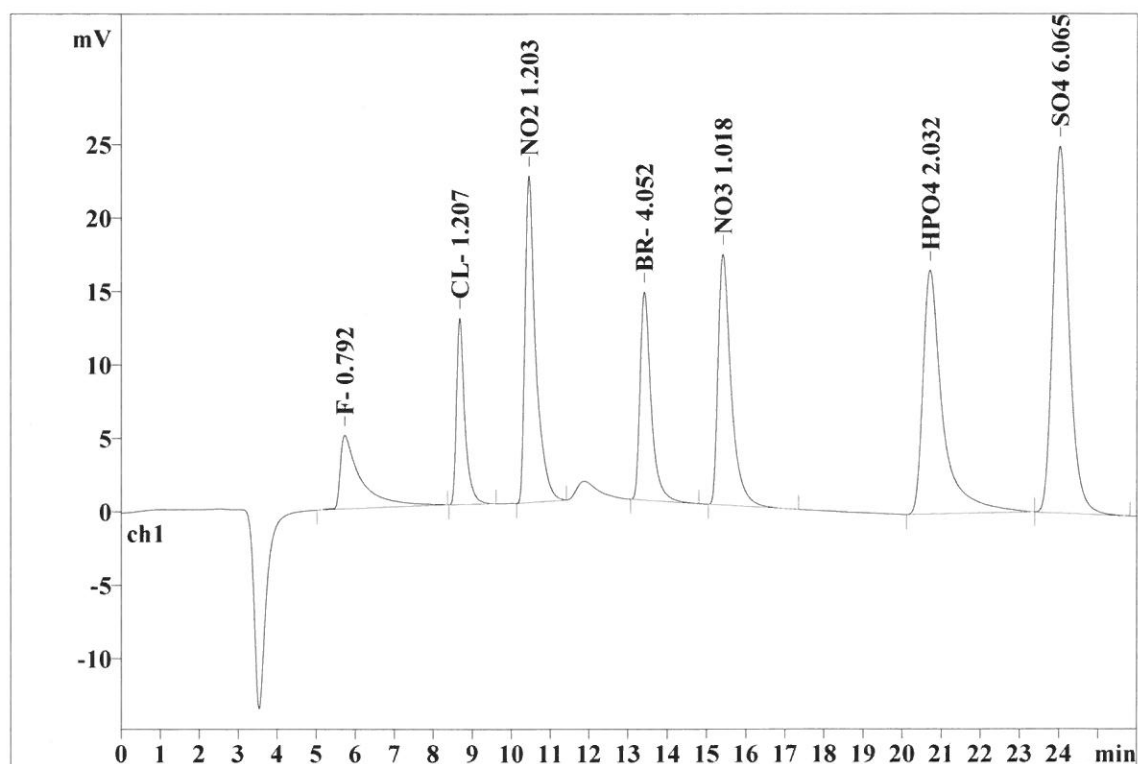

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.72	0.442	5.02	4.45	183.476	6.60
2	8.66	0.211	12.68	11.24	188.743	6.79
3	10.43	0.260	22.26	19.73	419.875	15.11
4	13.40	0.288	14.18	12.57	281.364	10.13
5	15.40	0.338	17.08	15.14	397.403	14.30
6	20.70	0.461	16.61	14.72	586.574	21.11
7	24.02	0.431	24.99	22.15	721.152	25.95
7	26.00	0.347	112.82	99.99	2778.588	100.00

This report has been created by IC Net
METROHM LTD

Report date: 7/12/2021 3:22:45 PM
Printed by: wet


Ident: STD4
Analysis from: 7/9/2021 11:07:59 AM
File: _2021-07-09_

Last save: 7/12/2021 3:21:23 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27532

Last save: 7/9/2021 12:31:

SAMPLE:
: AM/AP
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

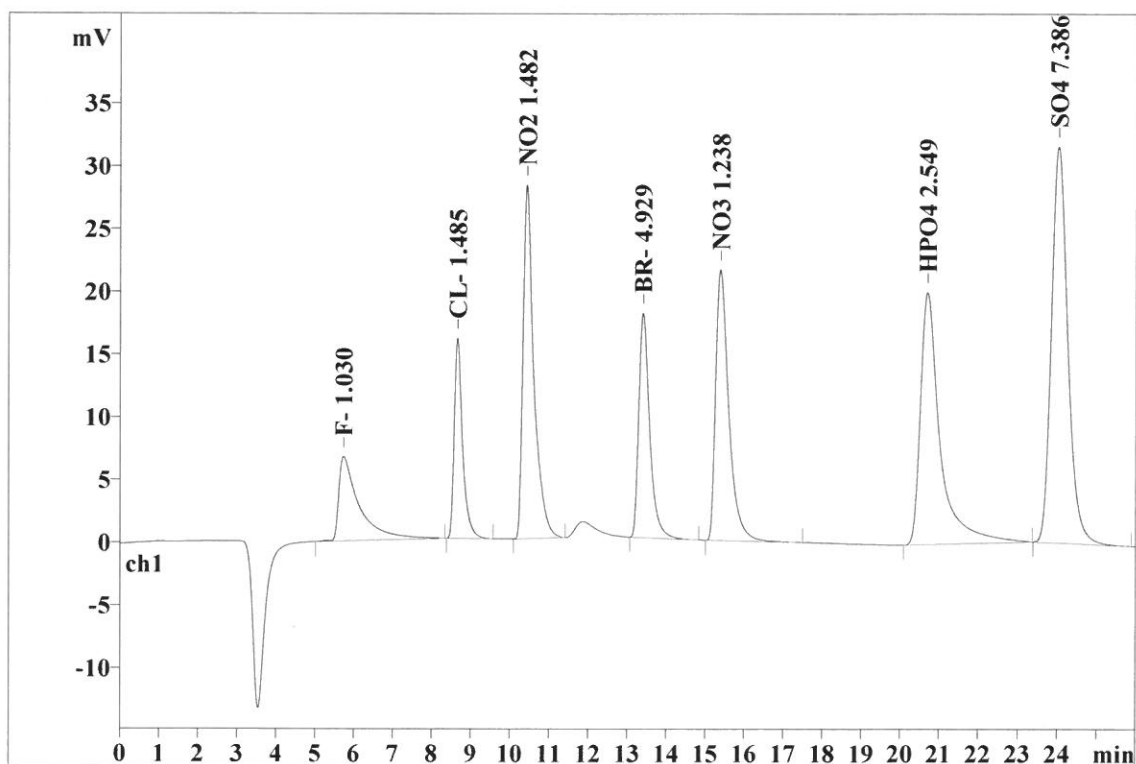

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.73	0.463	6.72	4.74	246.804	7.11
2	8.64	0.212	15.95	11.23	237.133	6.84
3	10.41	0.259	28.16	19.84	529.064	15.25
4	13.39	0.287	17.89	12.60	350.308	10.10
5	15.38	0.336	21.57	15.19	497.876	14.35
6	20.69	0.457	20.09	14.15	703.257	20.27
7	24.02	0.429	31.58	22.24	904.879	26.08
7	26.00	0.349	141.96	100.00	3469.319	100.00

This report has been created by IC Net
METROHM LTD

Report date: 7/12/2021 3:22:51 PM
Printed by: wet


Ident: STD5
Analysis from: 7/9/2021 11:36:37 AM
File: _2021-07-09_

Last save: 7/12/2021 3:21:23 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27533

Last save: 7/9/2021 12:31:

SAMPLE:
: AM/AP
Vial number: 6
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

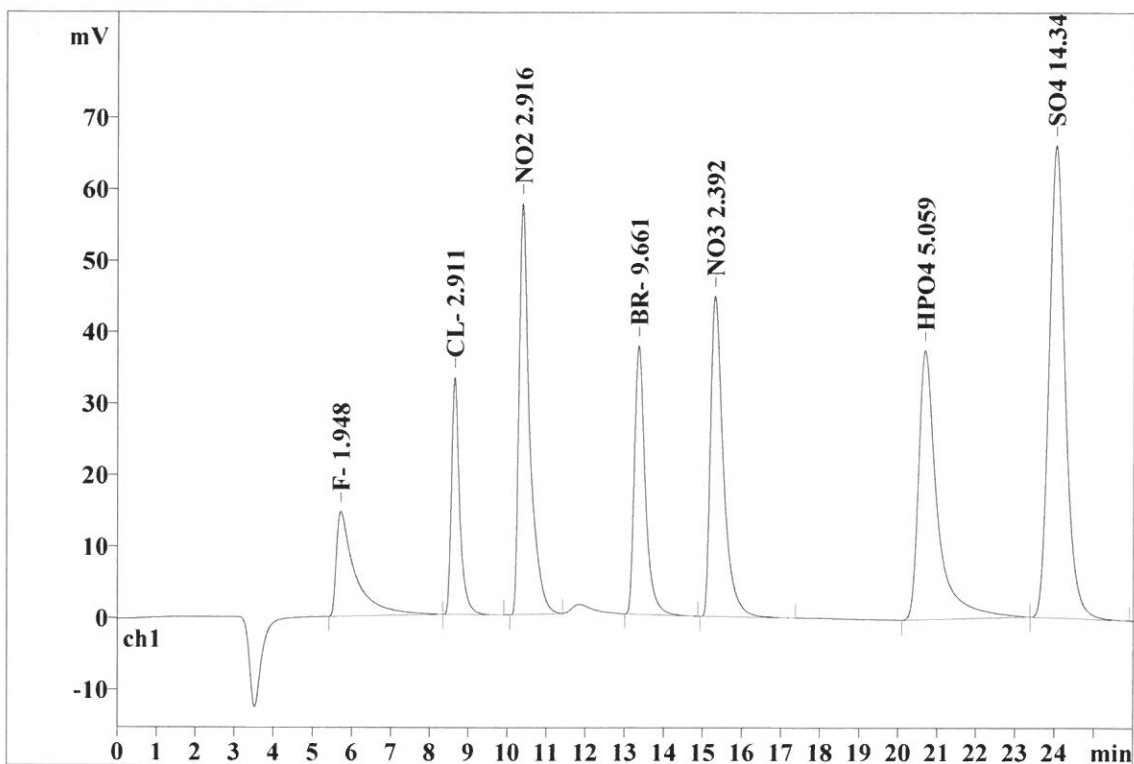

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.71	0.419	14.65	5.02	491.359	7.06
2	8.62	0.207	33.19	11.38	485.218	6.98
3	10.38	0.260	57.52	19.73	1090.401	15.67
4	13.34	0.280	37.57	12.89	722.244	10.38
5	15.30	0.332	44.85	15.38	1024.583	14.73
6	20.68	0.444	37.65	12.91	1270.020	18.26
7	24.02	0.423	66.09	22.67	1872.658	26.92
7	26.00	0.338	291.51	100.00	6956.483	100.00

This report has been created by IC Net
METROHM LTD

Report date: 7/12/2021 3:22:58 PM
Printed by: wet


Ident: STD6
Analysis from: 7/9/2021 12:05:13 PM
File: _2021-07-09_

Last save: 7/12/2021 3:21:23 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27534

Last save: 7/9/2021 12:31:

SAMPLE:
: AM/AP
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

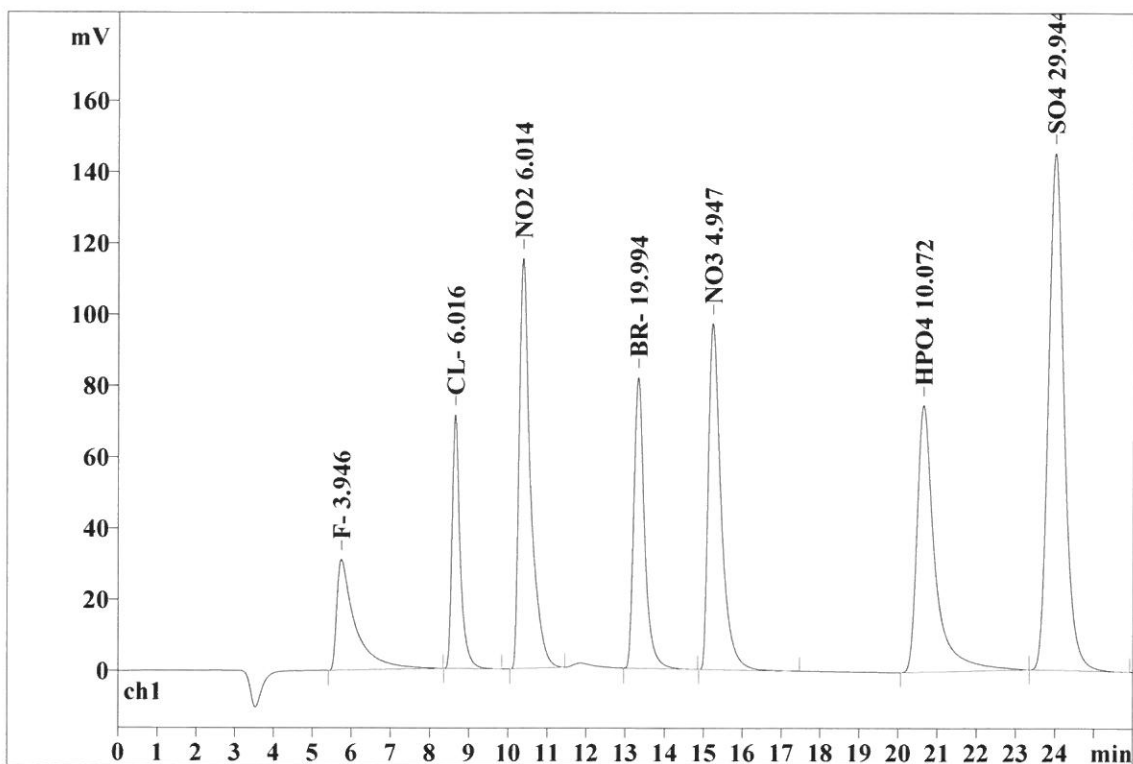

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.74	0.420	31.01	5.03	1023.332	7.05
2	8.63	0.203	71.27	11.56	1025.455	7.06
3	10.36	0.278	115.20	18.69	2302.532	15.86
4	13.31	0.273	81.68	13.25	1534.445	10.57
5	15.22	0.326	97.19	15.77	2191.307	15.09
6	20.63	0.428	74.91	12.15	2401.858	16.54
7	23.98	0.416	145.08	23.54	4041.385	27.83
7	26.00	0.335	616.34	100.00	14520.314	100.00

This report has been created by IC Net
METROHM LTD

Report date: 7/12/2021 3:23:05 PM
Printed by: wet


Ident: STD7
Analysis from: 7/9/2021 12:33:49 PM
File: _2021-07-09_

Last save: 7/12/2021 3:21:23 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27535

Last save: 7/9/2021 12:31:

SAMPLE:
: AM/AP
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

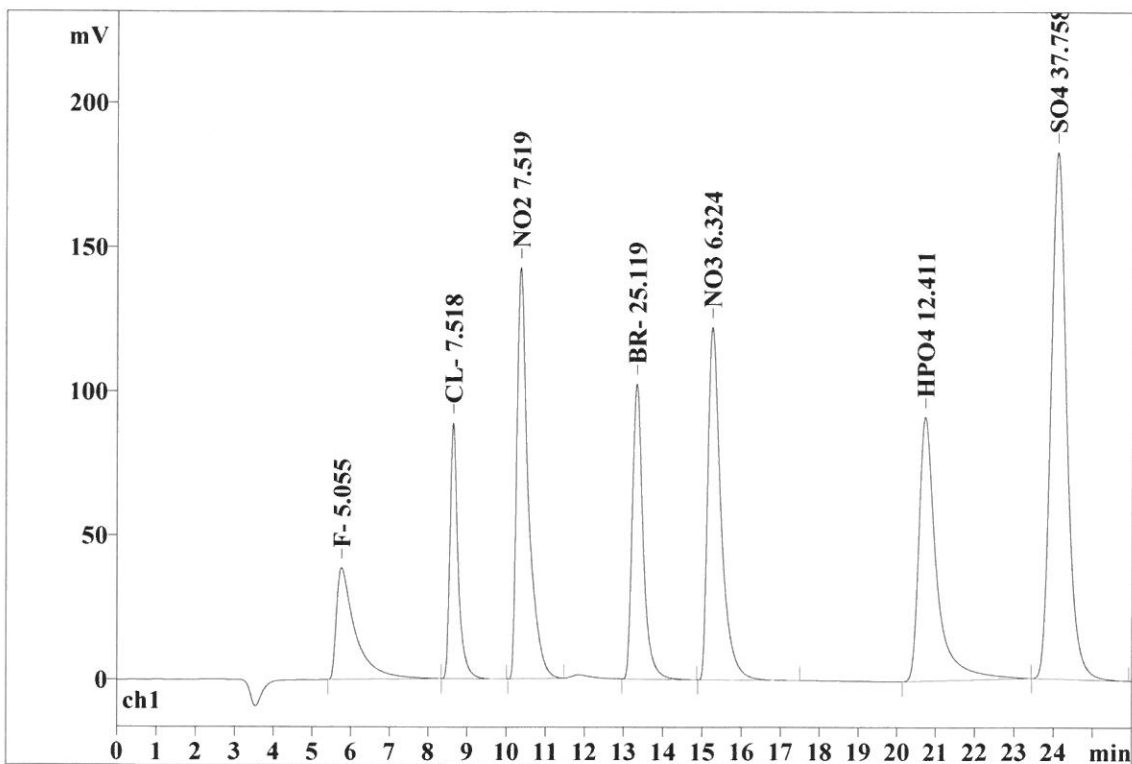

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.75	0.452	38.73	5.04	1318.856	7.20
2	8.62	0.204	88.63	11.53	1286.609	7.03
3	10.34	0.281	142.57	18.55	2891.454	15.79
4	13.32	0.275	102.34	13.31	1937.333	10.58
5	15.24	0.333	122.27	15.91	2820.037	15.40
6	20.71	0.429	91.49	11.90	2930.072	16.00
7	24.08	0.420	182.57	23.75	5127.796	28.00
7	26.00	0.342	768.59	100.00	18312.159	100.00

This report has been created by IC Net
METROHM LTD

Report date: 7/12/2021 3:23:12 PM
Printed by: wet


Ident: ICV
Analysis from: 7/9/2021 1:05:41 PM
File: _2021-07-09_

Last save: 7/9/2021 1:31:41 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27536

Last save: 7/9/2021 12:59:

SAMPLE:
: AM/AP
Vial number: 9
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

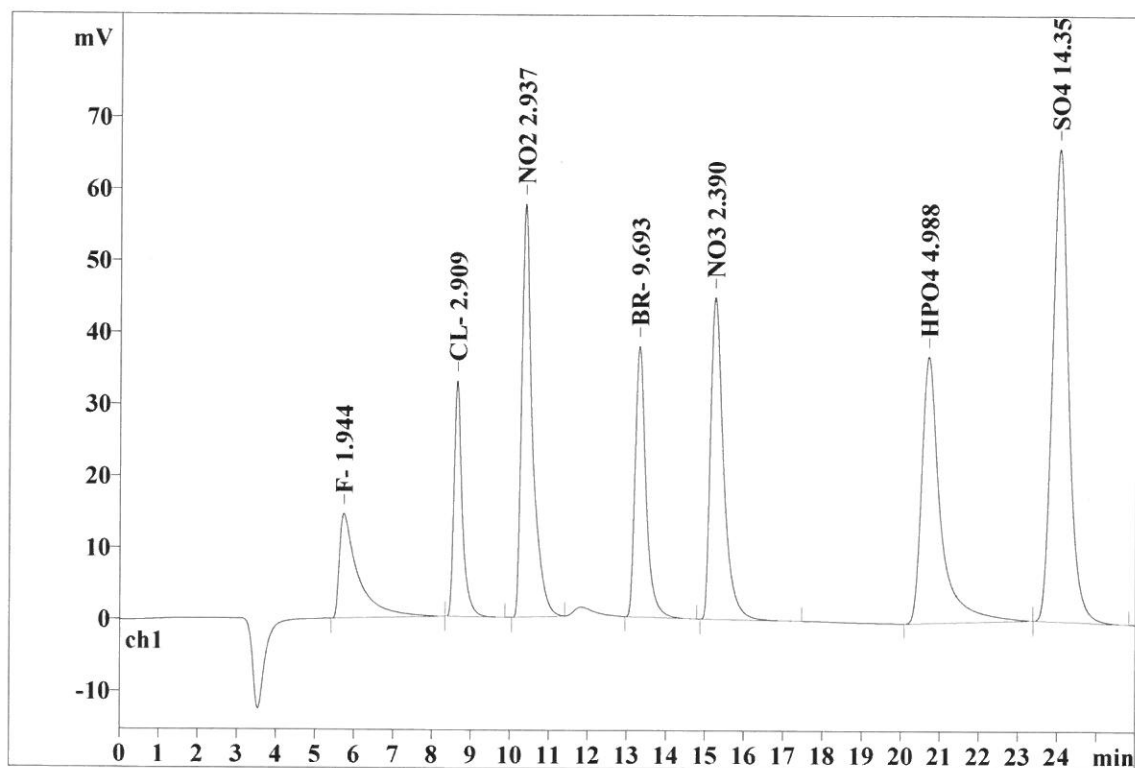

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.72	0.423	14.56	5.01	490.144	7.05
2	8.62	0.208	32.84	11.31	484.812	6.98
3	10.36	0.261	57.55	19.81	1098.352	15.80
4	13.29	0.280	37.73	12.99	724.773	10.43
5	15.23	0.331	44.83	15.43	1024.024	14.73
6	20.68	0.445	37.09	12.77	1254.043	18.04
7	24.02	0.425	65.85	22.67	1873.591	26.96
7	26.00	0.339	290.45	100.00	6949.740	100.00

This report has been created by IC Net
METROHM LTD

Report date: 7/12/2021 3:23:24 PM
Printed by: wet


Ident: ICB
Analysis from: 7/9/2021 1:34:44 PM
File: _2021-07-09_

Last save: 7/9/2021 2:00:44 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27537

Last save: 7/9/2021 12:59:

SAMPLE:
: AP/MA
Vial number: 10
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

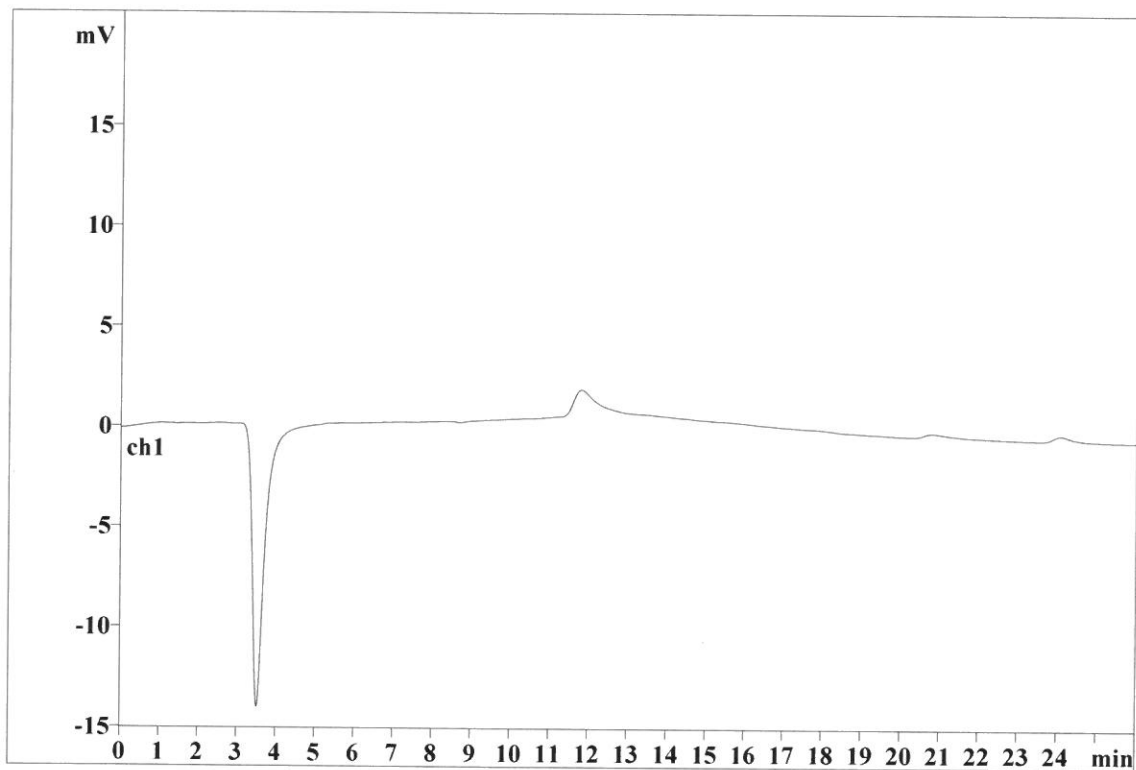

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 7/23/2021 4:17:21 PM
Printed by: wet


Ident: CCV
Analysis from: 7/23/2021 9:18:14 AM
File: _2021-07-23_

Last save: 7/23/2021 9:44:14 AM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27661

Last save: 7/12/2021 3:21:

SAMPLE:
: AP/MA
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

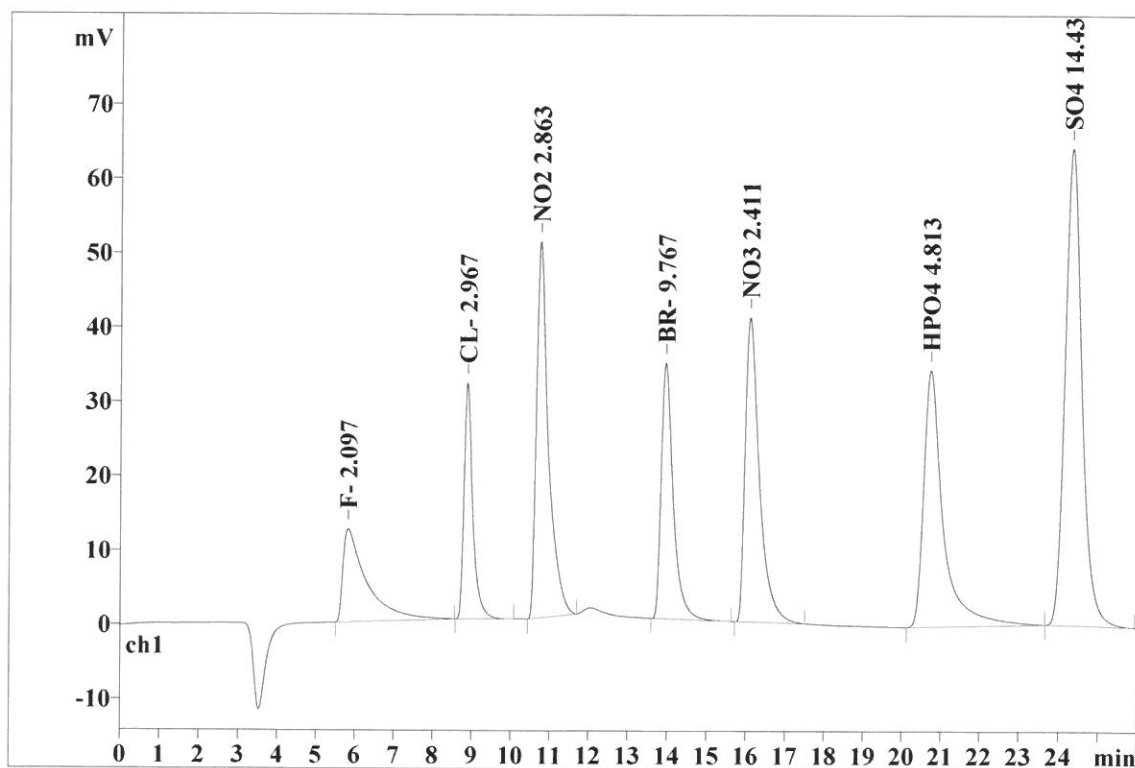

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.82	0.545	12.52	4.65	530.967	7.63
2	8.86	0.221	31.76	11.81	494.885	7.11
3	10.73	0.290	50.60	18.81	1069.459	15.37
4	13.95	0.308	34.42	12.80	730.581	10.50
5	16.09	0.367	40.95	15.22	1033.274	14.85
6	20.72	0.456	34.50	12.83	1214.484	17.45
7	24.31	0.437	64.19	23.87	1885.514	27.09
7	26.00	0.375	268.94	99.99	6959.163	100.00

This report has been created by IC Net
METROHM LTD

Report date: 7/23/2021 4:17:29 PM
Printed by: wet


Ident: CCB
Analysis from: 7/23/2021 10:10:28 AM
File: _2021-07-23_

Last save: 7/23/2021 10:36:28 AM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27662

Last save: 7/12/2021 3:21:

SAMPLE:
: AP/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

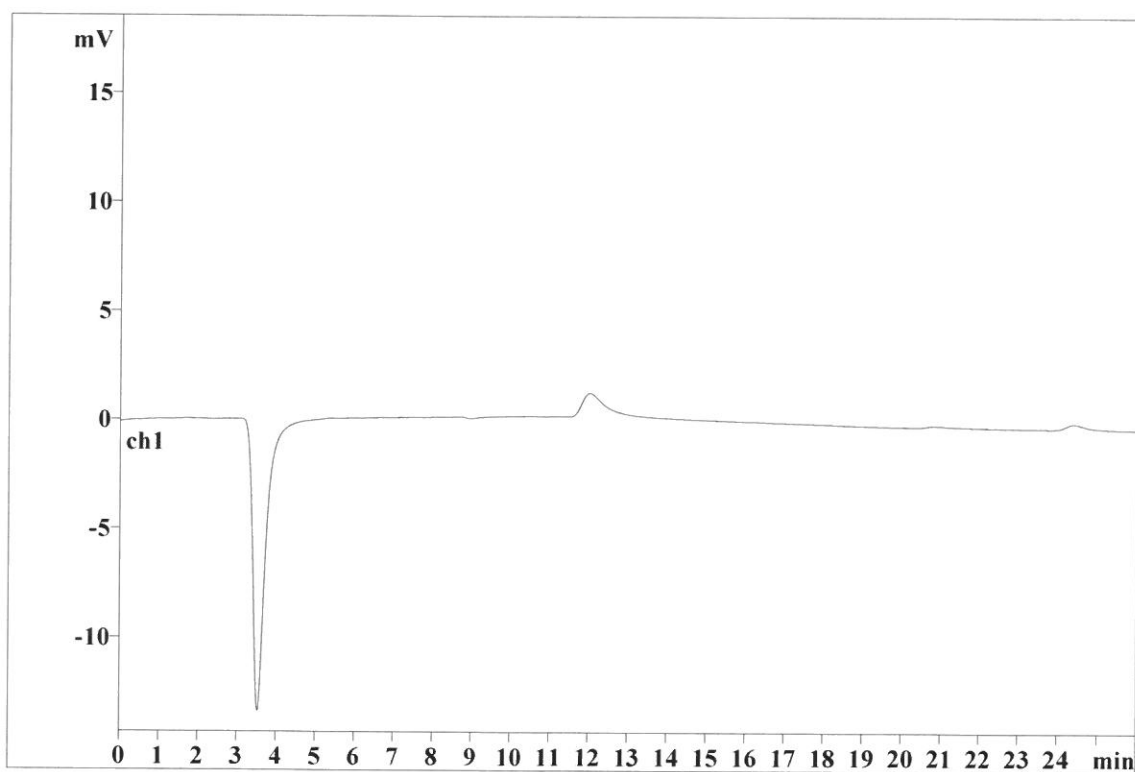

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 7/23/2021 4:17:36 PM
Printed by: wet


Ident: LB115504BLS
Analysis from: 7/23/2021 10:39:03 AM
File: _2021-07-23_

Last save: 7/23/2021 1:53:38 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27663

Last save: 7/12/2021 3:21:

SAMPLE: 5.00G/100mL
: AP/MA
Vial number: 13
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

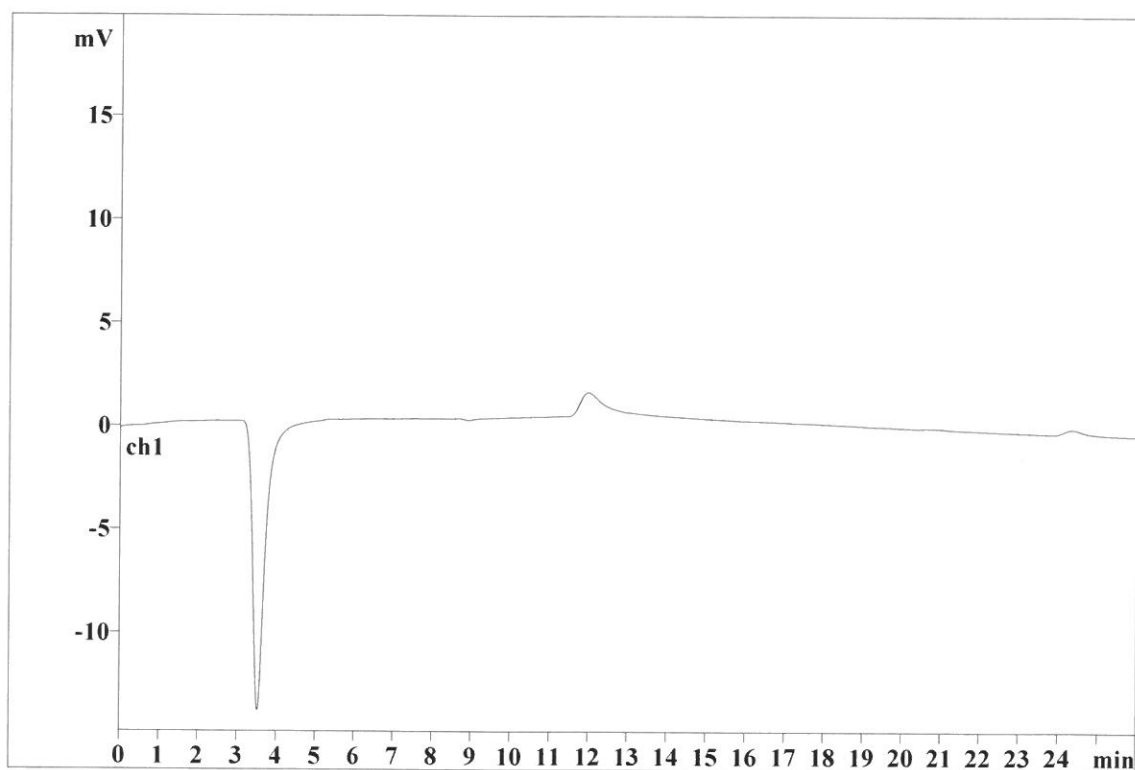

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 7/23/2021 4:17:42 PM
Printed by: wet


Ident: LB115504BSS
Analysis from: 7/23/2021 11:07:38 AM
File: _2021-07-23_

Last save: 7/23/2021 1:53:38 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27664

Last save: 7/12/2021 3:21:

SAMPLE: 5.00G/100mL
: AP/MA
Vial number: 14
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

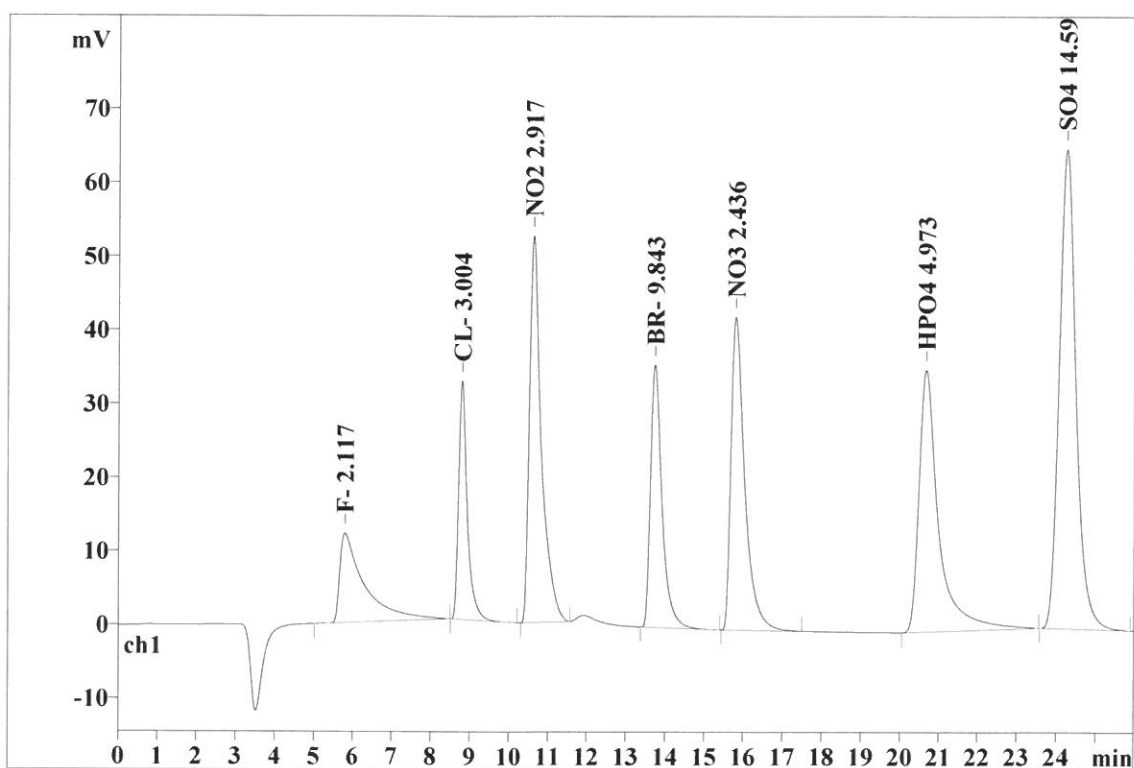

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.79	0.555	12.11	4.39	536.286	7.59
2	8.78	0.219	32.38	11.75	501.468	7.09
3	10.60	0.286	52.43	19.02	1090.886	15.43
4	13.72	0.300	35.63	12.93	736.556	10.42
5	15.79	0.356	42.46	15.41	1044.897	14.78
6	20.66	0.455	35.54	12.89	1250.579	17.69
7	24.22	0.436	65.06	23.60	1907.606	26.99
7	26.00	0.372	275.61	100.00	7068.278	100.00

This report has been created by IC Net
METROHM LTD

Report date: 7/23/2021 4:17:49 PM
Printed by: wet


Ident: M3151-01
Analysis from: 7/23/2021 11:55:06 AM
File: _2021-07-23_

Last save: 7/23/2021 12:21:06 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27665

Last save: 7/12/2021 3:21:

SAMPLE: 5.06g/100mL
: AP/MA
Vial number: 15
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

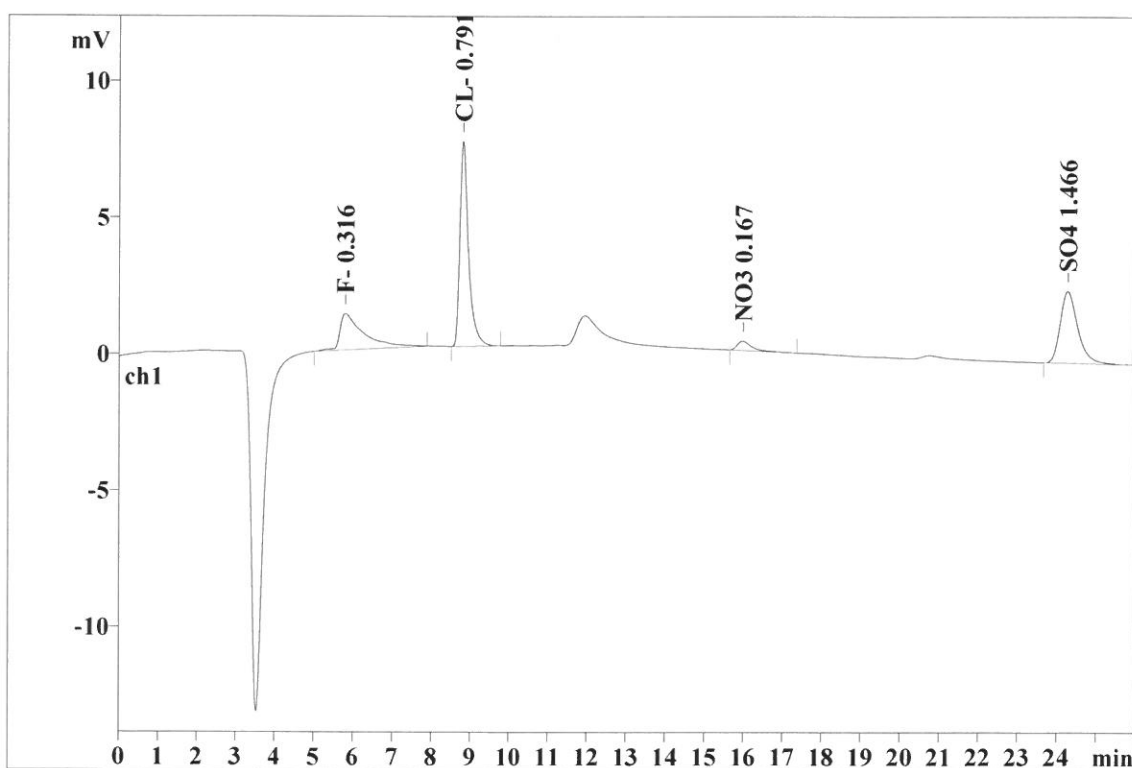

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.78	0.558	1.33	11.25	56.589	21.45
2	8.77	0.220	7.51	63.53	116.399	44.12
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	15.97	0.371	0.34	2.89	9.025	3.42
6	0.00	0.000	0.00	0.00	0.000	0.00
7	24.25	0.459	2.63	22.29	81.805	31.01
7	26.00	0.230	11.81	99.96	263.818	100.00

This report has been created by IC Net
METROHM LTD

Report date: 7/23/2021 4:17:56 PM
Printed by: wet


Ident: M3151-02
Analysis from: 7/23/2021 12:42:01 PM
File: _2021-07-23_

Last save: 7/23/2021 1:08:02 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27666

Last save: 7/12/2021 3:21:

SAMPLE: 5..25g/100mL
: AP/MA
Vial number: 25
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

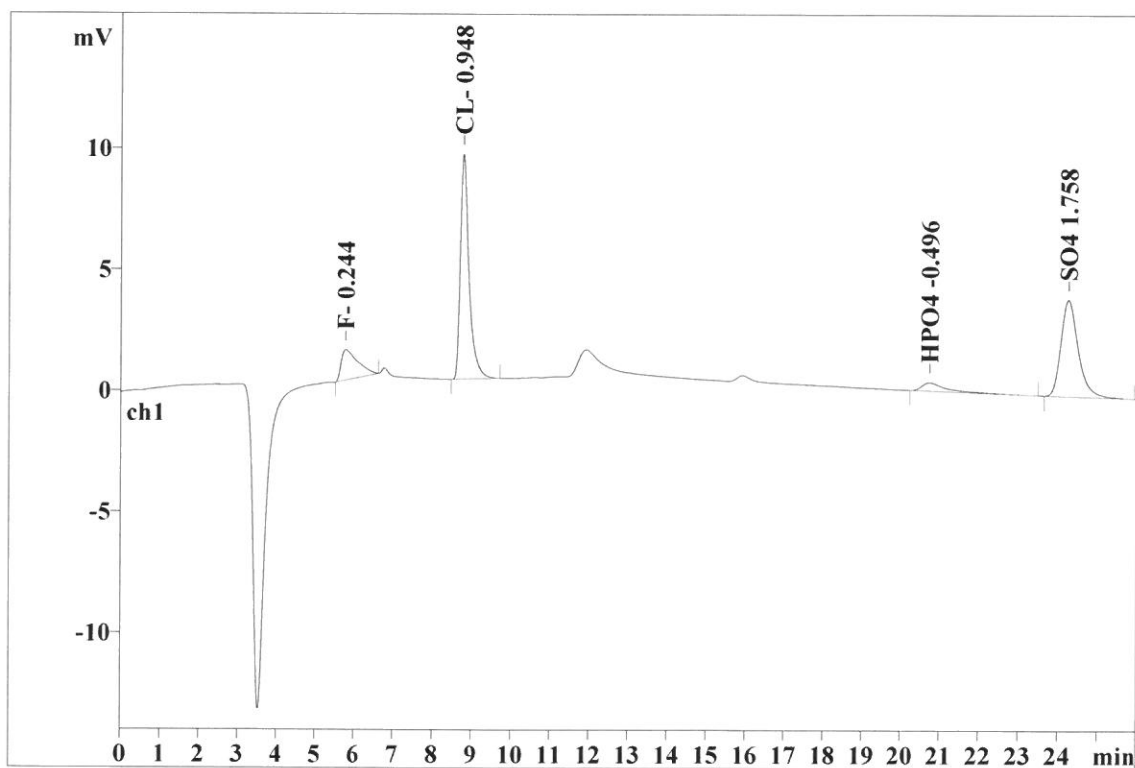

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.76	0.464	1.26	8.44	37.311	11.69
2	8.75	0.219	9.29	62.41	143.736	45.04
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	20.73	0.568	0.35	2.34	15.689	4.92
7	24.24	0.455	3.99	26.78	122.376	38.35
7	26.00	0.244	14.88	99.96	319.112	100.00

This report has been created by IC Net
METROHM LTD

Report date: 7/23/2021 4:18:05 PM
Printed by: wet


Ident: M3151-03
Analysis from: 7/23/2021 1:11:04 PM
File: _2021-07-23_

Last save: 7/23/2021 1:37:04 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27667

Last save: 7/12/2021 3:21:

SAMPLE: 5..21g/100mL
: AP/MA
Vial number: 17
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

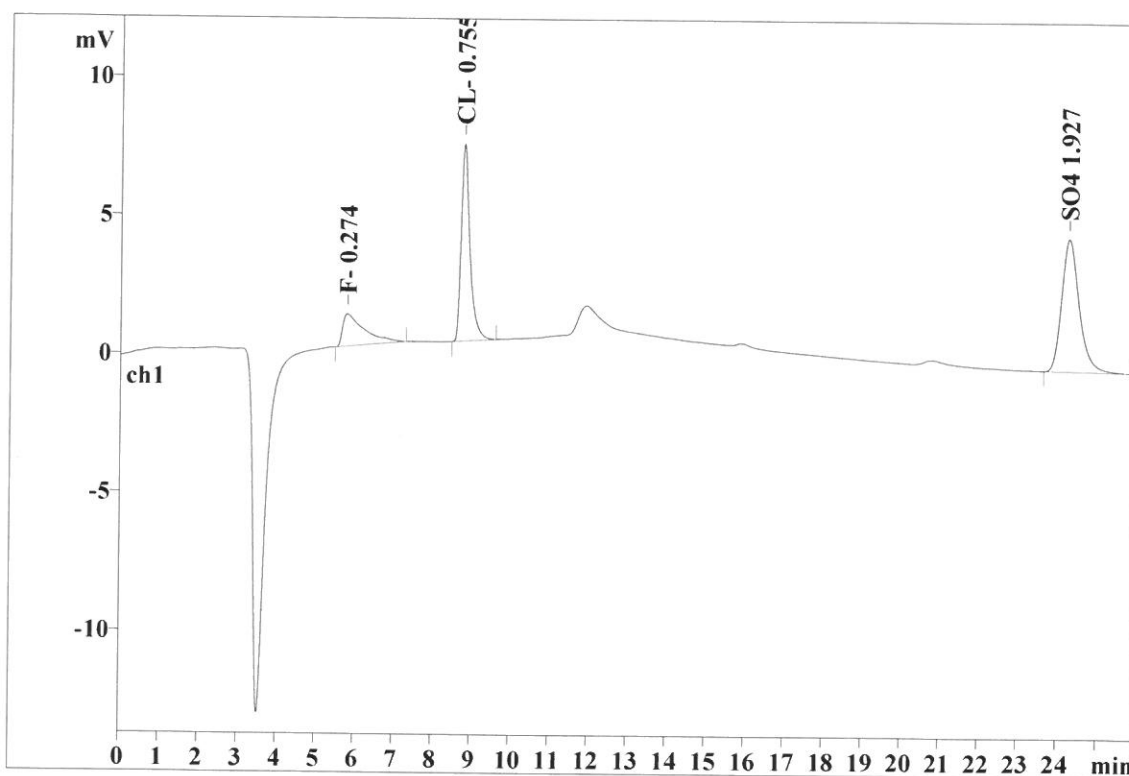

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.77	0.557	1.16	8.91	45.450	15.08
2	8.75	0.221	7.12	54.47	110.175	36.55
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	24.24	0.453	4.78	36.59	145.823	48.37
7	26.00	0.176	13.06	99.97	301.448	100.00

This report has been created by IC Net
METROHM LTD

Report date: 7/23/2021 4:18:26 PM
Printed by: wet


Ident: M3151-03MS
Analysis from: 7/23/2021 1:39:46 PM
File: _2021-07-23_

Last save: 7/23/2021 2:05:46 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27668

Last save: 7/12/2021 3:21:

SAMPLE: 5..20g/100mL
: AP/MA
Vial number: 18
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

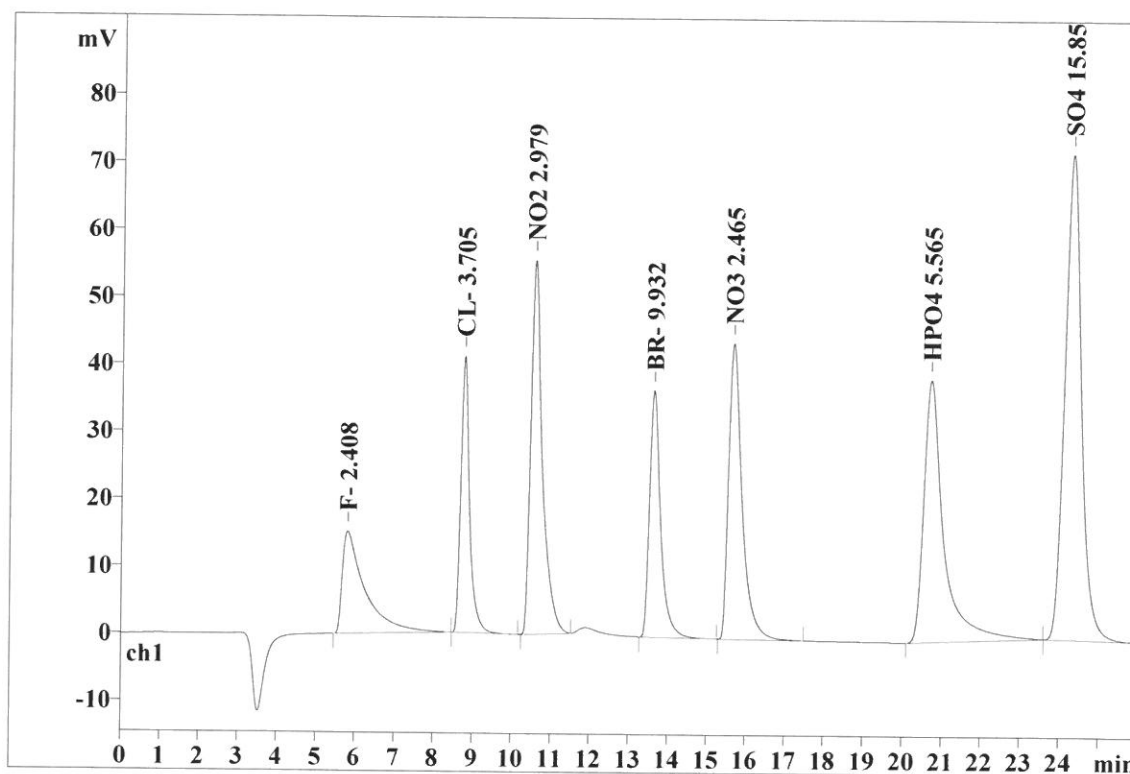

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.80	0.526	15.19	5.01	613.765	8.06
2	8.75	0.215	41.02	13.53	623.331	8.18
3	10.54	0.279	55.50	18.31	1114.995	14.63
4	13.61	0.295	36.61	12.08	743.558	9.76
5	15.65	0.349	43.89	14.48	1058.041	13.89
6	20.69	0.457	38.85	12.82	1384.155	18.17
7	24.26	0.430	72.06	23.77	2081.667	27.32
7	26.00	0.364	303.11	100.00	7619.512	100.00

This report has been created by IC Net
METROHM LTD

Report date: 7/23/2021 4:18:33 PM
Printed by: wet


Ident: M3151-03MSD
Analysis from: 7/23/2021 2:08:28 PM
File: _2021-07-23_

Last save: 7/23/2021 2:34:28 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27669

Last save: 7/12/2021 3:21:

SAMPLE: 5..22g/100mL
: AP/MA
Vial number: 19
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

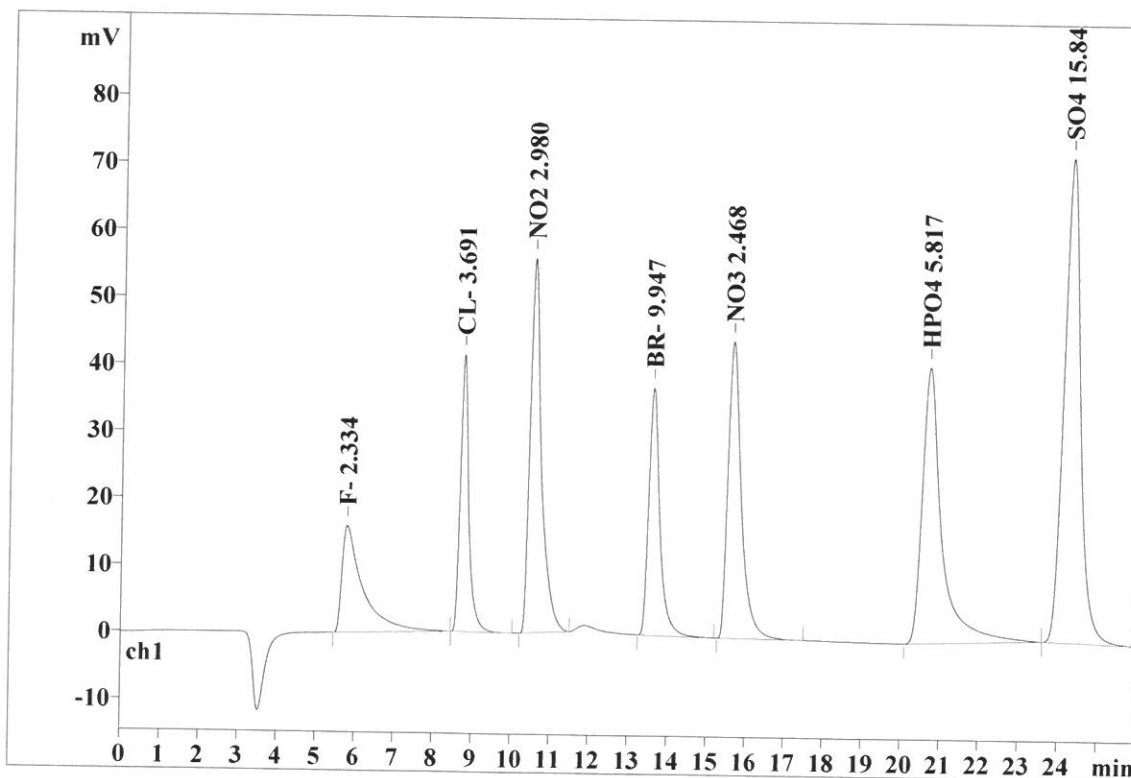

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.78	0.477	15.88	5.16	594.107	7.76
2	8.73	0.213	41.30	13.43	620.906	8.11
3	10.52	0.277	55.81	18.15	1115.289	14.57
4	13.58	0.293	36.90	12.00	744.737	9.73
5	15.61	0.347	44.23	14.39	1059.487	13.84
6	20.67	0.450	41.11	13.37	1441.089	18.82
7	24.24	0.429	72.24	23.50	2080.670	27.18
7	26.00	0.355	307.48	100.00	7656.285	100.00

This report has been created by IC Net
METROHM LTD

Report date: 7/23/2021 4:18:42 PM
Printed by: wet


Ident: CCV
Analysis from: 7/23/2021 2:37:07 PM
File: _2021-07-23_

Last save: 7/23/2021 3:03:07 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27670

Last save: 7/12/2021 3:21:

SAMPLE:
: AP/MA
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

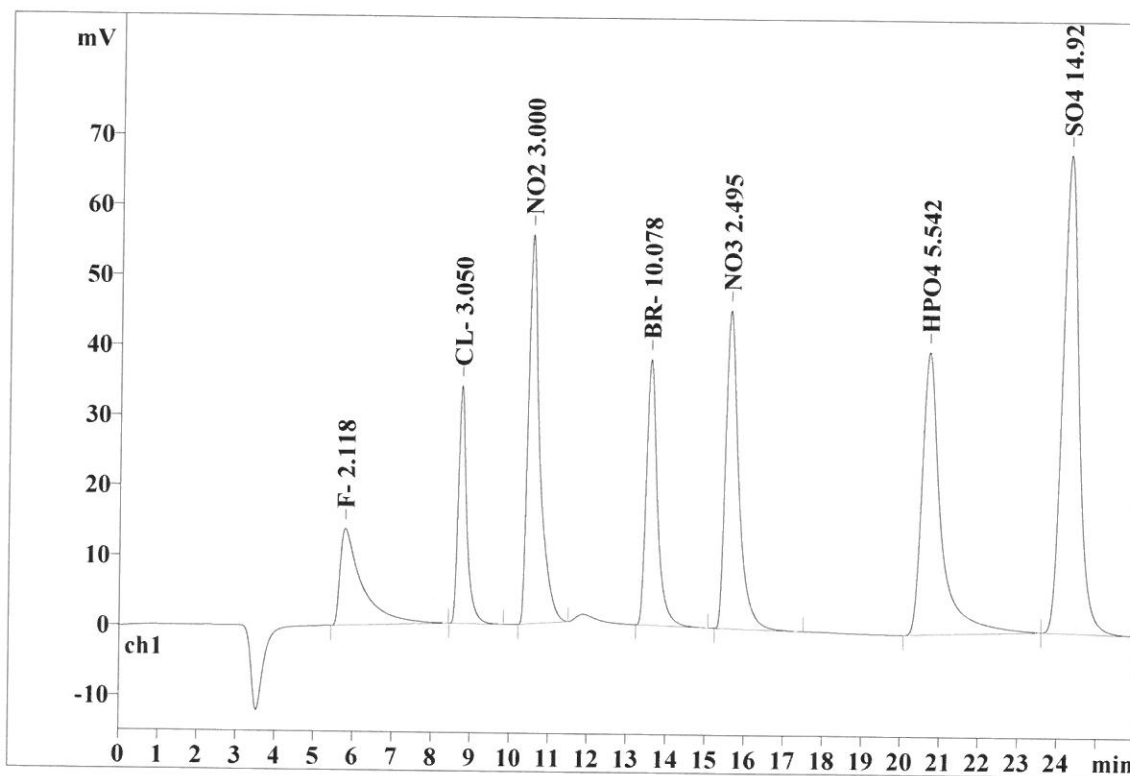

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.78	0.499	13.78	4.67	536.577	7.32
2	8.72	0.214	33.92	11.50	509.367	6.95
3	10.51	0.279	55.52	18.82	1123.015	15.33
4	13.56	0.290	37.92	12.85	755.050	10.30
5	15.58	0.343	45.36	15.37	1071.612	14.62
6	20.67	0.443	40.30	13.66	1379.074	18.82
7	24.24	0.427	68.20	23.12	1953.030	26.65
7	26.00	0.356	295.01	100.00	7327.726	100.00

This report has been created by IC Net
METROHM LTD

Report date: 7/23/2021 4:18:58 PM
Printed by: wet


Ident: CCB
Analysis from: 7/23/2021 3:44:28 PM
File: _2021-07-23_

Last save: 7/23/2021 4:10:28 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27671

Last save: 7/12/2021 3:21:

SAMPLE:
: AP/MA
Vial number: 12
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

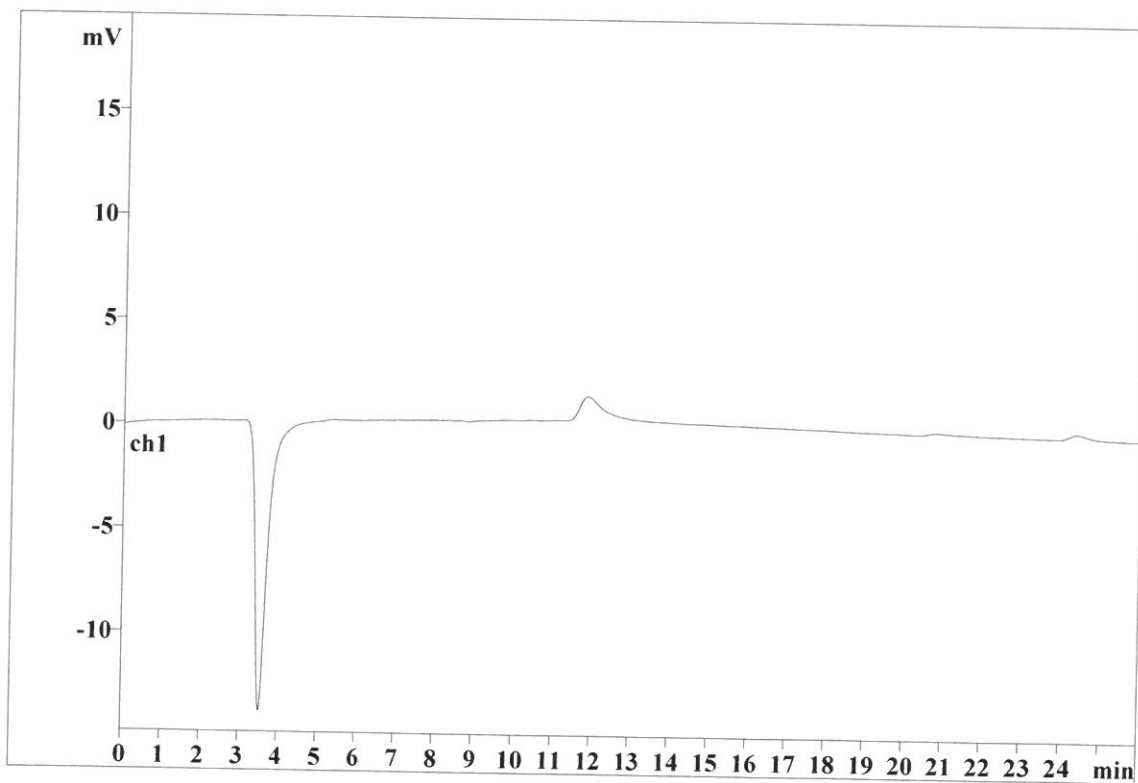

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD