


LB 115527

7471B

INSTRUMENT ID: CV1

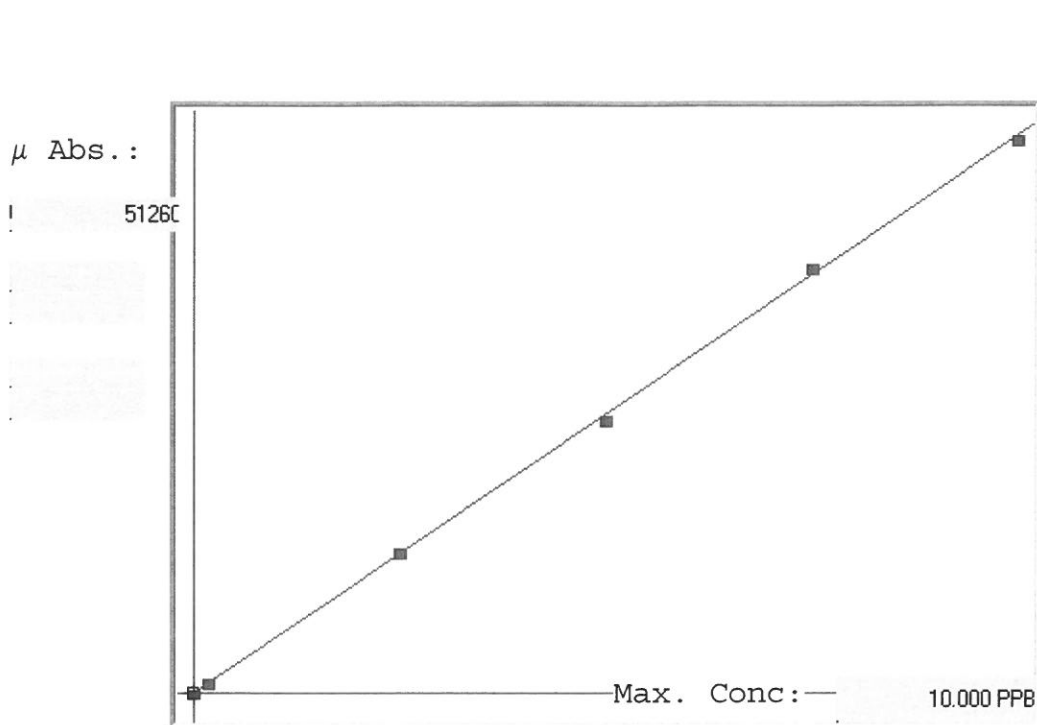

Linear

A= 0.0000e+000

B= 1.9392e-004

C= 7.9917e-003

Rho= 0.9998319

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	o/e))
0.0	0.000	0.008	0.008	-1	0.000	-1					-
0.2	0.200	0.197	-0.003	977	0.0 %	977					-2
2.5	2.500	2.520	0.020	12952	0.0 %	12952					1
5.0	5.000	4.904	-0.096	25248	0.0 %	25248					-2
7.5	7.500	7.623	0.123	39269	0.0 %	39269					2
10.0	10.000	9.948	-0.052	51260	0.0 %	51260					-1

LB115527 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 26 Jul 2021 11:47:49

Sample ID	Extended ID	μ Abs.	Conc.	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	50	-1	-	0.00007471B	PPB	26 Jul 2021 11:48:48	S	Std
0.2 - 1	50.2	977	-	0.20007471B	PPB	26 Jul 2021 11:51:05	S	Std
2.5 - 1	52.5	12952	-	2.50007471B	PPB	26 Jul 2021 11:53:22	S	Std
5.0 - 1	55	25248	-	5.00007471B	PPB	26 Jul 2021 11:55:38	S	Std
7.5 - 1	57.5	39269	-	7.50007471B	PPB	26 Jul 2021 11:57:55	S	Std
10.0 - 1	59	51260	-	10.00007471B	PPB	26 Jul 2021 12:00:11	S	Std
ICV20 - 1	ICV20	20228	3.9306	-7471B	PPB	26 Jul 2021 12:03:01	U	SMPL
ICB20 - 1	ICB20	-132	-0.0176	-7471B	PPB	26 Jul 2021 12:05:15	U	SMPL
CCV23 - 1	CCV23	25360	4.9257	-7471B	PPB	26 Jul 2021 12:07:31	U	SMPL
CCB23 - 1	CCB23	-143	-0.0197	-7471B	PPB	26 Jul 2021 12:09:46	U	SMPL
CRA - 1	CRA	960	0.1942	-7471B	PPB	26 Jul 2021 12:12:01	U	SMPL
HighStd - 1	HighStd	51504	9.9955	-7471B	PPB	26 Jul 2021 12:14:15	U	SMPL
ChkStd - 1	ChkStd	36894	7.1624	-7471B	PPB	26 Jul 2021 12:16:31	U	SMPL
PB137928BL - 1	PBS	-153	-0.0217	-7471B	PPB	26 Jul 2021 12:18:48	U	SMPL
PB137928BS - 1	LCSS	21390	4.1559	-7471B	PPB	26 Jul 2021 12:21:04	U	SMPL
M3148-02 - 1	SI-2-EXCA-SOIL	1103	0.2219	-7471B	PPB	26 Jul 2021 12:23:20	U	SMPL
M3148-02DUP - 1	SI-2-EXCA-SOILDUP	1140	0.2291	-7471B	PPB	26 Jul 2021 12:25:36	U	SMPL
M3148-02MS - 1	SI-2-EXCA-SOILMS	20200	3.9251	-7471B	PPB	26 Jul 2021 12:27:53	U	SMPL
M3148-02MSD - 1	SI-2-EXCA-SOILMSD	20325	3.9494	-7471B	PPB	26 Jul 2021 12:30:10	U	SMPL
M3148-04 - 1	SI-2-CLEAN-SOIL	855	0.1738	-7471B	PPB	26 Jul 2021 12:32:25	U	SMPL
CCV24 - 1	CCV24	25057	4.8670	-7471B	PPB	26 Jul 2021 12:34:41	U	SMPL
CCB24 - 1	CCB24	-140	-0.0192	-7471B	PPB	26 Jul 2021 12:36:56	U	SMPL
M3151-01 - 1	COMP-1	1767	0.3506	-7471B	PPB	26 Jul 2021 12:39:12	U	SMPL
M3151-02 - 1	COMP-2	7624	1.4864	-7471B	PPB	26 Jul 2021 12:41:28	U	SMPL
M3151-03 - 1	COMP-3	5249	1.0259	-7471B	PPB	26 Jul 2021 12:43:43	U	SMPL
M3158-01 - 1	WASTE	2644	0.5207	-7471B	PPB	26 Jul 2021 12:45:58	U	SMPL
M3159-11 - 1	20210535-COM-8	33413	6.4874	-7471B	PPB	26 Jul 2021 12:48:14	U	SMPL
M3159-12 - 1	20210539-COM-12	27465	5.3339	-7471B	PPB	26 Jul 2021 12:50:31	U	SMPL
M3159-13 - 1	20210545-COM-18	25340	4.9219	-7471B	PPB	26 Jul 2021 12:52:48	U	SMPL
M3159-14 - 1	20210554-COM-27	55456	10.7619	-7471B	PPB	26 Jul 2021 12:55:05	U	SMPL
M3159-15 - 1	20210556-COM-29	21647	4.2057	-7471B	PPB	26 Jul 2021 12:57:22	U	SMPL
CCV25 - 1	CCV25	25315	4.9170	-7471B	PPB	26 Jul 2021 12:59:40	U	SMPL
CCB25 - 1	CCB25	-132	-0.0176	-7471B	PPB	26 Jul 2021 13:01:56	U	SMPL
M3148-02LX5 - 1		210	0.0487	-7471B	PPB	26 Jul 2021 13:04:11	U	SMPL
M3148-02A - 1		20784	4.0384	-7471B	PPB	26 Jul 2021 13:06:27	U	SMPL
M3159-14DLX2 - 1		27382	5.3178	-7471B	PPB	26 Jul 2021 13:08:42	U	SMPL
CCV26 - 1	CCV26	25417	4.9368	-7471B	PPB	26 Jul 2021 13:10:57	U	SMPL
CCB26 - 1	CCB26	-113	-0.0139	-7471B	PPB	26 Jul 2021 13:13:14	U	SMPL