

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : AM Instrument ID : Konelab

7/27/2021 11:45

Test: ~~Total~~ CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	94.897	0.0	0.074	
ICB1	1.390	0.0	0.001	
CCV1	239.913	0.0	0.188	
CCB1	1.676	0.0	0.001	
PB137999BL	1.366	0.0	0.001	
M3176-02	1.610	0.0	0.001	
M3176-02DUP	1.849	0.0	0.001	
M3183-02	1.629	0.0	0.001	
CCV2	244.992	0.0	0.192	
CCB2	1.793	0.0	0.001	

N	10
Mean	59.111
SD	100.9188
CV%	170.73

Aquakem v. 7.2AQ1

Results from time period:

Tue Jul 27 11:00:12 2021

Tue Jul 27 11:43:30 2021

Sample Id	Sam/Ctr/c/	Test short na	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	1.0114	µg/l	7/27/2021 11:17:00.	
5.OPPBCN	A	Reactive CN	P	5.3567	µg/l	7/27/2021 11:17:01.	
10PPBCN	A	Reactive CN	P	10.2811	µg/l	7/27/2021 11:17:02.	
50PPBCN	A	Reactive CN	P	48.3779	µg/l	7/27/2021 11:17:03.	
100PPBCN	A	Reactive CN	P	98.3047	µg/l	7/27/2021 11:17:04.	
250PPBCN	A	Reactive CN	P	252.3522	µg/l	7/27/2021 11:17:05.	
500PPBCN	A	Reactive CN	P	499.3159	µg/l	7/27/2021 11:17:06.	
ICV1	S	Reactive CN	P	94.8967	µg/l	7/27/2021 11:40:42.	
ICB1	S	Reactive CN	P	1.3898	µg/l	7/27/2021 11:40:43.	
CCV1	S	Reactive CN	P	239.9126	µg/l	7/27/2021 11:40:44.	
CCB1	S	Reactive CN	P	1.6764	µg/l	7/27/2021 11:40:45.	
PB137999BL	S	Reactive CN	P	1.3656	µg/l	7/27/2021 11:40:46.	
M3176-02	S	Reactive CN	P	1.6101	µg/l	7/27/2021 11:40:47.	
M3176-02DUP	S	Reactive CN	P	1.849	µg/l	7/27/2021 11:40:48.	
M3183-02	S	Reactive CN	P	1.6291	µg/l	7/27/2021 11:40:49.	
CCV2	S	Reactive CN	P	244.9923	µg/l	7/27/2021 11:40:50.	
CCB2	S	Reactive CN	P	1.7931	µg/l	7/27/2021 11:40:51.	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : AS

Instrument ID : Konelab

7/27/2021 11:17


Test Total CN

Accepted 7/27/2021 11:17

Factor 1276
Bias 0

Coeff. of det. 0.999938

Errors

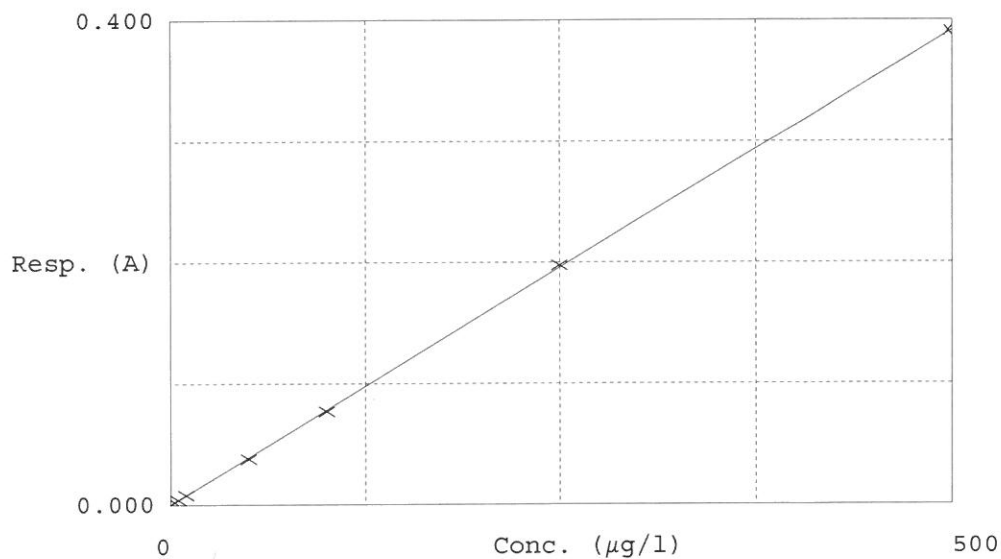

	Calibrator	Response	Calc. con.	Conc.	Relative Errors
1	0.0PPBCN	0.001	1.0114	0.0000	9.1
2	5.0PPBCN	0.004	5.3567	5.0000	2.8
3	10PPBCN	0.008	10.2811	10.0000	-3.2
4	50PPBCN	0.038	48.3779	50.0000	-1.2
5	100PPBCN	0.077	98.3047	100.0000	0.9
6	250PPBCN	0.198	252.3522	250.0000	-0.1
7	500PPBCN	0.391	499.3159	500.0000	

Relative Errors

AS

7/27/21

7/27/21