


LB115584

7470A

INSTRUMENT ID: CV4

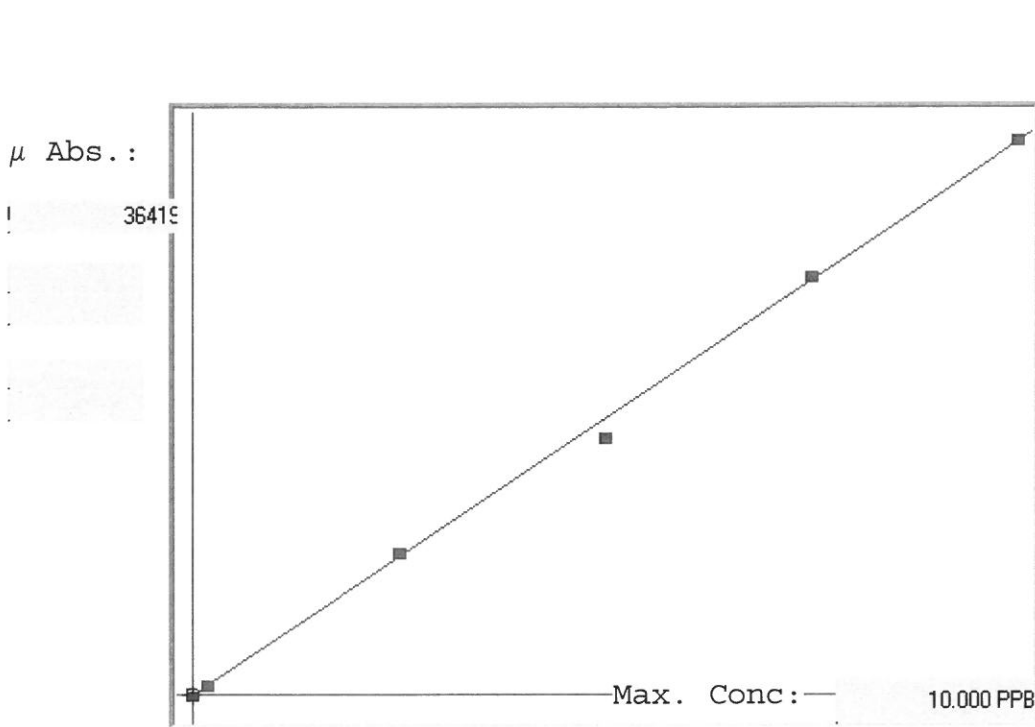

Linear

A= 0.0000e+000

B= 2.7513e-004

C= 2.5733e-002

Rho= 0.9992170

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.034	0.034	30	0.000	30					-
0.2	0.200	0.222	0.022	715	0.0 %	715					11
2.5	2.500	2.623	0.123	9441	0.0 %	9441					5
5.0	5.000	4.683	-0.317	16927	0.0 %	16927					-6
7.5	7.500	7.592	0.092	27499	0.0 %	27499					1
10.0	10.000	10.046	0.046	36419	0.0 %	36419					0

LB115584 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 28 Jul 2021 16:08:06

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	30	-	0.0000	7470A	PPB	28 Jul 2021 16:09:04	S	Std
0.2 - 1	50.2	715	-	0.2000	7470A	PPB	28 Jul 2021 16:11:20	S	Std
2.5 - 1	52.5	9441	-	2.5000	7470A	PPB	28 Jul 2021 16:13:37	S	Std
5.0 - 1	55	16927	-	5.0000	7470A	PPB	28 Jul 2021 16:15:54	S	Std
7.5 - 1	57.5	27499	-	7.5000	7470A	PPB	28 Jul 2021 16:18:10	S	Std
10.0 - 1	518	36419	-	10.0000	7470A	PPB	28 Jul 2021 16:23:01	S	Std
ICV26 - 1	ICV26	15249	4.2212	-	7470A	PPB	28 Jul 2021 16:25:45	U	SMPL
ICB26 - 1	ICB26	-93	0.0001	-	7470A	PPB	28 Jul 2021 16:27:59	U	SMPL
CCV43 - 1	CCV43	16651	4.6070	-	7470A	PPB	28 Jul 2021 16:30:14	U	SMPL
CCB43 - 1	CCB43	-80	0.0037	-	7470A	PPB	28 Jul 2021 16:32:29	U	SMPL
CRA - 1	CRA	686	0.2145	-	7470A	PPB	28 Jul 2021 16:34:43	U	SMPL
HighStd - 1	HighStd	35894	9.9013	-	7470A	PPB	28 Jul 2021 16:36:58	U	SMPL
ChkStd - 1	ChkStd	25124	6.9382	-	7470A	PPB	28 Jul 2021 16:39:13	U	SMPL
PB138027BL - 1	PBW	-149	-0.0153	-	7470A	PPB	28 Jul 2021 16:41:30	U	SMPL
PB138027BS - 1	LCSW	14514	4.0190	-	7470A	PPB	28 Jul 2021 16:43:45	U	SMPL
M3198-02 - 1	TP-7	-87	0.0018	-	7470A	PPB	28 Jul 2021 16:46:02	U	SMPL
M3198-06 - 1	TP-8	9	0.0282	-	7470A	PPB	28 Jul 2021 16:48:18	U	SMPL
M3198-06DUP - 1	TP-8DUP	29	0.0337	-	7470A	PPB	28 Jul 2021 16:50:35	U	SMPL
M3198-06MS - 1	TP-8MS	15710	4.3481	-	7470A	PPB	28 Jul 2021 16:52:52	U	SMPL
M3198-06MSD - 1	TP-8MSD	14395	3.9863	-	7470A	PPB	28 Jul 2021 16:55:07	U	SMPL
CCV44 - 1	CCV44	16421	4.5437	-	7470A	PPB	28 Jul 2021 16:57:22	U	SMPL
CCB44 - 1	CCB44	-90	0.0010	-	7470A	PPB	28 Jul 2021 16:59:37	U	SMPL
PB138027TB - 1	PB138006TB	-17	0.0211	-	7470A	PPB	28 Jul 2021 17:01:52	U	SMPL
M3198-06LX5 - 1		8	0.0279	-	7470A	PPB	28 Jul 2021 17:04:07	U	SMPL
M3198-06A - 1		15715	4.3494	-	7470A	PPB	28 Jul 2021 17:06:22	U	SMPL
CCV45 - 1	CCV45	16530	4.5737	-	7470A	PPB	28 Jul 2021 17:08:37	U	SMPL
CCB45 - 1	CCB45	-83	0.0029	-	7470A	PPB	28 Jul 2021 17:10:53	U	SMPL