


LB115595

7471B

INSTRUMENT ID: CV2

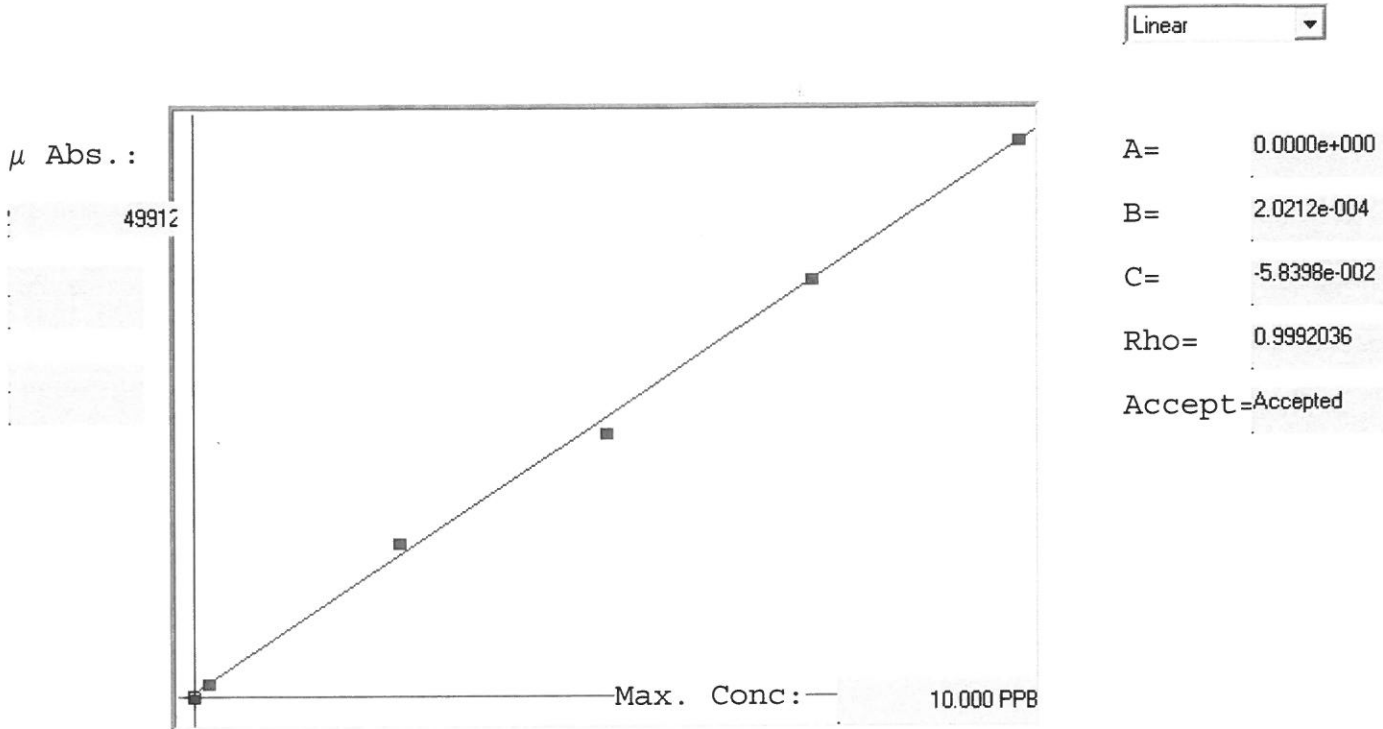

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	0/0
0.0	0.000	-0.048	-0.048	49	0.000	49					-2
0.2	0.200	0.196	-0.004	1260	0.0 %	1260					10
2.5	2.500	2.747	0.247	13878	0.0 %	13878					-5
5.0	5.000	4.745	-0.255	23765	0.0 %	23765					0
7.5	7.500	7.531	0.031	37550	0.0 %	37550					0
10.0	10.000	10.030	0.030	49912	0.0 %	49912					0

LB115595 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 29 Jul 2021 10:54:02

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	49	-	0.0000	7471B	PPB	29 Jul 2021 11:05:23	S	Std
0.2 - 1	50.2	1260	-	0.2000	7471B	PPB	29 Jul 2021 11:07:39	S	Std
2.5 - 1	52.5	13878	-	2.5000	7471B	PPB	29 Jul 2021 11:09:57	S	Std
5.0 - 1	55	23765	-	5.0000	7471B	PPB	29 Jul 2021 11:12:13	S	Std
7.5 - 1	57.5	37550	-	7.5000	7471B	PPB	29 Jul 2021 11:17:10	S	Std
10.0 - 1	510	49912	-	10.0000	7471B	PPB	29 Jul 2021 11:24:33	S	Std
ICV27 - 1	ICV27	21265	4.2396	-	7471B	PPB	29 Jul 2021 11:27:24	U	SMPL
ICB27 - 1	ICB27	12	-0.0560	-	7471B	PPB	29 Jul 2021 11:29:39	U	SMPL
CCV46 - 1	CCV46	24784	4.9509	-	7471B	PPB	29 Jul 2021 11:31:55	U	SMPL
CCB46 - 1	CCB46	39	-0.0505	-	7471B	PPB	29 Jul 2021 11:34:11	U	SMPL
CRA - 1	CRA	1223	0.1888	-	7471B	PPB	29 Jul 2021 11:36:27	U	SMPL
HighStd - 1	HighStd	50025	10.0525	-	7471B	PPB	29 Jul 2021 11:38:42	U	SMPL
ChkStd - 1	ChkStd	35769	7.1711	-	7471B	PPB	29 Jul 2021 11:40:57	U	SMPL
PB138056BL - 1	PBS	185	-0.0210	-	7471B	PPB	29 Jul 2021 11:43:14	U	SMPL
PB138056BS - 1	LCSS	21464	4.2798	-	7471B	PPB	29 Jul 2021 11:45:30	U	SMPL
M3198-01 - 1	TP-7	28485	5.6989	-	7471B	PPB	29 Jul 2021 11:47:46	U	SMPL
M3198-05 - 1	TP-8	79865	16.0837	-	7471B	PPB	29 Jul 2021 11:50:03	U	SMPL
M3202-01 - 1	CL-02-072721	17461	3.4708	-	7471B	PPB	29 Jul 2021 11:52:21	U	SMPL
M3204-01 - 1	EO-01-072721	4302	0.8111	-	7471B	PPB	29 Jul 2021 11:54:40	U	SMPL
M3204-03 - 1	EO-03-072721	8993	1.7592	-	7471B	PPB	29 Jul 2021 11:56:55	U	SMPL
CCV47 - 1	CCV47	24856	4.9654	-	7471B	PPB	29 Jul 2021 11:59:11	U	SMPL
CCB47 - 1	CCB47	54	-0.0475	-	7471B	PPB	29 Jul 2021 12:01:26	U	SMPL
M3204-03DUP - 1	EO-03-072721DUP	7545	1.4666	-	7471B	PPB	29 Jul 2021 12:03:42	U	SMPL
M3204-03MS - 1	EO-03-072721MS	27171	5.4333	-	7471B	PPB	29 Jul 2021 12:05:58	U	SMPL
M3204-03MSD - 1	EO-03-072721MSD	27750	5.5503	-	7471B	PPB	29 Jul 2021 12:08:13	U	SMPL
M3205-02 - 1	VNJ-209	21073	4.2008	-	7471B	PPB	29 Jul 2021 12:10:30	U	SMPL
M3205-04 - 1	VNJ-211	2881	0.5239	-	7471B	PPB	29 Jul 2021 12:12:47	U	SMPL
M3215-01 - 1	PS-1	2056	0.3572	-	7471B	PPB	29 Jul 2021 12:15:04	U	SMPL
M3215-02 - 1	PS-2	1488	0.2424	-	7471B	PPB	29 Jul 2021 12:17:20	U	SMPL
M3219-01 - 1	TR-05-072821	851	0.1136	-	7471B	PPB	29 Jul 2021 12:19:37	U	SMPL
M3204-03LX5 - 1		1934	0.3325	-	7471B	PPB	29 Jul 2021 12:21:54	U	SMPL
M3204-03A - 1		27146	5.4283	-	7471B	PPB	29 Jul 2021 12:24:09	U	SMPL
CCV48 - 1	CCV48	25024	4.9994	-	7471B	PPB	29 Jul 2021 12:26:25	U	SMPL
CCB48 - 1	CCB48	42	-0.0499	-	7471B	PPB	29 Jul 2021 12:28:41	U	SMPL
M3198-05DLX5 - 1		15500	3.0744	-	7471B	PPB	29 Jul 2021 12:30:57	U	SMPL
CCV49 - 1	CCV49	24838	4.9618	-	7471B	PPB	29 Jul 2021 12:33:12	U	SMPL
CCB49 - 1	CCB49	-80	-0.0746	-	7471B	PPB	29 Jul 2021 12:35:28	U	SMPL