


LB115629

7471B

INSTRUMENT ID: CV2

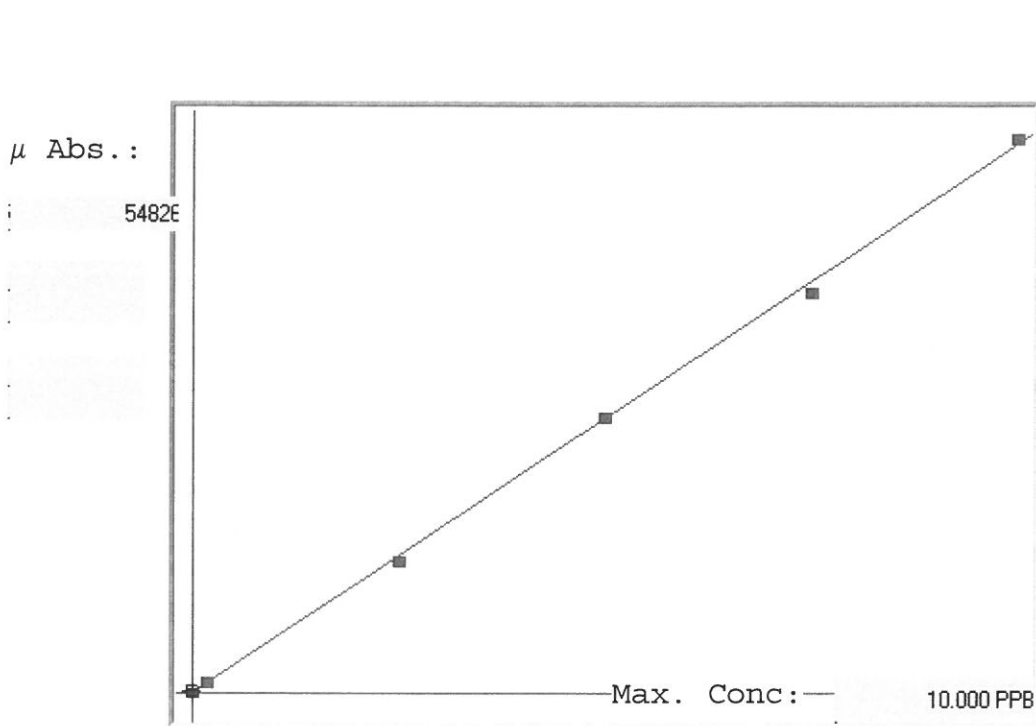

Linear

A= 0.0000e+000

B= 1.8449e-004

C= -2.2039e-003

Rho= 0.9997012

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.058	0.058	326	0.000	326					
0.2	0.200	0.219	0.019	1200	0.0 %	1200					-9
2.5	2.500	2.431	-0.069	13187	0.0 %	13187					-3
5.0	5.000	5.041	0.041	27336	0.0 %	27336					1
7.5	7.500	7.339	-0.161	39792	0.0 %	39792					-2
10.0	10.000	10.112	0.112	54826	0.0 %	54826					1

LB115629 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 30 Jul 2021 15:56:43

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	326	-	0.0000	7471B	PPB	30 Jul 2021 15:57:35	S	Std
0.2 - 1	50.2	1200	-	0.2000	7471B	PPB	30 Jul 2021 15:59:52	S	Std
2.5 - 1	52.5	13187	-	2.5000	7471B	PPB	30 Jul 2021 16:02:09	S	Std
5.0 - 1	55	27336	-	5.0000	7471B	PPB	30 Jul 2021 16:04:27	S	Std
7.5 - 1	57.5	39792	-	7.5000	7471B	PPB	30 Jul 2021 16:06:43	S	Std
10.0 - 1	51.1	54826	-	10.0000	7471B	PPB	30 Jul 2021 16:11:34	S	Std
ICV32 - 1	ICV32	20784	3.8322	-	7471B	PPB	30 Jul 2021 16:15:21	U	SMPL
ICB32 - 1	ICB32	181	0.0312	-	7471B	PPB	30 Jul 2021 16:17:36	U	SMPL
CCV64 - 1	CCV64	27327	5.0393	-	7471B	PPB	30 Jul 2021 16:19:51	U	SMPL
CCB64 - 1	CCB64	186	0.0321	-	7471B	PPB	30 Jul 2021 16:22:06	U	SMPL
CRA - 1	CRA	1215	0.2219	-	7471B	PPB	30 Jul 2021 16:24:22	U	SMPL
HighStd - 1	HighStd	55919	10.3141	-	7471B	PPB	30 Jul 2021 16:26:36	U	SMPL
ChkStd - 1	ChkStd	39053	7.2025	-	7471B	PPB	30 Jul 2021 16:28:51	U	SMPL
PB138097BL - 1	PBS	109	0.0179	-	7471B	PPB	30 Jul 2021 16:31:08	U	SMPL
PB138097BS - 1	LCSS	22088	4.0727	-	7471B	PPB	30 Jul 2021 16:33:26	U	SMPL
M3228-03 - 1	20210549-COM-22	105221	19.4097	-	7471B	PPB	30 Jul 2021 16:35:43	U	SMPL
M3228-04 - 1	20210552-COM-25	70866	13.0716	-	7471B	PPB	30 Jul 2021 16:38:00	U	SMPL
M3229-01 - 1	SOLID-A-E	4587	0.8440	-	7471B	PPB	30 Jul 2021 16:40:19	U	SMPL
M3234-01 - 1	OR-03-072921	2445	0.4489	-	7471B	PPB	30 Jul 2021 16:42:38	U	SMPL
M3235-01 - 1	MH-457-COMP	1786	0.3273	-	7471B	PPB	30 Jul 2021 16:44:53	U	SMPL
CCV65 - 1	CCV65	28207	5.2016	-	7471B	PPB	30 Jul 2021 16:53:32	U	SMPL
CCB65 - 1	CCB65	185	0.0319	-	7471B	PPB	30 Jul 2021 16:55:47	U	SMPL
M3235-03 - 1	MH-462-COMP	657	0.1190	-	7471B	PPB	30 Jul 2021 16:58:02	U	SMPL
M3238-01 - 1	282	5709	1.0510	-	7471B	PPB	30 Jul 2021 17:00:17	U	SMPL
M3238-03 - 1	221	1483	0.2714	-	7471B	PPB	30 Jul 2021 17:02:33	U	SMPL
M3238-03DUP - 1	221DUP	1578	0.2889	-	7471B	PPB	30 Jul 2021 17:04:48	U	SMPL
M3238-03MS - 1	221MS	25585	4.7179	-	7471B	PPB	30 Jul 2021 17:07:04	U	SMPL
M3238-03MSD - 1	221MSD	23810	4.3904	-	7471B	PPB	30 Jul 2021 17:11:55	U	SMPL
M3238-03LX5 - 1		443	0.0795	-	7471B	PPB	30 Jul 2021 17:14:11	U	SMPL
M3238-03A - 1		23811	4.3906	-	7471B	PPB	30 Jul 2021 17:16:28	U	SMPL
M3228-03DLX5 - 1		20207	3.7257	-	7471B	PPB	30 Jul 2021 17:18:44	U	SMPL
M3228-04DLX5 - 1		13224	2.4374	-	7471B	PPB	30 Jul 2021 17:21:00	U	SMPL
CCV66 - 1	CCV66	26546	4.8952	-	7471B	PPB	30 Jul 2021 17:31:01	U	SMPL
CCB66 - 1	CCB66	199	0.0345	-	7471B	PPB	30 Jul 2021 17:33:16	U	SMPL