


LB 115650

7470A

INSTRUMENT 115, CVL

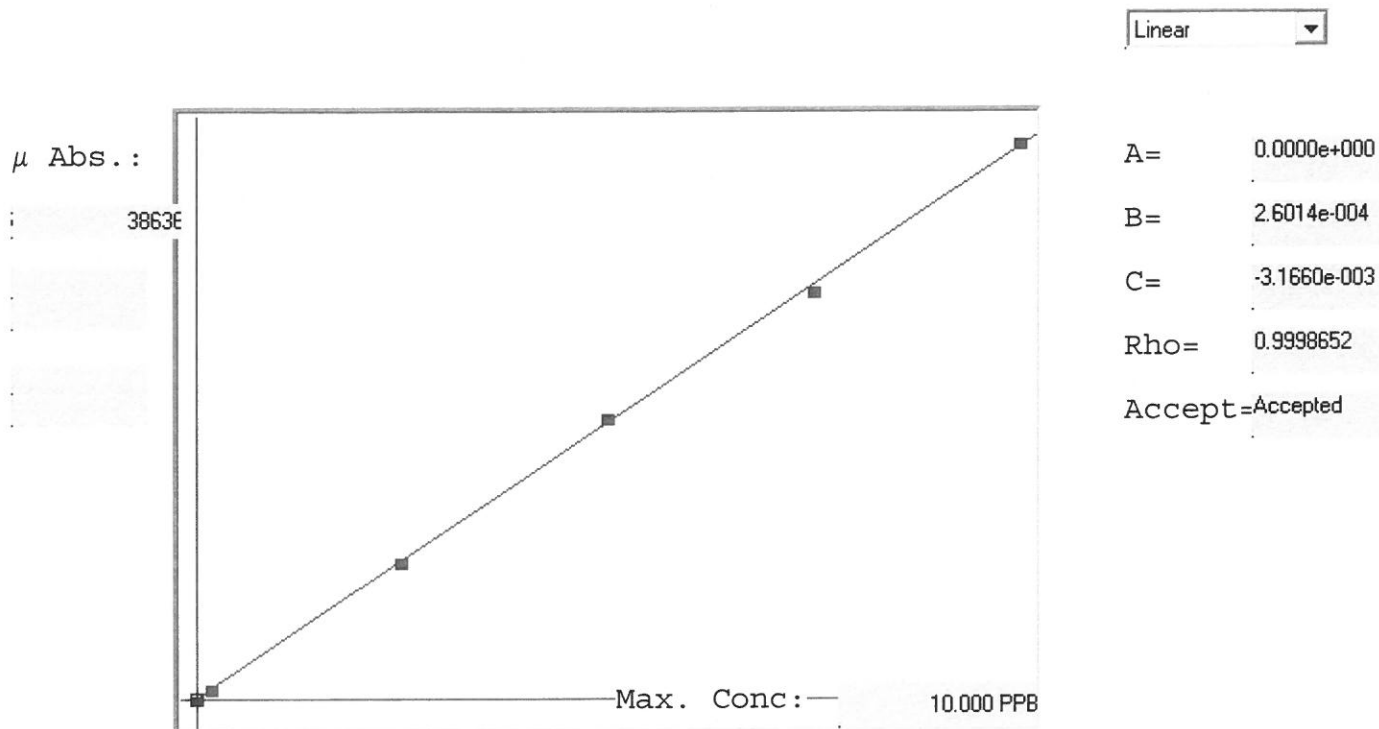

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	1/0 1)
0.0	0.000	0.004	0.004	29	0.000	29					1
0.2	0.200	0.201	0.001	785	0.0 %	785					-1
2.5	2.500	2.480	-0.020	9545	0.0 %	9545					2
5.0	5.000	5.080	0.080	19542	0.0 %	19542					-2
7.5	7.500	7.387	-0.113	28407	0.0 %	28407					0
10.0	10.000	10.048	0.048	38636	0.0 %	38636					

LB115650 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 02 Aug 2021 11:21:15

Sample ID	Extended ID	μ Abs	Conc	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	50	29	-	0.00007470A	PPB	02 Aug 2021 11:33:50	S	Std
0.2 - 1	50.2	785	-	0.20007470A	PPB	02 Aug 2021 11:36:07	S	Std
2.5 - 1	52.5	9545	-	2.50007470A	PPB	02 Aug 2021 11:38:24	S	Std
5.0 - 1	55	19542	-	5.00007470A	PPB	02 Aug 2021 11:40:41	S	Std
7.5 - 1	57.5	28407	-	7.50007470A	PPB	02 Aug 2021 11:42:57	S	Std
10.0 - 1	51	38636	-	10.00007470A	PPB	02 Aug 2021 11:45:13	S	Std
ICV33 - 1	ICV33	15578	4.0493	-7470A	PPB	02 Aug 2021 11:49:54	U	SMPL
ICB33 - 1	ICB33	-35	-0.0123	-7470A	PPB	02 Aug 2021 11:52:09	U	SMPL
CCV67 - 1	CCV67	18215	4.7353	-7470A	PPB	02 Aug 2021 11:54:24	U	SMPL
CCB67 - 1	CCB67	-21	-0.0086	-7470A	PPB	02 Aug 2021 11:56:39	U	SMPL
CRA - 1	CRA	769	0.1969	-7470A	PPB	02 Aug 2021 11:58:54	U	SMPL
HighStd - 1	HighStd	36832	9.5783	-7470A	PPB	02 Aug 2021 12:01:09	U	SMPL
ChkStd - 1	ChkStd	25793	6.7066	-7470A	PPB	02 Aug 2021 12:03:24	U	SMPL
PB138082BL - 1	PBW	-66	-0.0203	-7470A	PPB	02 Aug 2021 12:05:41	U	SMPL
PB138082BS - 1	LCSW	13649	3.5475	-7470A	PPB	02 Aug 2021 12:07:57	U	SMPL
M3206-05 - 1	SPLP-LEACHATE-AMENDED-COM-4	-46	-0.0151	-7470A	PPB	02 Aug 2021 12:10:13	U	SMPL
M3206-05DUP - 1	SPLP-LEACHATE-AMENDED-COM-4DUP	2	-0.0026	-7470A	PPB	02 Aug 2021 12:12:30	U	SMPL
M3206-05MS - 1	SPLP-LEACHATE-AMENDED-COM-4MS	14708	3.8230	-7470A	PPB	02 Aug 2021 12:14:46	U	SMPL
M3206-05MSD - 1	SPLP-LEACHATE-AMENDED-COM-4MSD	14854	3.8610	-7470A	PPB	02 Aug 2021 12:17:03	U	SMPL
M3216-11 - 1	SPLP-LEACHATE-AMENDED-COM-7	6	-0.0016	-7470A	PPB	02 Aug 2021 12:19:18	U	SMPL
CCV68 - 1	CCV68	18987	4.9361	-7470A	PPB	02 Aug 2021 12:21:34	U	SMPL
CCB68 - 1	CCB68	-30	-0.0110	-7470A	PPB	02 Aug 2021 12:23:49	U	SMPL
M3223-02 - 1	BACKFILL-ASHCROFT-REAR-09	389	0.0980	-7470A	PPB	02 Aug 2021 12:26:04	U	SMPL
M3223-04 - 1	BACKFILL-ASHCROFT-REAR-10	90	0.0202	-7470A	PPB	02 Aug 2021 12:28:19	U	SMPL
M3223-06 - 1	BACKFILL-ASHCROFT-REAR-11	55	0.0111	-7470A	PPB	02 Aug 2021 12:30:34	U	SMPL
PB138082TB - 1	PB138024TB	10	-0.0006	-7470A	PPB	02 Aug 2021 12:32:50	U	SMPL
M3206-05LX5 - 1		62	0.0130	-7470A	PPB	02 Aug 2021 12:35:05	U	SMPL
M3206-05A - 1		15447	4.0152	-7470A	PPB	02 Aug 2021 12:37:22	U	SMPL
CCV69 - 1	CCV69	18670	4.8536	-7470A	PPB	02 Aug 2021 12:39:38	U	SMPL
CCB69 - 1	CCB69	10	-0.0006	-7470A	PPB	02 Aug 2021 12:41:55	U	SMPL