


LB115665

7470A

INSTRUMENT ID: CV1

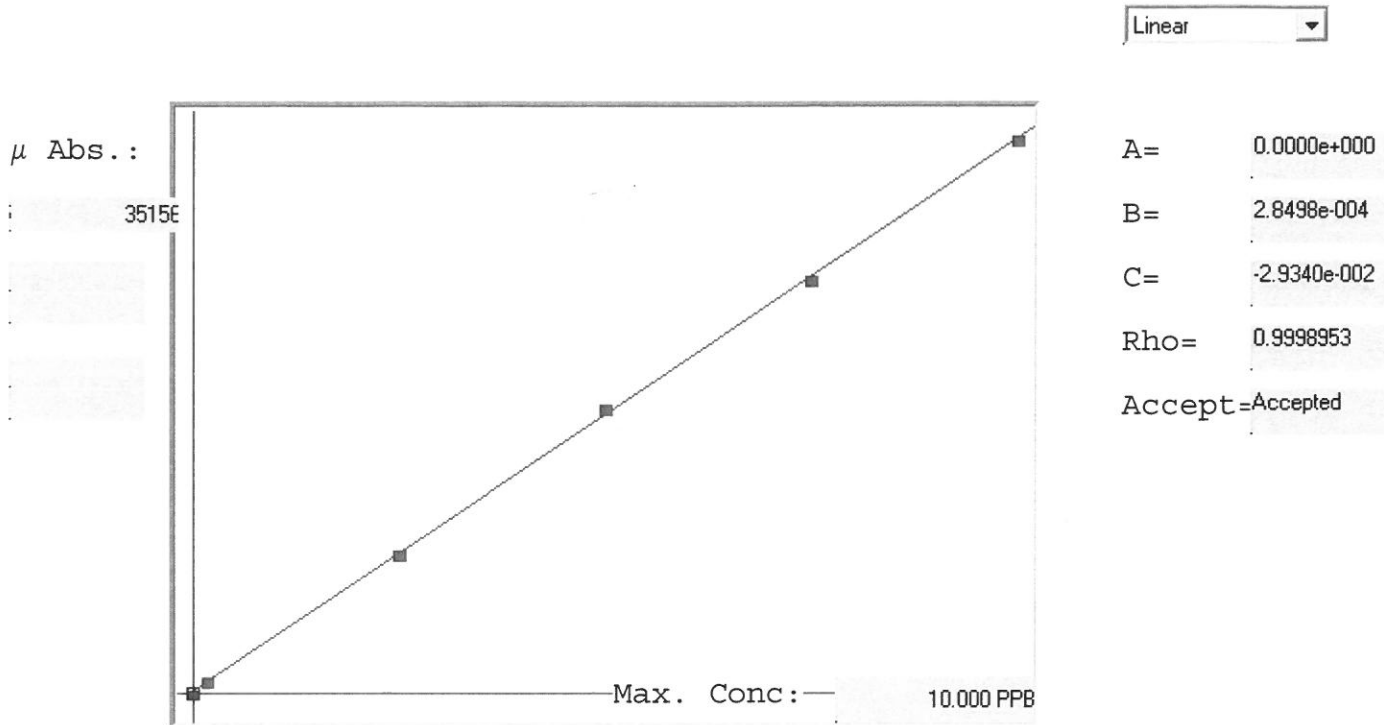

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	-0.030	-0.030	-4	0.000	-4					1
0.2	0.200	0.196	-0.004	791	0.0 %	791					-2
2.5	2.500	2.494	-0.006	8854	0.0 %	8854					0
5.0	5.000	5.111	0.111	18039	0.0 %	18039					2
7.5	7.500	7.440	-0.060	26210	0.0 %	26210					-1
10.0	10.000	9.989	-0.011	35156	0.0 %	35156					0

LB115665 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 03 Aug 2021 09:49:59				
Sample ID	Extended ID	μ Abs	Conc.	Std CondMethod	Units	Date	Type	Type
0.0 - 1	50	-4	-	0.00007470A	PPB	03 Aug 2021 10:16:55	S	Std
0.2 - 1	50.2	791	-	0.20007470A	PPB	03 Aug 2021 10:19:12	S	Std
2.5 - 1	52.5	8854	-	2.50007470A	PPB	03 Aug 2021 10:21:29	S	Std
5.0 - 1	55	18039	-	5.00007470A	PPB	03 Aug 2021 10:23:45	S	Std
7.5 - 1	57.5	26210	-	7.50007470A	PPB	03 Aug 2021 10:28:49	S	Std
10.0 - 1	518	35156	-	10.00007470A	PPB	03 Aug 2021 10:31:05	S	Std
ICV34 - 1	ICV34	14731	4.1687	-7470A	PPB	03 Aug 2021 10:35:53	U	SMPL
ICB34 - 1	ICB34	-77	-0.0513	-7470A	PPB	03 Aug 2021 10:38:08	U	SMPL
CCV74 - 1	CCV74	18202	5.1578	-7470A	PPB	03 Aug 2021 10:40:22	U	SMPL
CCB74 - 1	CCB74	-108	-0.0601	-7470A	PPB	03 Aug 2021 10:42:37	U	SMPL
CRA - 1	CRA	762	0.1878	-7470A	PPB	03 Aug 2021 10:44:52	U	SMPL
HighStd - 1	HighStd	35900	10.2013	-7470A	PPB	03 Aug 2021 10:47:07	U	SMPL
ChkStd - 1	ChkStd	25869	7.3427	-7470A	PPB	03 Aug 2021 10:49:22	U	SMPL
PB138132BL - 1	PBW	-96	-0.0567	-7470A	PPB	03 Aug 2021 10:51:38	U	SMPL
PB138132BS - 1	LCSW	13838	3.9142	-7470A	PPB	03 Aug 2021 10:53:54	U	SMPL
M3217-03 - 1	280	2	-0.0288	-7470A	PPB	03 Aug 2021 10:56:10	U	SMPL
M3229-02 - 1	SOLID-A-E	47	-0.0159	-7470A	PPB	03 Aug 2021 10:58:26	U	SMPL
M3229-02DUP - 1	SOLID-A-EDUP	44	-0.0168	-7470A	PPB	03 Aug 2021 11:00:43	U	SMPL
M3229-02MS - 1	SOLID-A-EMS	14380	4.0686	-7470A	PPB	03 Aug 2021 11:05:39	U	SMPL
M3229-02MSD - 1	SOLID-A-EMSD	14406	4.0760	-7470A	PPB	03 Aug 2021 11:07:53	U	SMPL
CCV75 - 1	CCV75	17999	5.1000	-7470A	PPB	03 Aug 2021 11:10:09	U	SMPL
CCB75 - 1	CCB75	-99	-0.0576	-7470A	PPB	03 Aug 2021 11:12:24	U	SMPL
PB138142BS - 1	LCSW	14146	4.0019	-7470A	PPB	03 Aug 2021 11:16:54	U	SMPL
M3229-06 - 1	WATER-A-B	251	0.0422	-7470A	PPB	03 Aug 2021 11:19:10	U	SMPL
M3229-06DUP - 1	WATER-A-BDUP	303	0.0570	-7470A	PPB	03 Aug 2021 11:21:26	U	SMPL
M3229-06MS - 1	WATER-A-BMS	15919	4.5072	-7470A	PPB	03 Aug 2021 11:23:41	U	SMPL
M3229-06MSD - 1	WATER-A-BMSD	16397	4.6434	-7470A	PPB	03 Aug 2021 11:25:58	U	SMPL
M3242-01 - 1	257392	-50	-0.0436	-7470A	PPB	03 Aug 2021 11:28:14	U	SMPL
PB138142BL - 1	PBW	-43	-0.0416	-7470A	PPB	03 Aug 2021 11:30:31	U	SMPL
CCV76 - 1	CCV76	18185	5.1530	-7470A	PPB	03 Aug 2021 11:32:48	U	SMPL
CCB76 - 1	CCB76	-57	-0.0456	-7470A	PPB	03 Aug 2021 11:35:03	U	SMPL
M3223-02 - 1	BACKFILL-ASHCROFT-REAR-09	102	-0.0003	-7470A	PPB	03 Aug 2021 11:39:53	U	SMPL
PB138132TB - 1	PB138061TB	109	0.0017	-7470A	PPB	03 Aug 2021 11:42:08	U	SMPL
M3229-02LX5 - 1		2	-0.0288	-7470A	PPB	03 Aug 2021 11:44:23	U	SMPL
M3229-02A - 1		15410	4.3622	-7470A	PPB	03 Aug 2021 11:46:39	U	SMPL
M3229-06LX5 - 1		-2	-0.0299	-7470A	PPB	03 Aug 2021 11:48:55	U	SMPL
M3229-06A - 1		14745	4.1726	-7470A	PPB	03 Aug 2021 11:51:10	U	SMPL
CCV77 - 1	CCV77	18424	5.2211	-7470A	PPB	03 Aug 2021 11:53:25	U	SMPL
CCB77 - 1	CCB77	-63	-0.0473	-7470A	PPB	03 Aug 2021 11:55:41	U	SMPL