

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : AL

Instrument ID : Konelab

8/3/2021 12:48

DeactiveTest: ~~Total~~ CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	90.204	0.0	0.065	
ICB1	0.796	0.0	0.001	
CCV1	241.661	0.0	0.174	
CCB1	0.894	0.0	0.001	
PB138150BL	0.716	0.0	0.001	
M3217-02	0.693	0.0	0.001	
M3217-02DUP	0.575	0.0	0.001	
PB138151BL	0.651	0.0	0.001	
M3242-01	0.605	0.0	0.001	
M3242-01DUP	0.614	0.0	0.001	
CCV2	245.325	0.0	0.177	
CCB2	0.256	0.0	0.000	

N	12
Mean	48.582
SD	94.5813
CV%	194.68

Aquakem v. 7.2AQ1

Results from time period:

Tue Aug 03 11:06:34 2021

Tue Aug 03 12:46:43 2021

Sample Id	Sam/Ctr/c/	Test short nam	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Reactive CN	P	0.6223	µg/l	8/3/2021 12:09:27	
5.0PPBCN	A	Reactive CN	P	6.0376	µg/l	8/3/2021 12:09:28	
10PPBCN	A	Reactive CN	P	10.0525	µg/l	8/3/2021 12:09:29	
50PPBCN	A	Reactive CN	P	47.8393	µg/l	8/3/2021 12:09:30	
100PPBCN	A	Reactive CN	P	97.669	µg/l	8/3/2021 12:09:31	
250PPBCN	A	Reactive CN	P	254.2168	µg/l	8/3/2021 12:09:32	
500PPBCN	A	Reactive CN	P	498.5625	µg/l	8/3/2021 12:09:33	
ICV1	S	Reactive CN	P	90.2036	µg/l	8/3/2021 12:42:50	
ICB1	S	Reactive CN	P	0.7959	µg/l	8/3/2021 12:42:51	
CCV1	S	Reactive CN	P	241.6606	µg/l	8/3/2021 12:42:52	
CCB1	S	Reactive CN	P	0.8936	µg/l	8/3/2021 12:42:53	
PB138150BL	S	Reactive CN	P	0.7157	µg/l	8/3/2021 12:42:54	
M3217-02	S	Reactive CN	P	0.6929	µg/l	8/3/2021 12:42:55	
M3217-02DUP	S	Reactive CN	P	0.5747	µg/l	8/3/2021 12:42:56	
PB138151BL	S	Reactive CN	P	0.6512	µg/l	8/3/2021 12:42:57	
M3242-01	S	Reactive CN	P	0.6047	µg/l	8/3/2021 12:42:58	
M3242-01DUP	S	Reactive CN	P	0.6143	µg/l	8/3/2021 12:42:59	
CCV2	S	Reactive CN	P	245.325	µg/l	8/3/2021 12:43:00	
CCB2	S	Reactive CN	P	0.2564	µg/l	8/3/2021 12:46:41	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : *pl*

Instrument ID : Konelab

8/3/2021 12:16


Test Total CN

Accepted 8/3/2021 12:15

Factor 1391
Bias 0

Coeff. of det. 0.999847

Errors

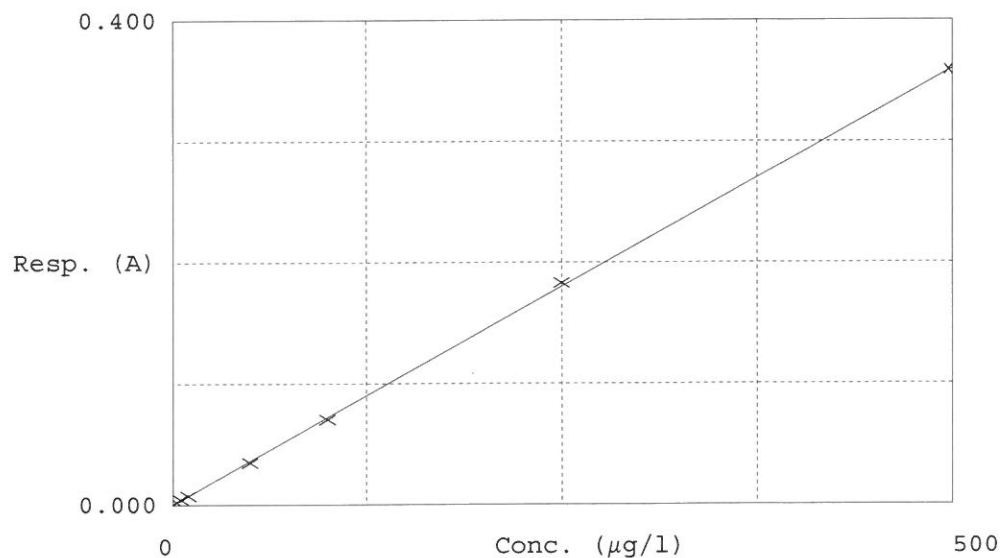

	Calibrator	Response	Calc. con.	Conc.	Relative Errors
1	0.0PPBCN	0.001	0.6223	0.0000	20.8
2	5.0PPBCN	0.005	6.0376	5.0000	0.5
3	10PPBCN	0.008	10.0525	10.0000	-4.3
4	50PPBCN	0.035	47.8393	50.0000	-2.3
5	100PPBCN	0.071	97.6690	100.0000	1.7
6	250PPBCN	0.183	254.2168	250.0000	-0.3
7	500PPBCN	0.359	498.5625	500.0000	

pl
8/3/21