

=====

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : AS

Instrument ID : Konelab

8/3/2021 14:08

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	92.551	0.0	0.067	
ICB1	0.989	0.0	0.001	
CCV1	247.808	0.0	0.179	
CCB1	0.795	0.0	0.001	
PB138154BL	0.737	0.0	0.001	
PB138154BS	94.696	0.0	0.068	
MIDPB138154	247.260	0.0	0.178	
M3265-02	6.004	0.0	0.005	
M3265-02DUP	6.379	0.0	0.005	
M3265-02MS	43.601	0.0	0.032	
M3265-02MSD	44.301	0.0	0.032	
CCV2	253.514	0.0	0.183	
CCB2	0.596	0.0	0.001	

N	13
Mean	79.941
SD	102.1495
CV%	127.78

Aquakem v. 7.2AQ1

Results from time period:

Tue Aug 03 14:00:25 2021

Tue Aug 03 14:06:14 2021

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	0.6223	µg/l	8/3/2021 12:09:27	
5.0PPBCN	A	Total CN	P	6.0376	µg/l	8/3/2021 12:09:28	
10PPBCN	A	Total CN	P	10.0525	µg/l	8/3/2021 12:09:29	
50PPBCN	A	Total CN	P	47.8393	µg/l	8/3/2021 12:09:30	
100PPBCN	A	Total CN	P	97.669	µg/l	8/3/2021 12:09:31	
250PPBCN	A	Total CN	P	254.2168	µg/l	8/3/2021 12:09:32	
500PPBCN	A	Total CN	P	498.5625	µg/l	8/3/2021 12:09:33	
ICV1	S	Total CN	P	92.5506	µg/l	8/3/2021 14:00:26	
ICB1	S	Total CN	P	0.9887	µg/l	8/3/2021 14:00:27	
CCV1	S	Total CN	P	247.8078	µg/l	8/3/2021 14:00:30	
CCB1	S	Total CN	P	0.7947	µg/l	8/3/2021 14:00:32	
PB138154BL	S	Total CN	P	0.7375	µg/l	8/3/2021 14:00:33	
PB138154BS	S	Total CN	P	94.6961	µg/l	8/3/2021 14:00:34	
MIDPB138154	S	Total CN	P	247.2595	µg/l	8/3/2021 14:00:35	
M3265-02	S	Total CN	P	6.0043	µg/l	8/3/2021 14:06:08	
M3265-02DUP	S	Total CN	P	6.3793	µg/l	8/3/2021 14:06:09	
M3265-02MS	S	Total CN	P	43.6011	µg/l	8/3/2021 14:06:10	
M3265-02MSD	S	Total CN	P	44.3006	µg/l	8/3/2021 14:06:11	
CCV2	S	Total CN	P	253.5141	µg/l	8/3/2021 14:06:12	
CCB2	S	Total CN	P	0.5959	µg/l	8/3/2021 14:06:13	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : *pl*

Instrument ID : Konelab

8/3/2021 12:16

Test Total CN


Accepted 8/3/2021 12:15

Factor 1391

Bias 0

Coeff. of det. 0.999847

Errors

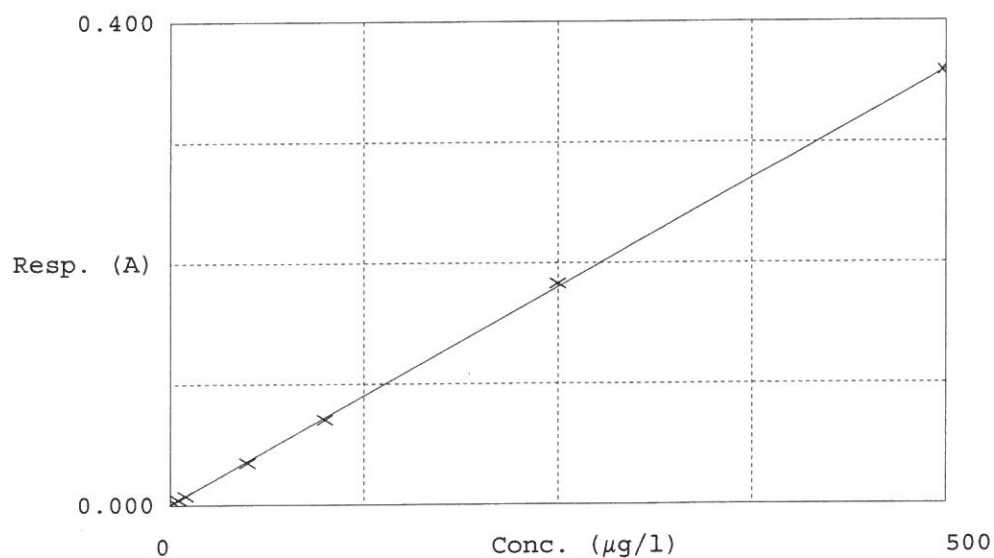

	Calibrator	Response	Calc. con.	Conc.	Relative Errors
1	0.0PPBCN	0.001	0.6223	0.0000	20.8
2	5.0PPBCN	0.005	6.0376	5.0000	0.5
3	10PPBCN	0.008	10.0525	10.0000	-4.8
4	50PPBCN	0.035	47.8393	50.0000	-2.3
5	100PPBCN	0.071	97.6690	100.0000	1.2
6	250PPBCN	0.183	254.2168	250.0000	-0.3
7	500PPBCN	0.359	498.5625	500.0000	

pl
8/3/21