


Clear table

Instrument ID: IC-2									
Method: 300.0 / 9856A									
Analyst : AP									
ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time
									Initial wt/ Final Vol
Analyst									
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-07-09_	7/9/21 9:42
STD2	0.4290	0.6630	0.6670	2.2450	0.5810	0.8760	3.5010	2021-07-09_	7/9/21 10:10
STD3	0.7920	1.2070	1.2030	4.0520	1.0180	2.0320	6.0650	2021-07-09_	7/9/21 10:39
STD4	1.0300	1.4850	1.4820	4.9290	1.2380	2.5490	7.3860	2021-07-09_	7/9/21 11:07
STD5	1.9480	2.9110	2.9160	9.6610	2.3920	5.0590	14.3460	2021-07-09_	7/9/21 11:36
STD6	3.9460	6.0160	6.0140	19.9940	4.9470	10.0720	29.9440	2021-07-09_	7/9/21 12:05
STD7	5.0550	7.5180	7.5190	25.1190	6.3240	12.4110	37.7580	2021-07-09_	7/9/21 12:33
ICV	1.9440	2.9090	2.9370	9.6930	2.3900	4.9880	14.3530	2021-07-09_	7/9/21 13:05
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-07-09_	7/9/21 13:34
CCV	1.9600	2.9660	2.9630	9.8010	2.4160	3.5520	14.4320	2021-08-04_	8/4/21 11:19
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-08-04_	8/4/21 11:49
LB115702BLW	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-08-04_	8/4/21 13:14
LB115702BSW	2.2290	3.1400	3.1420	10.4330	2.5740	5.5500	15.4890	2021-08-04_	8/4/21 13:43
M3281-03	0.0000	744.7530	0.0000	2.0140	0.1730	-0.1460	33.5980	2021-08-04_	8/4/21 14:23
M3281-05	0.5920	1345.3230	0.0000	9.3000	0.1710	0.0000	77.9280	2021-08-04_	8/4/21 14:53
M3281-05MS	3.1400	1289.4410	3.1510	19.5430	2.5290	-0.1490	92.8100	2021-08-04_	8/4/21 15:23
M3281-05MSD	3.0040	1298.8120	2.9560	19.3240	2.4560	-0.4020	92.3010	2021-08-04_	8/4/21 15:52
CCV	2.1430	3.6880	3.1120	10.7740	2.5530	8.2210	15.5660	2021-08-04_	8/4/21 17:00
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-08-04_	8/4/21 17:59

CALIBRATION OF COMPONENT F-

Method: AnionsIC2-070921.mtw
 Equation: $Q = 0.0750899 \cdot A + 2.06898$
 RSD: 2.325 %
 Correlation coefficient: 0.999705

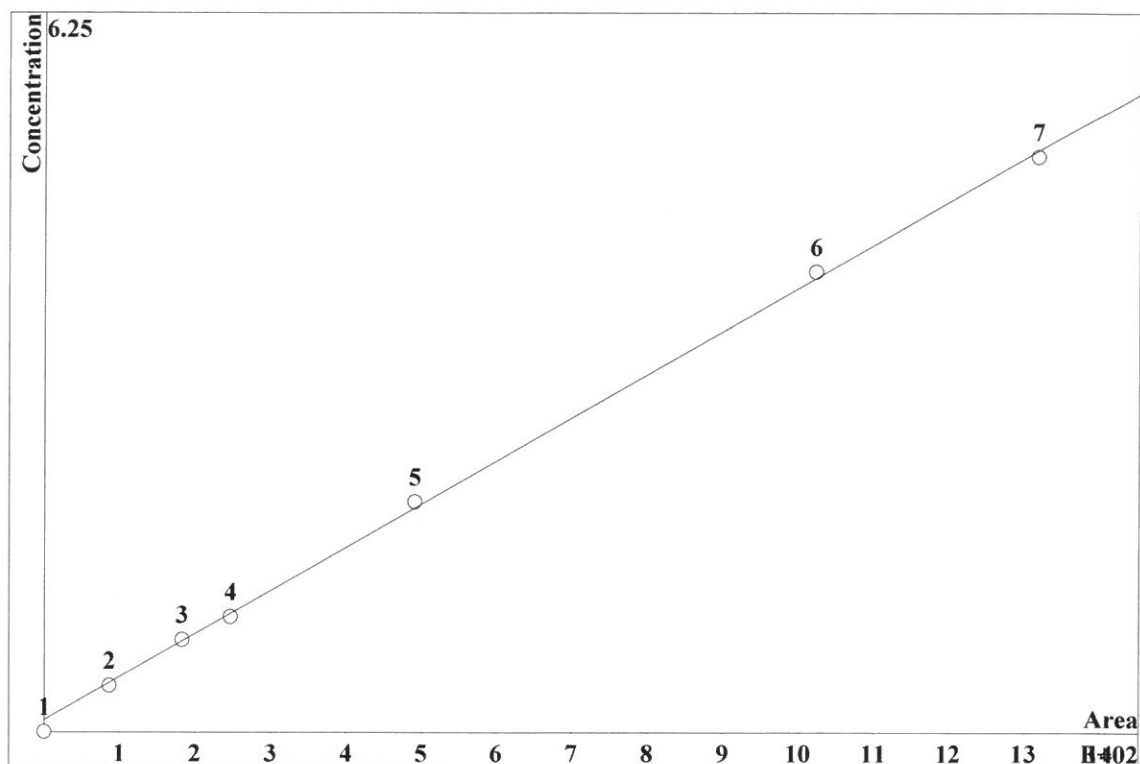

K3 = 0 K2 = 0 K1 = 0.0750899 K0 = 2.06898

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	2.336	86.64	0.4	20	5.75		
3	5.02	183.5	0.8	20	5.75		
4	6.724	246.8	1	20	5.75		
5	14.65	491.4	2	20	5.75		
6	31.01	1023	4	20	5.75		
7	38.73	1319	5	20	5.75		

CALIBRATION OF COMPONENT CL-

Method: AnionsIC2-070921.mtw
 Equation: $Q = 0.114962 \cdot A + 2.44005$
 RSD: 1.709 %
 Correlation coefficient: 0.999841

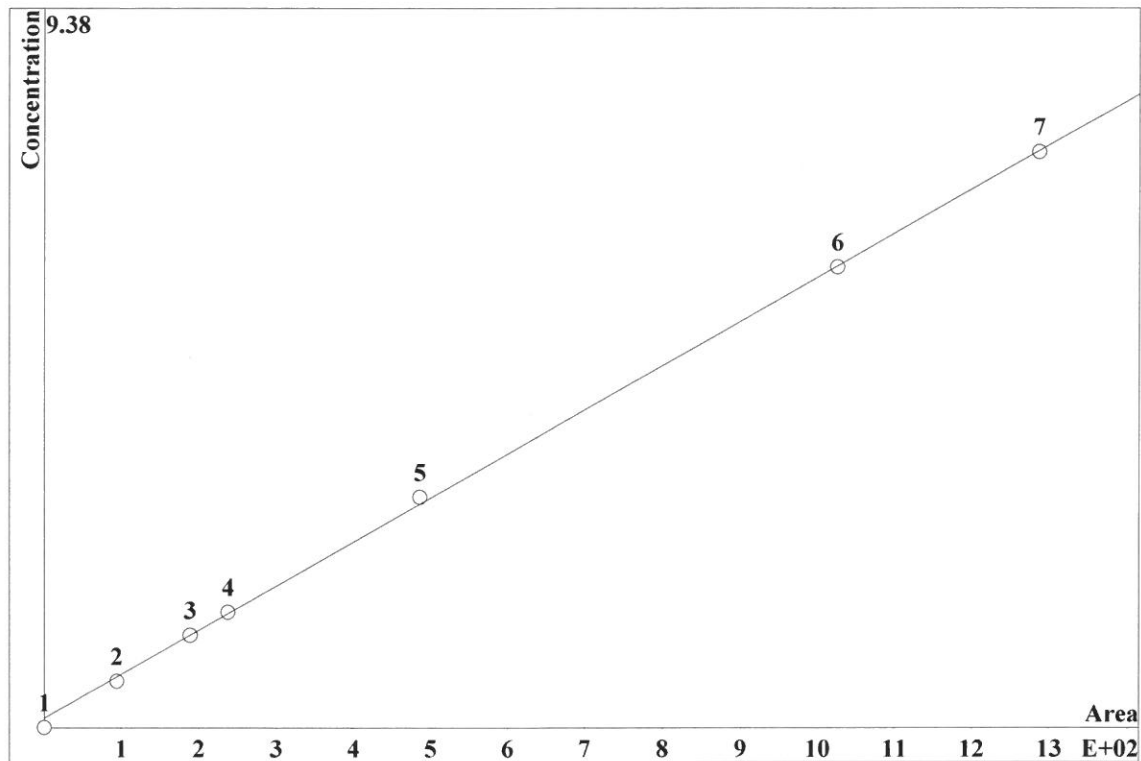

K3 = 0 K2 = 0 K1 = 0.114962 K0 = 2.44005

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	6.27	94.1	0.6	20	8.834		
3	12.68	188.7	1.2	20	8.834		
4	15.95	237.1	1.5	20	8.834		
5	33.19	485.2	3	20	8.834		
6	71.27	1025	6	20	8.834		
7	88.63	1287	7.5	20	8.834		

CALIBRATION OF COMPONENT NO2

Method: AnionsIC2-070921.mtw
 Equation: $Q = 0.051109 \cdot A + 2.59501$
 RSD: 1.685 %
 Correlation coefficient: 0.999845

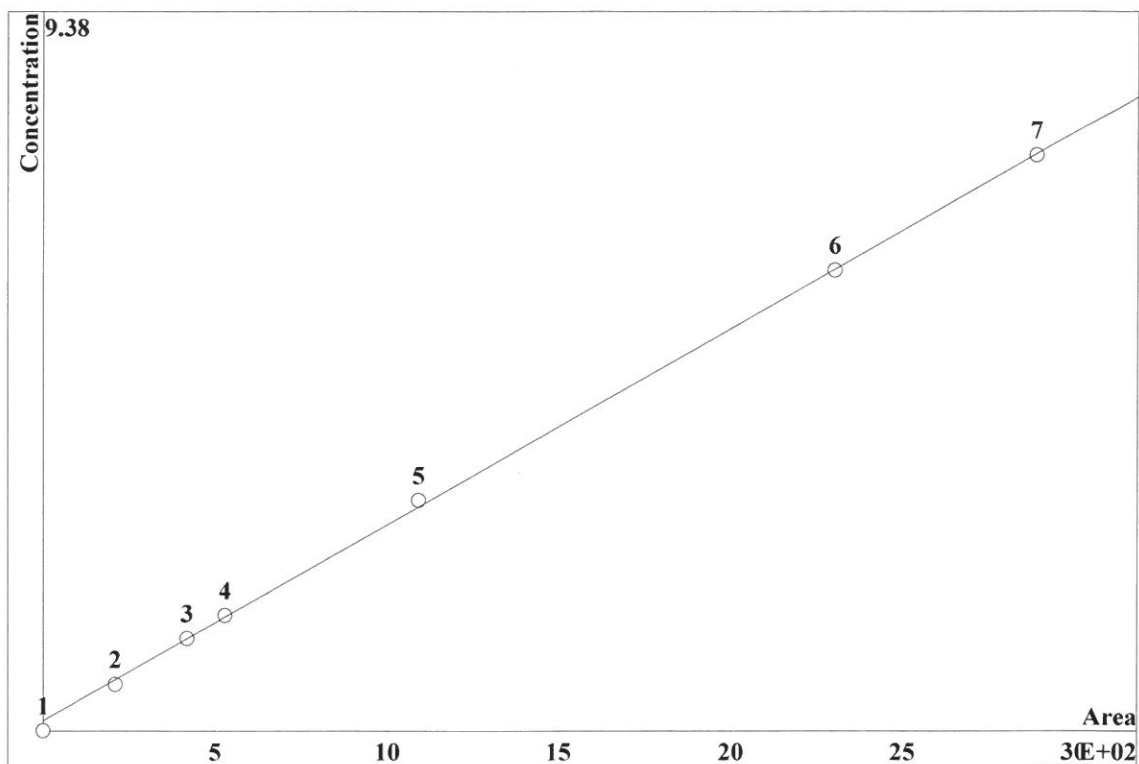

K3 = 0 K2 = 0 K1 = 0.051109 K0 = 2.59501

Base: Area

Ref.channel: ch1

ISTD:

Formula: Linear


Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	11.22	210.2	0.6	20	10.64		
3	22.26	419.9	1.2	20	10.64		
4	28.16	529.1	1.5	20	10.64		
5	57.52	1090	3	20	10.64		
6	115.2	2303	6	20	10.64		
7	142.6	2891	7.5	20	10.64		

±□:□

CALIBRATION OF COMPONENT BR-

Method: AnionsIC2-070921.mtw
 Equation: $Q = 0.254436 \cdot A + 9.45477$
 RSD: 2.017 %
 Correlation coefficient: 0.999778

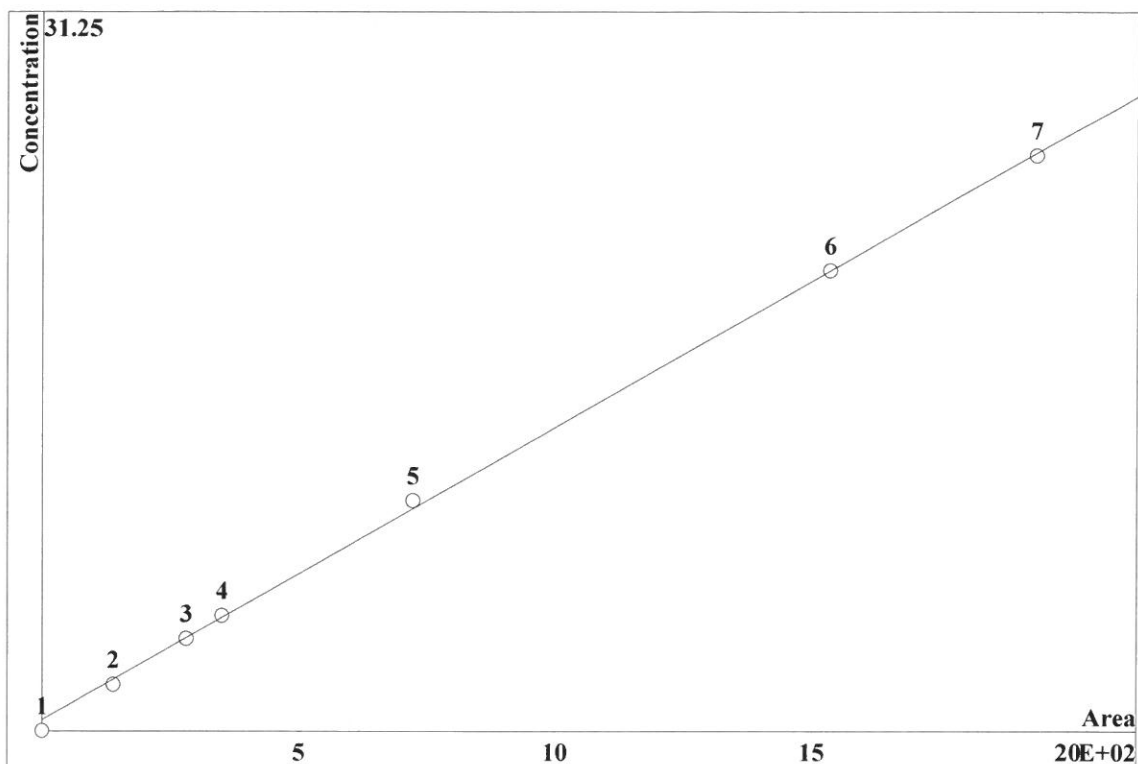

K3 = 0 K2 = 0 K1 = 0.254436 K0 = 9.45477

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	6.921	139.3	2	20			14
3	14.18	281.4	4	20			14
4	17.89	350.3	5	20			14
5	37.58	722.2	10	20			14
6	81.68	1534	20	20			14
7	102.3	1937	25	20			14

CALIBRATION OF COMPONENT NO3

Method: AnionsIC2-070921.mtw
 Equation: $Q = 0.0438083 \cdot A + 2.94619$
 RSD: 2.995 %
 Correlation coefficient: 0.999511

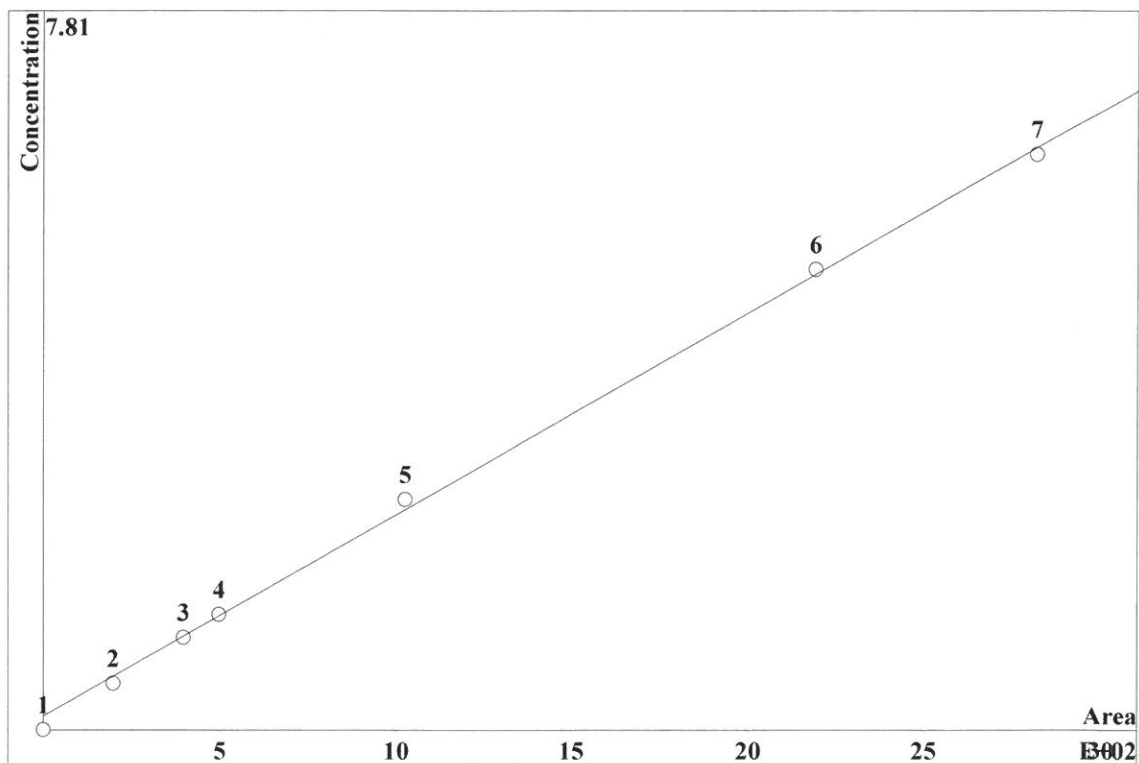

K3 = 0 K2 = 0 K1 = 0.0438083 K0 = 2.94619

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	8.418	198.1	0.5	20	16.28		
3	17.08	397.4	1	20	16.28		
4	21.57	497.9	1.25	20	16.28		
5	44.85	1025	2.5	20	16.28		
6	97.19	2191	5	20	16.28		
7	122.3	2820	6.25	20	16.28		

CALIBRATION OF COMPONENT HPO4

Method: AnionsIC2-070921.mtw
 Equation: $Q = 0.0885729 \cdot A - 11.3055$
 RSD: 1.708 %
 Correlation coefficient: 0.999841



K3 = 0 K2 = 0 K1 = 0.0885729 K0 = -11.3055

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	8.78	325.5	1	20	21.2		
3	16.61	586.6	2	20	21.2		
4	20.09	703.3	2.5	20	21.2		
5	37.65	1270	5	20	21.2		
6	74.91	2402	10	20	21.2		
7	91.49	2930	12.5	20	21.2		

CALIBRATION OF COMPONENT SO4

Method: AnionsIC2-070921.mtw
 Equation: $Q = 0.143844 \cdot A + 17.5564$
 RSD: 2.650 %
 Correlation coefficient: 0.999617

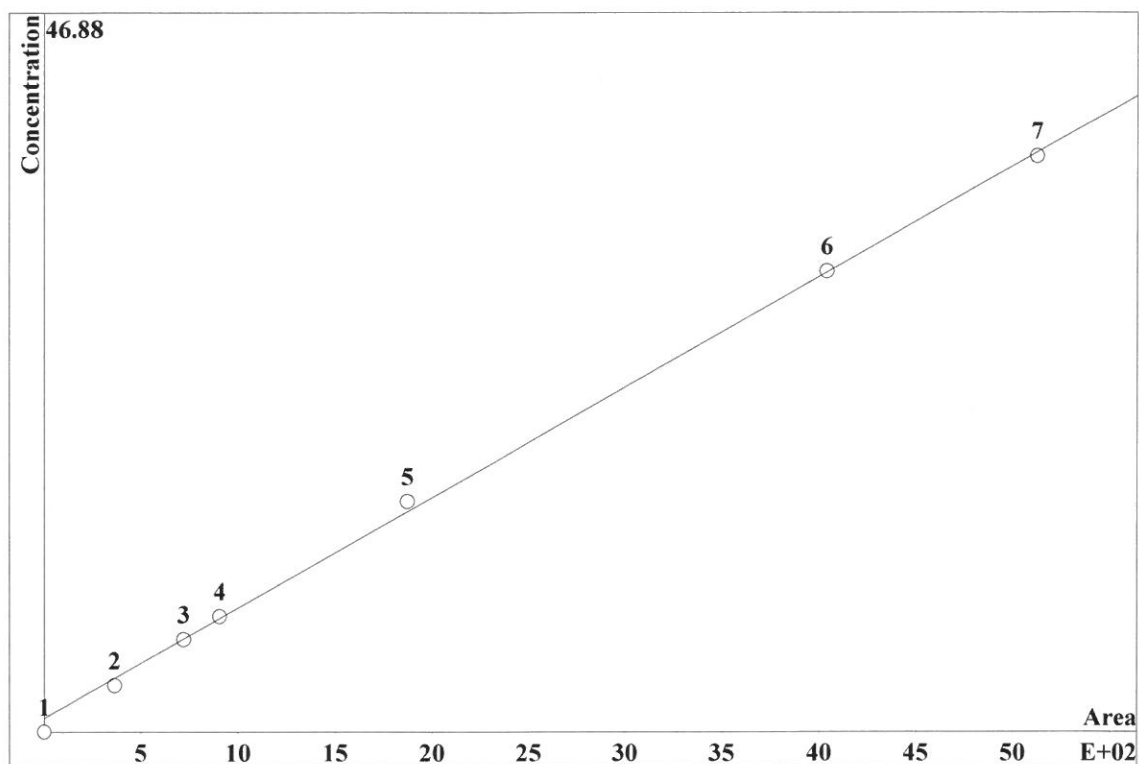

K3 = 0 K2 = 0 K1 = 0.143844 K0 = 17.5564

Base: Area

Ref.channel: ch1

ISTD:

Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	12.45	364.7	3	20	24.73		
3	24.99	721.2	6	20	24.73		
4	31.58	904.9	7.5	20	24.73		
5	66.09	1873	15	20	24.73		
6	145.1	4041	30	20	24.73		
7	182.6	5128	37.5	20	24.73		

æ#□

Clear table

Instrument ID: IC-2 Analyst: AP Method: 300 / 9056A

ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time	Initial wt/ Final Vol	Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-07-09_	7/9/21 9:42		AP/MA
STD2	0.4290	0.6630	0.6670	2.2450	0.5810	0.8760	3.5010	2021-07-09_	7/9/21 10:10		AP/MA
STD3	0.7920	1.2070	1.2030	4.0520	1.0180	2.0320	6.0650	2021-07-09_	7/9/21 10:39		AP/MA
STD4	1.0300	1.4850	1.4820	4.9290	1.2380	2.5490	7.3860	2021-07-09_	7/9/21 11:07		AP/MA
STD5	1.9480	2.9110	2.9160	9.6610	2.3920	5.0590	14.3460	2021-07-09_	7/9/21 11:36		AP/MA
STD6	3.9460	6.0160	6.0140	19.9940	4.9470	10.0720	29.9440	2021-07-09_	7/9/21 12:05		AP/MA
STD7	5.0550	7.5180	7.5190	25.1190	6.3240	12.4110	37.7580	2021-07-09_	7/9/21 12:33		AP/MA

ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.5000

ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4
STD1							
STD2	7.2500	10.5000	11.1667	12.2500	16.2000	-12.4000	16.7000
STD3	-1.0000	0.5833	0.2500	1.3000	1.8000	1.6000	1.0833
STD4	3.0000	-1.0000	-1.2000	-1.4200	-0.9600	1.9600	-1.5200
STD5	-2.6000	-2.9667	-2.8000	-3.3900	-4.3200	1.1800	-4.3600
STD6	-1.3500	0.2667	0.2333	-0.0300	-1.0600	0.7200	-0.1867
STD7	1.1000	0.2400	0.2533	0.4760	1.1840	-0.7120	0.6880

Report date: 7/12/2021 3:22:09 PM
Printed by: wet


Ident: STD1
Analysis from: 7/9/2021 9:42:11 AM
File: _2021-07-09_

Last save: 7/12/2021 3:21:23 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27529

Last save: 7/9/2021 12:31:

SAMPLE:
: AM/AP
Vial number: 2
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

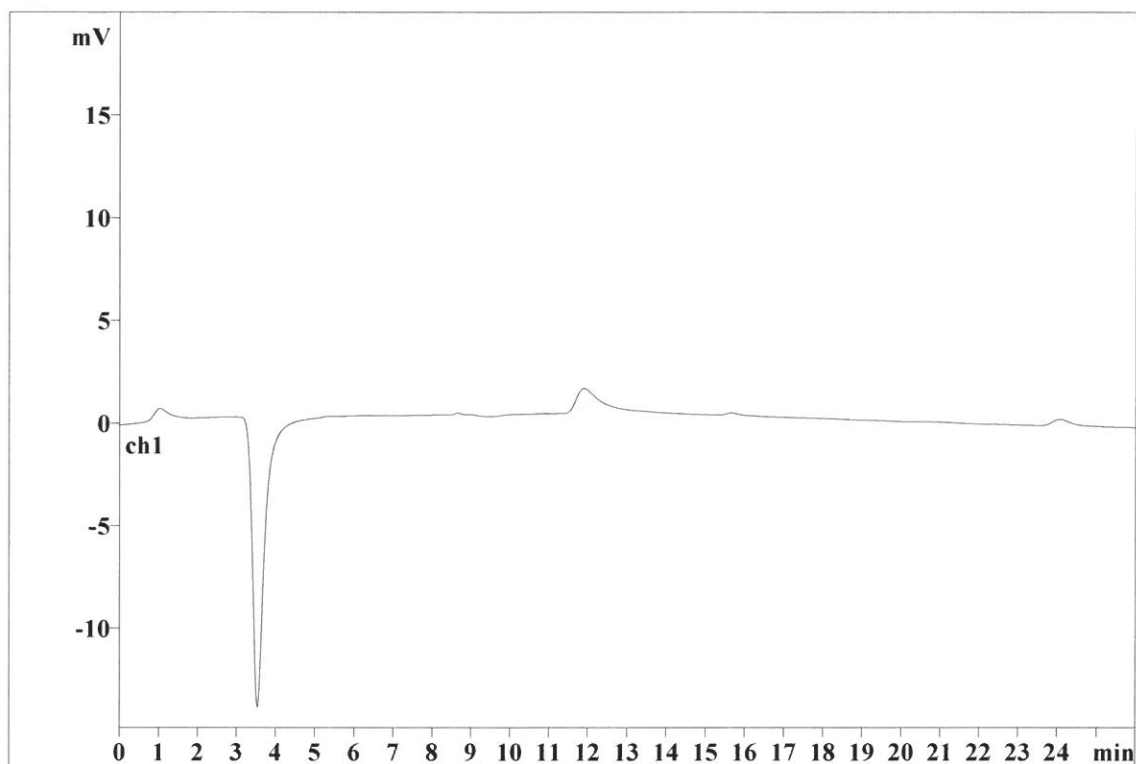

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 7/12/2021 3:22:24 PM
Printed by: wet


Ident: STD2
Analysis from: 7/9/2021 10:10:47 AM
File: _2021-07-09_

Last save: 7/12/2021 3:21:23 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27530

Last save: 7/9/2021 12:31:

SAMPLE:
: AM/AP
Vial number: 3
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

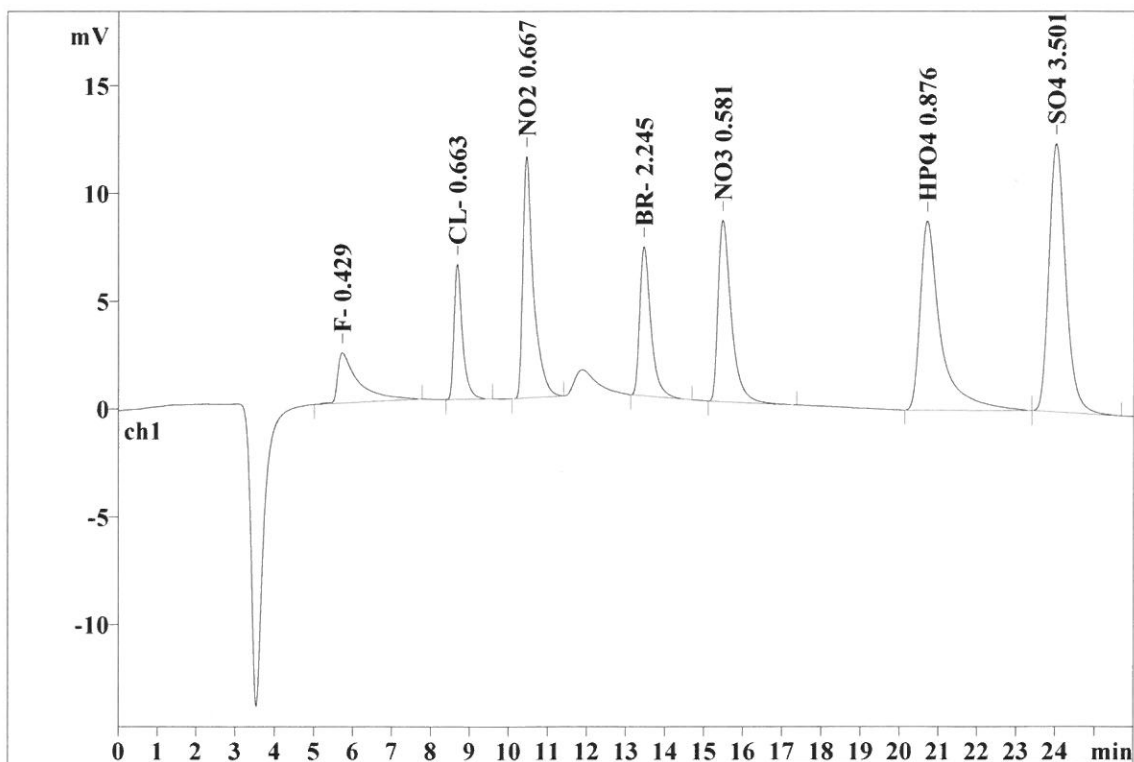

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.72	0.459	2.33	4.14	86.639	6.11
2	8.66	0.212	6.27	11.12	94.105	6.63
3	10.45	0.257	11.21	19.89	210.169	14.82
4	13.45	0.294	6.92	12.27	139.302	9.82
5	15.48	0.342	8.42	14.93	198.098	13.96
6	20.71	0.480	8.78	15.57	325.546	22.95
7	24.02	0.438	12.45	22.08	364.708	25.71
7	26.00	0.355	56.39	99.99	1418.567	100.00

This report has been created by IC Net
METROHM LTD

Report date: 7/12/2021 3:22:35 PM
Printed by: wet


Ident: STD3
Analysis from: 7/9/2021 10:39:23 AM
File: _2021-07-09_

Last save: 7/12/2021 3:21:23 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27531

Last save: 7/9/2021 12:31:

SAMPLE:
: AM/AP
Vial number: 4
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.72	0.442	5.02	4.45	183.476	6.60
2	8.66	0.211	12.68	11.24	188.743	6.79
3	10.43	0.260	22.26	19.73	419.875	15.11
4	13.40	0.288	14.18	12.57	281.364	10.13
5	15.40	0.338	17.08	15.14	397.403	14.30
6	20.70	0.461	16.61	14.72	586.574	21.11
7	24.02	0.431	24.99	22.15	721.152	25.95
7	26.00	0.347	112.82	99.99	2778.588	100.00

This report has been created by IC Net
METROHM LTD

Report date: 7/12/2021 3:22:45 PM
Printed by: wet


Ident: STD4
Analysis from: 7/9/2021 11:07:59 AM
File: _2021-07-09_

Last save: 7/12/2021 3:21:23 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27532

Last save: 7/9/2021 12:31:

SAMPLE:
: AM/AP
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

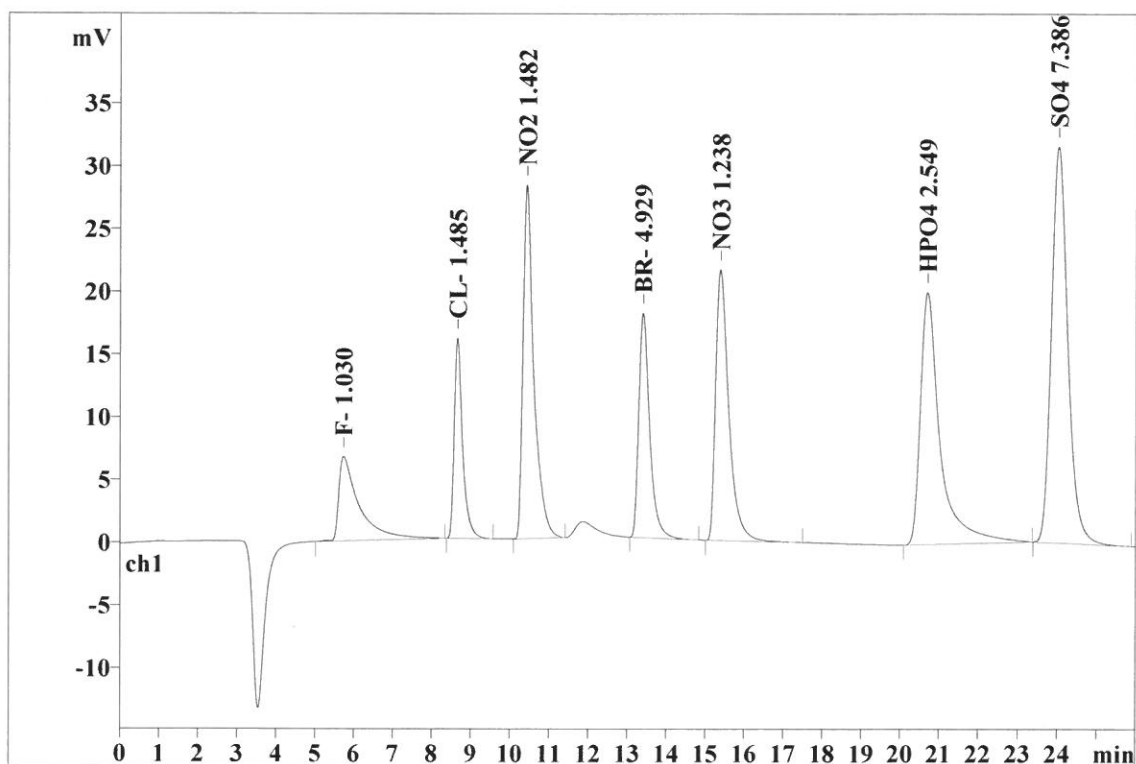

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.73	0.463	6.72	4.74	246.804	7.11
2	8.64	0.212	15.95	11.23	237.133	6.84
3	10.41	0.259	28.16	19.84	529.064	15.25
4	13.39	0.287	17.89	12.60	350.308	10.10
5	15.38	0.336	21.57	15.19	497.876	14.35
6	20.69	0.457	20.09	14.15	703.257	20.27
7	24.02	0.429	31.58	22.24	904.879	26.08
7	26.00	0.349	141.96	100.00	3469.319	100.00

This report has been created by IC Net
METROHM LTD

Report date: 7/12/2021 3:22:51 PM
Printed by: wet


Ident: STD5
Analysis from: 7/9/2021 11:36:37 AM
File: _2021-07-09_

Last save: 7/12/2021 3:21:23 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27533

Last save: 7/9/2021 12:31:

SAMPLE:
: AM/AP
Vial number: 6
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

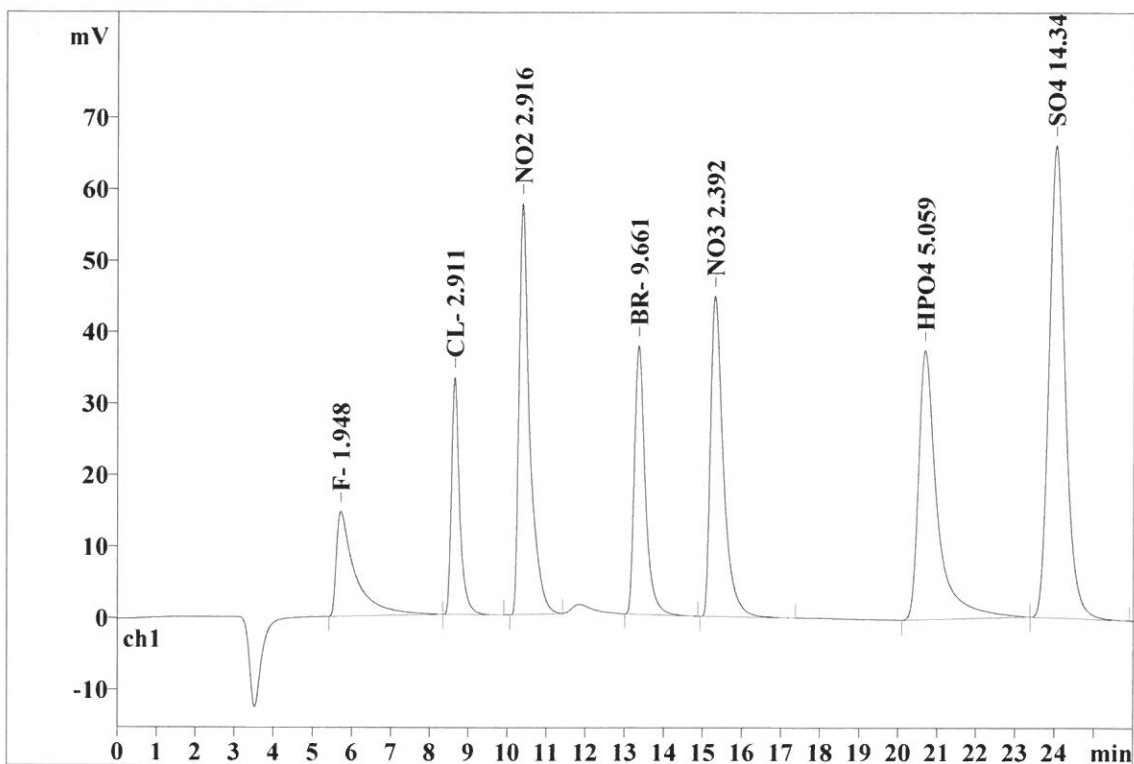

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.71	0.419	14.65	5.02	491.359	7.06
2	8.62	0.207	33.19	11.38	485.218	6.98
3	10.38	0.260	57.52	19.73	1090.401	15.67
4	13.34	0.280	37.57	12.89	722.244	10.38
5	15.30	0.332	44.85	15.38	1024.583	14.73
6	20.68	0.444	37.65	12.91	1270.020	18.26
7	24.02	0.423	66.09	22.67	1872.658	26.92
7	26.00	0.338	291.51	100.00	6956.483	100.00

This report has been created by IC Net
METROHM LTD

Report date: 7/12/2021 3:22:58 PM
Printed by: wet


Ident: STD6
Analysis from: 7/9/2021 12:05:13 PM
File: _2021-07-09_

Last save: 7/12/2021 3:21:23 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27534

Last save: 7/9/2021 12:31:

SAMPLE:
: AM/AP
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

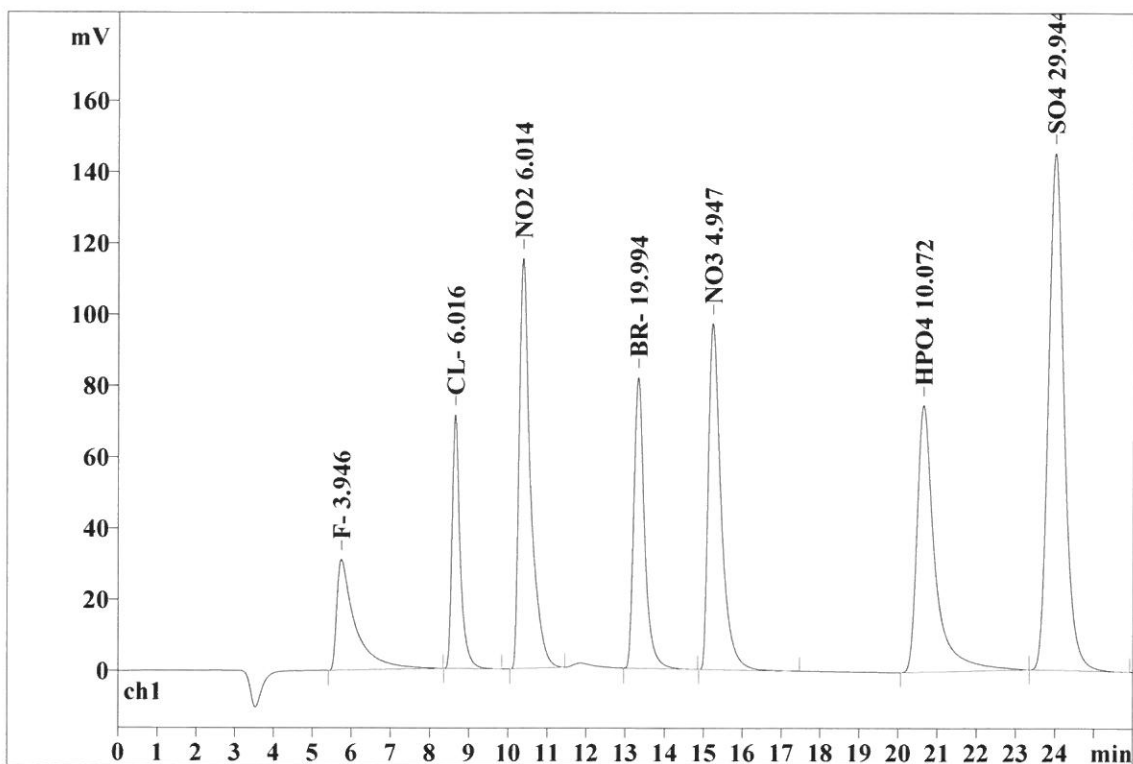

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.74	0.420	31.01	5.03	1023.332	7.05
2	8.63	0.203	71.27	11.56	1025.455	7.06
3	10.36	0.278	115.20	18.69	2302.532	15.86
4	13.31	0.273	81.68	13.25	1534.445	10.57
5	15.22	0.326	97.19	15.77	2191.307	15.09
6	20.63	0.428	74.91	12.15	2401.858	16.54
7	23.98	0.416	145.08	23.54	4041.385	27.83
7	26.00	0.335	616.34	100.00	14520.314	100.00

This report has been created by IC Net
METROHM LTD

Report date: 7/12/2021 3:23:05 PM
Printed by: wet


Ident: STD7
Analysis from: 7/9/2021 12:33:49 PM
File: _2021-07-09_

Last save: 7/12/2021 3:21:23 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27535

Last save: 7/9/2021 12:31:

SAMPLE:
: AM/AP
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.75	0.452	38.73	5.04	1318.856	7.20
2	8.62	0.204	88.63	11.53	1286.609	7.03
3	10.34	0.281	142.57	18.55	2891.454	15.79
4	13.32	0.275	102.34	13.31	1937.333	10.58
5	15.24	0.333	122.27	15.91	2820.037	15.40
6	20.71	0.429	91.49	11.90	2930.072	16.00
7	24.08	0.420	182.57	23.75	5127.796	28.00
7	26.00	0.342	768.59	100.00	18312.159	100.00

This report has been created by IC Net
METROHM LTD

Report date: 7/12/2021 3:23:12 PM
Printed by: wet


Ident: ICV
Analysis from: 7/9/2021 1:05:41 PM
File: _2021-07-09_

Last save: 7/9/2021 1:31:41 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27536

Last save: 7/9/2021 12:59:

SAMPLE:
: AM/AP
Vial number: 9
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

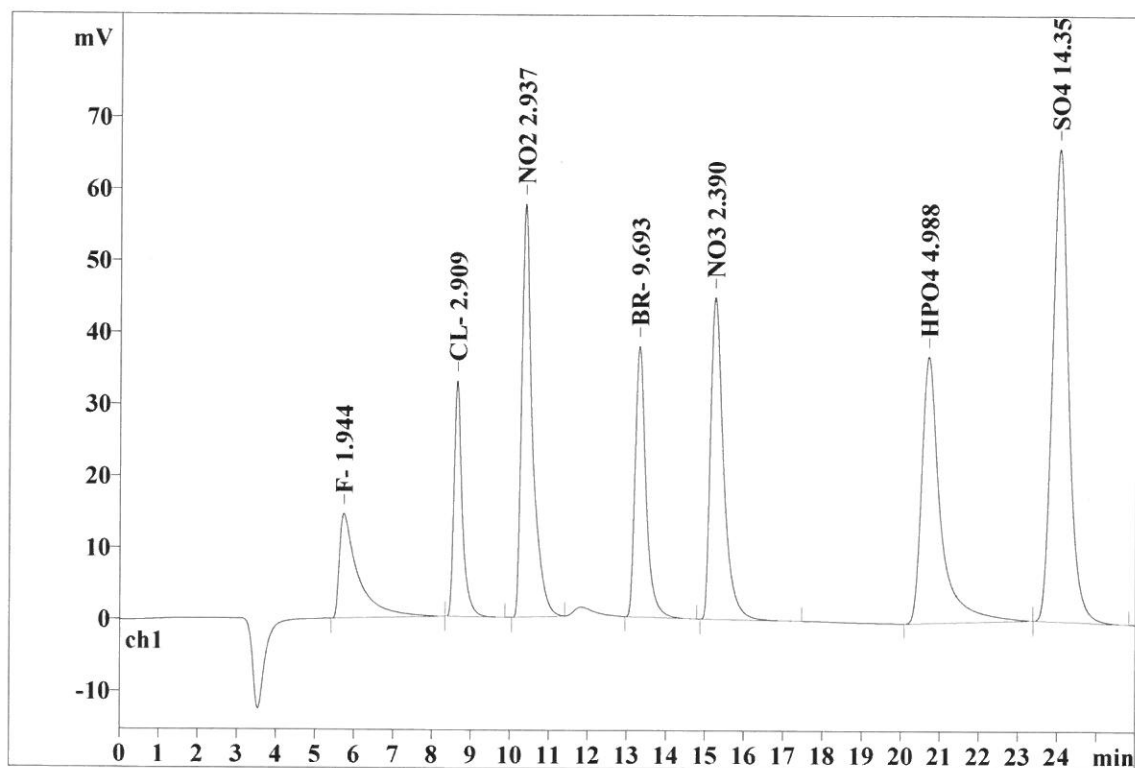

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.72	0.423	14.56	5.01	490.144	7.05
2	8.62	0.208	32.84	11.31	484.812	6.98
3	10.36	0.261	57.55	19.81	1098.352	15.80
4	13.29	0.280	37.73	12.99	724.773	10.43
5	15.23	0.331	44.83	15.43	1024.024	14.73
6	20.68	0.445	37.09	12.77	1254.043	18.04
7	24.02	0.425	65.85	22.67	1873.591	26.96
7	26.00	0.339	290.45	100.00	6949.740	100.00

This report has been created by IC Net
METROHM LTD

Report date: 7/12/2021 3:23:24 PM
Printed by: wet


Ident: ICB
Analysis from: 7/9/2021 1:34:44 PM
File: _2021-07-09_

Last save: 7/9/2021 2:00:44 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27537

Last save: 7/9/2021 12:59:

SAMPLE:
: AP/MA
Vial number: 10
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

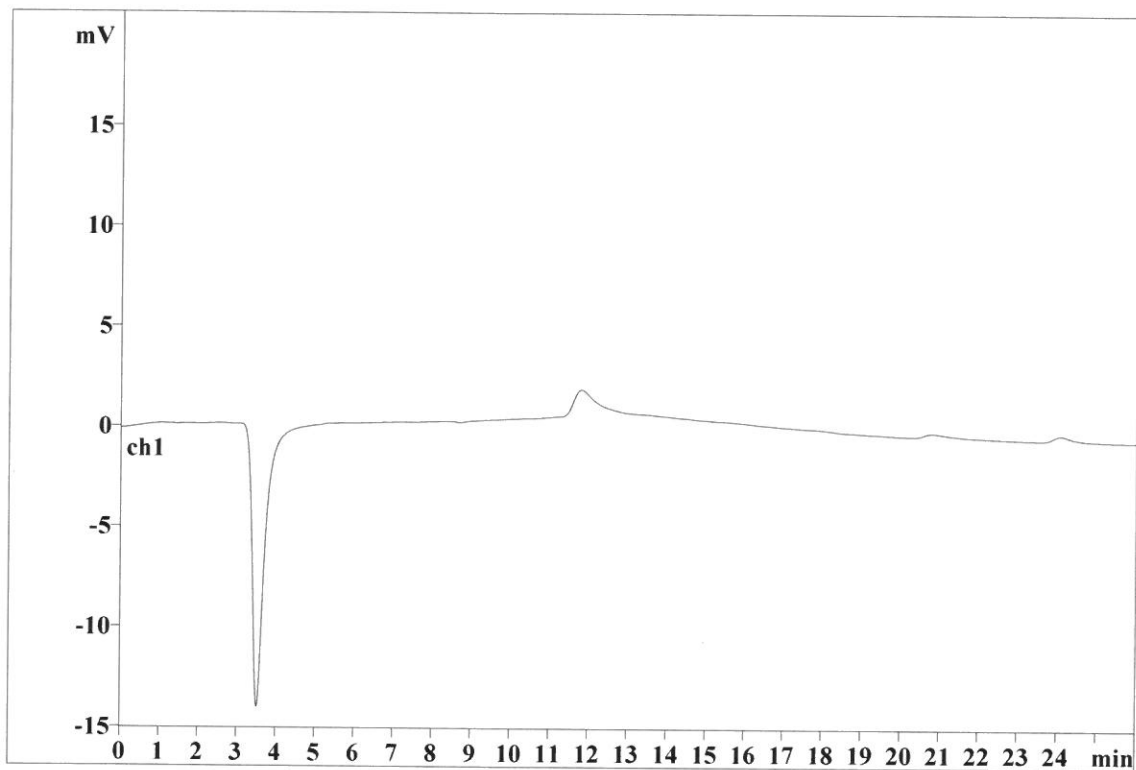

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 8/5/2021 10:52:13 AM
Printed by: wet


Ident: CCV
Analysis from: 8/4/2021 11:19:13 AM
File: _2021-08-04_

Last save: 8/4/2021 11:46:13 AM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27761

Last save: 8/4/2021 9:22:1

SAMPLE:
: AP/MA
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.72	0.501	12.91	5.23	494.373	7.40
2	8.70	0.229	31.13	12.62	494.759	7.41
3	10.52	0.283	55.37	22.44	1108.594	16.59
4	13.56	0.330	33.14	13.43	733.261	10.97
5	15.66	0.383	39.58	16.04	1035.817	15.50
6	20.90	0.554	23.47	9.51	929.793	13.92
7	24.55	0.570	51.14	20.73	1884.613	28.21
7	27.00	0.407	246.74	100.00	6681.209	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/5/2021 10:52:20 AM
Printed by: wet


Ident: CCB
Analysis from: 8/4/2021 11:49:14 AM
File: _2021-08-04_

Last save: 8/4/2021 12:16:14 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27762

Last save: 8/4/2021 9:22:1

SAMPLE:
: AP/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 8/5/2021 10:52:28 AM
Printed by: wet


Ident: LB115702BLW
Analysis from: 8/4/2021 1:14:18 PM
File: _2021-08-04_

Last save: 8/5/2021 10:51:59 AM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27768

Last save: 8/4/2021 9:22:1

SAMPLE:
: AP/MA
Vial number: 13
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 8/5/2021 10:52:35 AM
Printed by: wet


Ident: LB115702BSW
Analysis from: 8/4/2021 1:43:56 PM
File: _2021-08-04_

Last save: 8/5/2021 10:52:00 AM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27769

Last save: 8/4/2021 9:22:1

SAMPLE:
: AP/MA
Vial number: 14
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.71	0.427	16.54	4.84	566.055	7.47
2	8.69	0.186	40.01	11.70	525.017	6.93
3	10.49	0.237	68.05	19.91	1178.677	15.56
4	13.53	0.255	44.77	13.10	782.935	10.34
5	15.58	0.303	52.63	15.39	1107.742	14.63
6	20.95	0.410	43.46	12.71	1380.935	18.24
7	24.62	0.400	76.40	22.35	2031.548	26.83
7	27.00	0.317	341.86	100.00	7572.909	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/5/2021 10:52:49 AM
Printed by: wet


Ident: M3281-03
Analysis from: 8/4/2021 2:23:56 PM
File: _2021-08-04_

Last save: 8/4/2021 3:03:59 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27770

Last save: 8/4/2021 9:22:1

SAMPLE:
: AP/MA
Vial number: 15
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.63	1.297	1710.40	90.20	129543.728	96.37
3	0.00	0.000	0.00	0.00	0.000	0.00
4	13.81	0.233	7.87	0.42	121.132	0.09
5	15.93	0.297	0.62	0.03	11.940	0.01
6	21.09	0.519	2.32	0.12	94.639	0.07
7	24.64	0.398	170.83	9.01	4549.443	3.38
7	27.00	0.392	1892.04	99.78	134320.881	99.92

This report has been created by IC Net
METROHM LTD

Report date: 8/5/2021 10:53:18 AM
Printed by: wet


Ident: M3281-05
Analysis from: 8/4/2021 2:53:34 PM
File: _2021-08-04_

Last save: 8/5/2021 10:53:07 AM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27771

Last save: 8/4/2021 9:22:1

SAMPLE:
: AP/MA
Vial number: 16
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.84	1.302	1.80	0.08	130.077	0.05
2	10.04	2.251	1714.80	79.55	234024.955	95.28
3	0.00	0.000	0.00	0.00	0.000	0.00
4	14.20	0.221	47.35	2.20	693.847	0.28
5	16.25	0.274	0.61	0.03	10.975	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	24.63	0.413	389.30	18.06	10712.970	4.36
7	27.00	0.637	2153.86	99.92	245572.823	99.98

This report has been created by IC Net
METROHM LTD

Report date: 8/5/2021 10:57:00 AM
Printed by: wet


Ident: M3281-05MS
Analysis from: 8/4/2021 3:23:13 PM
File: _2021-08-04_

Last save: 8/5/2021 10:56:25 AM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27772

Last save: 8/4/2021 9:22:1

SAMPLE:
: AP/MA
Vial number: 17
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.86	1.344	9.58	0.40	808.785	0.33
2	10.11	2.157	1715.38	71.26	224303.147	92.78
3	12.64	0.327	49.80	2.07	1182.105	0.49
4	14.09	0.216	104.86	4.36	1499.031	0.62
5	15.95	0.265	60.93	2.53	1087.180	0.45
6	21.12	0.596	1.96	0.08	93.905	0.04
7	24.54	0.414	464.54	19.30	12782.235	5.29
7	27.00	0.760	2407.05	100.00	241756.388	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/5/2021 10:57:08 AM
Printed by: wet


Ident: M3281-05MSD
Analysis from: 8/4/2021 3:52:51 PM
File: _2021-08-04_

Last save: 8/5/2021 10:56:44 AM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27773

Last save: 8/4/2021 9:22:1

SAMPLE:
: AP/MA
Vial number: 18
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.87	1.347	9.19	0.38	772.489	0.32
2	10.11	2.178	1714.69	71.61	225933.452	92.94
3	12.63	0.364	46.50	1.94	1105.805	0.45
4	14.09	0.217	103.24	4.31	1481.795	0.61
5	15.96	0.266	58.94	2.46	1053.888	0.43
6	21.13	0.723	0.69	0.03	36.867	0.02
7	24.52	0.415	461.24	19.26	12711.469	5.23
7	27.00	0.787	2394.48	100.00	243095.764	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/5/2021 10:57:21 AM
Printed by: wet


Ident: CCV
Analysis from: 8/4/2021 5:00:01 PM
File: _2021-08-04_

Last save: 8/4/2021 5:27:01 PM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27776

Last save: 8/4/2021 9:22:1

SAMPLE:
: AP/MA
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.72	0.461	15.00	4.13	543.254	6.57
2	8.71	0.179	49.10	13.51	620.336	7.51
3	10.53	0.235	68.25	18.78	1166.939	14.12
4	13.59	0.256	45.48	12.52	809.741	9.80
5	15.65	0.301	53.07	14.61	1098.405	13.29
6	21.01	0.438	55.34	15.23	1984.024	24.01
7	24.67	0.399	77.12	21.22	2042.299	24.71
7	27.00	0.324	363.37	100.00	8264.998	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/5/2021 10:57:47 AM
Printed by: wet


Ident: CCB
Analysis from: 8/4/2021 5:59:21 PM
File: _2021-08-04_

Last save: 8/5/2021 10:57:37 AM

Method: AnionsIC2-070921.mtw
Run operator: wet
Analysis number: 27778

Last save: 8/4/2021 9:22:1

SAMPLE:
: AP/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD