


LB115708

7471B

INSTRUMENT ID : CYZ

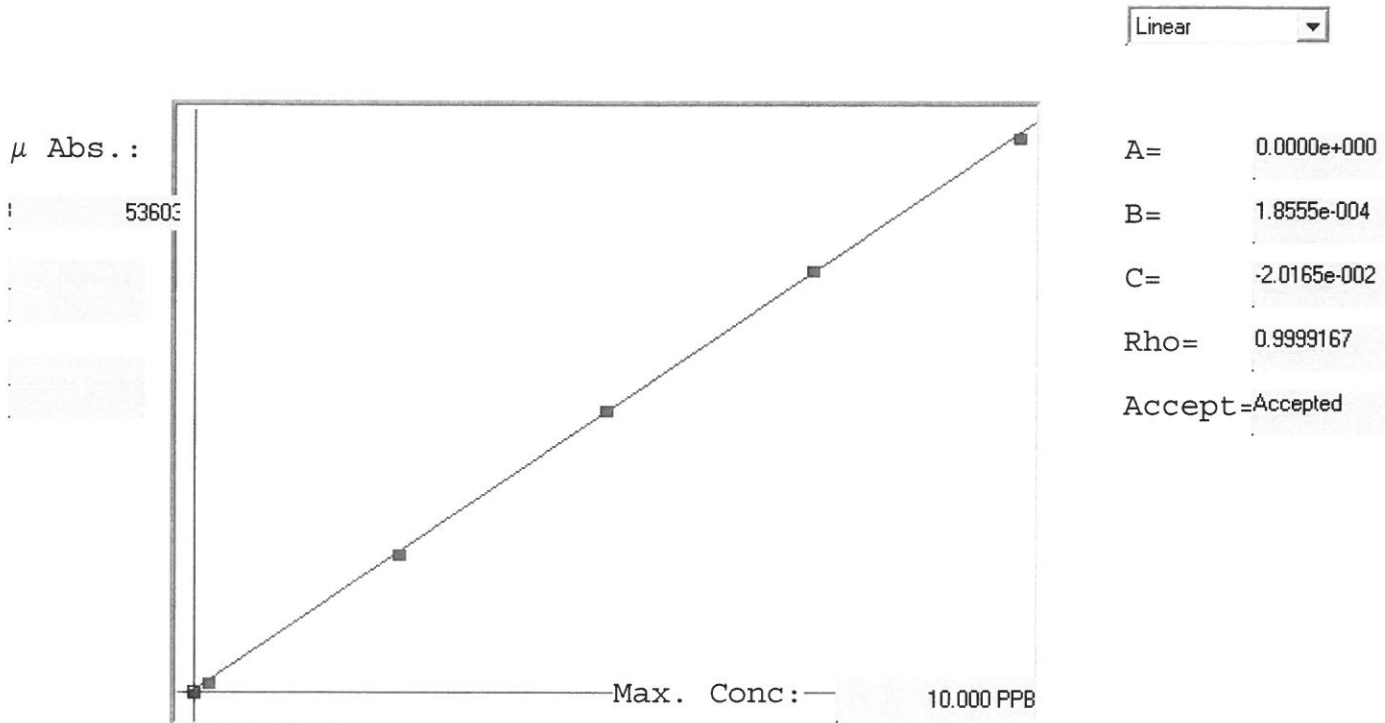

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	-0.015	-0.015	30	0.000	30					-8
0.2	0.200	0.185	-0.015	1108	0.0 %	1108					-1
2.5	2.500	2.482	-0.018	13485	0.0 %	13485					1
5.0	5.000	5.054	0.054	27345	0.0 %	27345					1
7.5	7.500	7.567	0.067	40890	0.0 %	40890					1
10.0	10.000	9.926	-0.074	53603	0.0 %	53603					-1

LB115708 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 05 Aug 2021 12:57:27

Sample ID	Extended ID	μ Abs.	Conc.	Std CondMethod	Units	Date	Type	Type
0.0 - 1	50	30	-	0.00007471B	PPB	05 Aug 2021 12:58:46	S	Std
0.2 - 1	50.2	1108	-	0.20007471B	PPB	05 Aug 2021 13:01:03	S	Std
2.5 - 1	52.5	13485	-	2.50007471B	PPB	05 Aug 2021 13:03:21	S	Std
5.0 - 1	55	27345	-	5.00007471B	PPB	05 Aug 2021 13:05:38	S	Std
7.5 - 1	57.5	40890	-	7.50007471B	PPB	05 Aug 2021 13:07:54	S	Std
10.0 - 1	510	53603	-	10.00007471B	PPB	05 Aug 2021 13:10:10	S	Std
ICV39 - 1	ICV39	21093	3.8937	-7471B	PPB	05 Aug 2021 13:12:59	U	SMPL
ICB39 - 1	ICB39	-92	-0.0372	-7471B	PPB	05 Aug 2021 13:15:14	U	SMPL
CCV94 - 1	CCV94	27289	5.0434	-7471B	PPB	05 Aug 2021 13:17:29	U	SMPL
CCB94 - 1	CCB94	-85	-0.0359	-7471B	PPB	05 Aug 2021 13:19:45	U	SMPL
CRA - 1	CRA	1075	0.1793	-7471B	PPB	05 Aug 2021 13:22:00	U	SMPL
HighStd - 1	HighStd	53424	9.8929	-7471B	PPB	05 Aug 2021 13:24:15	U	SMPL
ChkStd - 1	ChkStd	38242	7.0758	-7471B	PPB	05 Aug 2021 13:26:30	U	SMPL
PB138190BL - 1	PBS	-135	-0.0452	-7471B	PPB	05 Aug 2021 13:28:47	U	SMPL
PB138190BS - 1	LCSS	21658	3.9986	-7471B	PPB	05 Aug 2021 13:31:04	U	SMPL
M3268-12 - 1	20210574-COM-47	44817	8.2958	-7471B	PPB	05 Aug 2021 13:33:20	U	SMPL
M3268-13 - 1	20210575-COM-48	61537	11.3983	-7471B	PPB	05 Aug 2021 13:35:37	U	SMPL
M3268-14 - 1	20210576-COM-49	42557	7.8765	-7471B	PPB	05 Aug 2021 13:37:55	U	SMPL
M3271-01 - 1	TP-1	2812	0.5016	-7471B	PPB	05 Aug 2021 13:40:13	U	SMPL
M3271-04 - 1	TP-2	8973	1.6448	-7471B	PPB	05 Aug 2021 13:42:30	U	SMPL
CCV95 - 1	CCV95	26997	4.9893	-7471B	PPB	05 Aug 2021 13:44:46	U	SMPL
CCB95 - 1	CCB95	-83	-0.0356	-7471B	PPB	05 Aug 2021 13:47:01	U	SMPL
M3271-07 - 1	TP-3	9700	1.7797	-7471B	PPB	05 Aug 2021 13:49:17	U	SMPL
M3271-10 - 1	TP-4	2482	0.4404	-7471B	PPB	05 Aug 2021 13:51:32	U	SMPL
M3271-13 - 1	TP-5	1376	0.2352	-7471B	PPB	05 Aug 2021 13:53:47	U	SMPL
M3274-01 - 1	HD-01-080321	1039	0.1726	-7471B	PPB	05 Aug 2021 13:56:02	U	SMPL
M3274-01DUP - 1	HD-01-080321DUP	1054	0.1754	-7471B	PPB	05 Aug 2021 13:58:18	U	SMPL
M3274-01MS - 1	HD-01-080321MS	22999	4.2474	-7471B	PPB	05 Aug 2021 14:00:35	U	SMPL
M3274-01MSD - 1	HD-01-080321MSD	23906	4.4157	-7471B	PPB	05 Aug 2021 14:02:50	U	SMPL
M3276-01 - 1	PRE-MAEC-01	2094	0.3684	-7471B	PPB	05 Aug 2021 14:05:08	U	SMPL
M3276-03 - 1	PRE-MAEC-02	1165	0.1960	-7471B	PPB	05 Aug 2021 14:07:24	U	SMPL
CCV96 - 1	CCV96	27682	5.1164	-7471B	PPB	05 Aug 2021 14:09:40	U	SMPL
CCB96 - 1	CCB96	-77	-0.0345	-7471B	PPB	05 Aug 2021 14:11:55	U	SMPL
M3274-01LX5 - 1		225	0.0216	-7471B	PPB	05 Aug 2021 14:14:11	U	SMPL
M3274-01A - 1		23438	4.3289	-7471B	PPB	05 Aug 2021 14:16:26	U	SMPL
M3268-13DLX2 - 1		31076	5.7461	-7471B	PPB	05 Aug 2021 14:18:42	U	SMPL
CCV97 - 1	CCV97	27377	5.0598	-7471B	PPB	05 Aug 2021 14:20:59	U	SMPL
CCB97 - 1	CCB97	-74	-0.0339	-7471B	PPB	05 Aug 2021 14:23:14	U	SMPL