

Clear table

Instrument ID: IC-2											
Analyst : AP				Method:			300.0				
ident	concentra tion F-	concentratio n CL-	concentratio on NO2	concentratio on BR-	concentratio on NO3	concentratio on HPO4	concentratio on SO4	file name	date time	Initial wt/ Final Vol	Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-08-05	8/5/21 11:03		AP/MA
STD2	0.4150	0.6470	0.6420	2.1820	0.5520	0.7680	3.3920	2021-08-05	8/5/21 11:32		AP/MA
STD3	0.7740	1.2070	1.2010	4.0140	1.0070	2.0480	6.0450	2021-08-05	8/5/21 12:01		AP/MA
STD4	0.9690	1.4840	1.4840	4.9390	1.2300	2.5260	7.3750	2021-08-05	8/5/21 12:30		AP/MA
STD5	2.0470	2.9460	2.9530	9.8060	2.4420	5.2380	14.5520	2021-08-05	8/5/21 12:59		AP/MA
STD6	4.0260	5.9880	6.0110	19.9470	4.9880	10.1130	29.9090	2021-08-05	8/5/21 13:28		AP/MA
STD7	4.9680	7.5290	7.5090	25.1120	6.2800	12.3070	37.7270	2021-08-05	8/5/21 13:57		AP/MA
ICV	1.9650	2.9530	2.9220	9.8230	2.4440	5.0570	14.5200	2021-08-05	8/5/21 15:36		AP/MA
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-08-05	8/5/21 16:08		AP/MA
CCV	2.1250	3.1200	2.8970	9.7250	2.4300	5.4730	14.3260	2021-08-06	8/6/21 8:47		AP/MA
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-08-06	8/6/21 9:18		AP/MA
LB115709BLW	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-08-06	8/6/21 9:47		AP/MA
LB115709BSW	2.0510	3.0310	2.8640	9.5650	2.3890	5.3550	14.1160	2021-08-06	8/6/21 10:16		AP/MA
M3311-01	0.0000	0.2150	0.0000	0.0000	0.3980	0.0000	0.9390	2021-08-06	8/6/21 10:45		AP/MA
M3301-01	0.0000	691.4080	0.0000	4.8660	0.3460	0.0000	241.2230	2021-08-06	8/6/21 11:14		AP/MA
M3325-01	0.0000	63.0910	0.0000	0.0000	0.1560	0.0000	14.8620	2021-08-06	8/6/21 13:47		AP/MA
M3311-01MS	2.1750	2.9440	2.9660	9.7180	2.6920	5.8480	14.1040	2021-08-06	8/6/21 14:16		AP/MA
M3311-01MSD	2.0320	2.8510	2.8840	9.4170	2.6210	5.4370	13.6490	2021-08-06	8/6/21 14:45		AP/MA
CCV	2.0240	3.0190	2.8200	9.4400	2.3500	5.4230	13.6800	2021-08-06	8/6/21 15:14		AP/MA
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-08-06	8/6/21 15:44		AP/MA


8/5/21

Clear table

Instrument ID: IC-2											
Analyst : AP Method: 300 / 9056A											
ident	concentra tion F-	concentratio n CL-	concentratio on NO2	concentratio on BR-	concentratio on NO3	concentratio on HPO4	concentratio on SO4	file name	date time	Initial wt/ Final Vol	Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-08-05_	8/5/21 11:03		AP/MA
STD2	0.4150	0.6470	0.6420	2.1820	0.5520	0.7680	3.3920	2021-08-05_	8/5/21 11:32		AP/MA
STD3	0.7740	1.2070	1.2010	4.0140	1.0070	2.0480	6.0450	2021-08-05_	8/5/21 12:01		AP/MA
STD4	0.9690	1.4840	1.4840	4.9390	1.2300	2.5260	7.3750	2021-08-05_	8/5/21 12:30		AP/MA
STD5	2.0470	2.9460	2.9530	9.8060	2.4420	5.2380	14.5520	2021-08-05_	8/5/21 12:59		AP/MA
STD6	4.0260	5.9880	6.0110	19.9470	4.9880	10.1130	29.9090	2021-08-05_	8/5/21 13:28		AP/MA
STD7	4.9680	7.5290	7.5090	25.1120	6.2800	12.3070	37.7270	2021-08-05_	8/5/21 13:57		AP/MA
ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4				
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000				
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000				
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000				
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000				
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000				
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000				
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.5000				
ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4				
STD1		7.8333	7.0000	9.1000	10.4000	-23.2000	13.0667				
STD2	3.7500	0.5833	0.0833	0.3500	0.7000	2.4000	0.7500				
STD3	-3.2500	-1.0667	-1.0667	-1.2200	-1.6000	1.0400	-1.6667				
STD4	-3.1000	-1.8000	-1.5667	-1.9400	-2.3200	4.7600	-2.9867				
STD5	2.3500	-0.2000	0.1833	-0.2650	-0.2400	1.1300	-0.3033				
STD6	0.6500	0.3867	0.1200	0.4480	0.4800	-1.5440	0.6053				
STD7	-0.6400										

CALIBRATION OF COMPONENT F-

Method: AnionsIC2-080521.mtw
 Equation: $Q = 0.076853 \cdot A + 1.58934$
 RSD: 1.722 %
 Correlation coefficient: 0.999838

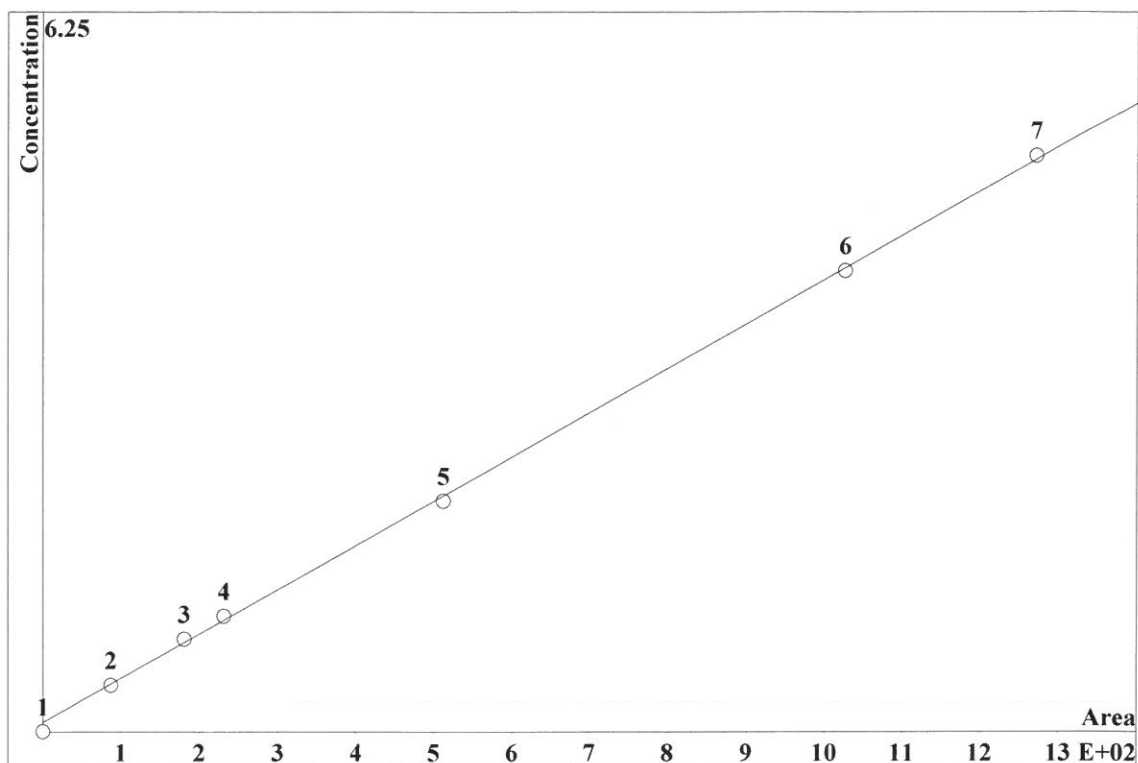


K3 = 0 K2 = 0 K1 = 0.076853 K0 = 1.58934
 Base: Area
 Ref.channel: chl
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	2.124	87.42	0.4	20	5.75		
3	5.031	180.8	0.8	20	5.75		
4	5.873	231.5	1	20	5.75		
5	13.38	512	2	20	5.75		
6	30.2	1027	4	20	5.75		
7	35.05	1272	5	20	5.75		

CALIBRATION OF COMPONENT CL-

Method: AnionsIC2-080521.mtw
 Equation: $Q = 0.112709 \cdot A + 2.35274$
 RSD: 1.216 %
 Correlation coefficient: 0.999919

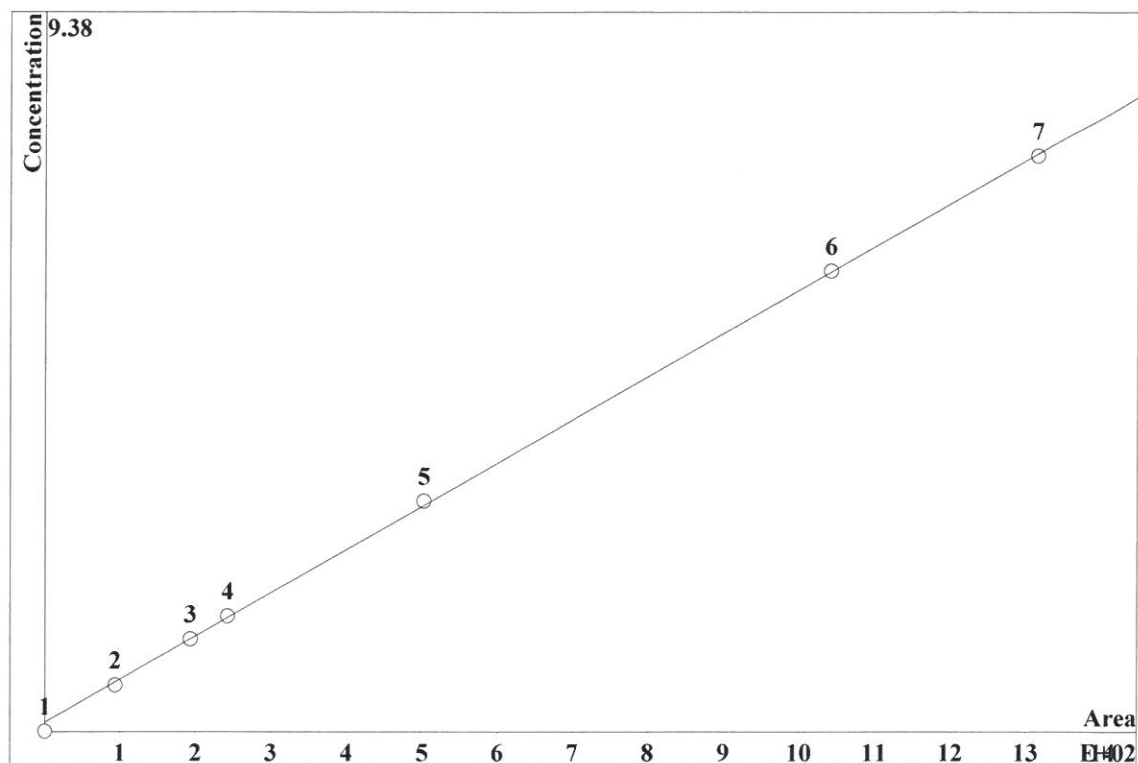

K3 = 0 K2 = 0 K1 = 0.112709 K0 = 2.35274

Base: Area

Ref.channel: chl

ISTD:

Formula: Linear


Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	7.009	93.9	0.6	20	8.834		
3	14.45	193.3	1.2	20	8.834		
4	18.53	242.4	1.5	20	8.834		
5	38.45	501.8	3	20	8.834		
6	81.17	1042	6	20	8.834		
7	104.4	1315	7.5	20	8.834		

1.□

CALIBRATION OF COMPONENT NO2

Method: AnionsIC2-080521.mtw
 Equation: $Q = 0.0506157 \cdot A + 2.28106$
 RSD: 1.009 %
 Correlation coefficient: 0.999945

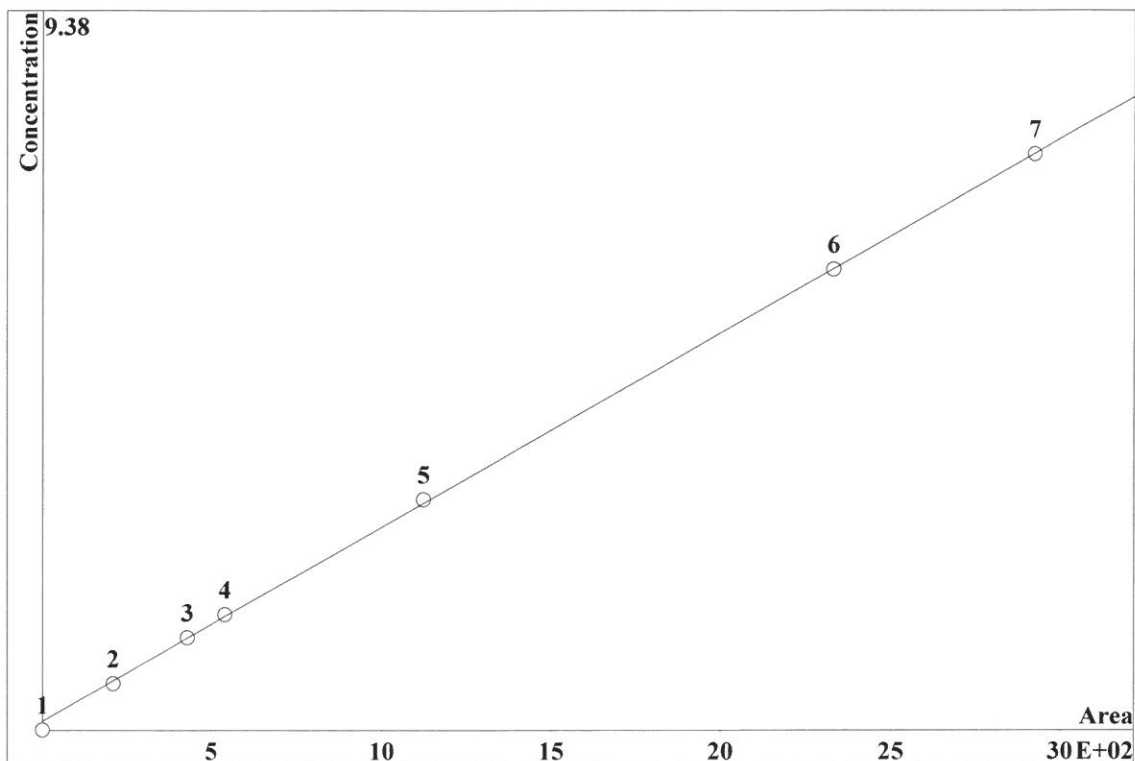


K3 = 0 K2 = 0 K1 = 0.0506157 K0 = 2.28106
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used File
1	0	0	0	0	0	0
2	12.64	208.6	0.6	20	10.64	
3	25.8	429.7	1.2	20	10.64	
4	32.48	541.1	1.5	20	10.64	
5	66.63	1122	3	20	10.64	
6	131.9	2330	6	20	10.64	
7	160.2	2922	7.5	20	10.64	

CALIBRATION OF COMPONENT BR-

Method: AnionsIC2-080521.mtw
 Equation: $Q = 0.25162 \cdot A + 8.79014$
 RSD: 1.364 %
 Correlation coefficient: 0.999899

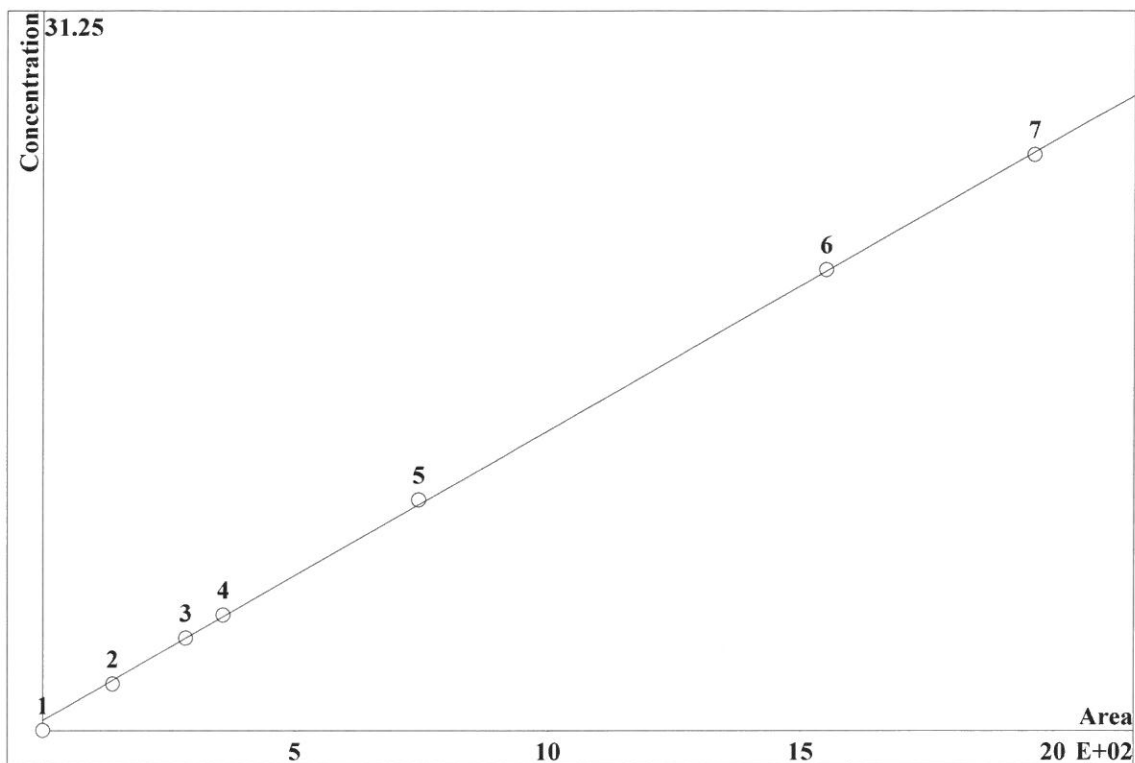

K3 = 0 K2 = 0 K1 = 0.25162 K0 = 8.79014

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	7.412	138.5	2	20			14
3	15.53	284.1	4	20			14
4	19.8	357.6	5	20			14
5	41.64	744.5	10	20			14
6	87.57	1551	20	20			14
7	111.3	1961	25	20			14

CALIBRATION OF COMPONENT NO3

Method: AnionsIC2-080521.mtw
 Equation: $Q = 0.0439491 \cdot A + 2.36059$
 RSD: 1.576 %
 Correlation coefficient: 0.999865

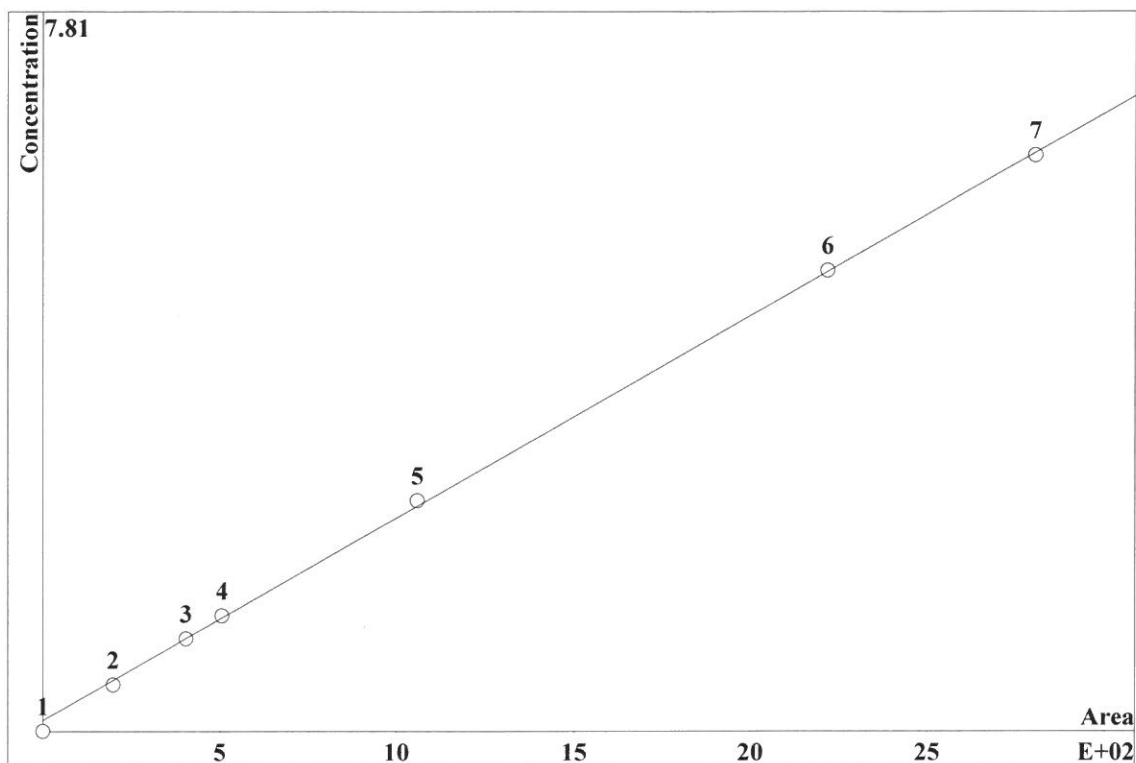


K3 = 0 K2 = 0 K1 = 0.0439491 K0 = 2.36059

Base: Area
 Ref.channel: chl
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	8.937	197.6	0.5	20	16.28		
3	18.53	404.7	1	20	16.28		
4	23.54	506	1.25	20	16.28		
5	49.34	1058	2.5	20	16.28		
6	104.4	2216	5	20	16.28		
7	133.8	2804	6.25	20	16.28		

CALIBRATION OF COMPONENT HPO4

Method: AnionsIC2-080521.mtw
 Equation: $Q = 0.0803488 \cdot A - 18.9323$
 RSD: 3.677 %
 Correlation coefficient: 0.999263

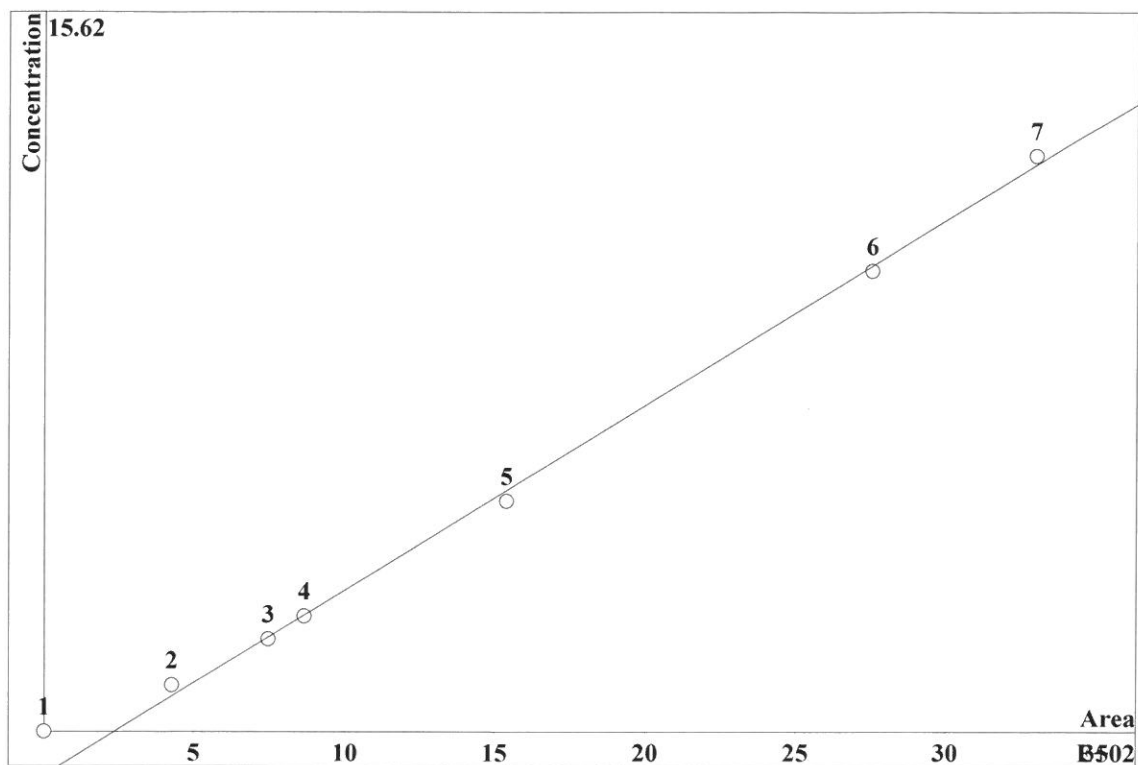

K3 = 0 K2 = 0 K1 = 0.0803488 K0 = -18.9323

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	11.13	426.7	1	20	21.2		
3	20.4	745.3	2	20	21.2		
4	24.18	864.5	2.5	20	21.2		
5	45.25	1540	5	20	21.2		
6	85.4	2753	10	20	21.2		
7	104.4	3299	12.5	20	21.2		

CALIBRATION OF COMPONENT SO4

Method: AnionsIC2-080521.mtw
 Equation: $Q = 0.141941 \cdot A + 16.2145$
 RSD: 1.991 %
 Correlation coefficient: 0.999784

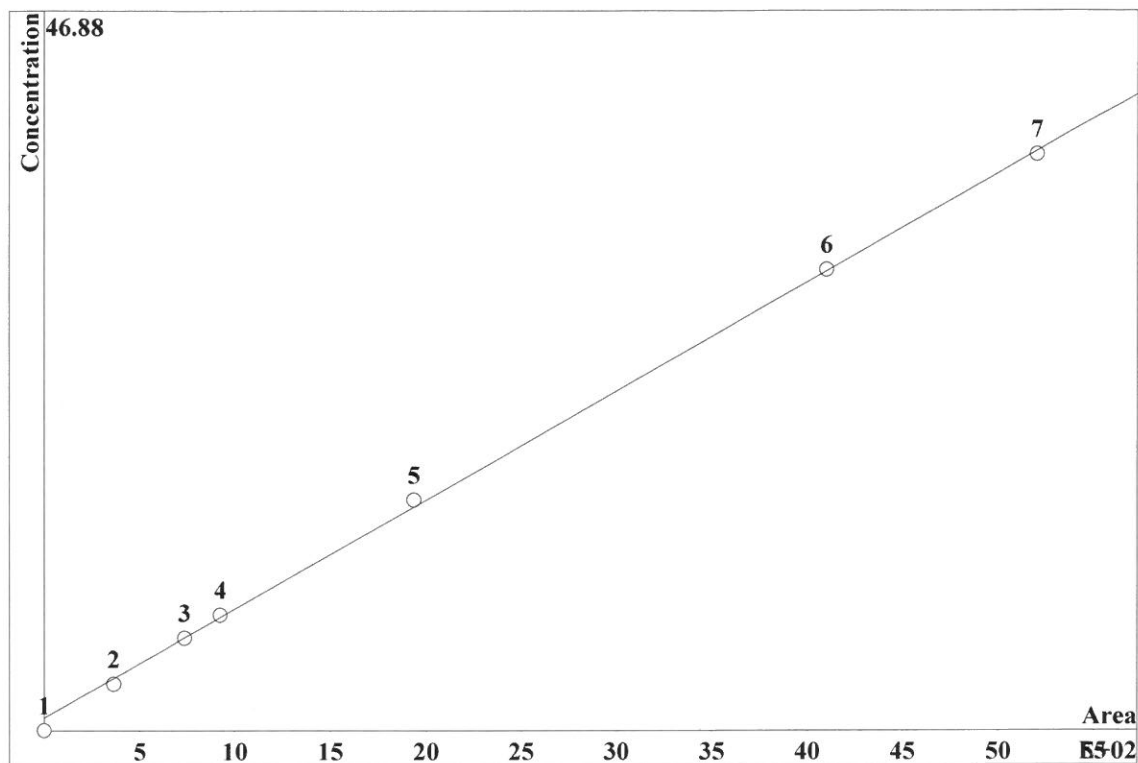

K3 = 0 K2 = 0 K1 = 0.141941 K0 = 16.2145

Base: Area

Ref.channel: ch1

ISTD:

Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used File
1	0	0	0	0	0	0
2	12.9	363.8	3	20	24.73	
3	26.54	737.5	6	20	24.73	
4	33.53	924.9	7.5	20	24.73	
5	70.85	1936	15	20	24.73	
6	151.6	4100	30	20	24.73	
7	192.9	5202	37.5	20	24.73	

Report date: 8/6/2021 4:44:20 PM
Printed by: wet


Ident: STD1
Analysis from: 8/5/2021 11:03:05 AM
File: _2021-08-05_

Last save: 8/5/2021 4:06:12 PM

Method: AnionsIC2-080521.mtw
Run operator: wet
Analysis number: 27788

Last save: 8/5/2021 10:25:

SAMPLE:
: AP/MA
Vial number: 2
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

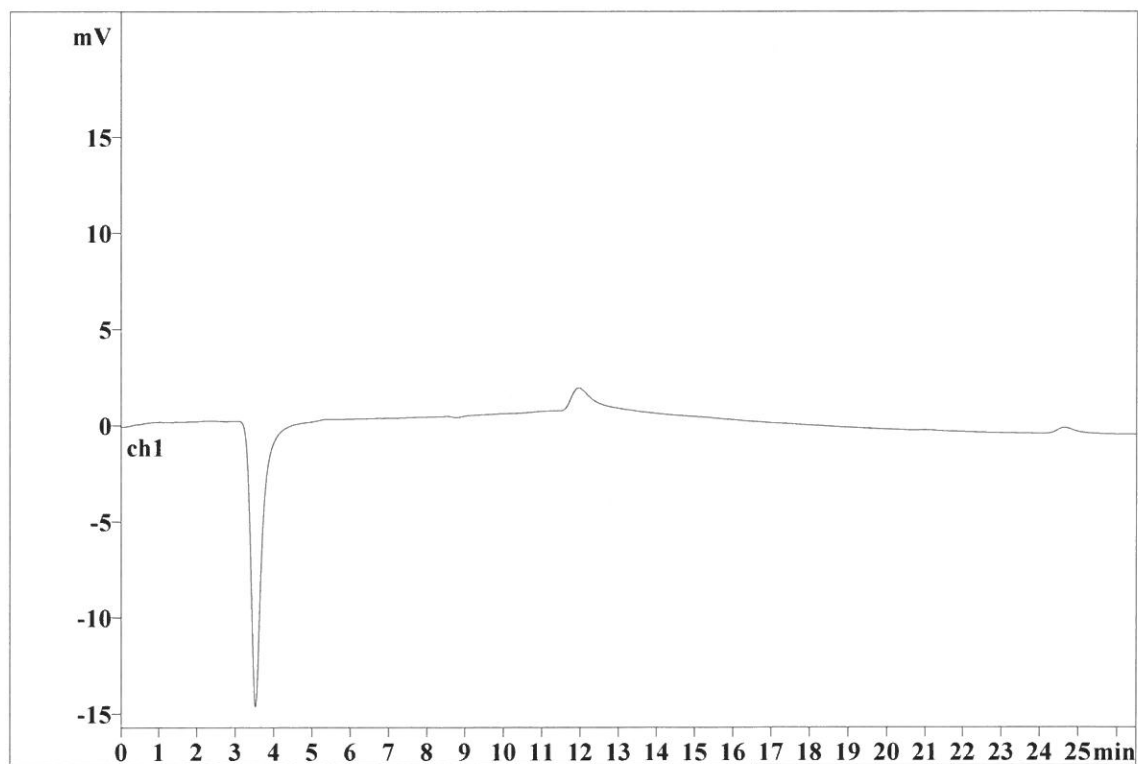

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 8/6/2021 4:44:37 PM
Printed by: wet


Ident: STD2
Analysis from: 8/5/2021 11:32:13 AM
File: _2021-08-05_

Last save: 8/5/2021 4:06:12 PM

Method: AnionsIC2-080521.mtw
Run operator: wet
Analysis number: 27789

Last save: 8/5/2021 10:25:

SAMPLE:
: AP/MA
Vial number: 3
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

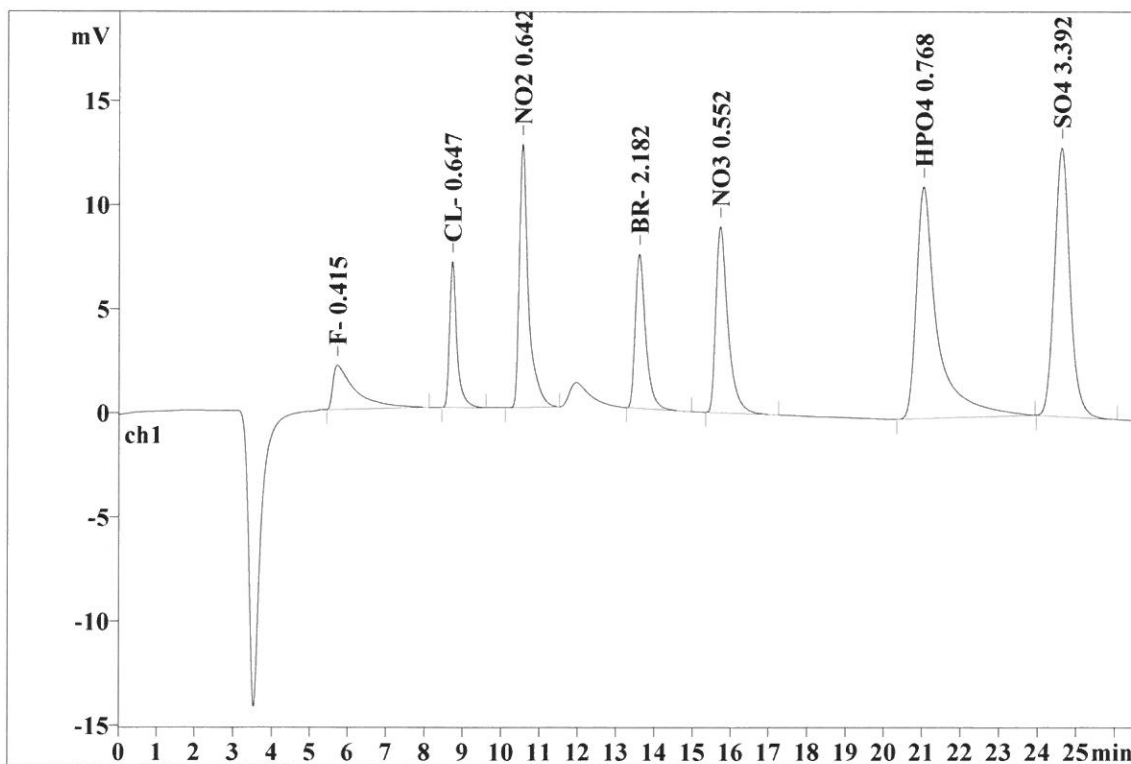

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.72	0.529	2.12	3.42	87.416	5.76
2	8.70	0.185	7.01	11.28	93.898	6.19
3	10.54	0.221	12.64	20.33	208.575	13.75
4	13.59	0.271	7.41	11.92	138.522	9.13
5	15.70	0.318	8.94	14.38	197.597	13.03
6	21.01	0.473	11.13	17.91	426.742	28.14
7	24.58	0.423	12.90	20.76	363.768	23.99
7	26.50	0.346	62.15	99.99	1516.518	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/6/2021 4:44:44 PM
Printed by: wet


Ident: STD3
Analysis from: 8/5/2021 12:01:21 PM
File: _2021-08-05_

Last save: 8/5/2021 4:06:12 PM

Method: AnionsIC2-080521.mtw
Run operator: wet
Analysis number: 27790

Last save: 8/5/2021 10:25:

SAMPLE:
: AP/MA
Vial number: 4
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

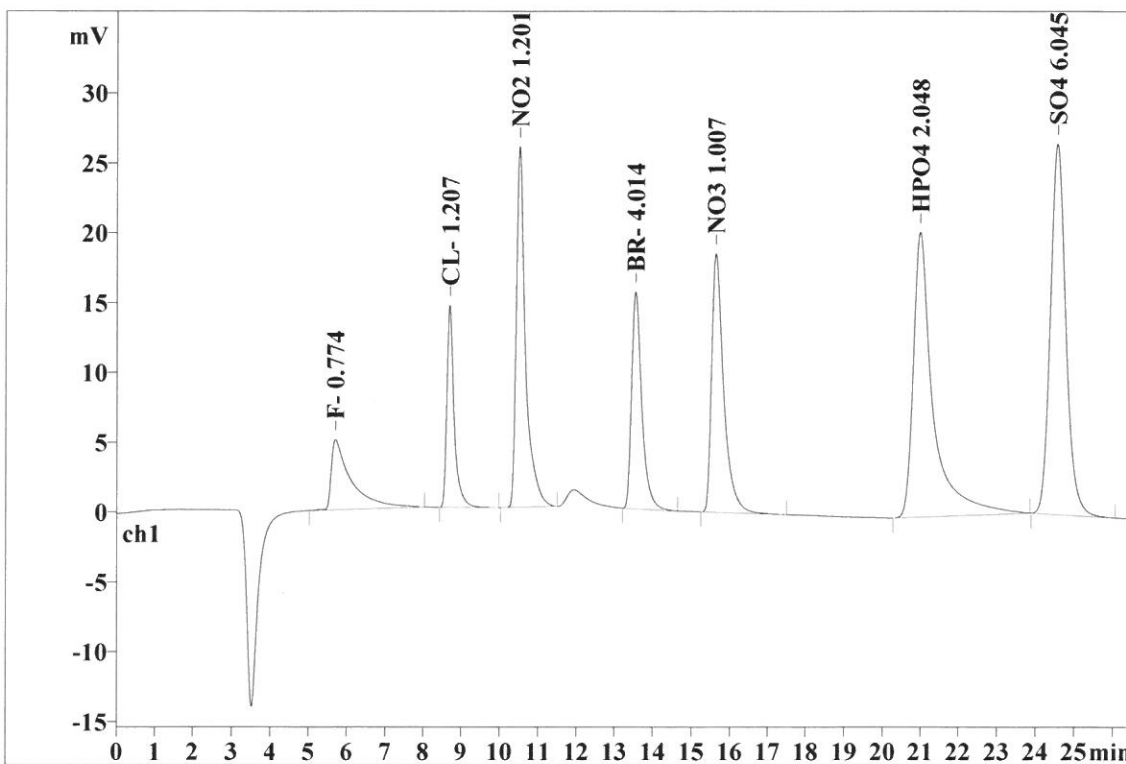

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.69	0.446	5.03	3.98	180.825	6.08
2	8.68	0.185	14.45	11.45	193.273	6.50
3	10.51	0.224	25.80	20.43	429.683	14.44
4	13.54	0.266	15.53	12.30	284.130	9.55
5	15.62	0.313	18.53	14.67	404.666	13.60
6	20.97	0.454	20.40	16.15	745.320	25.05
7	24.55	0.417	26.54	21.01	737.476	24.79
7	26.50	0.329	126.27	99.99	2975.373	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/6/2021 4:44:50 PM
Printed by: wet


Ident: STD4
Analysis from: 8/5/2021 12:30:30 PM
File: _2021-08-05_

Last save: 8/5/2021 4:06:12 PM

Method: AnionsIC2-080521.mtw
Run operator: wet
Analysis number: 27791

Last save: 8/5/2021 10:25:

SAMPLE:
: AP/MA
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

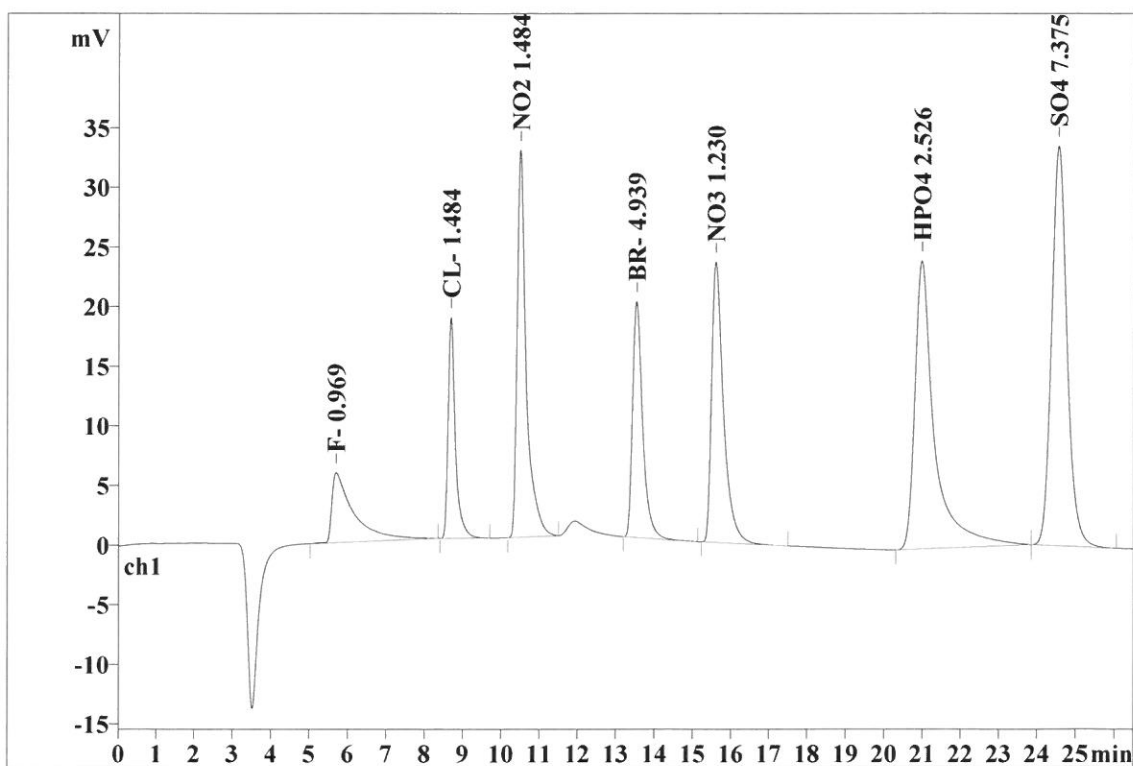

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.70	0.488	5.87	3.72	231.481	6.31
2	8.68	0.181	18.53	11.73	242.437	6.61
3	10.50	0.225	32.48	20.57	541.135	14.75
4	13.52	0.262	19.80	12.53	357.624	9.75
5	15.60	0.309	23.53	14.90	505.957	13.79
6	20.96	0.448	24.18	15.31	864.484	23.57
7	24.55	0.415	33.53	21.23	924.919	25.22
7	26.50	0.333	157.92	100.00	3668.038	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/6/2021 4:45:08 PM
Printed by: wet


Ident: STD5
Analysis from: 8/5/2021 12:59:38 PM
File: _2021-08-05_

Last save: 8/5/2021 4:06:12 PM

Method: AnionsIC2-080521.mtw
Run operator: wet
Analysis number: 27792

Last save: 8/5/2021 10:25:

SAMPLE:
: AP/MA
Vial number: 6
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

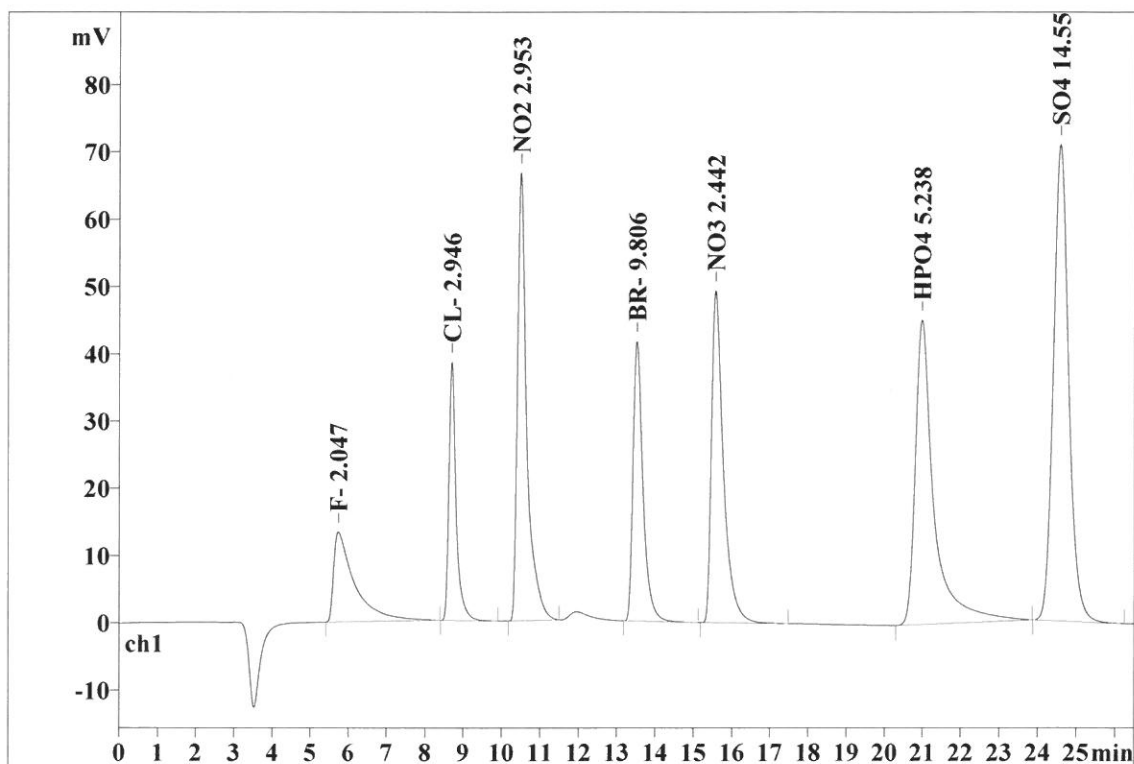

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.73	0.496	13.38	4.11	512.039	6.91
2	8.69	0.181	38.45	11.81	501.837	6.77
3	10.49	0.227	66.63	20.47	1121.786	15.13
4	13.52	0.259	41.63	12.79	744.499	10.04
5	15.56	0.306	49.34	15.16	1057.777	14.27
6	20.97	0.431	45.25	13.90	1539.537	20.77
7	24.57	0.410	70.85	21.76	1936.191	26.12
7	26.50	0.330	325.53	100.00	7413.666	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/6/2021 4:45:14 PM
Printed by: wet


Ident: STD6
Analysis from: 8/5/2021 1:28:46 PM
File: _2021-08-05_

Last save: 8/5/2021 4:06:12 PM

Method: AnionsIC2-080521.mtw
Run operator: wet
Analysis number: 27793

Last save: 8/5/2021 10:25:

SAMPLE:
: AP/MA
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

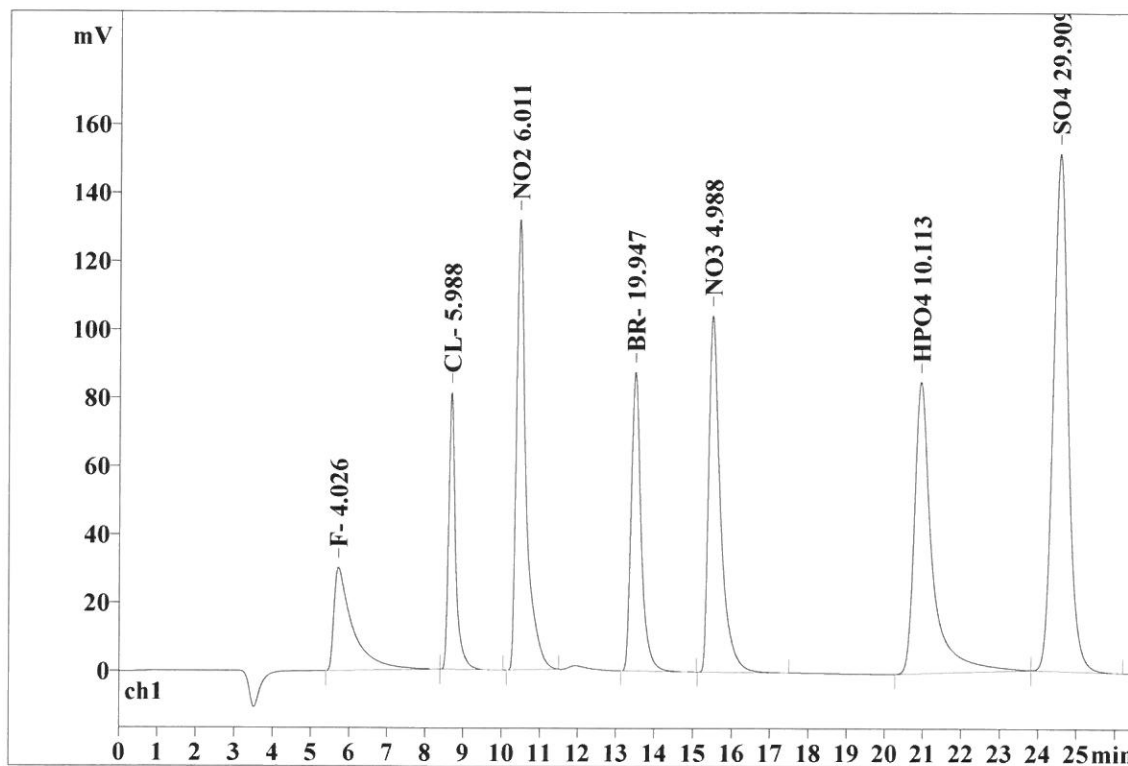

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.71	0.432	30.20	4.49	1026.995	6.84
2	8.67	0.176	81.17	12.07	1041.639	6.94
3	10.44	0.237	131.89	19.62	2329.898	15.51
4	13.48	0.256	87.57	13.03	1550.546	10.32
5	15.48	0.300	104.40	15.53	2216.399	14.76
6	20.92	0.415	85.39	12.70	2752.824	18.33
7	24.53	0.404	151.60	22.55	4100.118	27.30
7	26.50	0.317	672.22	100.00	15018.420	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/6/2021 4:45:21 PM
Printed by: wet


Ident: STD7
Analysis from: 8/5/2021 1:57:54 PM
File: _2021-08-05_

Last save: 8/5/2021 4:06:12 PM

Method: AnionsIC2-080521.mtw
Run operator: wet
Analysis number: 27794

Last save: 8/5/2021 10:25:

SAMPLE:
: AP/MA
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

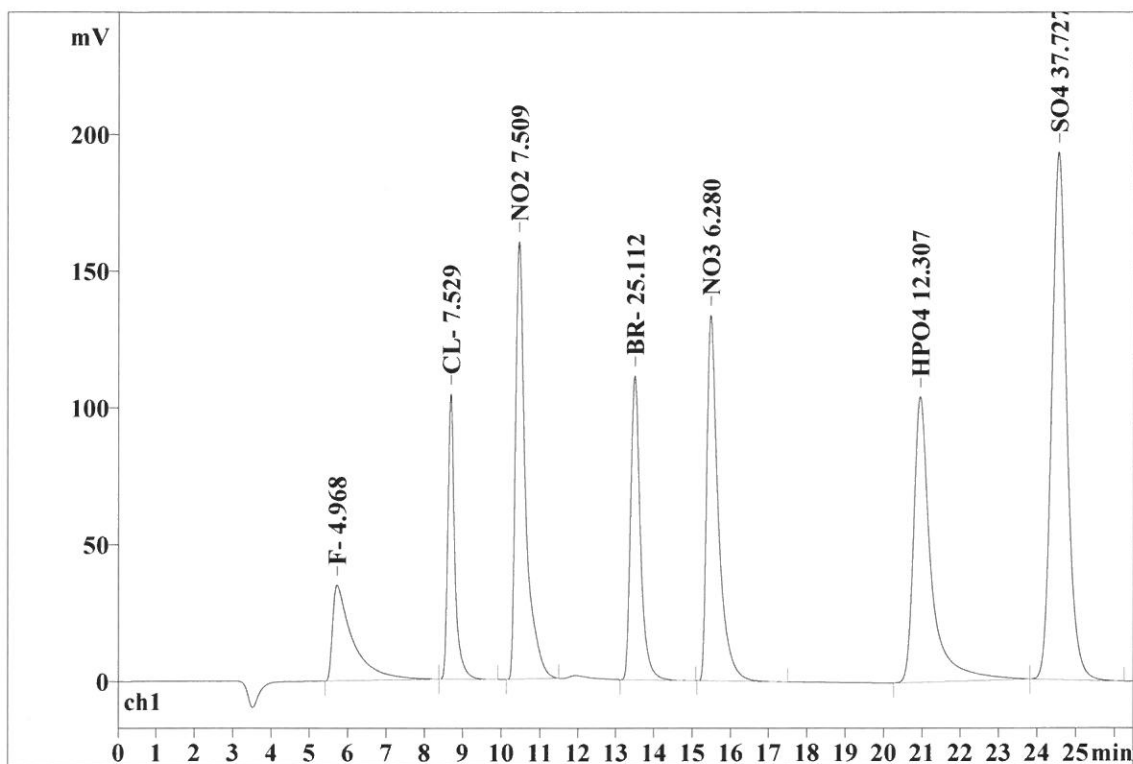

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.72	0.467	35.05	4.16	1272.291	6.78
2	8.67	0.173	104.43	12.40	1315.140	7.00
3	10.44	0.248	160.16	19.02	2922.178	15.56
4	13.48	0.256	111.32	13.22	1961.076	10.44
5	15.46	0.296	133.84	15.89	2804.019	14.93
6	20.92	0.411	104.45	12.40	3299.040	17.57
7	24.53	0.403	192.93	22.91	5201.581	27.70
7	26.50	0.322	842.17	100.00	18775.325	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/6/2021 4:45:27 PM
Printed by: wet


Ident: ICV
Analysis from: 8/5/2021 3:36:31 PM
File: _2021-08-05_

Last save: 8/5/2021 4:06:12 PM

Method: AnionsIC2-080521.mtw
Run operator: wet
Analysis number: 27797

Last save: 8/5/2021 10:25:

SAMPLE:
: AP/MA
Vial number: 9
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

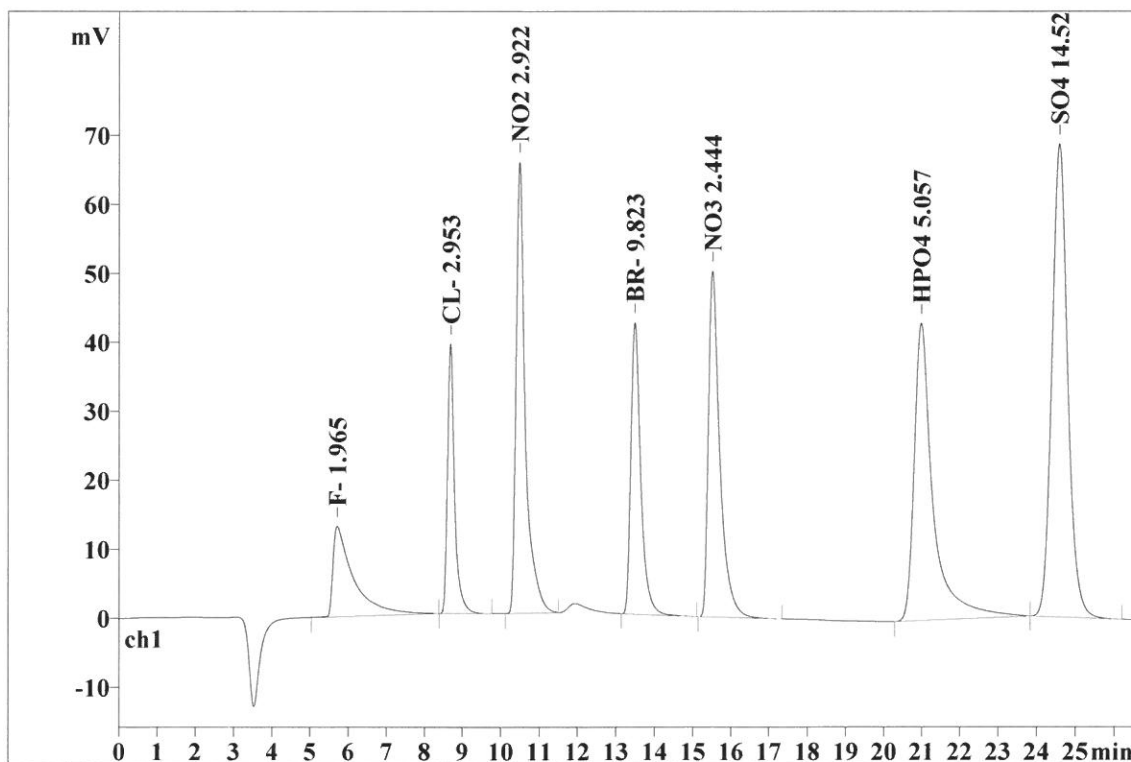

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.71	0.471	13.12	4.08	490.773	6.69
2	8.67	0.179	39.12	12.15	503.197	6.86
3	10.46	0.230	65.44	20.33	1109.466	15.13
4	13.47	0.256	42.29	13.14	745.880	10.17
5	15.50	0.302	50.18	15.59	1058.675	14.43
6	20.96	0.445	43.13	13.40	1494.473	20.38
7	24.55	0.423	68.62	21.32	1931.631	26.34
7	26.50	0.330	321.91	100.00	7334.096	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/6/2021 4:45:36 PM
Printed by: wet


Ident: ICB
Analysis from: 8/5/2021 4:08:17 PM
File: _2021-08-05_

Last save: 8/5/2021 4:39:37 PM

Method: AnionsIC2-080521.mtw
Run operator: wet
Analysis number: 27798

Last save: 8/5/2021 2:25:2

SAMPLE:
: AP/MA
Vial number: 10
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

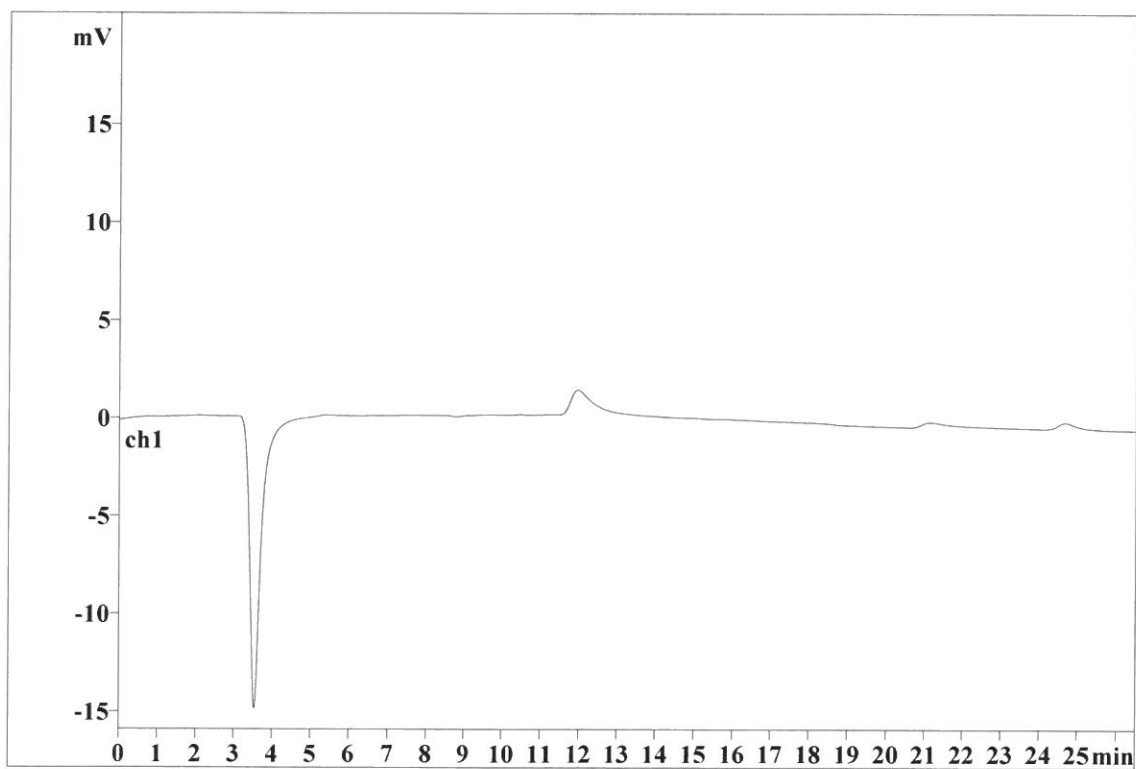

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 8/9/2021 11:16:29 AM
Printed by: wet


Ident: CCV
Analysis from: 8/6/2021 8:47:09 AM
File: _2021-08-06_

Last save: 8/6/2021 9:13:39 AM

Method: AnionsIC2-080521.mtw
Run operator: wet
Analysis number: 27812

Last save: 8/5/2021 2:25:2

SAMPLE:
: AP/MA
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

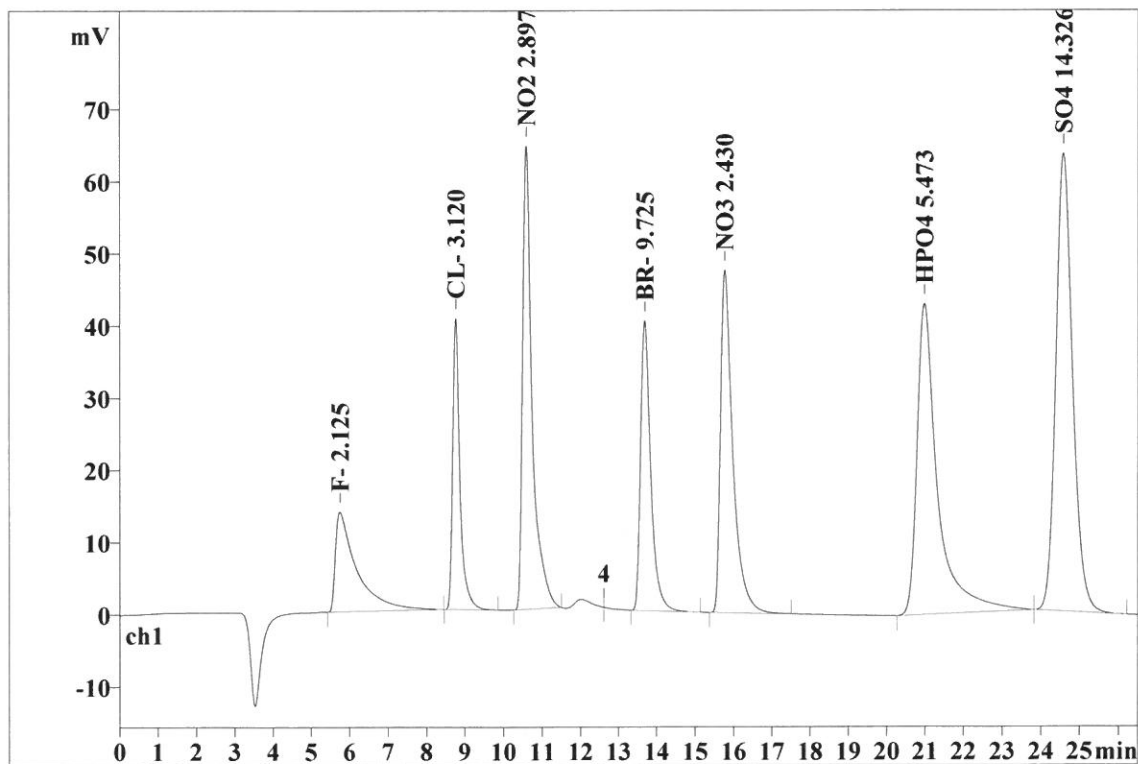

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.74	0.490	13.82	4.42	532.351	7.14
2	8.75	0.183	40.33	12.91	532.824	7.14
3	10.58	0.230	64.18	20.54	1099.732	14.75
4	13.68	0.266	40.14	12.85	738.028	9.90
5	15.77	0.316	47.44	15.18	1052.230	14.11
6	20.98	0.478	43.08	13.79	1598.019	21.43
7	24.59	0.453	63.47	20.31	1904.395	25.54
7	26.50	0.345	312.45	100.00	7457.579	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/9/2021 11:20:28 AM
Printed by: wet


Ident: CCB
Analysis from: 8/6/2021 9:18:07 AM
File: _2021-08-06_

Last save: 8/6/2021 9:45:18 AM

Method: AnionsIC2-080521.mtw
Run operator: wet
Analysis number: 27813

Last save: 8/6/2021 9:45:0

SAMPLE:
: AP/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

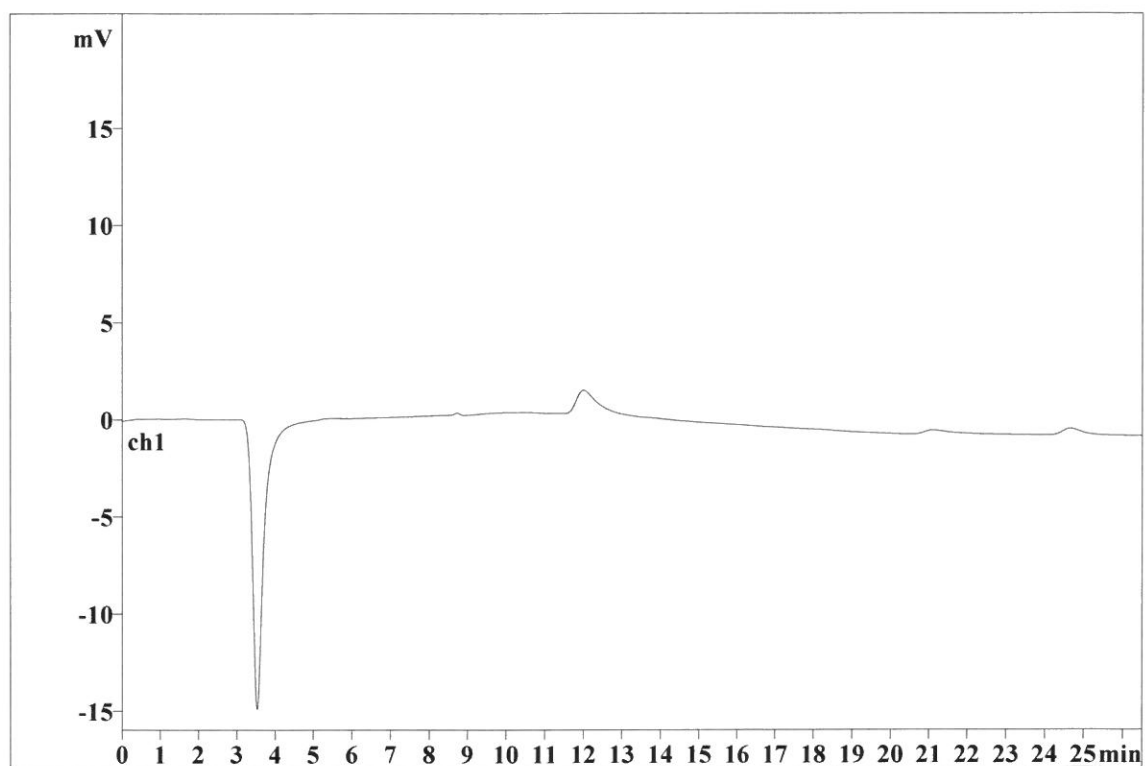

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 8/9/2021 11:20:57 AM
Printed by: wet


Ident: LB115709BLW
Analysis from: 8/6/2021 9:47:15 AM
File: _2021-08-06_

Last save: 8/9/2021 11:20:55 AM

Method: AnionsIC2-080521.mtw
Run operator: wet
Analysis number: 27814

Last save: 8/5/2021 2:25:2

SAMPLE:
: AP/MA
Vial number: 13
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

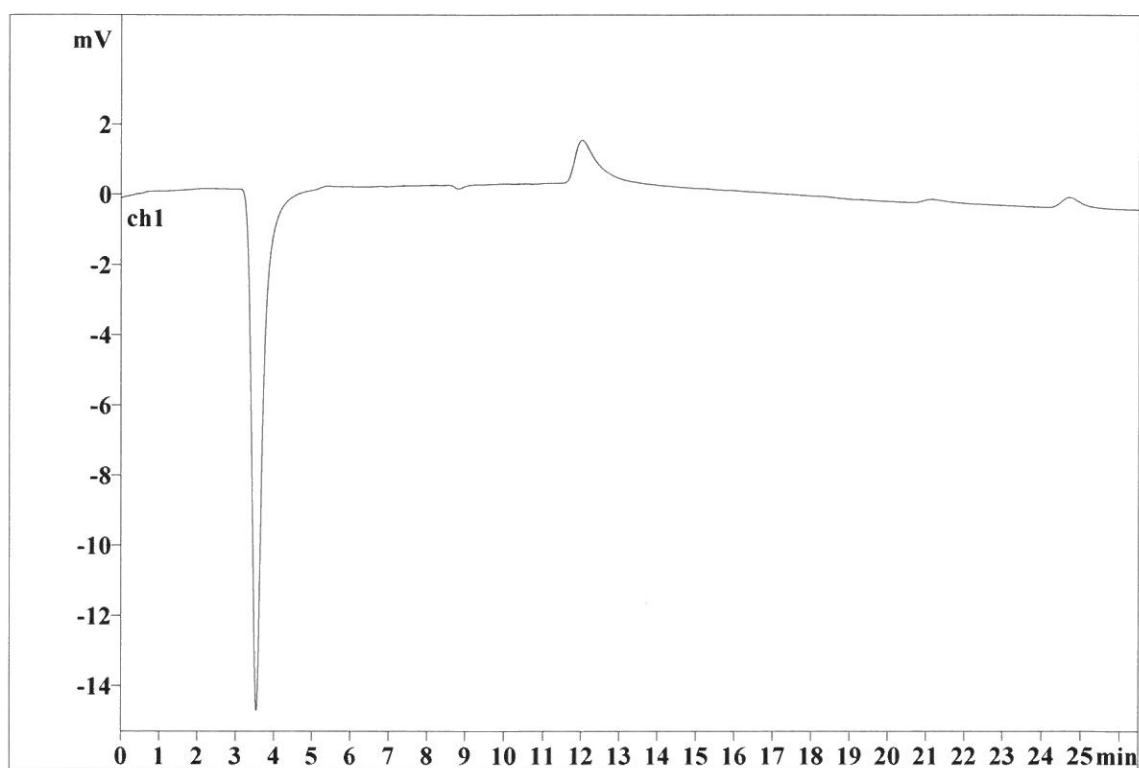

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 8/9/2021 11:21:07 AM
 Printed by: wet


Ident: LB115709BSW
 Analysis from: 8/6/2021 10:16:23 AM
 File: _2021-08-06_

Last save: 8/6/2021 10:42:53 AM

Method: AnionsIC2-080521.mtw
 Run operator: wet
 Analysis number: 27815

Last save: 8/6/2021 9:45:0

SAMPLE:
 : AP/MA
 Vial number: 14
 Volume: 20.0 µL
 Dilution: 1.00
 Amount: 1.0000

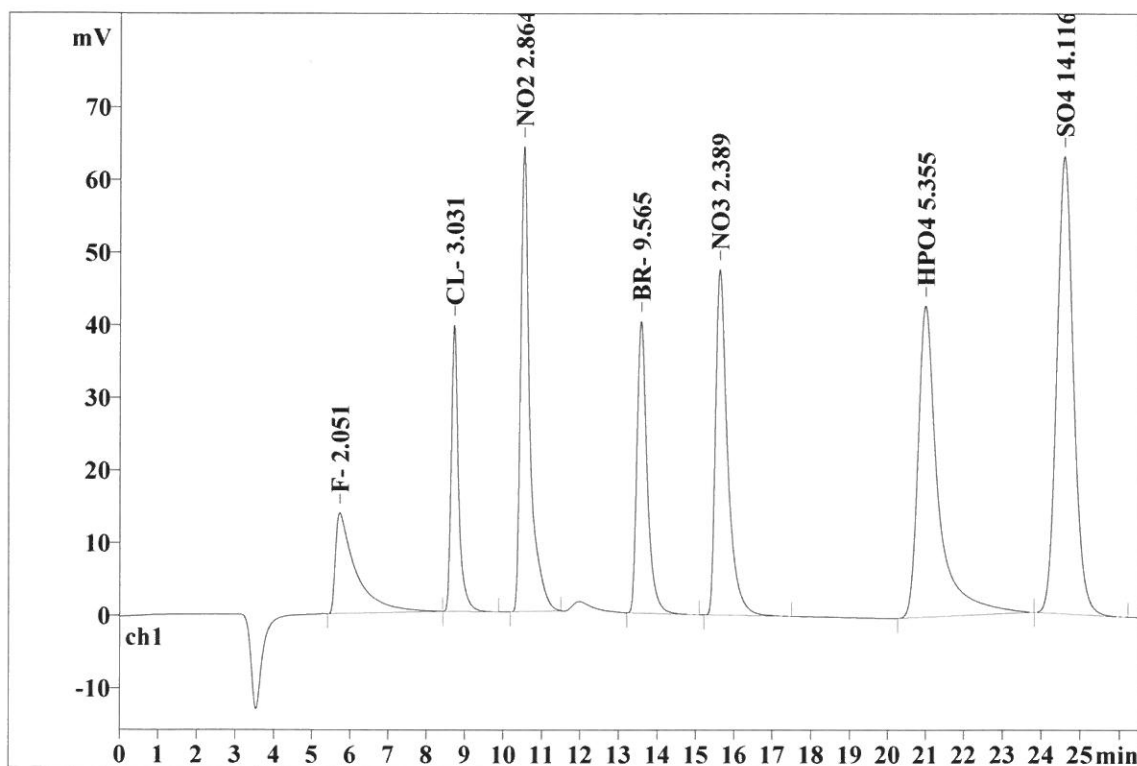

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.73	0.467	13.86	4.46	513.088	7.01
2	8.70	0.181	39.48	12.69	516.958	7.06
3	10.51	0.227	64.08	20.60	1086.478	14.85
4	13.56	0.262	40.21	12.93	725.375	9.91
5	15.61	0.310	47.57	15.29	1033.290	14.12
6	20.97	0.473	42.87	13.78	1568.625	21.43
7	24.57	0.450	63.00	20.25	1874.763	25.62
7	26.50	0.339	311.06	100.00	7318.577	100.00

This report has been created by IC Net
 METROHM LTD

Report date: 8/9/2021 11:21:30 AM
Printed by: wet


Ident: M3311-01
Analysis from: 8/6/2021 10:45:33 AM
File: _2021-08-06_

Last save: 8/6/2021 11:12:03 AM

Method: AnionsIC2-080521.mtw
Run operator: wet
Analysis number: 27816

Last save: 8/6/2021 9:45:0

SAMPLE:
: AP/MA
Vial number: 18
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

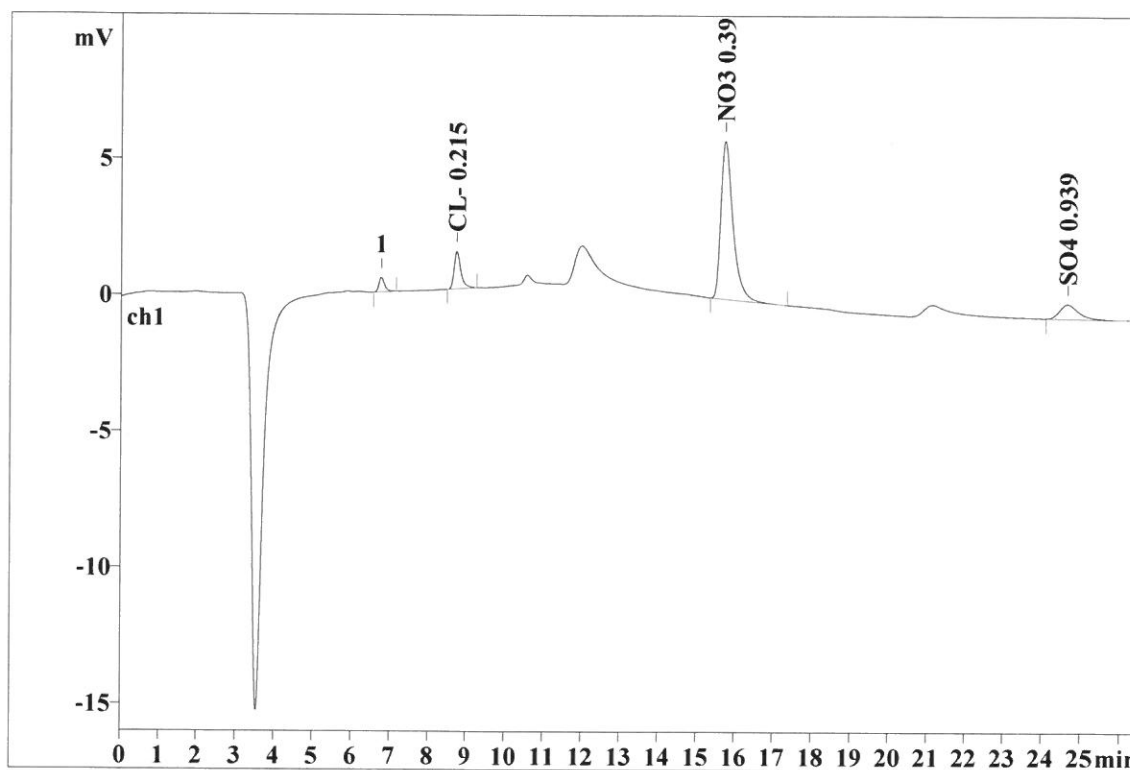

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	8.71	0.180	1.37	16.63	17.191	10.22
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	15.71	0.319	5.80	70.36	127.404	75.73
6	0.00	0.000	0.00	0.00	0.000	0.00
7	24.65	0.497	0.53	6.49	18.099	10.76
7	26.50	0.142	7.71	93.48	162.694	96.71

This report has been created by IC Net
METROHM LTD

Report date: 8/9/2021 11:21:41 AM
Printed by: wet


Ident: M3301-01
Analysis from: 8/6/2021 11:14:44 AM
File: _2021-08-06_

Last save: 8/6/2021 11:50:00 AM

Method: AnionsIC2-080521.mtw
Run operator: wet
Analysis number: 27817

Last save: 8/6/2021 9:45:0

SAMPLE:
: AP/MA
Vial number: 15
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

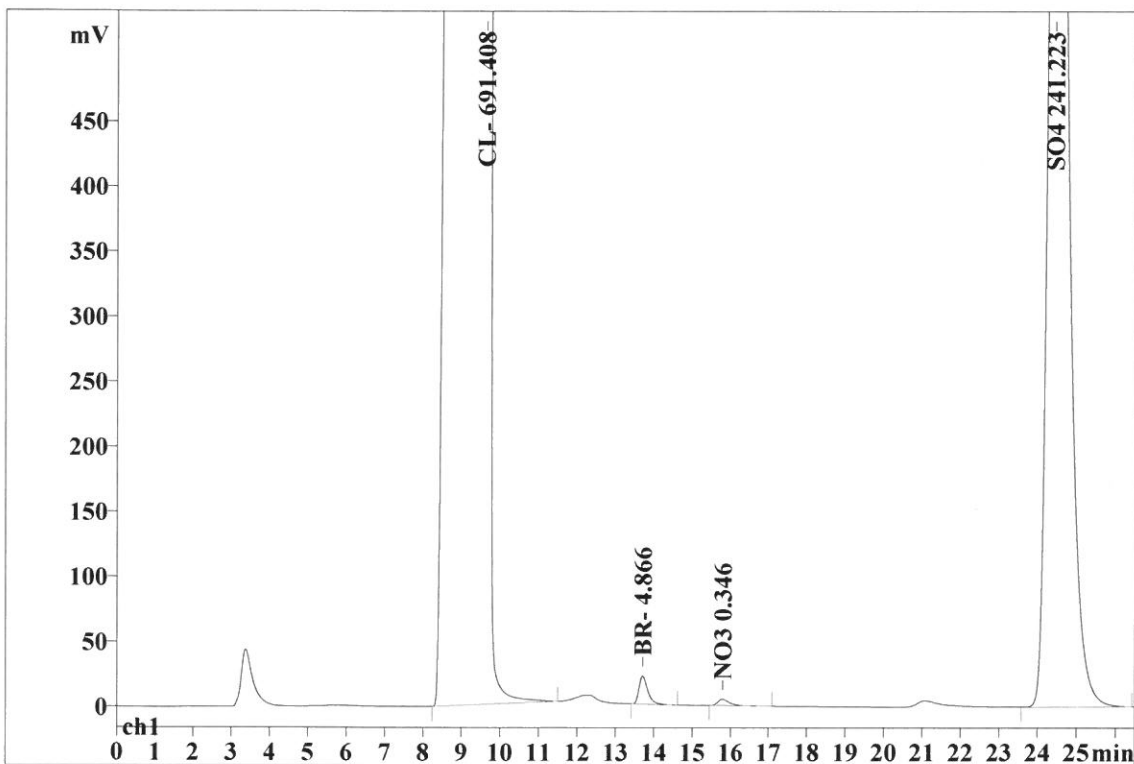

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.60	1.229	1706.46	61.05	122668.087	78.13
3	0.00	0.000	0.00	0.00	0.000	0.00
4	13.71	0.241	21.68	0.78	351.821	0.22
5	15.79	0.308	4.93	0.18	103.619	0.07
6	0.00	0.000	0.00	0.00	0.000	0.00
7	24.42	0.486	1062.05	38.00	33874.897	21.58
7	26.50	0.323	2795.12	100.00	156998.425	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/9/2021 11:21:51 AM
Printed by: wet


Ident: M3325-01
Analysis from: 8/6/2021 1:47:11 PM
File: _2021-08-06_

Last save: 8/6/2021 2:27:04 PM

Method: AnionsIC2-080521.mtw
Run operator: wet
Analysis number: 27822

Last save: 8/6/2021 9:45:0

SAMPLE:
: AP/MA
Vial number: 21
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

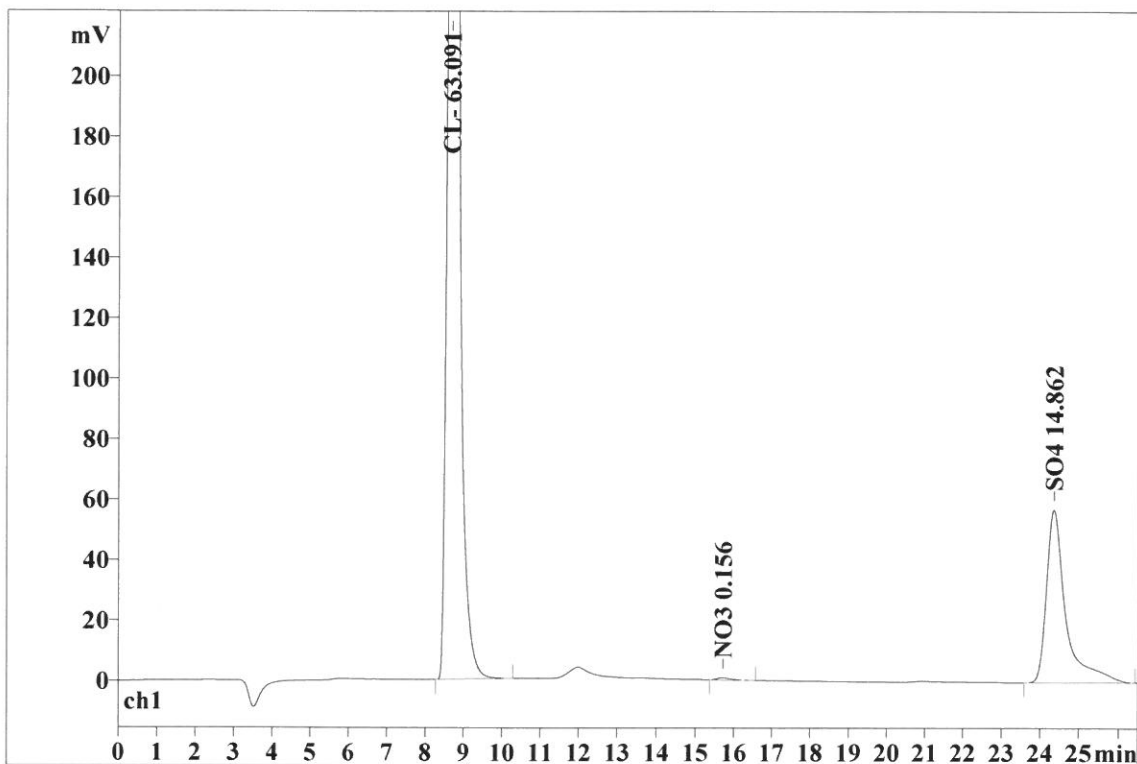

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	8.65	0.211	736.29	92.71	11174.579	84.84
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	15.71	0.364	0.70	0.09	17.163	0.13
6	0.00	0.000	0.00	0.00	0.000	0.00
7	24.36	0.451	57.17	7.20	1979.932	15.03
7	26.50	0.147	794.16	100.00	13171.675	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/9/2021 11:22:15 AM
Printed by: wet


Ident: M3311-01MS
Analysis from: 8/6/2021 2:16:21 PM
File: _2021-08-06_

Last save: 8/6/2021 3:13:22 PM

Method: AnionsIC2-080521.mtw
Run operator: wet
Analysis number: 27823

Last save: 8/6/2021 9:45:0

SAMPLE:
: AP/MA
Vial number: 19
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

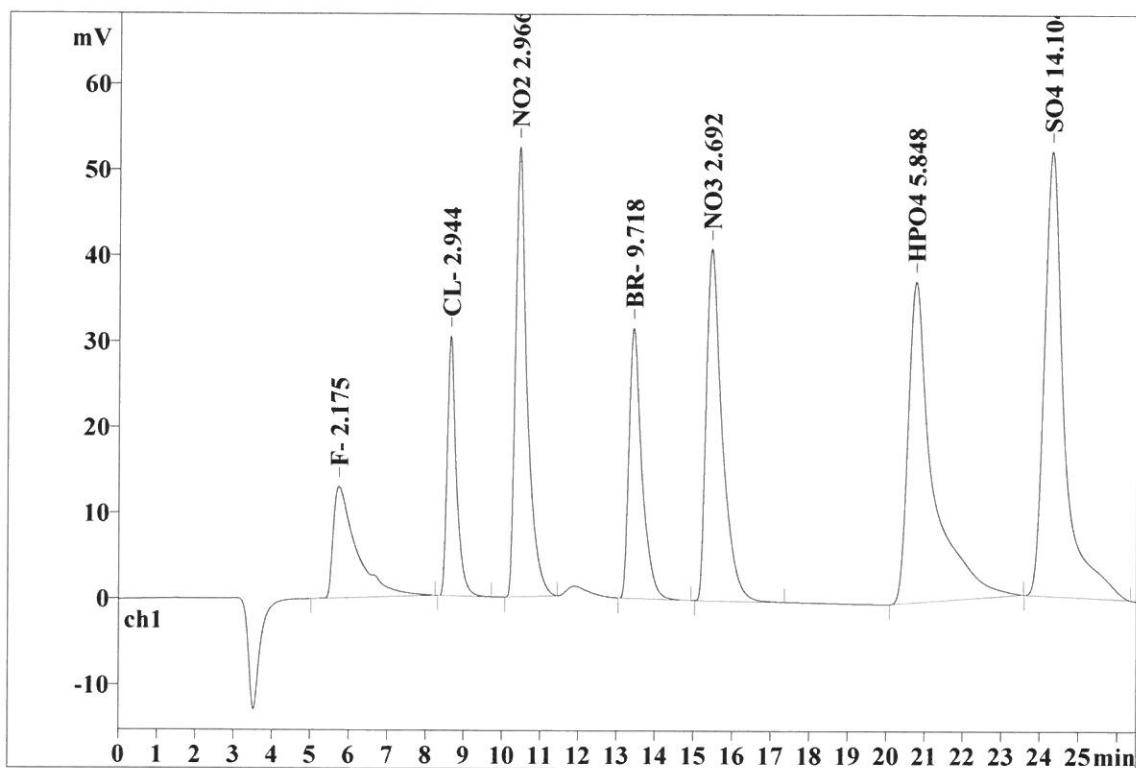

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.73	0.549	12.99	5.05	545.288	7.13
2	8.63	0.235	30.28	11.76	501.486	6.56
3	10.41	0.303	52.42	20.36	1126.819	14.74
4	13.42	0.337	31.51	12.24	737.467	9.64
5	15.43	0.415	41.00	15.92	1171.279	15.32
6	20.73	0.529	37.41	14.53	1691.229	22.12
7	24.28	0.479	51.85	20.14	1873.054	24.50
7	26.50	0.407	257.46	100.00	7646.621	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/9/2021 11:22:56 AM
Printed by: wet


Ident: M3311-01MSD
Analysis from: 8/6/2021 2:45:29 PM
File: _2021-08-06_

Last save: 8/6/2021 3:13:22 PM

Method: AnionsIC2-080521.mtw
Run operator: wet
Analysis number: 27824

Last save: 8/6/2021 9:45:0

SAMPLE:
: AP/MA
Vial number: 20
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

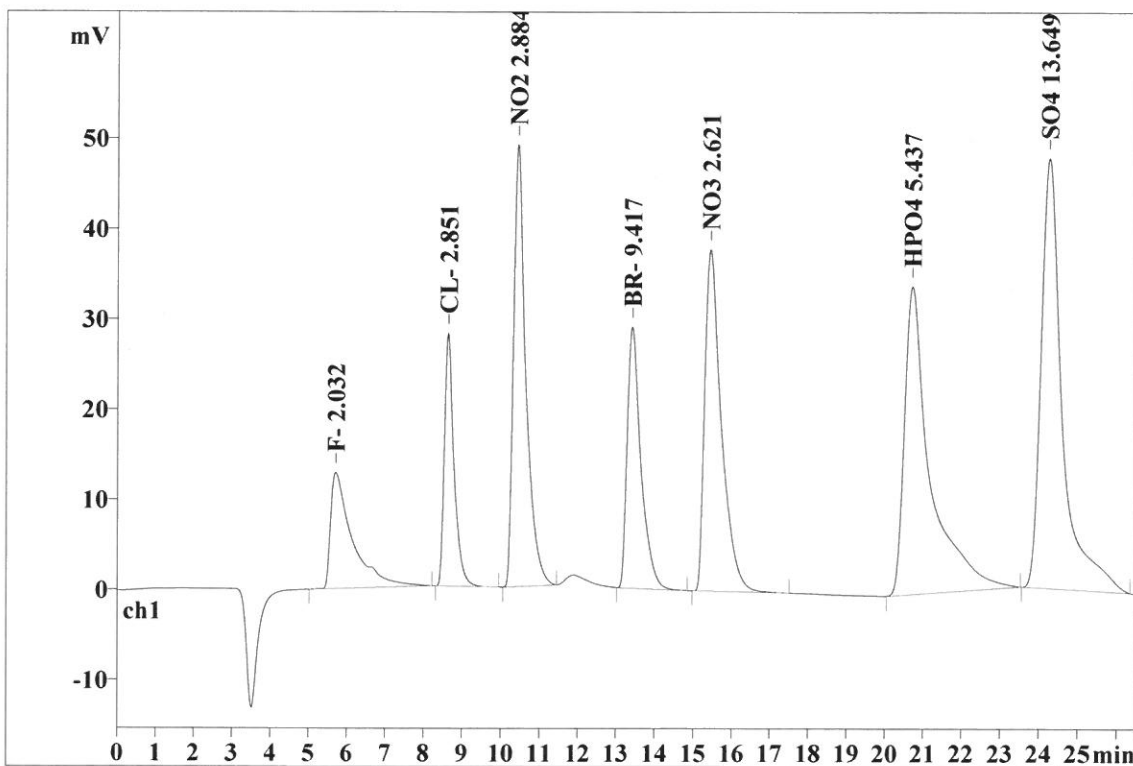

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.71	0.504	12.87	5.40	508.167	6.93
2	8.62	0.247	28.03	11.76	485.075	6.61
3	10.41	0.319	48.96	20.53	1094.307	14.91
4	13.41	0.358	28.95	12.14	713.595	9.72
5	15.43	0.439	37.83	15.87	1138.824	15.52
6	20.70	0.552	34.09	14.30	1589.066	21.66
7	24.24	0.506	47.68	20.00	1808.953	24.65
7	26.50	0.418	238.40	100.00	7337.987	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/9/2021 11:22:38 AM
Printed by: wet


Ident: CCV
Analysis from: 8/6/2021 3:14:41 PM
File: _2021-08-06_

Last save: 8/6/2021 3:41:11 PM

Method: AnionsIC2-080521.mtw
Run operator: wet
Analysis number: 27825

Last save: 8/6/2021 9:45:0

SAMPLE:
: AP/MA
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

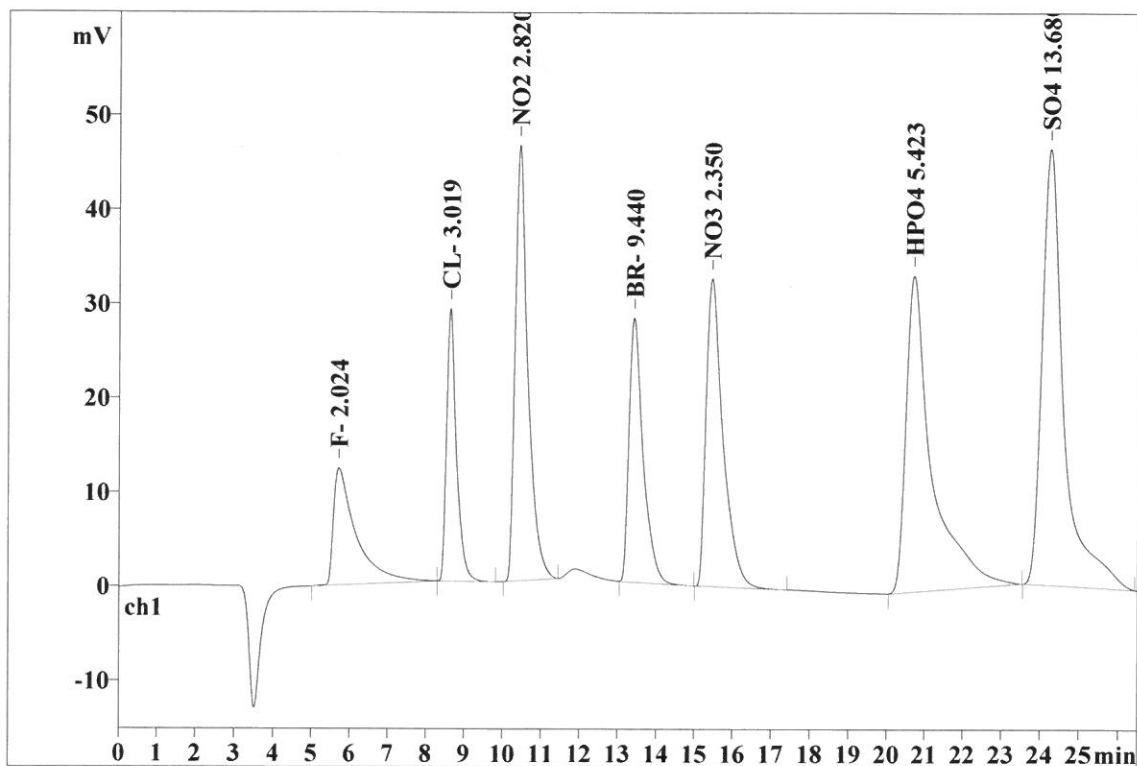

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.71	0.529	12.40	5.43	506.131	7.01
2	8.62	0.256	28.91	12.68	514.874	7.13
3	10.41	0.334	46.22	20.26	1069.174	14.81
4	13.41	0.371	28.04	12.29	715.364	9.91
5	15.44	0.457	32.67	14.32	1015.655	14.07
6	20.69	0.564	33.55	14.71	1585.375	21.96
7	24.24	0.522	46.29	20.29	1813.387	25.12
7	26.50	0.433	228.08	100.00	7219.959	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/9/2021 11:22:47 AM
Printed by: wet


Ident: CCB
Analysis from: 8/6/2021 3:44:27 PM
File: _2021-08-06_

Last save: 8/6/2021 4:10:58 PM

Method: AnionsIC2-080521.mtw
Run operator: wet
Analysis number: 27826

Last save: 8/6/2021 9:45:0

SAMPLE:
: AP/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

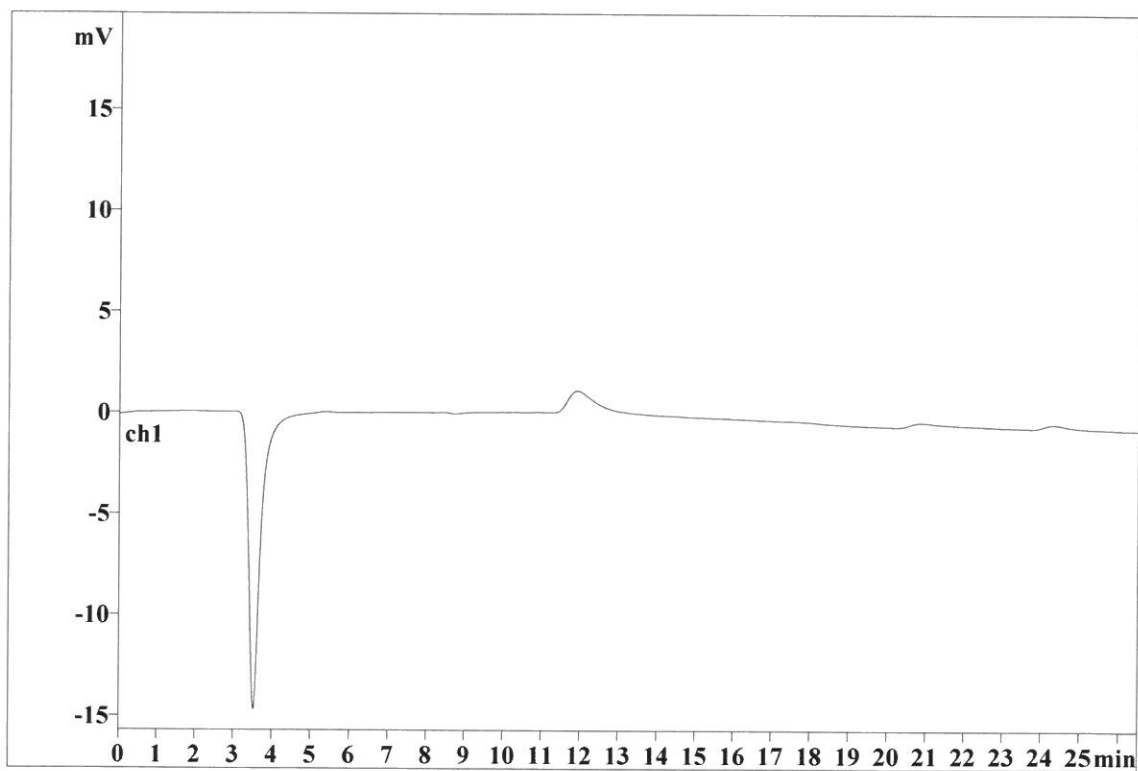

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD