

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : *AK* Instrument ID : Konelab

8/9/2021 13:36

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.115	0.0	0.072	
ICB1	1.227	0.0	0.001	
CCV1	247.897	0.0	0.186	
CCB1	1.174	0.0	0.001	
PB138272BL	1.373	0.0	0.001	
PB138272BS	97.137	0.0	0.073	
M3279-10	5.356	0.0	0.004	
M3279-10DUP	5.270	0.0	0.004	
M3279-10MS	48.049	0.0	0.036	
M3279-10MSD	48.559	0.0	0.037	
M3318-05	7.626	0.0	0.006	
CCV2	260.430	0.0	0.195	
CCB2	1.130	0.0	0.001	

N	13
Mean	63.180
SD	91.6721
CV%	145.10

Aquakem v. 7.2AQ1

Results from time period:

Mon Aug 09 13:26:18 2021

Mon Aug 09 13:31:38 2021

Sample Id	Sam/Ctr/c/	Test short r	Test type	Result	Result unit	Result date and tim	Stat
0.0PPBCN	A	Total CN	P	-1.2313	µg/l	8/9/2021 10:10:31	
5.0PPBCN	A	Total CN	P	5.6805	µg/l	8/9/2021 10:10:32	
10PPBCN	A	Total CN	P	9.8971	µg/l	8/9/2021 10:10:33	
50PPBCN	A	Total CN	P	46.9631	µg/l	8/9/2021 10:10:34	
100PPBCN	A	Total CN	P	101.1159	µg/l	8/9/2021 10:10:35	
250PPBCN	A	Total CN	P	254.9978	µg/l	8/9/2021 10:10:36	
500PPBCN	A	Total CN	P	497.5768	µg/l	8/9/2021 10:10:37	
ICV1	S	Total CN	P	96.1151	µg/l	8/9/2021 13:26:19	
ICB1	S	Total CN	P	1.2267	µg/l	8/9/2021 13:26:20	
CCV1	S	Total CN	P	247.8969	µg/l	8/9/2021 13:26:23	
CCB1	S	Total CN	P	1.1737	µg/l	8/9/2021 13:26:25	
PB138272BL	S	Total CN	P	1.3734	µg/l	8/9/2021 13:26:26	
PB138272BS	S	Total CN	P	97.137	µg/l	8/9/2021 13:26:27	
M3279-10	S	Total CN	P	5.3559	µg/l	8/9/2021 13:26:28	
M3279-10DUP	S	Total CN	P	5.2696	µg/l	8/9/2021 13:31:33	
M3279-10MS	S	Total CN	P	48.0489	µg/l	8/9/2021 13:31:34	
M3279-10MSD	S	Total CN	P	48.5586	µg/l	8/9/2021 13:31:35	
M3318-05	S	Total CN	P	7.6262	µg/l	8/9/2021 13:31:36	
CCV2	S	Total CN	P	260.4304	µg/l	8/9/2021 13:31:37	
CCB2	S	Total CN	P	1.1295	µg/l	8/9/2021 13:31:38	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

8/9/2021 10:15

Reviewed by : AL Instrument ID : Konelab


Test Total CN

Accepted 8/9/2021 10:15

Factor 1338
Bias 0

Coeff. of det. 0.999789

Errors

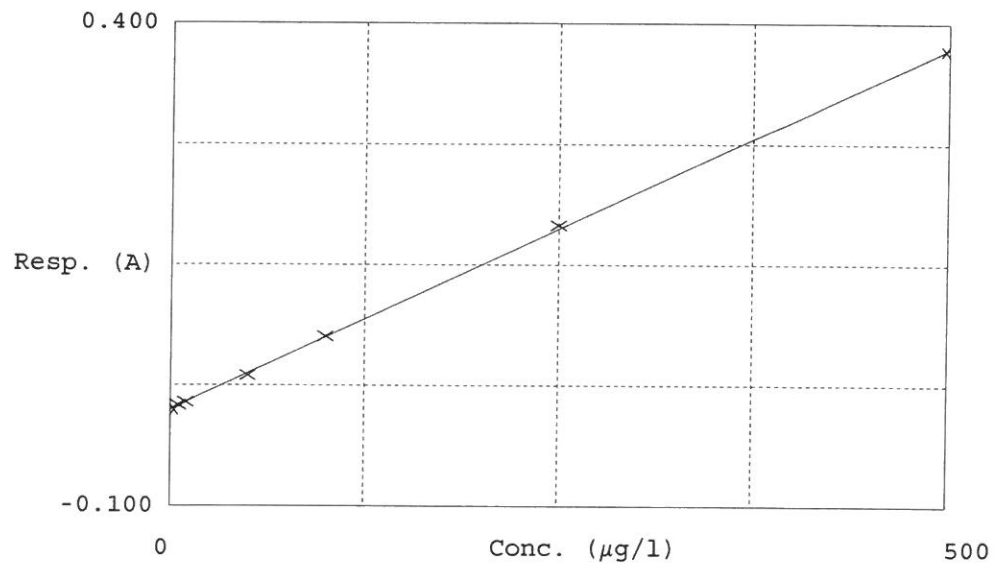

	Calibrator	Response	Calc. con.	Conc.	relative Errors
1	0.0PPBCN	-0.001	-1.2313	0.0000	
2	5.0PPBCN	0.005	5.6805	5.0000	
3	10PPBCN	0.008	9.8971	10.0000	
4	50PPBCN	0.035	46.9631	50.0000	
5	100PPBCN	0.076	101.1159	100.0000	
6	250PPBCN	0.191	254.9978	250.0000	
7	500PPBCN	0.372	497.5768	500.0000	

13.6
-1.0
-6.1
1.1
2.0
-0.5

AL
8/9/21