

LB 115843


7470A

INSTRUMENT ID: CV7

Linear

 μ Abs.:

40627

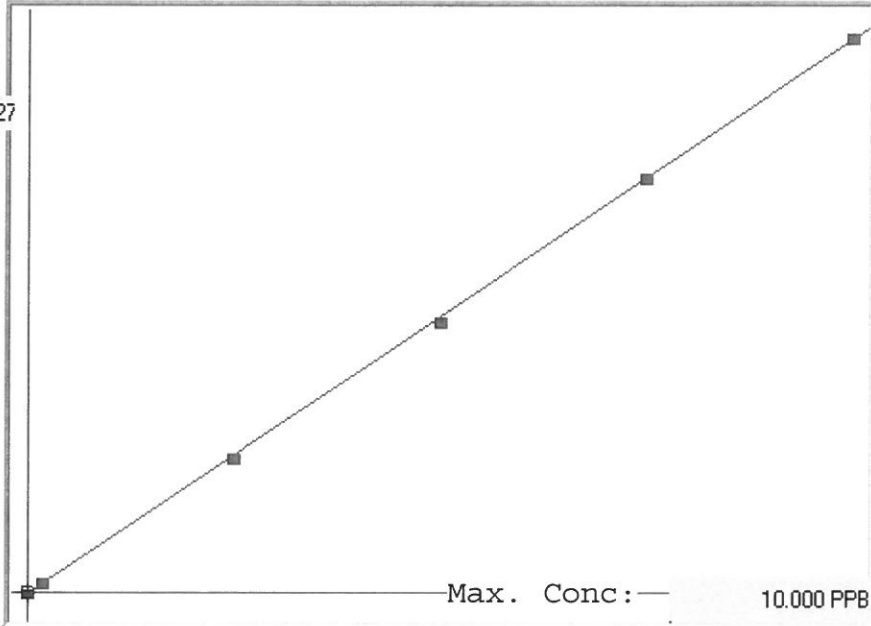

A= 0.0000e+000

B= 2.4610e-004

C= 3.2684e-002

Rho= 0.9999567

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.035	0.035	8	0.000	8					-
0.2	0.200	0.218	0.018	754	0.0 %	754					9
2.5	2.500	2.468	-0.032	9895	0.0 %	9895					-1
5.0	5.000	4.941	-0.059	19944	0.0 %	19944					-1
7.5	7.500	7.507	0.007	30373	0.0 %	30373					0
10.0	10.000	10.031	0.031	40627	0.0 %	40627					0

LB115843 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 13 Aug 2021 15:55:24

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	8	-	0.0000	7470A	PPB	13 Aug 2021 15:57:06	S	Std
0.2 - 1	50.2	754	-	0.2000	7470A	PPB	13 Aug 2021 15:59:24	S	Std
2.5 - 1	52.5	9895	-	2.5000	7470A	PPB	13 Aug 2021 16:01:43	S	Std
5.0 - 1	55	19944	-	5.0000	7470A	PPB	13 Aug 2021 16:04:00	S	Std
7.5 - 1	57.5	30373	-	7.5000	7470A	PPB	13 Aug 2021 16:06:17	S	Std
10.0 - 1	58	40627	-	10.0000	7470A	PPB	13 Aug 2021 16:13:38	S	Std
ICV53 - 1	ICV53	15129	3.7559	-	7470A	PPB	13 Aug 2021 16:16:14	U	SMPL
ICB53 - 1	ICB53	-45	0.0216	-	7470A	PPB	13 Aug 2021 16:18:28	U	SMPL
CCV49 - 1	CCV49	20144	4.9901	-	7470A	PPB	13 Aug 2021 16:20:48	U	SMPL
CCB49 - 1	CCB49	-56	0.0189	-	7470A	PPB	13 Aug 2021 16:23:03	U	SMPL
CRA - 1	CRA	733	0.2131	-	7470A	PPB	13 Aug 2021 16:25:17	U	SMPL
HighStd - 1	HighStd	40162	9.9165	-	7470A	PPB	13 Aug 2021 16:27:33	U	SMPL
ChkStd - 1	ChkStd	29013	7.1728	-	7470A	PPB	13 Aug 2021 16:29:48	U	SMPL
PB138395BL - 1	PBW	-100	0.0081	-	7470A	PPB	13 Aug 2021 16:32:05	U	SMPL
PB138395BS - 1	LCSW	16698	4.1420	-	7470A	PPB	13 Aug 2021 16:34:21	U	SMPL
M3371-02 - 1	JET-GROUT	-78	0.0135	-	7470A	PPB	13 Aug 2021 16:36:37	U	SMPL
M3371-02DUP - 1	JET-GROUTDUP	14	0.0361	-	7470A	PPB	13 Aug 2021 16:38:53	U	SMPL
M3371-02MS - 1	JET-GROUTMS	18499	4.5853	-	7470A	PPB	13 Aug 2021 16:41:10	U	SMPL
M3371-02MSD - 1	JET-GROUTMSD	18825	4.6655	-	7470A	PPB	13 Aug 2021 16:43:27	U	SMPL
M3388-02 - 1	VNJ-215	-47	0.0211	-	7470A	PPB	13 Aug 2021 16:45:42	U	SMPL
CCV50 - 1	CCV50	20570	5.0949	-	7470A	PPB	13 Aug 2021 16:47:57	U	SMPL
CCB50 - 1	CCB50	-48	0.0209	-	7470A	PPB	13 Aug 2021 16:50:13	U	SMPL
M3404-03 - 1	TP-1-6FT	0	0.0327	-	7470A	PPB	13 Aug 2021 16:52:28	U	SMPL
M3404-06 - 1	TP2-1-6FT	19	0.0374	-	7470A	PPB	13 Aug 2021 16:54:43	U	SMPL
M3404-09 - 1	TP3-1-6FT	12	0.0356	-	7470A	PPB	13 Aug 2021 16:56:58	U	SMPL
PB138395TB - 1	PB138357TB	27	0.0393	-	7470A	PPB	13 Aug 2021 16:59:13	U	SMPL
M3371-02LX5 - 1		33	0.0408	-	7470A	PPB	13 Aug 2021 17:01:29	U	SMPL
M3371-02A - 1		17200	4.2656	-	7470A	PPB	13 Aug 2021 17:03:45	U	SMPL
CCV51 - 1	CCV51	19865	4.9214	-	7470A	PPB	13 Aug 2021 17:06:01	U	SMPL
CCB51 - 1	CCB51	-152	-0.0047	-	7470A	PPB	13 Aug 2021 17:08:18	U	SMPL