


LB115269

7471B

INSTRUMENT ID: CV1

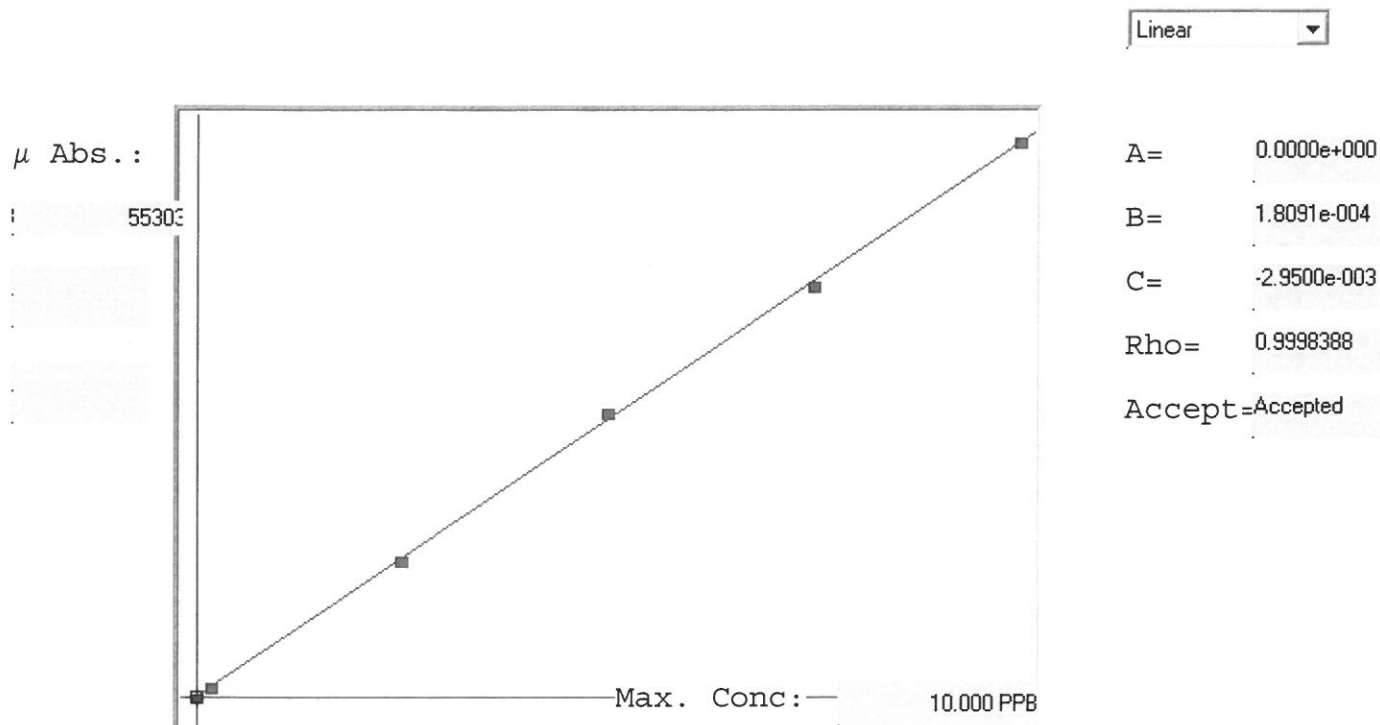

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	
0.0	0.000	0.002	0.002	30	0.000	30					101
0.2	0.200	0.186	-0.014	1043	0.0 %	1043					-7
2.5	2.500	2.456	-0.044	13595	0.0 %	13595					-2
5.0	5.000	5.134	0.134	28393	0.0 %	28393					3
7.5	7.500	7.420	-0.080	41032	0.0 %	41032					-1
10.0	10.000	10.002	0.002	55303	0.0 %	55303					0

Method: 7471B		Operator: Admin		Date of Analysis: 16 Aug 2021 09:53:07				Date	Type	Type
Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units				
0.0 - 1	50	30	-	0.0000	7471B	PPB		16 Aug 2021 10:04:03	S	Std
0.2 - 1	50.2	1043	-	0.2000	7471B	PPB		16 Aug 2021 10:06:21	S	Std
2.5 - 1	52.1	13595	-	2.5000	7471B	PPB		16 Aug 2021 10:08:39	S	Std
5.0 - 1	55	28393	-	5.0000	7471B	PPB		16 Aug 2021 10:10:58	S	Std
7.5 - 1	57.5	41032	-	7.5000	7471B	PPB		16 Aug 2021 10:13:14	S	Std
10.0 - 1	510	55303	-	10.0000	7471B	PPB		16 Aug 2021 10:15:31	S	Std
ICV54 - 1	ICV54	22464	4.0609	-	7471B	PPB		16 Aug 2021 10:27:35	U	SMPL
ICB54 - 1	ICB54	-34	-0.0091	-	7471B	PPB		16 Aug 2021 10:29:49	U	SMPL
CCV52 - 1	CCV52	28101	5.0807	-	7471B	PPB		16 Aug 2021 10:32:04	U	SMPL
CCB52 - 1	CCB52	-24	-0.0073	-	7471B	PPB		16 Aug 2021 10:34:19	U	SMPL
CRA - 1	CRA	1073	0.1912	-	7471B	PPB		16 Aug 2021 10:36:34	U	SMPL
HighStd - 1	HighStd	55215	9.9858	-	7471B	PPB		16 Aug 2021 10:38:49	U	SMPL
ChkStd - 1	ChkStd	38298	6.9254	-	7471B	PPB		16 Aug 2021 10:41:06	U	SMPL
PB138402BL - 1	PBS	-56	-0.0131	-	7471B	PPB		16 Aug 2021 10:43:26	U	SMPL
PB138402BS - 1	LCSS	22648	4.0942	-	7471B	PPB		16 Aug 2021 10:45:43	U	SMPL
M3407-02 - 1	25N	2831	0.5092	-	7471B	PPB		16 Aug 2021 10:47:59	U	SMPL
M3407-05 - 1	25S	2340	0.4204	-	7471B	PPB		16 Aug 2021 10:50:15	U	SMPL
M3407-08 - 1	26N	131630	23.8098	-	7471B	PPB		16 Aug 2021 10:52:32	U	SMPL
M3407-11 - 1	26S	13269	2.3975	-	7471B	PPB		16 Aug 2021 10:54:50	U	SMPL
M3407-14 - 1	27N	700	0.1237	-	7471B	PPB		16 Aug 2021 10:57:07	U	SMPL
CCV53 - 1	CCV53	27896	5.0436	-	7471B	PPB		16 Aug 2021 10:59:22	U	SMPL
CCB53 - 1	CCB53	-29	-0.0082	-	7471B	PPB		16 Aug 2021 11:01:38	U	SMPL
M3407-17 - 1	27S	11170	2.0178	-	7471B	PPB		16 Aug 2021 11:03:53	U	SMPL
M3407-20 - 1	28N	70966	12.8353	-	7471B	PPB		16 Aug 2021 11:06:08	U	SMPL
M3407-23 - 1	28S	204936	37.0714	-	7471B	PPB		16 Aug 2021 11:08:23	U	SMPL
M3407-26 - 1	29N	3621	0.6521	-	7471B	PPB		16 Aug 2021 11:10:41	U	SMPL
M3407-29 - 1	29S	197480	35.7225	-	7471B	PPB		16 Aug 2021 11:12:59	U	SMPL
M3408-02 - 1	31S	3924	0.7069	-	7471B	PPB		16 Aug 2021 11:15:15	U	SMPL
M3408-05 - 1	32S	775556	HIGH	-	7471B	PPB		16 Aug 2021 11:17:34	X	
M3408-08 - 1	33S	2815	0.5063	-	7471B	PPB		16 Aug 2021 11:19:22	U	SMPL
M3408-11 - 1	34S	32307	5.8416	-	7471B	PPB		16 Aug 2021 11:21:51	U	SMPL
M3408-14 - 1	34N	875	0.1553	-	7471B	PPB		16 Aug 2021 11:24:06	U	SMPL
CCV54 - 1	CCV54	27779	5.0225	-	7471					

LB115869 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 16 Aug 2021 09:53:07

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
CCB58 - 1	CCB58	-21	-0.0067	-7471B	PPB		16 Aug 2021 13:17:31	U	SMPL
M3401-01 - 1	BR-2-081221	3591	0.6467	-7471B	PPB		16 Aug 2021 13:19:48	U	SMPL
M3404-01 - 1	TP1-1-6FT	1803	0.3232	-7471B	PPB		16 Aug 2021 13:22:04	U	SMPL
M3404-04 - 1	TP2-1-6FT	4091	0.7371	-7471B	PPB		16 Aug 2021 13:24:20	U	SMPL
M3404-07 - 1	TP3-1-6FT	624	0.1099	-7471B	PPB		16 Aug 2021 13:26:38	U	SMPL
M3405-01 - 1	CL-01-081221	2480	0.4457	-7471B	PPB		16 Aug 2021 13:28:54	U	SMPL
M3405-01DUP - 1	CL-01-081221DUP	2254	0.4048	-7471B	PPB		16 Aug 2021 13:33:53	U	SMPL
M3405-01MS - 1	CL-01-081221MS	20428	3.6926	-7471B	PPB		16 Aug 2021 13:36:09	U	SMPL
M3405-01MSD - 1	CL-01-081221MSD	21706	3.9238	-7471B	PPB		16 Aug 2021 13:38:26	U	SMPL
CCV59 - 1	CCV59	28298	5.1164	-7471B	PPB		16 Aug 2021 13:44:24	U	SMPL
CCB59 - 1	CCB59	-68	-0.0153	-7471B	PPB		16 Aug 2021 13:46:40	U	SMPL
M3408-05DLX10 - 1		200529	36.2741	-7471B	PPB		16 Aug 2021 13:48:57	U	SMPL
M3408-14LX - 1		-433	-0.0813	-7471B	PPB		16 Aug 2021 13:51:13	U	SMPL
M3408-14A - 1		22726	4.1083	-7471B	PPB		16 Aug 2021 13:53:31	U	SMPL
M3394-01LX5 - 1		151	0.0244	-7471B	PPB		16 Aug 2021 13:55:47	U	SMPL
M3394-01A - 1		22254	4.0230	-7471B	PPB		16 Aug 2021 13:58:03	U	SMPL
M3405-01LX5 - 1		356	0.0615	-7471B	PPB		16 Aug 2021 14:00:19	U	SMPL
M3405-01A - 1		24880	4.4980	-7471B	PPB		16 Aug 2021 14:02:35	U	SMPL
CCV60 - 1	CCV60	28805	5.2081	-7471B	PPB		16 Aug 2021 14:15:10	U	SMPL
CCB60 - 1	CCB60	-52	-0.0124	-7471B	PPB		16 Aug 2021 14:17:26	U	SMPL
M3407-08DLX5 - 1		26581	4.8057	-7471B	PPB		16 Aug 2021 14:19:43	U	SMPL
M3407-20DLX2 - 1		35937	6.4983	-7471B	PPB		16 Aug 2021 14:21:59	U	SMPL
M3407-23DLX10 - 1		22999	4.1577	-7471B	PPB		16 Aug 2021 14:25:08	U	SMPL
M3707-29DLX10 - 1		21496	3.8858	-7471B	PPB		16 Aug 2021 14:27:23	U	SMPL
M3405-05DLX100 - 1		21436	3.8750	-7471B	PPB		16 Aug 2021 14:29:39	U	SMPL
M3397-03DLX2 - 1		29313	5.3000	-7471B	PPB		16 Aug 2021 14:31:56	U	SMPL
M3398-11DLX2 - 1		34970	6.3234	-7471B	PPB		16 Aug 2021 14:34:13	U	SMPL
CCV61 - 1	CCV61	28207	5.0999	-7471B	PPB		16 Aug 2021 14:36:29	U	SMPL
CCB61 - 1	CCB61	-47	-0.0115	-7471B	PPB		16 Aug 2021 14:38:46	U	SMPL