


LB115885

245.1

INSTRUMENT ID: CV1

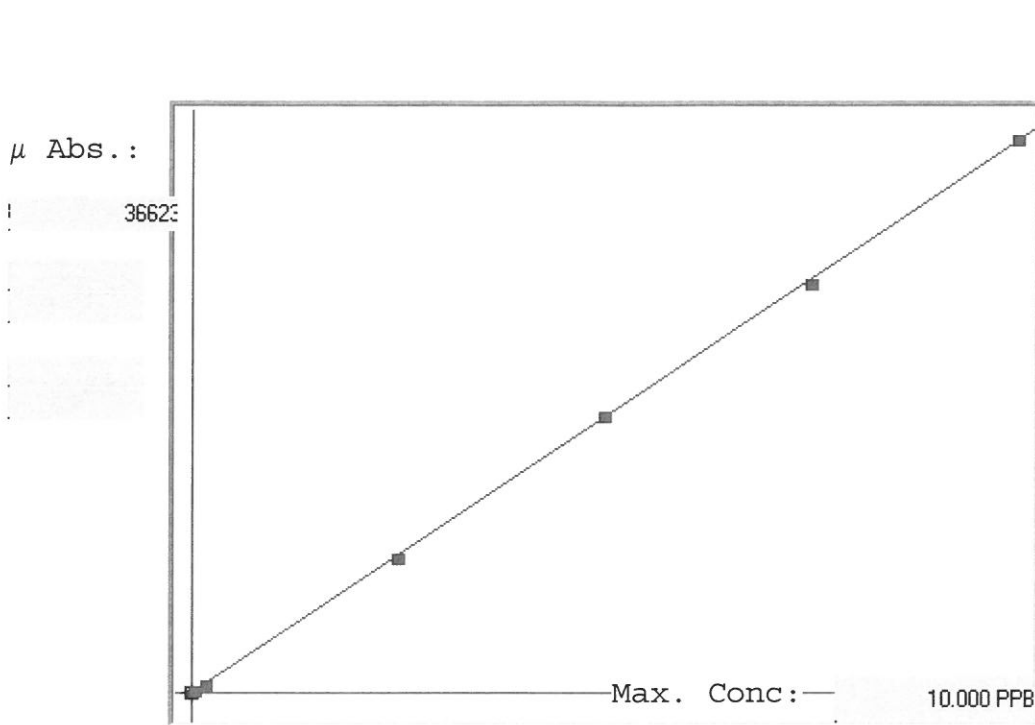

Linear

A= 0.0000e+000

B= 2.7380e-004

C= 2.1633e-002

Rho= 0.9999365

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%RSD
0.0	0.000	0.017	0.017	-16	0.000	-16					1
0.05	0.050	0.065	0.015	157	0.0 %	157	0				30
0.2	0.200	0.193	-0.007	625	0.0 %	625					4
2.5	2.500	2.470	-0.030	8943	0.0 %	8943					1
5.0	5.000	5.039	0.039	18326	0.0 %	18326					1
7.5	7.500	7.417	-0.083	27011	0.0 %	27011					1
10.0	10.000	10.049	0.049	36623	0.0 %	36623					0

LB115885

Method: 245.1

Operator: Admin

Date of Analysis: 16 Aug 2021 16:02:03

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-16	-	0.0000	245.1	PPB	16 Aug 2021 16:10:39	S	Std
0.05 - 1	50.05	157	-	0.0500	245.1	PPB	16 Aug 2021 16:12:55	S	Std
0.2 - 1	50.2	625	-	0.2000	245.1	PPB	16 Aug 2021 16:15:13	S	Std
2.5 - 1	52.5	8943	-	2.5000	245.1	PPB	16 Aug 2021 16:17:30	S	Std
5.0 - 1	55	18326	-	5.0000	245.1	PPB	16 Aug 2021 16:19:48	S	Std
7.5 - 1	57.5	27011	-	7.5000	245.1	PPB	16 Aug 2021 16:25:24	S	Std
10.0 - 1	510	36623	-	10.0000	245.1	PPB	16 Aug 2021 16:38:08	S	Std
ICV55 - 1	ICV55	15228	4.1910	-245.1		PPB	16 Aug 2021 16:42:36	U	SMPL
ICB55 - 1	ICB55	-86	-0.0019	-245.1		PPB	16 Aug 2021 16:44:51	U	SMPL
CCV62 - 1	CCV62	18725	5.1485	-245.1		PPB	16 Aug 2021 16:47:06	U	SMPL
CCB62 - 1	CCB62	-117	-0.0104	-245.1		PPB	16 Aug 2021 16:49:21	U	SMPL
CRA - 1	CRA	152	0.0632	-245.1		PPB	16 Aug 2021 16:51:36	U	SMPL
HighStd - 1	HighStd	35610	9.7715	-245.1		PPB	16 Aug 2021 16:53:51	U	SMPL
ChkStd - 1	ChkStd	25390	6.9733	-245.1		PPB	16 Aug 2021 16:56:06	U	SMPL
PB138475BL - 1	PBW	-93	-0.0038	-245.1		PPB	16 Aug 2021 16:58:22	U	SMPL
PB138475BS - 1	LCSW	14309	3.9394	-245.1		PPB	16 Aug 2021 17:00:38	U	SMPL
M3374-01 - 1	DEWATERING-DISCHARGE	752	0.2275	-245.1		PPB	16 Aug 2021 17:02:57	U	SMPL
M3374-01DUP - 1	DEWATERING-DISCHARGEDUP	809	0.2431	-245.1		PPB	16 Aug 2021 17:05:14	U	SMPL
M3374-01MS - 1	DEWATERING-DISCHARGEMS	17733	4.8769	-245.1		PPB	16 Aug 2021 17:07:31	U	SMPL
M3374-01MSD - 1	DEWATERING-DISCHARGEMSD	16038	4.4128	-245.1		PPB	16 Aug 2021 17:14:34	U	SMPL
CCV63 - 1	CCV63	18185	5.0006	-245.1		PPB	16 Aug 2021 17:16:49	U	SMPL
CCB63 - 1	CCB63	-111	-0.0088	-245.1		PPB	16 Aug 2021 17:19:04	U	SMPL
M3374-01LX5 - 1		100	0.0490	-245.1		PPB	16 Aug 2021 17:21:19	U	SMPL
M3374-01A - 1		15345	4.2230	-245.1		PPB	16 Aug 2021 17:23:34	U	SMPL
CCV64 - 1	CCV64	18509	5.0893	-245.1		PPB	16 Aug 2021 17:25:50	U	SMPL
CCB64 - 1	CCB64	-96	-0.0047	-245.1		PPB	16 Aug 2021 17:28:05	U	SMPL