


LB115891

7470A

INSTRUMENT ID: CV2

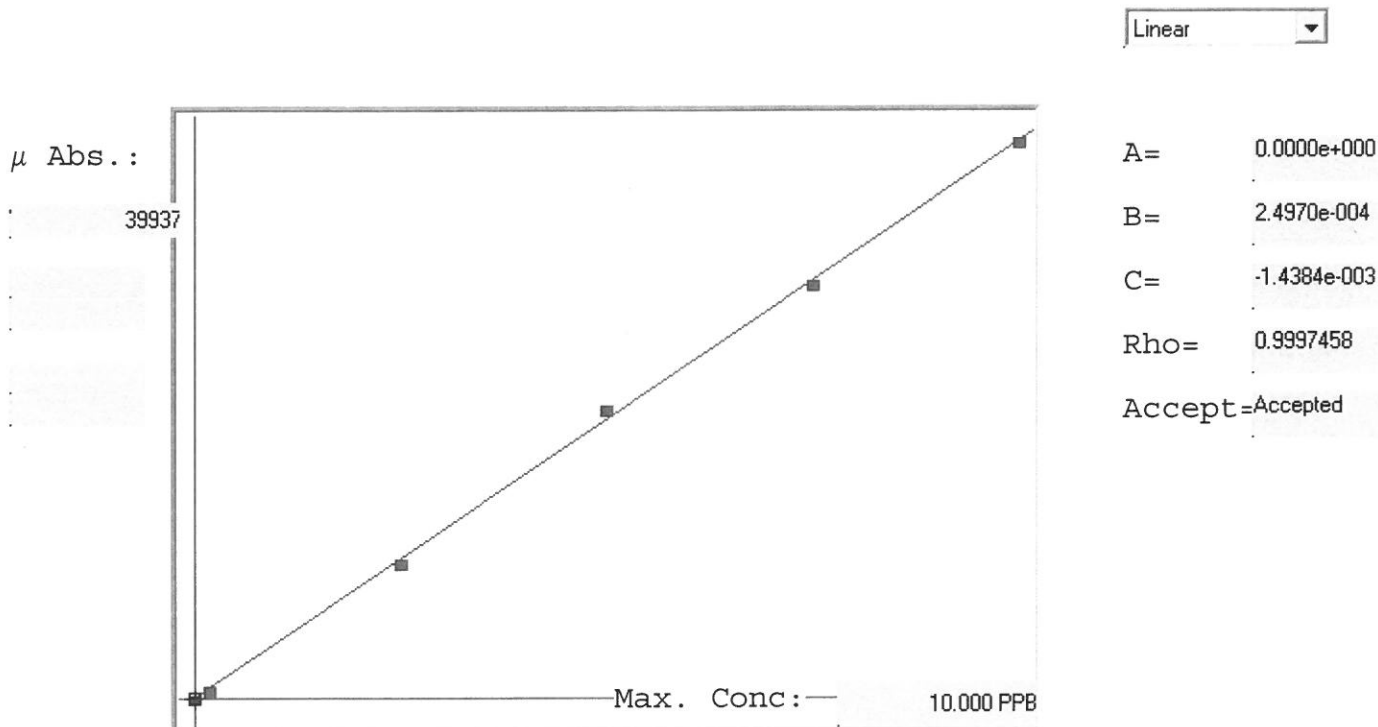

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.003	0.003	18	0.000	18				
0.2	0.200	0.167	-0.033	675	0.0 %	675				
2.5	2.500	2.447	-0.053	9807	0.0 %	9807				
5.0	5.000	5.180	0.180	20749	0.0 %	20749				
7.5	7.500	7.432	-0.068	29771	0.0 %	29771				
10.0	10.000	9.971	-0.029	39937	0.0 %	39937				

0/01)

1

-17

-2

4

-1

0

LB115891 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 17 Aug 2021 09:04:43					
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	18	-	0.0000	7470A	PPB	17 Aug 2021 09:07:54	S	Std
0.2 - 1	50.2	675	-	0.2000	7470A	PPB	17 Aug 2021 09:10:11	S	Std
2.5 - 1	52.5	9807	-	2.5000	7470A	PPB	17 Aug 2021 09:12:27	S	Std
5.0 - 1	55	20749	-	5.0000	7470A	PPB	17 Aug 2021 09:14:44	S	Std
7.5 - 1	57.5	29771	-	7.5000	7470A	PPB	17 Aug 2021 09:17:00	S	Std
10.0 - 1	510	39937	-	10.0000	7470A	PPB	17 Aug 2021 09:19:16	S	Std
ICV56 - 1	ICV56	16015	3.9975	-	7470A	PPB	17 Aug 2021 09:22:01	U	SMPL
ICB56 - 1	ICB56	-68	-0.0184	-	7470A	PPB	17 Aug 2021 09:24:16	U	SMPL
CCV65 - 1	CCV65	19459	4.8574	-	7470A	PPB	17 Aug 2021 09:26:31	U	SMPL
CCB65 - 1	CCB65	-73	-0.0197	-	7470A	PPB	17 Aug 2021 09:28:45	U	SMPL
CRA - 1	CRA	683	0.1691	-	7470A	PPB	17 Aug 2021 09:31:00	U	SMPL
HighStd - 1	HighStd	40645	10.1475	-	7470A	PPB	17 Aug 2021 09:33:14	U	SMPL
ChkStd - 1	ChkStd	28576	7.1339	-	7470A	PPB	17 Aug 2021 09:35:29	U	SMPL
PB138479BL - 1	PBW	-114	-0.0299	-	7470A	PPB	17 Aug 2021 09:37:45	U	SMPL
PB138479BS - 1	LCSW	16153	4.0319	-	7470A	PPB	17 Aug 2021 09:40:01	U	SMPL
M3407-03 - 1	25N	-72	-0.0194	-	7470A	PPB	17 Aug 2021 09:42:17	U	SMPL
M3407-03DUP - 1	25NDUP	3	-0.0007	-	7470A	PPB	17 Aug 2021 09:44:33	U	SMPL
M3407-03MS - 1	25NMS	14292	3.5672	-	7470A	PPB	17 Aug 2021 09:46:49	U	SMPL
M3407-03MSD - 1	25NMSD	15085	3.7652	-	7470A	PPB	17 Aug 2021 09:49:06	U	SMPL
M3407-06 - 1	25S	-28	-0.0084	-	7470A	PPB	17 Aug 2021 09:51:22	U	SMPL
CCV66 - 1	CCV66	19666	4.9091	-	7470A	PPB	17 Aug 2021 09:53:37	U	SMPL
CCB66 - 1	CCB66	-80	-0.0214	-	7470A	PPB	17 Aug 2021 09:55:51	U	SMPL
M3407-09 - 1	26N	21	0.0038	-	7470A	PPB	17 Aug 2021 09:58:06	U	SMPL
M3407-12 - 1	26S	13	0.0018	-	7470A	PPB	17 Aug 2021 10:00:22	U	SMPL
M3407-15 - 1	27N	26	0.0051	-	7470A	PPB	17 Aug 2021 10:02:38	U	SMPL
M3407-18 - 1	27S	17	0.0028	-	7470A	PPB	17 Aug 2021 10:04:54	U	SMPL
M3407-21 - 1	28N	15	0.0023	-	7470A	PPB	17 Aug 2021 10:07:09	U	SMPL
M3407-24 - 1	28S	24	0.0046	-	7470A	PPB	17 Aug 2021 10:09:25	U	SMPL
M3407-27 - 1	29N	3	-0.0007	-	7470A	PPB	17 Aug 2021 10:11:41	U	SMPL
M3407-30 - 1	29S	12	0.0016	-	7470A	PPB	17 Aug 2021 10:13:58	U	SMPL
M3408-03 - 1	31S	33	0.0068	-	7470A	PPB	17 Aug 2021 10:16:15	U	SMPL
M3408-06 - 1	32S	159	0.0383	-	7470A	PPB	17 Aug 2021 10:18:30	U	SMPL
CCV67 - 1	CCV67	19925	4.9738	-	7470A	PPB	17 Aug 2021 10:20:45	U	SMPL
CCB67 - 1	CCB67	-70	-0.0189	-	7470A	PPB	17 Aug 2021 10:23:01	U	SMPL
M3408-09 - 1	33S	-7	-0.0032	-	7470A	PPB	17 Aug 2021 10:25:16	U	SMPL
M3408-12 - 1	34S	336	0.0825	-	7470A	PPB	17 Aug 2021 10:27:32	U	SMPL
M3408-15 - 1	34N	13	0.0018	-	7470A	PPB	17 Aug 2021 10:29:47	U	SMPL
PB138480BL - 1	PBW	11	0.0013	-	7470A	PPB	17 Aug 2021 10:32:02	U	SMPL
PB138480BS - 1	LCSW	15412	3.8469	-	7470A	PPB	17 Aug 2021 10:34:18	U	SMPL
M3424-03 - 1	18N	-27	-0.0082	-	7470A	PPB	17 Aug 2021 10:36:34	U	SMPL
M3424-06 - 1	18S	21	0.0038	-	7470A	PPB	17 Aug 2021 10:38:51	U	SMPL
M3424-09 - 1	19N	1	-0.0012	-	7470A	PPB	17 Aug 2021 10:41:08	U	SMPL
M3424-12 - 1	19S	36	0.0076	-	7470A	PPB	17 Aug 2021 10:43:24	U	SMPL
M3424-15 - 1	20N	19	0.0033	-	7470A	PPB	17 Aug 2021 10:45:40	U	SMPL
CCV68 - 1	CCV68	19914	4.9710	-	7470A	PPB	17 Aug 2021 10:47:56	U	SMPL
CCB68 - 1	CCB68	-74	-0.0199	-	7470A	PPB	17 Aug 2021 10:50:13	U	SMPL
M3425-03 - 1	20S	-13	-0.0047	-	7470A	PPB	17 Aug 2021 10:52:29	U	SMPL
M3425-06 - 1	21N	22	0.0041	-	7470A	PPB	17 Aug 2021 10:54:45	U	SMPL
M3425-09 - 1	21S	105	0.0248	-	7470A	PPB	17 Aug 2021 10:57:01	U	SMPL
M3425-12 - 1	22N	245	0.0597	-	7470A	PPB	17 Aug 2021 11:00:17	U	SMPL
M3425-15 - 1	22S	43	0.0093	-	7470A	PPB	17 Aug 2021 11:02:33	U	SMPL
M3425-18 - 1	23N	17	0.0028	-	7470A	PPB	17 Aug 2021 11:04:49	U	SMPL
M3425-21 - 1	23S	41	0.0088	-	7470A	PPB	17 Aug 2021 11:07:05	U	SMPL
M3429-02 - 1	WC-1	53	0.0118	-	7470A	PPB	17 Aug 2021 11:09:21	U	SMPL
M3429-05 - 1	WC-2	33	0.0068	-	7470A	PPB	17 Aug 2021 11:11:37	U	SMPL
M3429-08 - 1	WC-3	23	0.0043	-	7470A	PPB	17 Aug 2021 11:13:53	U	SMPL
CCV69 - 1	CCV69	20148	5.0295	-	7470A	PPB	17 Aug 2021 11:16:09	U	SMPL
CCB69 - 1	CCB69	-73	-0.0197	-	7470A	PPB	17 Aug 2021 11:18:25	U	SMPL
M3429-08DUP - 1	WC-3DUP	11	0.0013	-	7470A	PPB	17 Aug 2021 11:20:41	U	SMPL
M3429-08MS - 1	WC-3MS	15820	3.9488	-	7470A	PPB	17 Aug 2021 11:22:57	U	SMPL
M3429-08MSD - 1	WC-3MSD	17427	4.3500	-	7470A	PPB	17 Aug 2021 11:25:13	U	SMPL
PB138481BL - 1	PBW	-59	-0.0162	-	7470A	PPB	17 Aug 2021 11:27:29	U	SMPL
PB138481BS - 1	LCSW	17228	4.3003	-	7470A	PPB	17 Aug 2021 11:29:45	U	SMPL
M3394-03 - 1	SWCS-01-0002	-51	-0.0142	-	7470A	PPB	17 Aug 2021 11:32:01	U	SMPL
M3394-06 - 1	SWCS-01-0205	-4	-0.0024	-	7470A	PPB	17 Aug 2021 11:34:17	U	SMPL
M3394-06DUP - 1	SWCS-01-0205DUP	1	-0.0012	-	7470A	PPB	17 Aug 2021 11:36:33	U	SMPL
M3394-06MS - 1	SWCS-01-0205MS	17407	4.3450	-	7470A	PPB	17 Aug 2021 11:38:49	U	SMPL
M3394-06MSD - 1	SWCS-01-0205MSD	17386	4.3398	-	7470A	PPB	17 Aug 2021 11:41:05	U	SMPL
CCV70 - 1	CCV70	20108	5.0195	-	7470A	PPB	17 Aug 2021 11:43:21	U	SMPL
CCB70 - 1	CCB70	-88	-0.0234	-	7470A	PPB	17 Aug 2021 11:45:37	U	SMPL
M3394-09 - 1	SWCS-01-0510	15	0.0023	-	7470A	PPB	17 Aug 2021 11:47:53	U	SMPL
M3394-12 - 1	SWCS-01-1015	-14	-0.0049	-	7470A	PPB	17 Aug 2021 11:50:09	U	SMPL
M3394-15 - 1	SWCS-02-0002	41	0.0088	-	7470A	PPB	17 Aug 2021 11:52:25	U	SMPL
M3394-18 - 1	SWCS-02-0205	112	0.0265	-	7470A	PPB	17 Aug 2021 11:54:41	U	SMPL
M3394-21 - 1	SWCS-02-0510	46	0.0100	-	7470A	PPB	17 Aug 2021 11:56:57	U	SMPL
M3397-02 - 1	SWCS-07-0002	0	-0.0014	-	7470A	PPB	17 Aug 2021 11:59:13	U	SMPL
M3397-05 - 1	SWCS-07-0205	-5	-0.0027	-	7470A	PPB	17 Aug 2021 12:01:29	U	SMPL
M3397-08 - 1	SWCS-07-0510	16	0.0026	-	7470A	PPB	17 Aug 2021 12:03:45	U	SMPL
M3397-11 - 1	SWCS-07-1015	4	-0.0004	-	7470A	PPB	17 Aug 2021 12:06:01	U	SMPL
M3397-14 - 1	SWCS-06-0002	122	0.0290	-	7470A	PPB	17 Aug 2021 12:08:17	U	SMPL
CCV71 - 1	CCV71	20193	5.0407	-	7470A	PPB	17 Aug 2021 12:10:33	U	SMPL

LB115891 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 17 Aug 2021 09:04:43

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
CCB71 - 1	CCB71	-56	-0.0154	-7470A	PPB		17 Aug 2021 12:17:48	U	SMPL
M3397-17 - 1	SWCS-06-0205	15	0.0023	-7470A	PPB		17 Aug 2021 12:20:04	U	SMPL
M3397-20 - 1	SWCS-06-0510	6	0.0001	-7470A	PPB		17 Aug 2021 12:22:19	U	SMPL
M3398-01 - 1	SWCS-06-1015	-3	-0.0022	-7470A	PPB		17 Aug 2021 12:24:36	U	SMPL
M3398-04 - 1	2021-08-10-FD-01	22	0.0041	-7470A	PPB		17 Aug 2021 12:26:52	U	SMPL
M3398-07 - 1	SWCS-05-0002	5	-0.0002	-7470A	PPB		17 Aug 2021 12:29:08	U	SMPL
M3398-10 - 1	SWCS-05-0205	40	0.0085	-7470A	PPB		17 Aug 2021 12:31:24	U	SMPL
M3398-13 - 1	SWCS-05-0510	73	0.0168	-7470A	PPB		17 Aug 2021 12:33:40	U	SMPL
PB138479TB - 1	PB138398TB	10	0.0011	-7470A	PPB		17 Aug 2021 12:35:57	U	SMPL
PB138480TB - 1	PB138429TB	2	-0.0009	-7470A	PPB		17 Aug 2021 12:38:14	U	SMPL
PB138481TB - 1	PB138431TB	-9	-0.0037	-7470A	PPB		17 Aug 2021 12:40:30	U	SMPL
CCV72 - 1	CCV72	19767	4.9343	-7470A	PPB		17 Aug 2021 12:42:46	U	SMPL
CCB72 - 1	CCB72	-61	-0.0167	-7470A	PPB		17 Aug 2021 12:45:02	U	SMPL
M3407-03LX5 - 1		-35	-0.0102	-7470A	PPB		17 Aug 2021 12:47:18	U	SMPL
M3407-03A - 1		16070	4.0112	-7470A	PPB		17 Aug 2021 12:49:34	U	SMPL
M3429-08LX5 - 1		-97	-0.0257	-7470A	PPB		17 Aug 2021 12:51:51	U	SMPL
M3429-08A - 1		16157	4.0329	-7470A	PPB		17 Aug 2021 12:54:07	U	SMPL
M3394-06LX5 - 1		-101	-0.0267	-7470A	PPB		17 Aug 2021 12:56:23	U	SMPL
M3394-06A - 1		17058	4.2579	-7470A	PPB		17 Aug 2021 12:58:38	U	SMPL
CCV73 - 1	CCV73	19155	4.7815	-7470A	PPB		17 Aug 2021 13:00:55	U	SMPL
CCB73 - 1	CCB73	-116	-0.0304	-7470A	PPB		17 Aug 2021 13:03:12	U	SMPL