


LB115914

7471B

INSTRUMENT ID: CV2

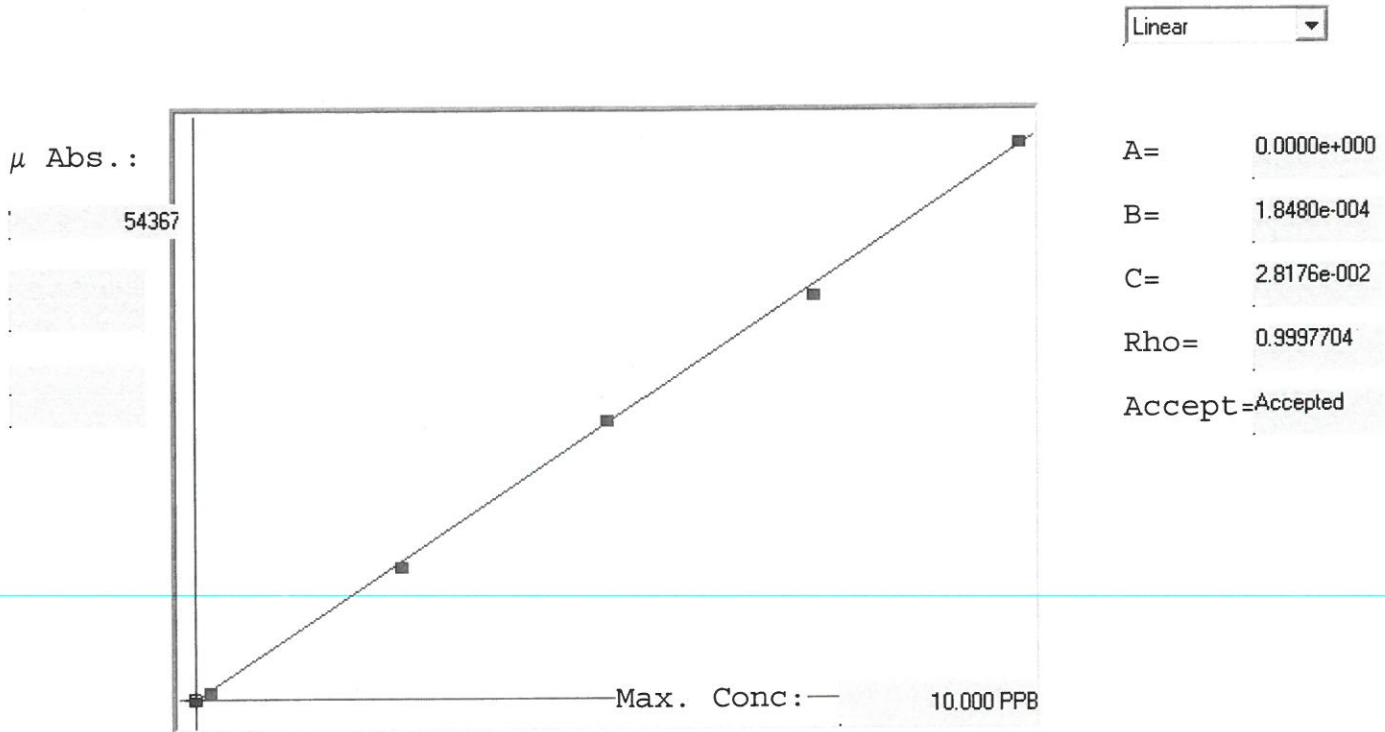

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.039	0.039	59	0.000	59					-
0.2	0.200	0.192	-0.008	889	0.0 %	889					-4
2.5	2.500	2.455	-0.045	13135	0.0 %	13135					-2
5.0	5.000	5.084	0.084	27358	0.0 %	27358					2
7.5	7.500	7.354	-0.146	39643	0.0 %	39643					-2
10.0	10.000	10.075	0.075	54367	0.0 %	54367					1

LB115914 INSTRUMENT ID : CV1

Method: 7471B		Operator: Admin		Date of Analysis: 18 Aug 2021 12:58:14					
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	59	-	0.00007471B	PPB		18 Aug 2021 12:59:43	S	Std
0.2 - 1	50.2	889	-	0.20007471B	PPB		18 Aug 2021 13:02:00	S	Std
2.5 - 1	52.5	13135	-	2.50007471B	PPB		18 Aug 2021 13:04:16	S	Std
5.0 - 1	55	27358	-	5.00007471B	PPB		18 Aug 2021 13:06:33	S	Std
7.5 - 1	57.5	39643	-	7.50007471B	PPB		18 Aug 2021 13:08:49	S	Std
10.0 - 1	510	54367	-	10.00007471B	PPB		18 Aug 2021 13:11:05	S	Std
ICV60 - 1	ICV60	21261	3.9571	-7471B	PPB		18 Aug 2021 13:13:51	U	SMPL
ICB60 - 1	ICB60	-64	0.0163	-7471B	PPB		18 Aug 2021 13:16:05	U	SMPL
CCV89 - 1	CCV89	26132	4.8573	-7471B	PPB		18 Aug 2021 13:18:20	U	SMPL
CCB89 - 1	CCB89	-59	0.0173	-7471B	PPB		18 Aug 2021 13:20:35	U	SMPL
CRA - 1	CRA	891	0.1928	-7471B	PPB		18 Aug 2021 13:22:51	U	SMPL
HighStd - 1	HighStd	54149	10.0348	-7471B	PPB		18 Aug 2021 13:25:05	U	SMPL
ChkStd - 1	ChkStd	37014	6.8683	-7471B	PPB		18 Aug 2021 13:27:21	U	SMPL
PB138545BL - 1	PBS	-106	0.0086	-7471B	PPB		18 Aug 2021 13:29:38	U	SMPL
PB138545BS - 1	LCSS	19326	3.5996	-7471B	PPB		18 Aug 2021 13:34:26	U	SMPL
M3435-01 - 1	SWCS-17-0003	23149	4.3060	-7471B	PPB		18 Aug 2021 13:36:42	U	SMPL
M3435-03 - 1	SWCS-17-0306	18546	3.4554	-7471B	PPB		18 Aug 2021 13:38:59	U	SMPL
M3435-05 - 1	SWCS-21-0002	3603	0.6940	-7471B	PPB		18 Aug 2021 13:41:15	U	SMPL
M3435-07 - 1	SWCS-21-0204	2596	0.5079	-7471B	PPB		18 Aug 2021 13:43:32	U	SMPL
M3435-09 - 1	SWCS-22-0306	340	0.0910	-7471B	PPB		18 Aug 2021 13:45:47	U	SMPL
CCV90 - 1	CCV90	26123	4.8556	-7471B	PPB		18 Aug 2021 13:48:02	U	SMPL
CCB90 - 1	CCB90	-70	0.0152	-7471B	PPB		18 Aug 2021 13:50:18	U	SMPL
M3435-11 - 1	2021-08-13-FD-04	3825	0.7350	-7471B	PPB		18 Aug 2021 13:52:34	U	SMPL
M3435-13 - 1	SWCS-24-0003	4763	0.9084	-7471B	PPB		18 Aug 2021 13:54:48	U	SMPL
M3435-15 - 1	SWCS-24-0306	1228	0.2551	-7471B	PPB		18 Aug 2021 13:57:04	U	SMPL
M3435-15DUP - 1	SWCS-24-0306DUP	1055	0.2231	-7471B	PPB		18 Aug 2021 13:59:20	U	SMPL
M3435-17 - 1	M3435-15MS	21167	3.9398	-7471B	PPB		18 Aug 2021 14:01:35	U	SMPL
M3435-18 - 1	M3435-15MSD	21004	3.9097	-7471B	PPB		18 Aug 2021 14:03:51	U	SMPL
M3435-21 - 1	SWCS-26-0003	515	0.1233	-7471B	PPB		18 Aug 2021 14:06:07	U	SMPL
M3435-23 - 1	SWCS-26-0306	100	0.0467	-7471B	PPB		18 Aug 2021 14:08:24	U	SMPL
M3435-25 - 1	SWCS-28-0003	632	0.1450	-7471B	PPB		18 Aug 2021 14:10:41	U	SMPL
M3435-27 - 1	SWCS-28-0306	90	0.0448	-7471B	PPB		18 Aug 2021 14:12:56	U	SMPL
CCV91 - 1	CCV91	26071	4.8460	-7471B	PPB		18 Aug 2021 14:15:11	U	SMPL
CCB91 - 1	CCB91	-67	0.0158	-7471B	PPB		18 Aug 2021 14:17:27	U	SMPL
M3435-29 - 1	SWCS-22-0003	733	0.1636	-7471B	PPB		18 Aug 2021 14:19:42	U	SMPL
M3438-01 - 1	RBR-2520561	4513	0.8622	-7471B	PPB		18 Aug 2021 14:21:58	U	SMPL
M3438-03 - 1	CHRT-26855	3339	0.6452	-7471B	PPB		18 Aug 2021 14:24:13	U	SMPL
M3439-01 - 1	HD-SOIL-COMP	937	0.2013	-7471B	PPB		18 Aug 2021 14:26:29	U	SMPL
M3441-01 - 1	WC-4	18906	3.5219	-7471B	PPB		18 Aug 2021 14:28:44	U	SMPL
M3441-04 - 1	WC-5	10723	2.0098	-7471B	PPB		18 Aug 2021 14:31:01	U	SMPL
M3451-01 - 1	TP-0-5-COMP	3381	0.6530	-7471B	PPB		18 Aug 2021 14:33:17	U	SMPL
M3451-04 - 1	TP-5-10-COMP	3179	0.6156	-7471B	PPB		18 Aug 2021 14:35:34	U	SMPL
PB138546BL - 1	PBS	60	0.0393	-7471B	PPB		18 Aug 2021 14:37:50	U	SMPL
PB138546BS - 1	LCSS	19570	3.6447	-7471B	PPB		18 Aug 2021 14:40:06	U	SMPL
CCV92 - 1	CCV92	25955	4.8246	-7471B	PPB		18 Aug 2021 14:42:21	U	SMPL
CCB92 - 1	CCB92	-64	0.0163	-7471B	PPB		18 Aug 2021 14:44:36	U	SMPL
M3419-01 - 1	SWCS-03-0002	4535	0.8662	-7471B	PPB		18 Aug 2021 14:46:53	U	SMPL
M3419-03 - 1	SWCS-03-0205	7453	1.4055	-7471B	PPB		18 Aug 2021 14:49:08	U	SMPL
M3419-05 - 1	SWCS-03-0510	268394	49.6266	-7471B	PPB		18 Aug 2021 14:51:24	U	SMPL
M3419-07 - 1	SWCS-03-1015	8725	1.6405	-7471B	PPB		18 Aug 2021 14:58:46	U	SMPL
M3419-07DUP - 1	SWCS-03-1015DUP	8519	1.6025	-7471B	PPB		18 Aug 2021 15:01:02	U	SMPL
M3419-09 - 1	M3419-07MS	30759	5.7123	-7471B	PPB		18 Aug 2021 15:03:18	U	SMPL
M3419-10 - 1	M3419-07MSD	31898	5.9228	-7471B	PPB		18 Aug 2021 15:08:17	U	SMPL
M3419-13 - 1	SWCS-08-0002	8496	1.5982	-7471B	PPB		18 Aug 2021 15:10:33	U	SMPL
M3419-15 - 1	SWCS-08-0205	169	0.0594	-7471B	PPB		18 Aug 2021 15:12:51	U	SMPL
M3419-17 - 1	SWCS-08-0510	234	0.0714	-7471B	PPB		18 Aug 2021 15:15:07	U	SMPL
CCV93 - 1	CCV93	27451	5.1010	-7471B	PPB		18 Aug 2021 15:17:23	U	SMPL
CCB93 - 1	CCB93	-64	0.0163	-7471B	PPB		18 Aug 2021 15:19:38	U	SMPL
M3419-19 - 1	SWCS-08-1015	233	0.0712	-7471B	PPB		18 Aug 2021 15:21:54	U	SMPL
M3419-21 - 1	SWCS-09-0002	8068	1.5191	-7471B	PPB		18 Aug 2021 15:24:10	U	SMPL
M3419-23 - 1	SWCS-09-0205	10420	1.9538	-7471B	PPB		18 Aug 2021 15:26:25	U	SMPL
M3426-01 - 1	SWCS-09-0510	543	0.1285	-7471B	PPB		18 Aug 2021 15:28:41	U	SMPL
M3426-03 - 1	2021-08-11-FD-02	840	0.1834	-7471B	PPB		18 Aug 2021 15:30:57	U	SMPL
M3426-05 - 1	SWCS-09-1015	341	0.0912	-7471B	PPB		18 Aug 2021 15:33:13	U	SMPL
M3426-07 - 1	SWCS-10-0002	7860	1.4807	-7471B	PPB		18 Aug 2021 15:35:30	U	SMPL
M3426-09 - 1	SWCS-10-0205	60582	11.2236	-7471B	PPB		18 Aug 2021 15:37:47	U	SMPL
M3426-11 - 1	SWCS-10-0510	445	0.1104	-7471B	PPB		18 Aug 2021 15:40:04	U	SMPL
M3426-13 - 1	M3426-11MS	22724	4.2275	-7471B	PPB		18 Aug 2021 15:43:53	U	SMPL
CCV94 - 1	CCV94	27253	5.0644	-7471B	PPB		18 Aug 2021 15:46:09	U	SMPL
CCB94 - 1	CCB94	-69	0.0154	-7471B	PPB		18 Aug 2021 15:48:25	U	SMPL
M3426-14 - 1	M3426-11MSD	20508	3.8180	-7471B	PPB		18 Aug 2021 15:50:41	U	SMPL
M3426-17 - 1	SWCS-10-1015	69	0.0409	-7471B	PPB		18 Aug 2021 15:52:57	U	SMPL
PB138547BL - 1	PBS	31	0.0339	-7471B	PPB		18 Aug 2021 15:55:13	U	SMPL
PB138547BS - 1	LCSS	21724	4.0427	-7471B	PPB		18 Aug 2021 16:00:24	U	SMPL
M3434-01 - 1	SWCS-11-0002	4550	0.8690	-7471B	PPB		18 Aug 2021 16:02:40	U	SMPL
M3434-01DUP - 1	SWCS-11-0002DUP	5215	0.9919	-7471B	PPB		18 Aug 2021 16:04:56	U	SMPL
M3434-01MS - 1	SWCS-11-0002MS	26245	4.8782	-7471B	PPB		18 Aug 2021 16:09:52	U	SMPL
M3434-01MSD - 1	SWCS-11-0002MSD	27189	5.0526	-7471B	PPB		18 Aug 2021 16:12:08	U	SMPL
M3434-03 - 1	SWCS-11-0205	6150	1.1647	-7471B	PPB		18 Aug 2021 16:14:25	U	SMPL
M3434-05 - 1	SWCS-11-0510	409	0.1038	-7471B	PPB		18 Aug 2021 16:16:41	U	SMPL
CCV95 - 1	CCV95	25984	4.8299	-7471B	PPB		18 Aug 2021 16:18:57	U	SMPL

LB115914 INSTRUMENT ID : CV1

Method: 7471B		Operator: Admin		Date of Analysis: 18 Aug 2021 12:58:14					
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
CCB95 - 1	CCB95	-72	0.0149	-7471B	PPB		18 Aug 2021 16:21:13	U	SMPL
M3434-07 - 1	SWCS-11-1015	145	0.0550	-7471B	PPB		18 Aug 2021 16:23:30	U	SMPL
M3434-09 - 1	SWCS-12-0002	4021	0.7712	-7471B	PPB		18 Aug 2021 16:25:46	U	SMPL
M3434-11 - 1	SWCS-12-0205	494	0.1195	-7471B	PPB		18 Aug 2021 16:28:02	U	SMPL
M3434-13 - 1	SWCS-12-0510	90	0.0448	-7471B	PPB		18 Aug 2021 16:30:18	U	SMPL
M3434-15 - 1	SWCS-12-1015	97	0.0461	-7471B	PPB		18 Aug 2021 16:32:34	U	SMPL
M3434-17 - 1	SWCS-13-0002	2640	0.5160	-7471B	PPB		18 Aug 2021 16:34:50	U	SMPL
M3434-19 - 1	SWCS-13-0205	1014	0.2156	-7471B	PPB		18 Aug 2021 16:37:06	U	SMPL
M3434-21 - 1	SWCS-13-0510	35462	6.5814	-7471B	PPB		18 Aug 2021 16:39:23	U	SMPL
M3434-23 - 1	SWCS-13-1015	-224	-0.0132	-7471B	PPB		18 Aug 2021 16:41:40	U	SMPL
M3434-25 - 1	SWCS-14-0002	5301	1.0078	-7471B	PPB		18 Aug 2021 16:43:58	U	SMPL
CCV96 - 1	CCV96	26161	4.8627	-7471B	PPB		18 Aug 2021 16:55:14	U	SMPL
CCB96 - 1	CCB96	-100	0.0097	-7471B	PPB		18 Aug 2021 16:57:30	U	SMPL
M3434-27 - 1	SWCS-14-0205	9303	1.7473	-7471B	PPB		18 Aug 2021 16:59:48	U	SMPL
M3434-29 - 1	SWCS-14-0515	5686	1.0789	-7471B	PPB		18 Aug 2021 17:02:04	U	SMPL
M3434-31 - 1	2021-08-12-FD-03	5690	1.0797	-7471B	PPB		18 Aug 2021 17:04:21	U	SMPL
M3434-33 - 1	SWCS-15-0002	9266	1.7405	-7471B	PPB		18 Aug 2021 17:06:37	U	SMPL
M3434-35 - 1	SWCS-15-0205	11991	2.2441	-7471B	PPB		18 Aug 2021 17:08:53	U	SMPL
M3434-37 - 1	SWCS-15-0510	1803	0.3614	-7471B	PPB		18 Aug 2021 17:11:09	U	SMPL
M3434-39 - 1	SWCS-15-1015	1015	0.2157	-7471B	PPB		18 Aug 2021 17:13:25	U	SMPL
CCV97 - 1	CCV97	26275	4.8837	-7471B	PPB		18 Aug 2021 17:15:42	U	SMPL
CCB97 - 1	CCB97	60	0.0393	-7471B	PPB		18 Aug 2021 17:17:59	U	SMPL
M3435-15LX5 - 1		218	0.0685	-7471B	PPB		18 Aug 2021 17:20:16	U	SMPL
M3435-15A - 1		21777	4.0525	-7471B	PPB		18 Aug 2021 17:22:33	U	SMPL
M3419-07LX5 - 1		1664	0.3357	-7471B	PPB		18 Aug 2021 17:24:49	U	SMPL
M3419-07A - 1		29157	5.4163	-7471B	PPB		18 Aug 2021 17:27:05	U	SMPL
M3434-01LX5 - 1		810	0.1779	-7471B	PPB		18 Aug 2021 17:29:21	U	SMPL
M3434-01A - 1		25796	4.7952	-7471B	PPB		18 Aug 2021 17:31:38	U	SMPL
M3419-05DLX10 - 1		28304	5.2587	-7471B	PPB		18 Aug 2021 17:33:55	U	SMPL
M3426-09DLX2 - 1		29218	5.4276	-7471B	PPB		18 Aug 2021 17:36:12	U	SMPL
CCV98 - 1	CCV98	26772	4.9756	-7471B	PPB		18 Aug 2021 17:38:28	U	SMPL
CCB98 - 1	CCB98	-116	0.0067	-7471B	PPB		18 Aug 2021 17:40:46	U	SMPL