

Clear table

Instrument ID: IC-2											Analyst :		AP		Method:		9056A	
ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time	Initial wt/ Final Vol	Analyst							
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-08-16_	8/16/21 10:41		AP/MA							
STD2	0.3910	0.6790	0.6640	2.2200	0.5610	0.8630	3.4380	2021-08-16_	8/16/21 11:10		AP/MA							
STD3	0.8120	1.1960	1.1960	4.0250	1.0110	1.9680	6.0560	2021-08-16_	8/16/21 11:40		AP/MA							
STD4	0.9680	1.4810	1.4890	4.9650	1.2390	2.5530	7.4120	2021-08-16_	8/16/21 12:09		AP/MA							
STD5	2.0210	2.9170	2.9320	9.7020	2.4140	5.1900	14.4290	2021-08-16_	8/16/21 12:38		AP/MA							
STD6	4.0620	5.9880	5.9780	19.9480	4.9860	10.0130	29.8970	2021-08-16_	8/16/21 13:07		AP/MA							
STD7	4.9450	7.5390	7.5410	25.1390	6.2890	12.4140	37.7680	2021-08-16_	8/16/21 13:37		AP/MA							
ICV	2.0750	3.0030	3.0150	10.0260	2.4820	5.3330	14.8330	2021-08-16_	8/16/21 14:22		AP/MA							
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-08-16_	8/16/21 14:51		AP/MA							
CCV	1.9550	2.8620	2.8420	9.6360	2.4030	4.6740	14.2780	2021-08-27_	8/27/21 8:45		AP/MA							
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-08-27_	8/27/21 9:28		AP/MA							
LB116044BL	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-08-27_	8/27/21 9:57	5.00g/100µ	AP/MA							
LB116044BS	1.9240	2.8900	2.8860	9.7070	2.4220	4.9190	14.3650	2021-08-27_	8/27/21 10:26	5.00g/100µ	AP/MA							
M3572-01	0.3950	0.1370	0.0000	0.0000	0.0000	0.0000	0.9630	2021-08-27_	8/27/21 13:50	5.05g/100µ	AP/MA							
M3572-02	0.3000	6.2090	0.0000	0.0000	0.0000	0.0000	1.0120	2021-08-27_	8/27/21 14:19	5.03g/100µ	AP/MA							
M3572-02MS	2.5560	9.3820	3.0400	10.2220	2.5400	6.2770	15.3640	2021-08-27_	8/27/21 15:17	5.02g/100µ	AP/MA							
M3572-02MSD	2.4820	9.3680	3.0470	10.2140	2.5380	6.4840	15.3220	2021-08-27_	8/27/21 15:47	5.04g/100µ	AP/MA							
CCV	2.0510	2.8830	2.8730	9.7270	2.4290	5.4850	14.4130	2021-08-27_	8/27/21 16:17		AP/MA							
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-08-27_	8/27/21 16:46		AP/MA							


AP 9/16/21

Clear table

Instrument ID: IC-2 Analyst: AP Method: 300 / 9056A											
ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time	Initial wt/ Final Vol	Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-08-16_	8/16/21 10:41		AP/MA
STD2	0.3910	0.6790	0.6640	2.2200	0.5610	0.8630	3.4380	2021-08-16_	8/16/21 11:10		AP/MA
STD3	0.8120	1.1960	1.1960	4.0250	1.0110	1.9680	6.0560	2021-08-16_	8/16/21 11:40		AP/MA
STD4	0.9680	1.4810	1.4890	4.9650	1.2390	2.5530	7.4120	2021-08-16_	8/16/21 12:09		AP/MA
STD5	2.0210	2.9170	2.9320	9.7020	2.4140	5.1900	14.4290	2021-08-16_	8/16/21 12:38		AP/MA
STD6	4.0620	5.9880	5.9780	19.9480	4.9860	10.0130	29.8970	2021-08-16_	8/16/21 13:07		AP/MA
STD7	4.9450	7.5390	7.5410	25.1390	6.2890	12.4140	37.7680	2021-08-16_	8/16/21 13:37		AP/MA
ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4				
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000				
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000				
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000				
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000				
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000				
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000				
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.5000				
ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4				
STD1											
STD2	-2.2500	13.1667	10.6667	11.0000	12.2000	-13.7000	14.6000				
STD3	1.5000	-0.3333	-0.3333	0.6250	1.1000	-1.6000	0.9333				
STD4	-3.2000	-1.2667	-0.7333	-0.7000	-0.8800	2.1200	-1.1733				
STD5	1.0500	-2.7667	-2.2667	-2.9800	-3.4400	3.8000	-3.8067				
STD6	1.5500	-0.2000	-0.3667	-0.2600	-0.2800	0.1300	-0.3433				
STD7	-1.1000	0.5200	0.5467	0.5560	0.6240	-0.6880	0.7147				

CALIBRATION OF COMPONENT F-

Method: AnionsIC2-081621.mtw
 Equation: $Q = 0.0787508 \cdot A + 1.63425$
 RSD: 2.096 %
 Correlation coefficient: 0.999761

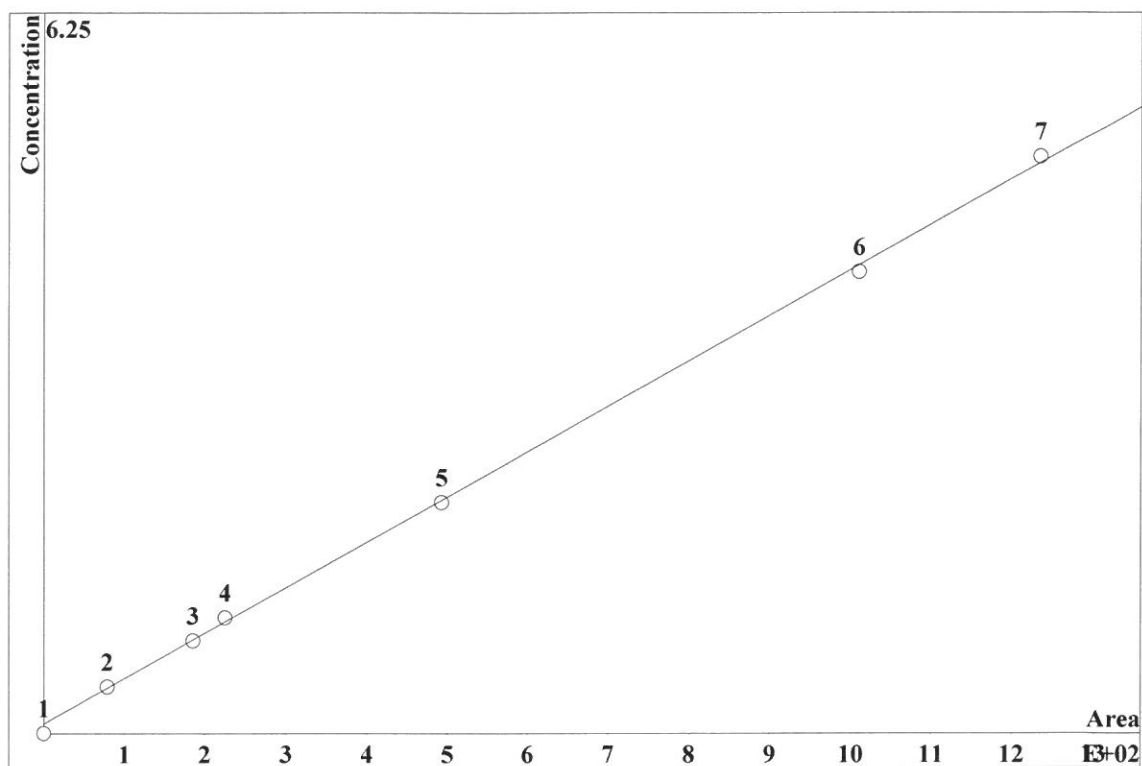

K3 = 0 K2 = 0 K1 = 0.0787508 K0 = 1.63425

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	2.039	78.64	0.4	20	5.75		
3	4.335	185.4	0.8	20	5.75		
4	5.553	225.1	1	20	5.75		
5	12.72	492.6	2	20	5.75		
6	25.53	1011	4	20	5.75		
7	32.96	1235	5	20	5.75		

CALIBRATION OF COMPONENT CL-

Method: AnionsIC2-081621.mtw
 Equation: $Q = 0.117224 \cdot A + 1.57793$
 RSD: 1.870 %
 Correlation coefficient: 0.999809

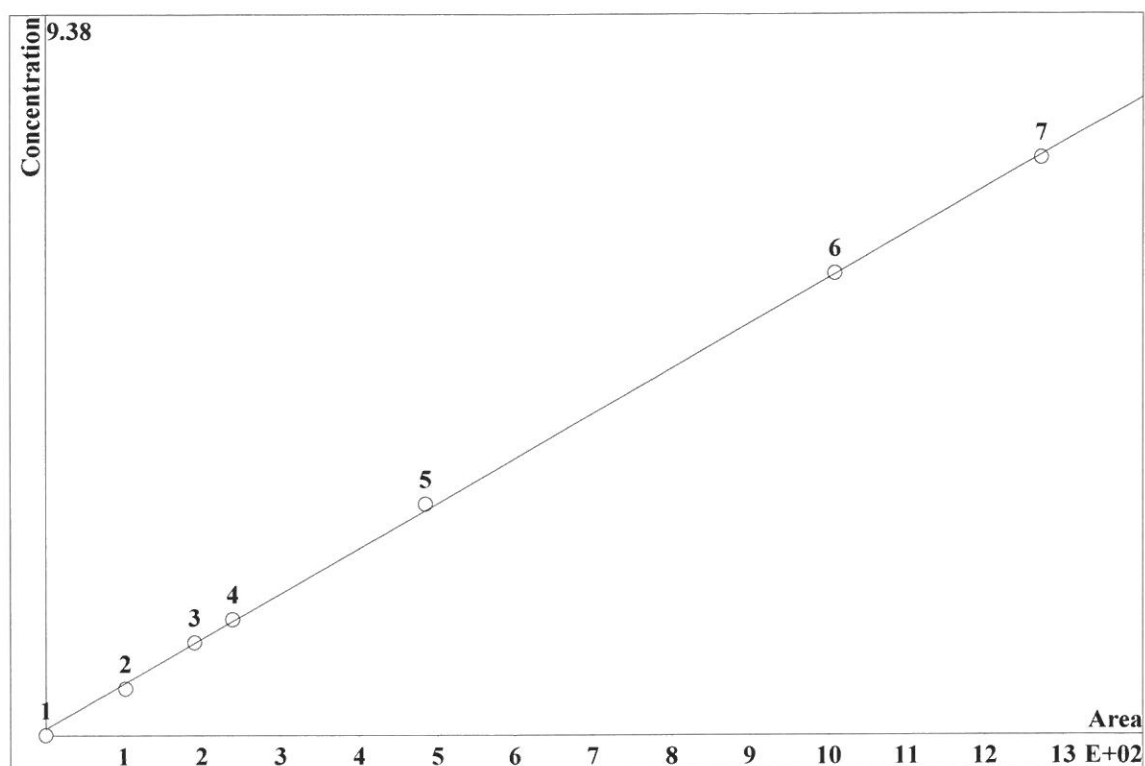

K3 = 0 K2 = 0 K1 = 0.117224 K0 = 1.57793

Base: Area

Ref.channel: chl

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	6.284	102.4	0.6	20	8.834		
3	12.17	190.6	1.2	20	8.834		
4	15.33	239.2	1.5	20	8.834		
5	31.62	484.2	3	20	8.834		
6	66.52	1008	6	20	8.834		
7	84.64	1273	7.5	20	8.834		

CALIBRATION OF COMPONENT NO2

Method: AnionsIC2-081621.mtw
 Equation: $Q = 0.0516801 \cdot A + 2.2891$
 RSD: 1.582 %
 Correlation coefficient: 0.999864

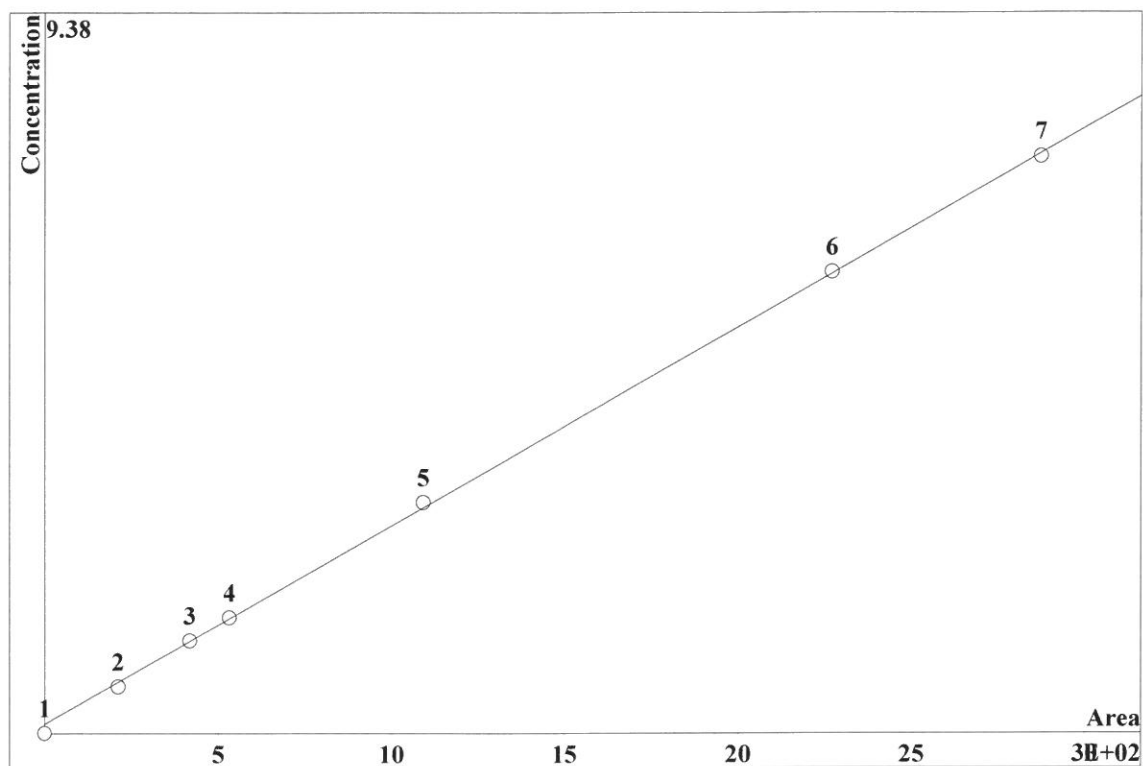


K3 = 0 K2 = 0 K1 = 0.0516801 K0 = 2.2891
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	10.82	212.6	0.6	20	10.64		
3	21.42	418.5	1.2	20	10.64		
4	27.07	531.9	1.5	20	10.64		
5	54.81	1091	3	20	10.64		
6	112.5	2269	6	20	10.64		
7	140.7	2874	7.5	20	10.64		

CALIBRATION OF COMPONENT BR-

Method: AnionsIC2-081621.mtw
 Equation: $Q = 0.260041 \cdot A + 9.18714$
 RSD: 1.824 %
 Correlation coefficient: 0.999819

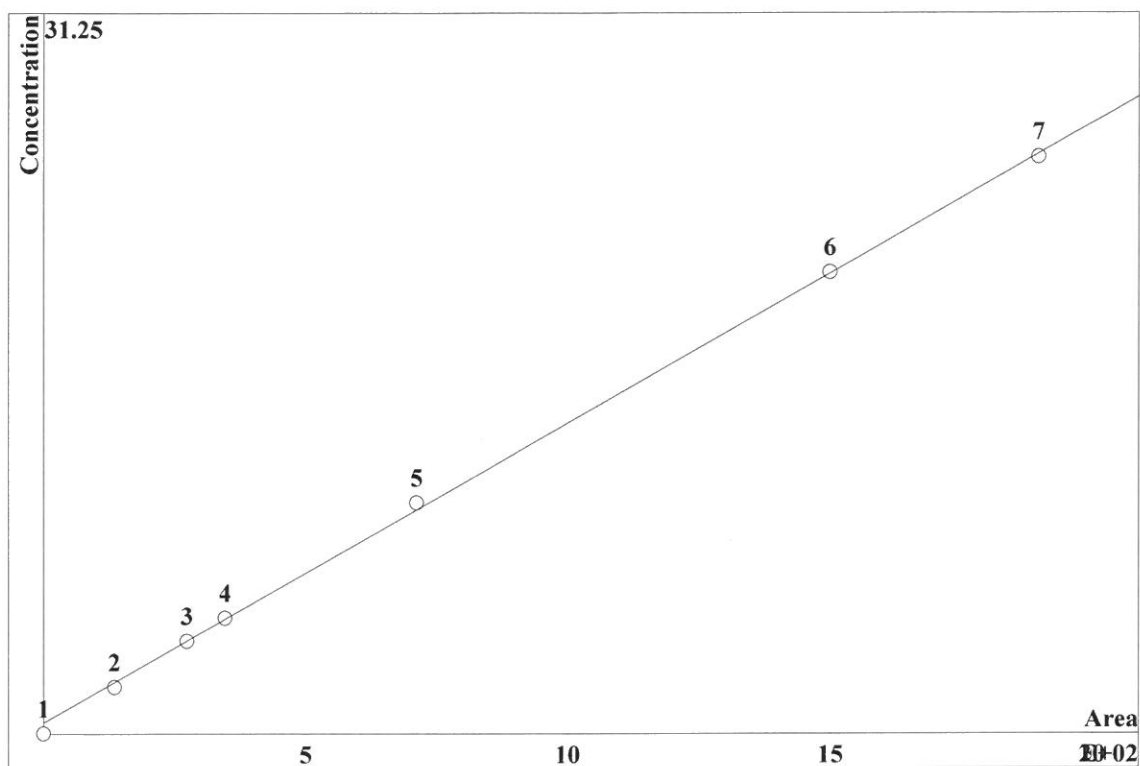


K3 = 0 K2 = 0 K1 = 0.260041 K0 = 9.18714
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	6.57	135.4	2	20			14
3	13.26	274.2	4	20			14
4	16.89	346.5	5	20			14
5	35.45	710.9	10	20			14
6	75.7	1499	20	20			14
7	96.72	1898	25	20			14

CALIBRATION OF COMPONENT NO3

Method: AnionsIC2-081621.mtw
 Equation: $Q = 0.0453375 \cdot A + 2.27775$
 RSD: 2.079 %
 Correlation coefficient: 0.999764

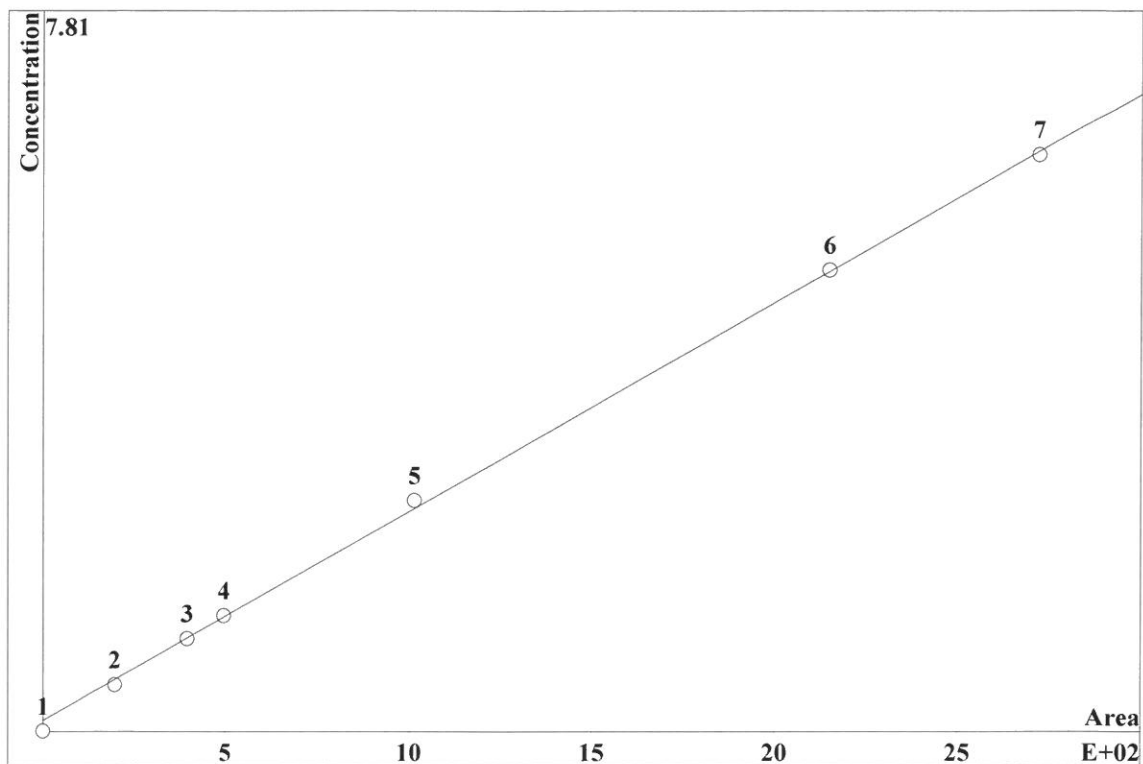

K3 = 0 K2 = 0 K1 = 0.0453375 K0 = 2.27775

Base: Area

Ref.channel: chl

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	7.929	197.1	0.5	20	16.28		
3	15.82	395.8	1	20	16.28		
4	20.05	496.5	1.25	20	16.28		
5	41.67	1015	2.5	20	16.28		
6	88.92	2149	5	20	16.28		
7	114	2724	6.25	20	16.28		

CALIBRATION OF COMPONENT HPO4

Method: AnionsIC2-081621.mtw
 Equation: $Q = 0.093688 \cdot A - 10.9491$
 RSD: 2.345 %
 Correlation coefficient: 0.999700



K3 = 0 K2 = 0 K1 = 0.093688 K0 = -10.9491

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	6.866	301	1	20	21.2		
3	12.55	536.9	2	20	21.2		
4	15.7	661.8	2.5	20	21.2		
5	30.88	1225	5	20	21.2		
6	58.85	2254	10	20	21.2		
7	73.57	2767	12.5	20	21.2		

CALIBRATION OF COMPONENT SO4

Method: AnionsIC2-081621.mtw
 Equation: $Q = 0.148108 \cdot A + 15.0956$
 RSD: 2.368 %
 Correlation coefficient: 0.999694

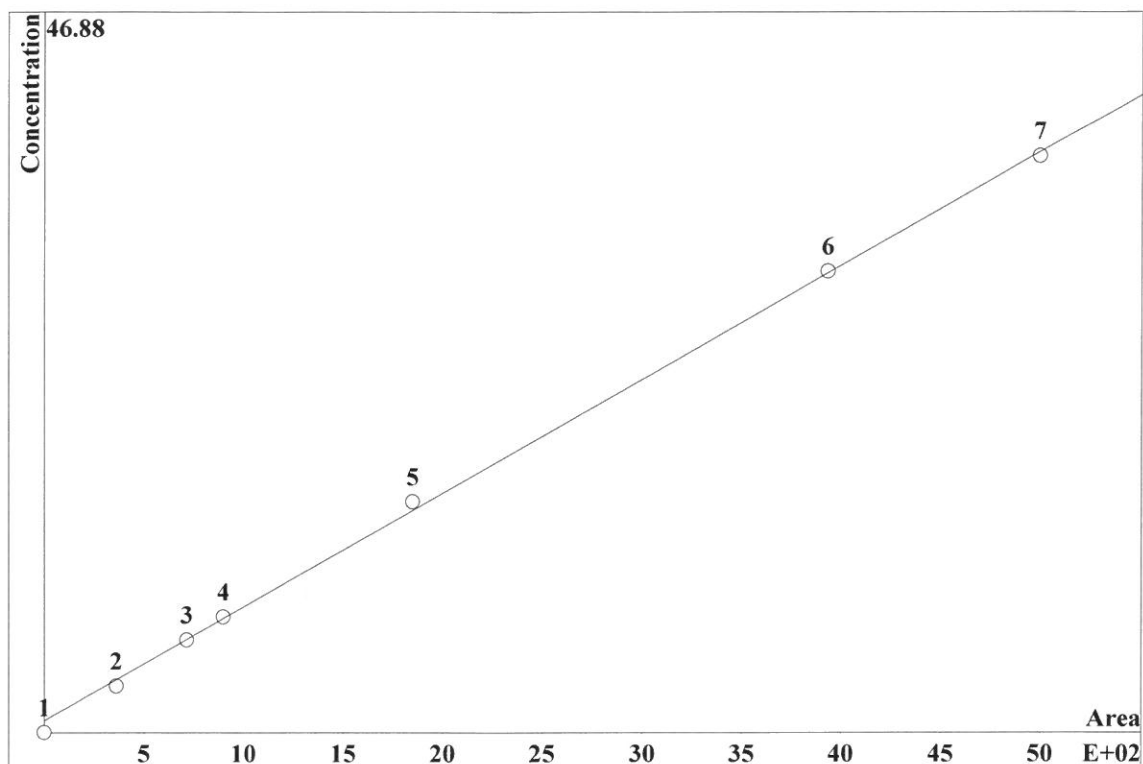

K3 = 0 K2 = 0 K1 = 0.148108 K0 = 15.0956

Base: Area

Ref.channel: ch1

ISTD:

Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	11.07	362.3	3	20	24.73		
3	21.95	715.9	6	20	24.73		
4	27.77	898.9	7.5	20	24.73		
5	57.89	1847	15	20	24.73		
6	124.1	3935	30	20	24.73		
7	158.5	4998	37.5	20	24.73		

Report date: 8/16/2021 2:41:00 PM
Printed by: wet


Ident: STD1
Analysis from: 8/16/2021 10:41:20 AM
File: _2021-08-16_

Last save: 8/16/2021 2:19:03 PM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 27902

Last save: 8/16/2021 1:34:

SAMPLE:
: AM/AP
Vial number: 2
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 8/16/2021 2:41:09 PM
Printed by: wet


Ident: STD2
Analysis from: 8/16/2021 11:10:29 AM
File: _2021-08-16_

Last save: 8/16/2021 2:19:03 PM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 27903

Last save: 8/16/2021 1:34:

SAMPLE:
: AM/AP
Vial number: 3
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

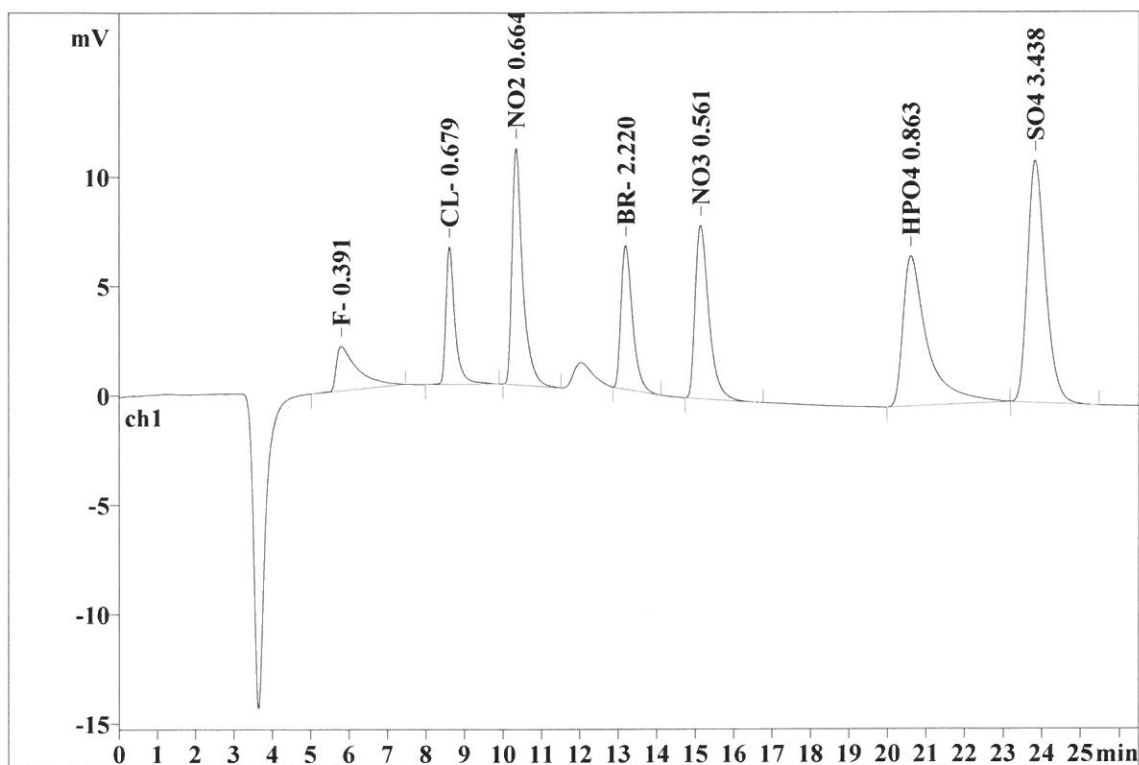

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.79	0.528	2.04	3.95	78.638	5.66
2	8.59	0.227	6.28	12.19	102.434	7.37
3	10.31	0.280	10.82	20.97	212.618	15.30
4	13.18	0.310	6.57	12.74	135.403	9.74
5	15.12	0.370	7.93	15.38	197.114	14.19
6	20.60	0.581	6.86	13.31	300.994	21.66
7	23.82	0.498	11.07	21.46	362.315	26.07
7	26.50	0.399	51.57	99.99	1389.516	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/16/2021 2:41:15 PM
Printed by: wet


Ident: STD3
Analysis from: 8/16/2021 11:40:29 AM
File: _2021-08-16_

Last save: 8/16/2021 2:19:03 PM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 27904

Last save: 8/16/2021 1:34:

SAMPLE:
: AM/AP
Vial number: 4
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

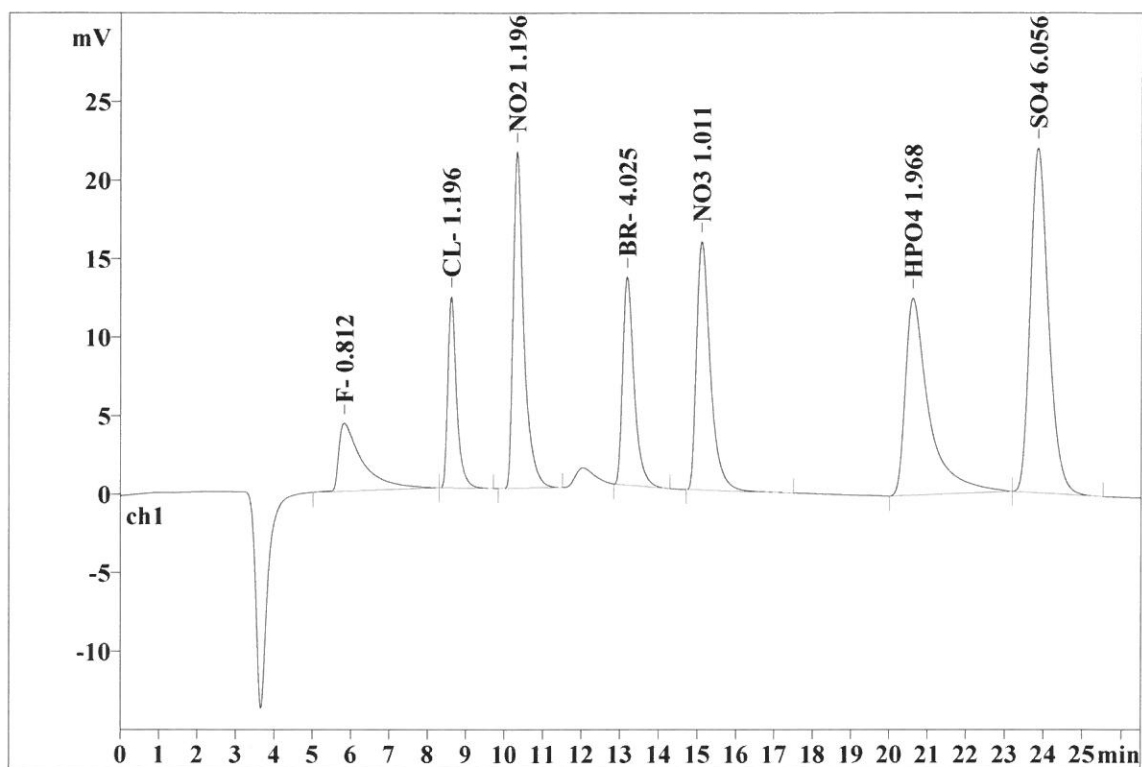

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.82	0.561	4.33	4.27	185.440	6.82
2	8.60	0.224	12.17	11.99	190.565	7.01
3	10.31	0.278	21.42	21.10	418.497	15.40
4	13.17	0.308	13.25	13.06	274.248	10.09
5	15.10	0.369	15.82	15.59	395.751	14.56
6	20.62	0.570	12.55	12.36	536.946	19.76
7	23.85	0.496	21.95	21.62	715.856	26.34
7	26.50	0.401	101.49	99.99	2717.303	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/16/2021 2:41:22 PM
Printed by: wet


Ident: STD4
Analysis from: 8/16/2021 12:09:38 PM
File: _2021-08-16_

Last save: 8/16/2021 2:19:03 PM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 27905

Last save: 8/16/2021 1:34:

SAMPLE:
: AM/AP
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.80	0.516	5.55	4.32	225.116	6.62
2	8.58	0.224	15.33	11.94	239.230	7.04
3	10.29	0.279	27.07	21.09	531.854	15.64
4	13.14	0.306	16.89	13.16	346.535	10.19
5	15.06	0.366	20.05	15.62	496.499	14.60
6	20.58	0.561	15.70	12.23	661.773	19.46
7	23.82	0.492	27.77	21.63	898.941	26.44
7	26.50	0.392	128.37	100.00	3399.949	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/16/2021 2:41:29 PM

Printed by: wet

Ident: STD5

Analysis from: 8/16/2021 12:38:45 PM

File: _2021-08-16_

Last save: 8/16/2021 2:19:03 PM

Method: AnionsIC2-081621.mtw

Last save: 8/16/2021 1:34:

Run operator: wet

Analysis number: 27906

SAMPLE:


: AM/AP

Vial number: 6

Volume: 20.0 µL

Dilution: 1.00

Amount: 1.0000



Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.80	0.504	12.72	4.80	492.593	7.18
2	8.58	0.220	31.62	11.93	484.207	7.05
3	10.28	0.284	54.81	20.68	1090.559	15.89
4	13.12	0.298	35.45	13.38	710.881	10.36
5	15.01	0.360	41.66	15.72	1014.578	14.78
6	20.56	0.532	30.87	11.65	1224.844	17.84
7	23.81	0.484	57.89	21.84	1846.544	26.90
7	26.50	0.383	265.03	100.00	6864.205	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/16/2021 2:41:36 PM
Printed by: wet


Ident: STD6
Analysis from: 8/16/2021 1:07:53 PM
File: _2021-08-16_

Last save: 8/16/2021 2:19:03 PM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 27907

Last save: 8/16/2021 1:34:

SAMPLE:
: AM/AP
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.84	0.534	25.53	4.62	1010.837	7.16
2	8.59	0.216	66.52	12.05	1008.142	7.14
3	10.27	0.286	112.49	20.37	2269.338	16.06
4	13.13	0.292	75.70	13.71	1498.913	10.61
5	14.97	0.354	88.92	16.10	2149.238	15.21
6	20.56	0.519	58.85	10.66	2254.471	15.96
7	23.83	0.480	124.14	22.48	3935.287	27.86
7	26.50	0.383	552.16	100.00	14126.227	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/16/2021 2:41:42 PM
Printed by: wet


Ident: STD7
Analysis from: 8/16/2021 1:37:00 PM
File: _2021-08-16_

Last save: 8/16/2021 2:19:03 PM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 27908

Last save: 8/16/2021 1:34:

SAMPLE:
: AM/AP
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

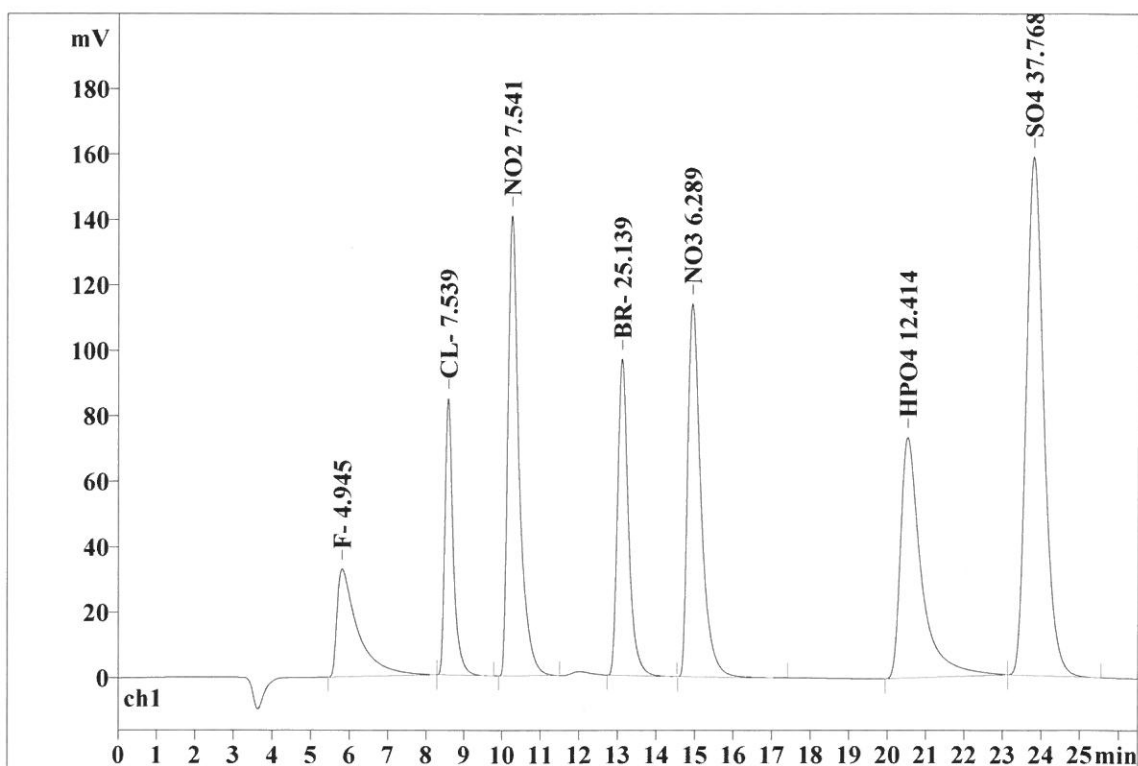

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.81	0.494	32.96	4.70	1235.210	6.95
2	8.57	0.214	84.64	12.07	1272.799	7.16
3	10.24	0.290	140.66	20.06	2873.891	16.17
4	13.11	0.290	96.71	13.79	1898.166	10.68
5	14.93	0.350	114.00	16.26	2724.121	15.33
6	20.52	0.512	73.57	10.49	2766.841	15.57
7	23.79	0.478	158.53	22.61	4998.116	28.13
7	26.50	0.375	701.07	100.00	17769.143	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/17/2021 4:31:35 PM
Printed by: wet


Ident: ICV
Analysis from: 8/16/2021 2:22:07 PM
File: _2021-08-16_

Last save: 8/16/2021 2:48:38 PM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 27909

Last save: 8/16/2021 2:03:

SAMPLE:
: AM/AP
Vial number: 9
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

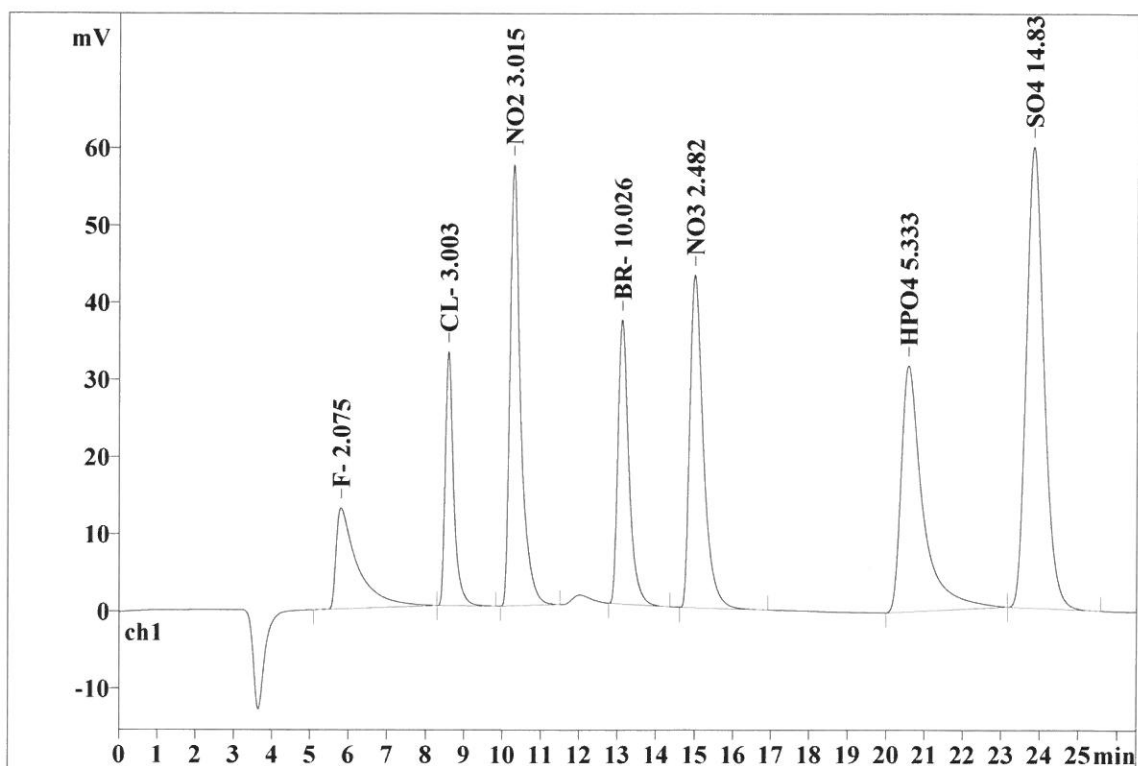

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.80	0.504	13.08	4.76	506.270	7.17
2	8.58	0.217	32.89	11.98	498.972	7.06
3	10.27	0.279	57.10	20.79	1122.328	15.89
4	13.11	0.296	36.82	13.41	735.757	10.41
5	14.99	0.358	43.10	15.69	1044.695	14.79
6	20.57	0.528	31.89	11.61	1255.288	17.77
7	23.82	0.482	59.76	21.76	1901.107	26.91
7	26.50	0.381	274.65	100.00	7064.419	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/17/2021 4:31:44 PM
Printed by: wet


Ident: ICB
Analysis from: 8/16/2021 2:51:40 PM
File: _2021-08-16_

Last save: 8/16/2021 3:22:33 PM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 27910

Last save: 8/16/2021 2:03:

SAMPLE:
: AP/MA
Vial number: 10
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

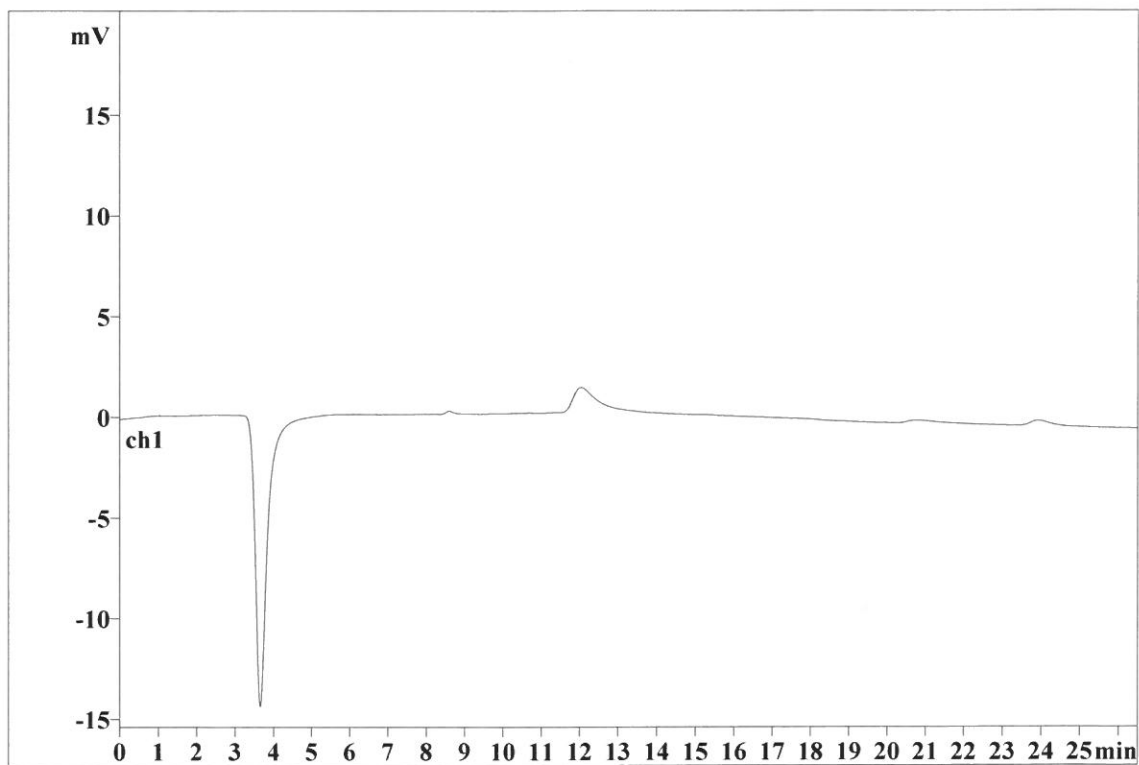

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 8/30/2021 8:58:17 AM
Printed by: wet


Ident: CCV
Analysis from: 8/27/2021 8:45:03 AM
File: _2021-08-27_

Last save: 8/27/2021 9:11:33 AM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 28004

Last save: 8/23/2021 10:23

SAMPLE:
: AP/MA
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.89	0.543	11.49	4.51	475.706	7.14
2	8.75	0.216	30.78	12.07	474.875	7.13
3	10.49	0.286	51.44	20.16	1055.482	15.84
4	13.45	0.299	34.48	13.52	705.747	10.59
5	15.42	0.361	40.70	15.95	1009.853	15.16
6	20.90	0.515	28.42	11.14	1114.714	16.73
7	24.54	0.473	57.79	22.65	1826.163	27.41
7	26.50	0.385	255.11	100.00	6662.539	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/30/2021 8:58:25 AM
Printed by: wet


Ident: CCB
Analysis from: 8/27/2021 9:28:16 AM
File: _2021-08-27_

Last save: 8/27/2021 9:54:46 AM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 28005

Last save: 8/23/2021 10:23

SAMPLE:
: AP/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 8/30/2021 8:58:33 AM
Printed by: wet


Ident: LB116044BL
Analysis from: 8/27/2021 9:57:22 AM
File: _2021-08-27_

Last save: 8/27/2021 2:48:21 PM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 28006

Last save: 8/23/2021 10:23

SAMPLE: 5.00g/100mL
: AP/MA
Vial number: 13
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 8/30/2021 8:58:39 AM
Printed by: wet


Ident: LB116044BS
Analysis from: 8/27/2021 10:26:27 AM
File: _2021-08-27_

Last save: 8/27/2021 2:48:21 PM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 28007

Last save: 8/23/2021 10:23

SAMPLE: 5.00g/100mL
: AP/MA
Vial number: 14
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.87	0.522	11.67	4.45	467.952	6.93
2	8.69	0.214	31.46	11.99	479.603	7.10
3	10.40	0.282	53.10	20.24	1072.398	15.88
4	13.29	0.292	35.69	13.60	711.278	10.53
5	15.21	0.352	42.28	16.11	1018.256	15.08
6	20.88	0.514	29.77	11.35	1166.935	17.28
7	24.51	0.473	58.38	22.25	1837.838	27.21
7	26.50	0.378	262.36	100.00	6754.260	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/30/2021 8:58:47 AM
Printed by: wet


Ident: M3572-01
Analysis from: 8/27/2021 1:50:12 PM
File: _2021-08-27_

Last save: 8/27/2021 2:16:42 PM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 28010

Last save: 8/23/2021 10:23

SAMPLE: 5.05g/100mL
: AM/AP
Vial number: 15
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.90	0.575	1.90	55.32	79.597	67.74
2	8.73	0.197	0.70	20.46	9.840	8.37
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	24.62	0.491	0.83	24.04	28.069	23.89
7	26.50	0.180	3.43	99.83	117.507	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/30/2021 8:58:56 AM
Printed by: wet


Ident: M3572-02
Analysis from: 8/27/2021 2:19:17 PM
File: _2021-08-27_

Last save: 8/27/2021 2:46:15 PM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 28011

Last save: 8/23/2021 10:23

SAMPLE: 5.03g/100mL
: AM/AP
Vial number: 16
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.87	0.569	1.37	1.85	55.373	4.87
2	8.70	0.203	71.43	96.73	1045.894	92.07
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	24.58	0.488	1.05	1.42	34.706	3.06
7	26.50	0.180	73.84	100.00	1135.972	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/30/2021 8:59:04 AM
Printed by: wet


Ident: M3572-02MS
Analysis from: 8/27/2021 3:17:34 PM
File: _2021-08-27_

Last save: 8/27/2021 4:15:10 PM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 28013

Last save: 8/23/2021 10:23

SAMPLE: 5.02g/100mL
: AM/AP
Vial number: 17
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.90	0.548	15.36	4.11	628.277	7.31
2	8.69	0.199	111.27	29.75	1587.234	18.46
3	10.39	0.270	57.83	15.46	1132.173	13.17
4	13.27	0.279	39.44	10.55	750.869	8.73
5	15.17	0.336	46.38	12.40	1070.317	12.45
6	20.94	0.492	38.17	10.21	1456.805	16.94
7	24.58	0.454	65.55	17.53	1972.781	22.94
7	26.50	0.368	374.00	100.00	8598.456	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/30/2021 8:59:12 AM
Printed by: wet


Ident: M3572-02MSD
Analysis from: 8/27/2021 3:47:52 PM
File: _2021-08-27_

Last save: 8/27/2021 4:15:10 PM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 28014

Last save: 8/23/2021 10:23

SAMPLE: 5.04g/100mL
: AM/AP
Vial number: 18
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.87	0.514	15.49	4.13	609.544	7.07
2	8.67	0.198	111.21	29.63	1584.842	18.39
3	10.37	0.268	57.98	15.45	1134.899	13.17
4	13.24	0.277	39.64	10.56	750.256	8.71
5	15.13	0.334	46.57	12.41	1069.335	12.41
6	20.93	0.491	39.39	10.49	1500.946	17.42
7	24.57	0.457	65.07	17.33	1967.038	22.83
7	26.50	0.363	375.35	100.00	8616.861	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/30/2021 8:59:19 AM
Printed by: wet


Ident: CCV
Analysis from: 8/27/2021 4:17:02 PM
File: _2021-08-27_

Last save: 8/27/2021 4:43:32 PM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 28015

Last save: 8/23/2021 10:23

SAMPLE:
: AP/MA
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.87	0.525	12.55	4.55	500.068	7.23
2	8.66	0.205	32.41	11.75	478.500	6.92
3	10.36	0.269	54.36	19.70	1067.550	15.44
4	13.21	0.278	37.42	13.56	712.773	10.31
5	15.10	0.334	44.37	16.08	1021.115	14.77
6	20.93	0.489	34.26	12.41	1287.779	18.63
7	24.57	0.459	60.57	21.95	1844.352	26.68
7	26.50	0.365	275.94	100.00	6912.137	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/30/2021 8:59:29 AM
Printed by: wet


Ident: CCB
Analysis from: 8/27/2021 4:46:07 PM
File: _2021-08-27_

Last save: 8/27/2021 5:12:37 PM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 28016

Last save: 8/23/2021 10:23

SAMPLE:
: AP/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD