


LB116086

7471B

INSTRUMENT ID: CV1

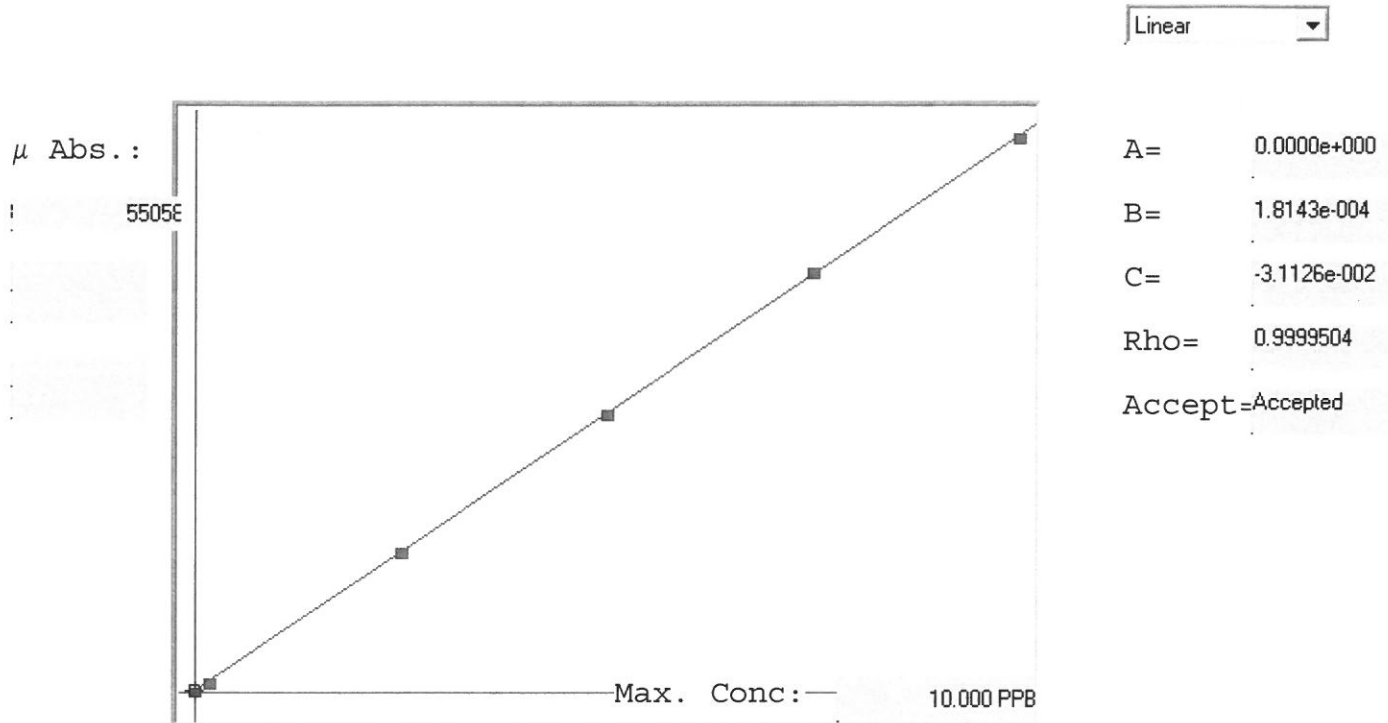

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.023	0.023	300	0.000	300					-
0.2	0.200	0.160	-0.040	1055	0.0 %	1055					-20
2.5	2.500	2.511	0.011	14011	0.0 %	14011					0
5.0	5.000	4.985	-0.015	27651	0.0 %	27651					0
7.5	7.500	7.562	0.062	41854	0.0 %	41854					0
10.0	10.000	9.958	-0.042	55058	0.0 %	55058					10

LB116086 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 31 Aug 2021 11:38:34

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	300	-	0.0000	7471B	PPB	31 Aug 2021 13:02:53	S	Std
0.2 - 1	52.2	1055	-	0.2000	7471B	PPB	31 Aug 2021 13:05:10	S	Std
2.5 - 1	52.5	14011	-	2.5000	7471B	PPB	31 Aug 2021 13:07:27	S	Std
5.0 - 1	55	27651	-	5.0000	7471B	PPB	31 Aug 2021 13:09:44	S	Std
7.5 - 1	57.5	41854	-	7.5000	7471B	PPB	31 Aug 2021 13:12:00	S	Std
10.0 - 1	51.0	55058	-	10.0000	7471B	PPB	31 Aug 2021 13:32:17	S	Std
ICV75 - 1	ICV75	21488	3.8674	-	7471B	PPB	31 Aug 2021 13:34:55	U	SMPL
ICB75 - 1	ICB75	-25	-0.0357	-	7471B	PPB	31 Aug 2021 13:37:09	U	SMPL
CCV66 - 1	CCV66	27652	4.9857	-	7471B	PPB	31 Aug 2021 13:39:24	U	SMPL
CCB66 - 1	CCB66	-40	-0.0384	-	7471B	PPB	31 Aug 2021 13:41:39	U	SMPL
CRA - 1	CRA	1205	0.1875	-	7471B	PPB	31 Aug 2021 13:46:51	U	SMPL
HighStd - 1	HighStd	56018	10.1320	-	7471B	PPB	31 Aug 2021 13:49:05	U	SMPL
ChkStd - 1	ChkStd	39466	7.1290	-	7471B	PPB	31 Aug 2021 13:51:21	U	SMPL
PB138846BL - 1	PBS	39	-0.0241	-	7471B	PPB	31 Aug 2021 13:56:14	U	SMPL
PB138846BS - 1	LCSS	22950	4.1326	-	7471B	PPB	31 Aug 2021 13:58:29	U	SMPL
M3564-02 - 1	VNJ-237	1522	0.2450	-	7471B	PPB	31 Aug 2021 14:00:46	U	SMPL
M3569-01 - 1	S-1	4324	0.7534	-	7471B	PPB	31 Aug 2021 14:03:02	U	SMPL
M3569-02 - 1	S-2	7081	1.2536	-	7471B	PPB	31 Aug 2021 14:05:19	U	SMPL
M3571-01 - 1	BL-1	5189	0.9103	-	7471B	PPB	31 Aug 2021 14:07:36	U	SMPL
M3574-01 - 1	TPR-12-13-COMP	745	0.1040	-	7471B	PPB	31 Aug 2021 14:09:51	U	SMPL
CCV67 - 1	CCV67	27856	5.0227	-	7471B	PPB	31 Aug 2021 14:12:06	U	SMPL
CCB67 - 1	CCB67	-21	-0.0349	-	7471B	PPB	31 Aug 2021 14:14:21	U	SMPL
M3577-01 - 1	191-0827-B1-0-2	3562	0.6151	-	7471B	PPB	31 Aug 2021 14:16:36	U	SMPL
M3577-02 - 1	191-0827-B1-DP	3962	0.6877	-	7471B	PPB	31 Aug 2021 14:18:51	U	SMPL
M3584-01 - 1	OF-2-20210827	28009	5.0504	-	7471B	PPB	31 Aug 2021 14:21:07	U	SMPL
M3584-02 - 1	OF-3-20210827	18129	3.2579	-	7471B	PPB	31 Aug 2021 14:23:23	U	SMPL
M3584-02DUP - 1	OF-3-20210827DUP	18297	3.2884	-	7471B	PPB	31 Aug 2021 14:25:38	U	SMPL
M3584-03 - 1	M3584-02MS	37505	6.7733	-	7471B	PPB	31 Aug 2021 14:27:54	U	SMPL
M3584-04 - 1	M3584-02MSD	37426	6.7589	-	7471B	PPB	31 Aug 2021 14:30:10	U	SMPL
M3584-05 - 1	OF-4-20210827	10043	1.7909	-	7471B	PPB	31 Aug 2021 14:32:28	U	SMPL
M3584-06 - 1	DUP03-20210827	9098	1.6195	-	7471B	PPB	31 Aug 2021 14:34:46	U	SMPL
M3593-01 - 1	ETGI-280	7448	1.3201	-	7471B	PPB	31 Aug 2021 14:37:02	U	SMPL
CCV68 - 1	CCV68	27682	4.9911	-	7471B	PPB	31 Aug 2021 14:39:17	U	SMPL
CCB68 - 1	CCB68	-29	-0.0364	-	7471B	PPB	31 Aug 2021 14:41:33	U	SMPL
M3597-01 - 1	RO-124030	12480	2.2331	-	7471B	PPB	31 Aug 2021 14:43:48	U	SMPL
M3597-03 - 1	RO-PSC124042	6432	1.1358	-	7471B	PPB	31 Aug 2021 14:46:03	U	SMPL
M3602-09 - 1	TP-1COMP	4165	0.7245	-	7471B	PPB	31 Aug 2021 14:48:19	U	SMPL
M3584-02LX5 - 1		3717	0.6432	-	7471B	PPB	31 Aug 2021 14:50:34	U	SMPL
M3584-02A - 1		40192	7.2607	-	7471B	PPB	31 Aug 2021 14:52:50	U	SMPL
CCV69 - 1	CCV69	27590	4.9744	-	7471B	PPB	31 Aug 2021 14:55:06	U	SMPL
CCB69 - 1	CCB69	-38	-0.0380	-	7471B	PPB	31 Aug 2021 14:57:23	U	SMPL