

Clear table

Instrument ID: IC-2										Analyst : AP		Method: 300.0	
ident	concentra tion F-	concentratio n CL-	concentratio on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time	Initial wt/ Final Vol	Analyst		
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-08-16_	8/16/21 10:41		AP/MA		
STD2	0.3910	0.6790	0.6640	2.2200	0.5610	0.8630	3.4380	2021-08-16_	8/16/21 11:10		AP/MA		
STD3	0.8120	1.1960	1.1960	4.0250	1.0110	1.9680	6.0560	2021-08-16_	8/16/21 11:40		AP/MA		
STD4	0.9680	1.4810	1.4890	4.9650	1.2390	2.5530	7.4120	2021-08-16_	8/16/21 12:09		AP/MA		
STD5	2.0210	2.9170	2.9320	9.7020	2.4140	5.1900	14.4290	2021-08-16_	8/16/21 12:38		AP/MA		
STD6	4.0620	5.9880	5.9780	19.9480	4.9860	10.0130	29.8970	2021-08-16_	8/16/21 13:07		AP/MA		
STD7	4.9450	7.5390	7.5410	25.1390	6.2890	12.4140	37.7680	2021-08-16_	8/16/21 13:37		AP/MA		
ICV	2.0750	3.0030	3.0150	10.0260	2.4820	5.3330	14.8330	2021-08-16_	8/16/21 14:22		AP/MA		
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-08-16_	8/16/21 14:51		AP/MA		
CCV	2.1310	2.9130	2.9040	9.7500	2.4490	4.8150	14.5200	2021-08-31_	8/31/21 8:49		AP/MA		
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-08-31_	8/31/21 9:19		AP/MA		
LB116093BLW	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-08-31_	8/31/21 9:47		AP/MA		
LB116093BSW	2.1160	2.9630	2.9160	9.6780	2.4350	5.0870	14.4500	2021-08-31_	8/31/21 10:16		AP/MA		
M3610-01	0.0000	57.9990	0.2000	0.0000	0.7100	0.3940	17.5770	2021-08-31_	8/31/21 12:00		AP/MA		
M3610-02	0.0000	71.1150	0.0000	0.7960	0.3010	-0.2890	6.9840	2021-08-31_	8/31/21 12:29		AP/MA		
M3610-01MS	2.4190	58.7290	3.1110	10.1300	3.1400	8.6610	32.8830	2021-08-31_	8/31/21 12:58		AP/MA		
M3610-01MSD	2.3680	58.8920	2.9660	9.6840	3.0390	8.3810	32.2420	2021-08-31_	8/31/21 13:26		AP/MA		
CCV	2.0230	2.8920	2.8950	9.6680	2.4330	5.8740	14.4180	2021-08-31_	8/31/21 13:56		AP/MA		
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-08-31_	8/31/21 14:25		AP/MA		


AP 9/16/21

Clear table

Instrument ID: IC-2									
Analyst : AP				Method: 300 / 9056A					
ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time
ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4		Initial wt/ Final Vol
ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4		Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-08-16_	8/16/21 10:41
STD2	0.3910	0.6790	0.6640	2.2200	0.5610	0.8630	3.4380	2021-08-16_	8/16/21 11:10
STD3	0.8120	1.1960	1.1960	4.0250	1.0110	1.9680	6.0560	2021-08-16_	8/16/21 11:40
STD4	0.9680	1.4810	1.4890	4.9650	1.2390	2.5530	7.4120	2021-08-16_	8/16/21 12:09
STD5	2.0210	2.9170	2.9320	9.7020	2.4140	5.1900	14.4290	2021-08-16_	8/16/21 12:38
STD6	4.0620	5.9880	5.9780	19.9480	4.9860	10.0130	29.8970	2021-08-16_	8/16/21 13:07
STD7	4.9450	7.5390	7.5410	25.1390	6.2890	12.4140	37.7680	2021-08-16_	8/16/21 13:37
ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4		
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000		AP/MA
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000		AP/MA
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000		AP/MA
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000		AP/MA
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000		AP/MA
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000		AP/MA
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.5000		AP/MA
ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4		
STD1									
STD2	-2.2500	13.1667	10.6667	11.0000	12.2000	-13.7000	14.6000		
STD3	1.5000	-0.3333	-0.3333	0.6250	1.1000	-1.6000	0.9333		
STD4	-3.2000	-1.2667	-0.7333	-0.7000	-0.8800	2.1200	-1.1733		
STD5	1.0500	-2.7667	-2.2667	-2.9800	-3.4400	3.8000	-3.8067		
STD6	1.5500	-0.2000	-0.3667	-0.2600	-0.2800	0.1300	-0.3433		
STD7	-1.1000	0.5200	0.5467	0.5560	0.6240	-0.6880	0.7147		

CALIBRATION OF COMPONENT F-

Method: AnionsIC2-081621.mtw
 Equation: $Q = 0.0787508 \cdot A + 1.63425$
 RSD: 2.096 %
 Correlation coefficient: 0.999761

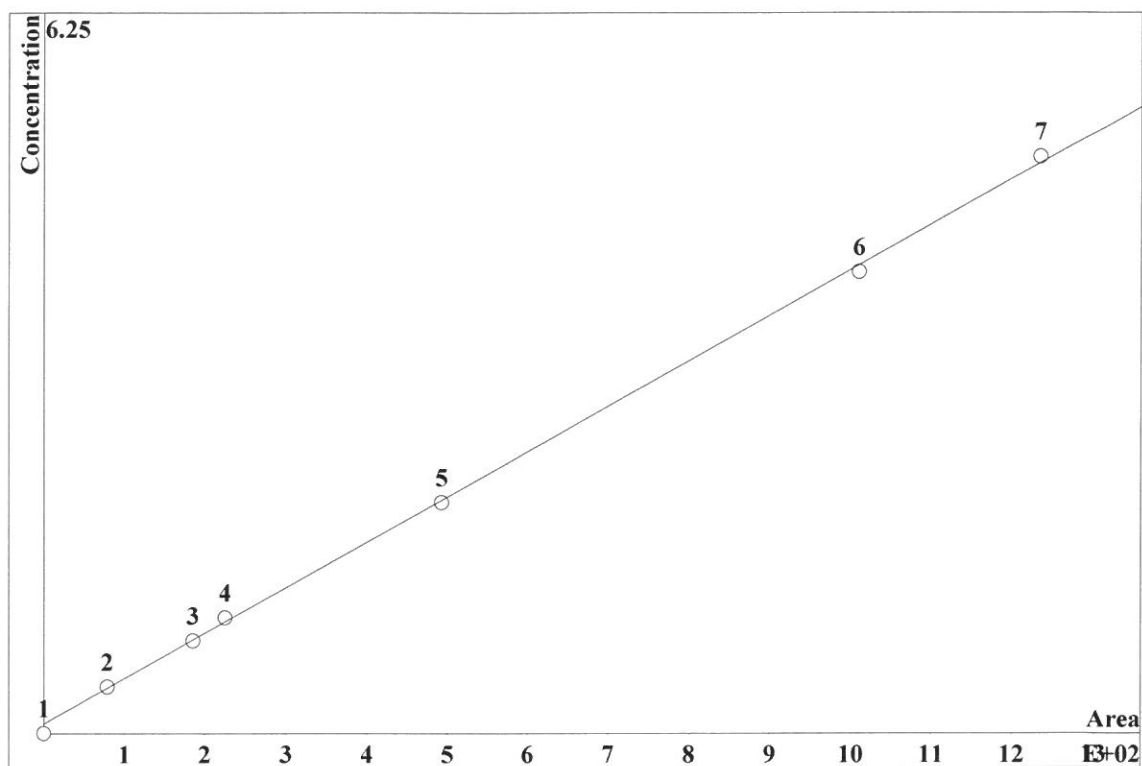

K3 = 0 K2 = 0 K1 = 0.0787508 K0 = 1.63425

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	2.039	78.64	0.4	20	5.75		
3	4.335	185.4	0.8	20	5.75		
4	5.553	225.1	1	20	5.75		
5	12.72	492.6	2	20	5.75		
6	25.53	1011	4	20	5.75		
7	32.96	1235	5	20	5.75		

CALIBRATION OF COMPONENT CL-

Method: AnionsIC2-081621.mtw
 Equation: $Q = 0.117224 \cdot A + 1.57793$
 RSD: 1.870 %
 Correlation coefficient: 0.999809

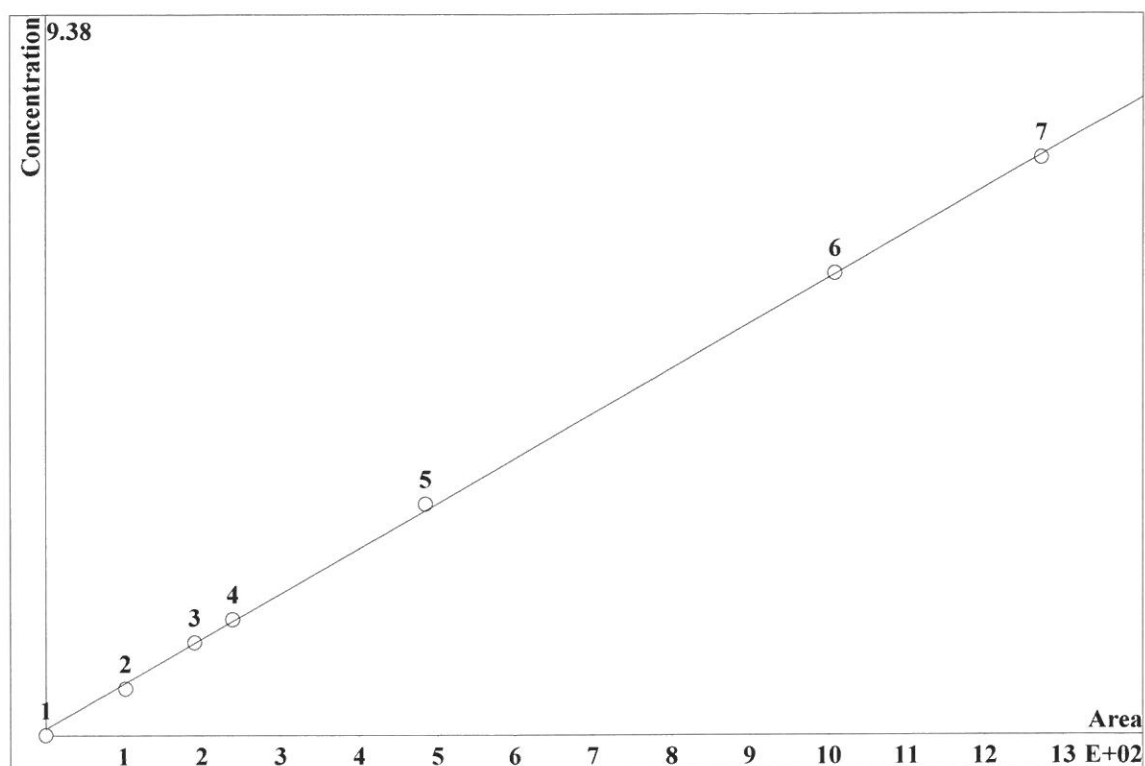

K3 = 0 K2 = 0 K1 = 0.117224 K0 = 1.57793

Base: Area

Ref.channel: chl

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	6.284	102.4	0.6	20	8.834		
3	12.17	190.6	1.2	20	8.834		
4	15.33	239.2	1.5	20	8.834		
5	31.62	484.2	3	20	8.834		
6	66.52	1008	6	20	8.834		
7	84.64	1273	7.5	20	8.834		

CALIBRATION OF COMPONENT NO2

Method: AnionsIC2-081621.mtw
 Equation: $Q = 0.0516801 \cdot A + 2.2891$
 RSD: 1.582 %
 Correlation coefficient: 0.999864

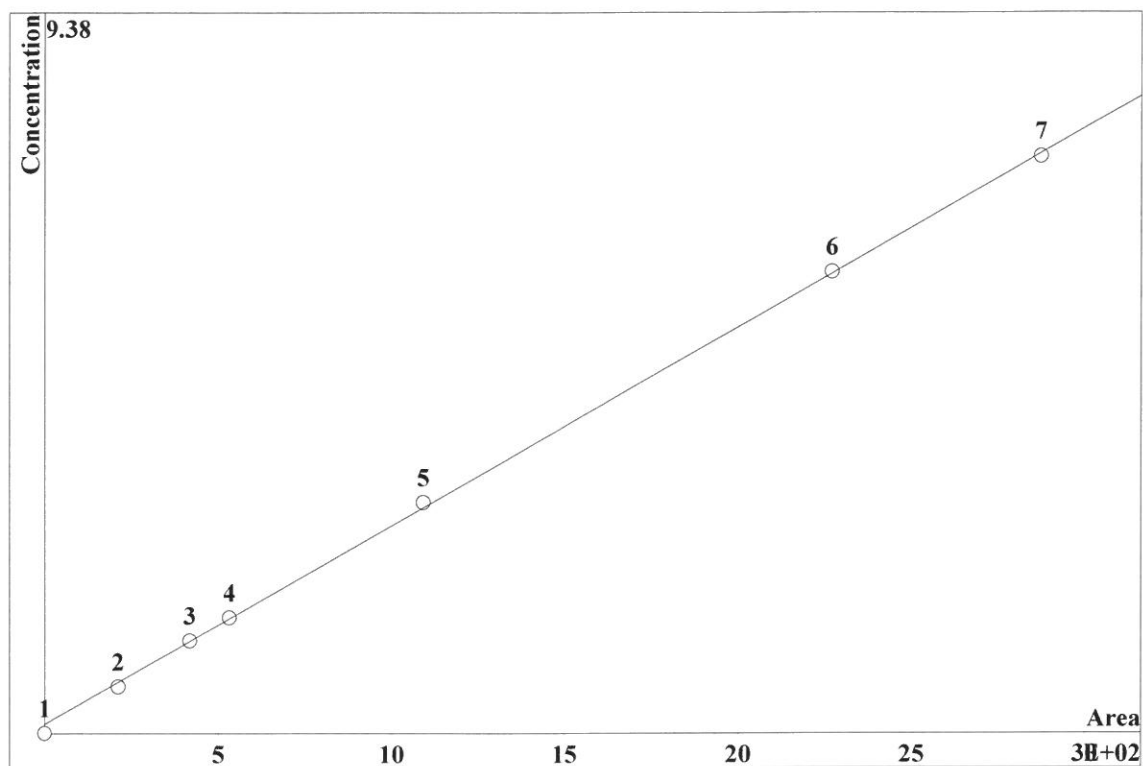

K3 = 0 K2 = 0 K1 = 0.0516801 K0 = 2.2891

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	10.82	212.6	0.6	20	10.64		
3	21.42	418.5	1.2	20	10.64		
4	27.07	531.9	1.5	20	10.64		
5	54.81	1091	3	20	10.64		
6	112.5	2269	6	20	10.64		
7	140.7	2874	7.5	20	10.64		

CALIBRATION OF COMPONENT BR-

Method: AnionsIC2-081621.mtw
 Equation: $Q = 0.260041 \cdot A + 9.18714$
 RSD: 1.824 %
 Correlation coefficient: 0.999819

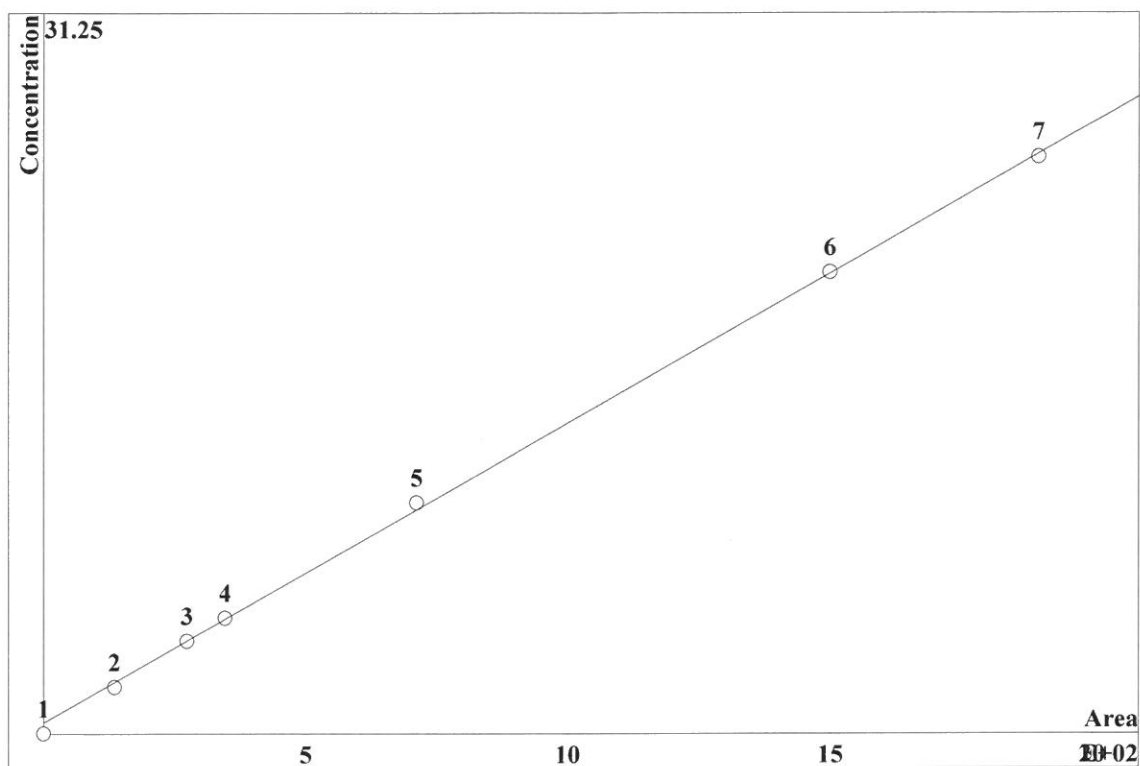

K3 = 0 K2 = 0 K1 = 0.260041 K0 = 9.18714

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	6.57	135.4	2	20			14
3	13.26	274.2	4	20			14
4	16.89	346.5	5	20			14
5	35.45	710.9	10	20			14
6	75.7	1499	20	20			14
7	96.72	1898	25	20			14

CALIBRATION OF COMPONENT NO3

Method: AnionsIC2-081621.mtw
 Equation: $Q = 0.0453375 \cdot A + 2.27775$
 RSD: 2.079 %
 Correlation coefficient: 0.999764

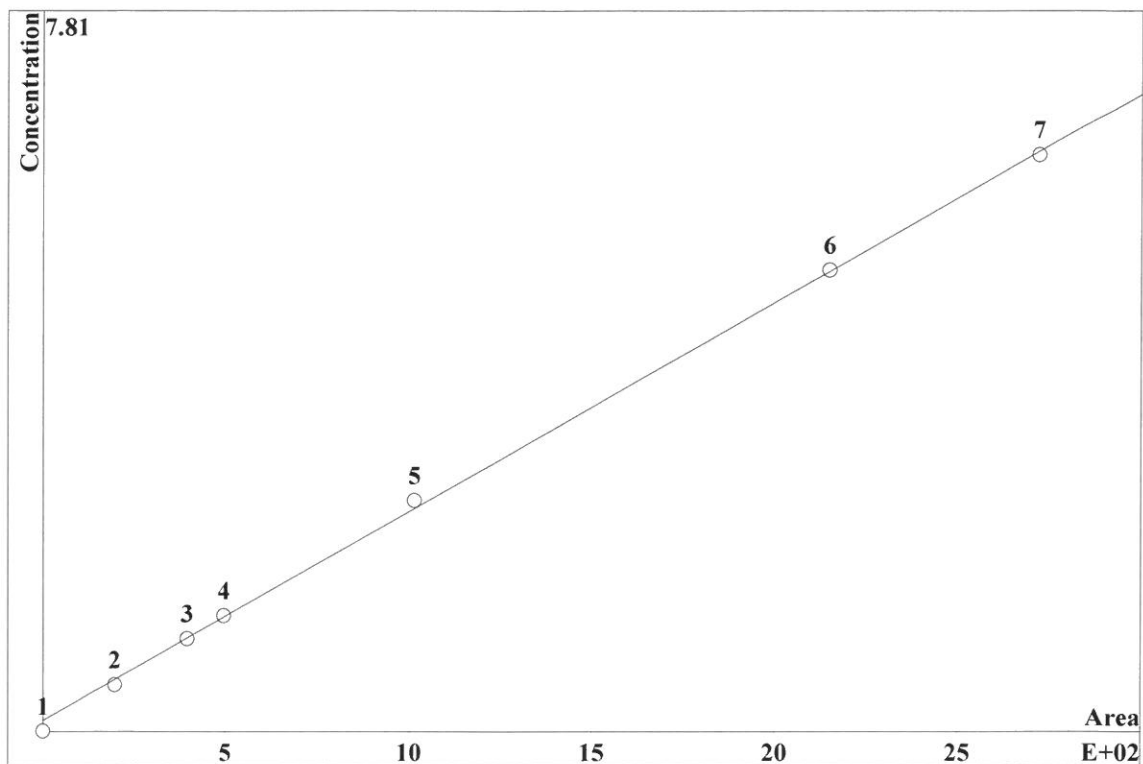

K3 = 0 K2 = 0 K1 = 0.0453375 K0 = 2.27775

Base: Area

Ref.channel: chl

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used File
1	0	0	0	0	0	0
2	7.929	197.1	0.5	20	16.28	
3	15.82	395.8	1	20	16.28	
4	20.05	496.5	1.25	20	16.28	
5	41.67	1015	2.5	20	16.28	
6	88.92	2149	5	20	16.28	
7	114	2724	6.25	20	16.28	

CALIBRATION OF COMPONENT HPO4

Method: AnionsIC2-081621.mtw
 Equation: $Q = 0.093688 \cdot A - 10.9491$
 RSD: 2.345 %
 Correlation coefficient: 0.999700

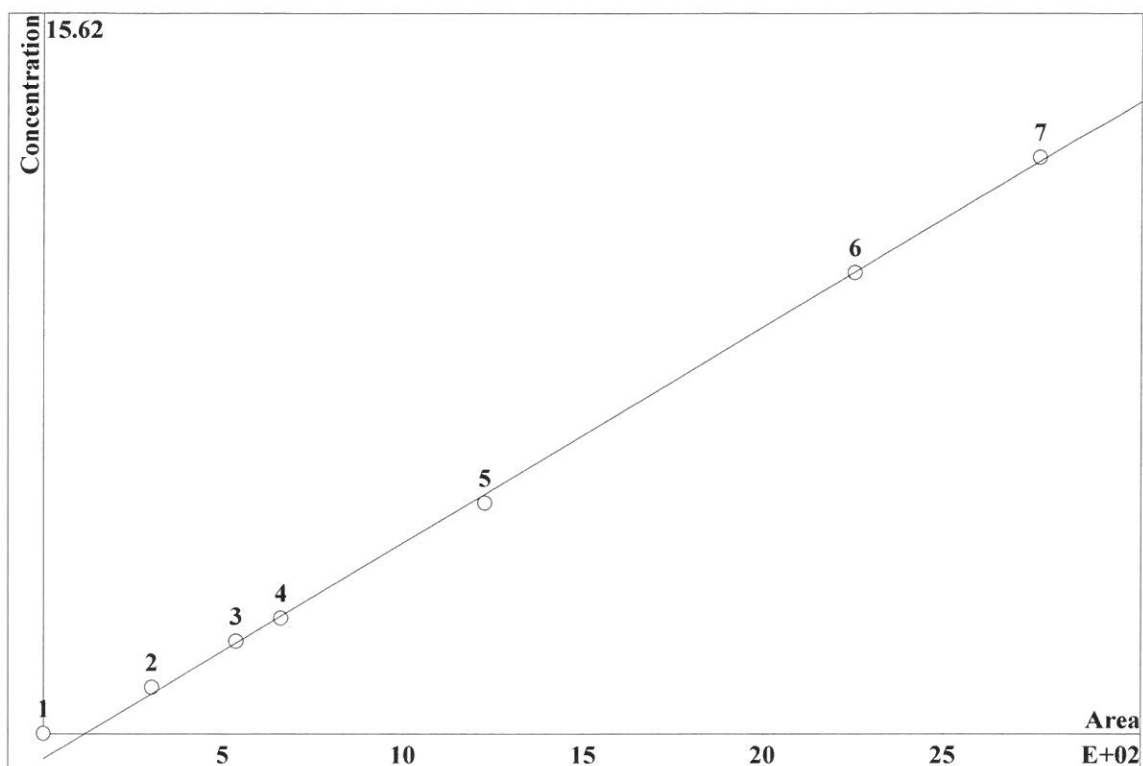

K3 = 0 K2 = 0 K1 = 0.093688 K0 = -10.9491

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	6.866	301	1	20	21.2		
3	12.55	536.9	2	20	21.2		
4	15.7	661.8	2.5	20	21.2		
5	30.88	1225	5	20	21.2		
6	58.85	2254	10	20	21.2		
7	73.57	2767	12.5	20	21.2		

CALIBRATION OF COMPONENT SO4

Method: AnionsIC2-081621.mtw
 Equation: $Q = 0.148108 \cdot A + 15.0956$
 RSD: 2.368 %
 Correlation coefficient: 0.999694

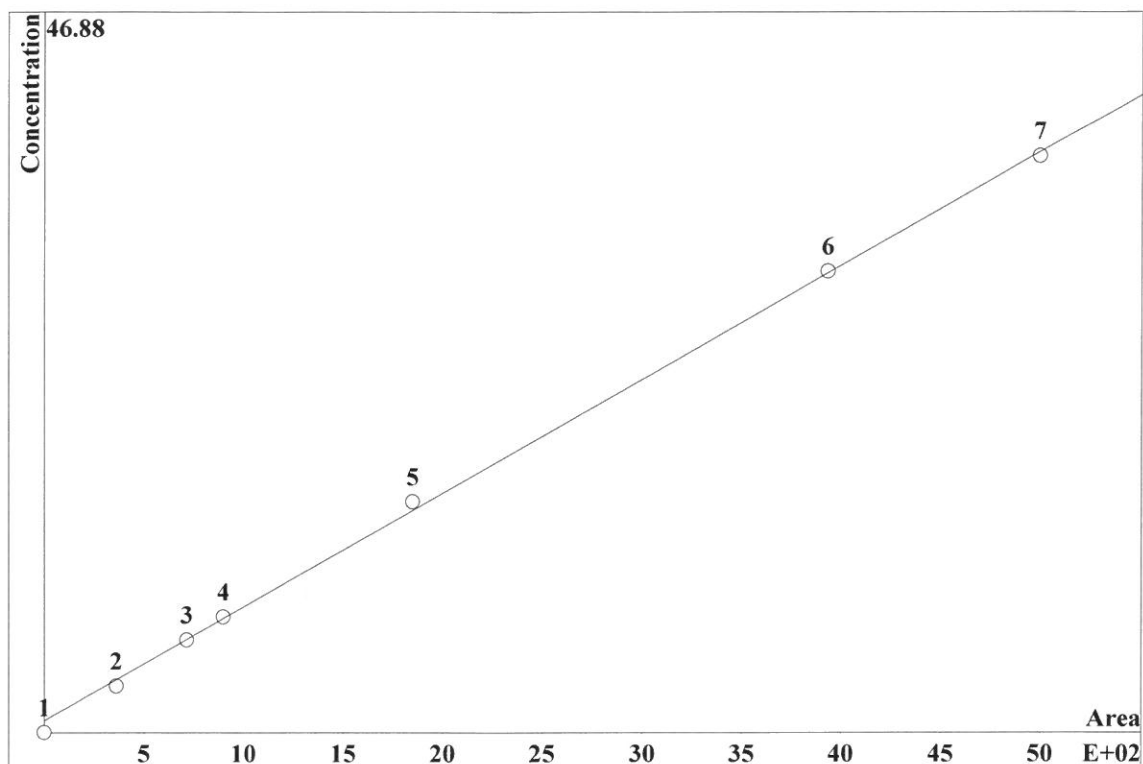

K3 = 0 K2 = 0 K1 = 0.148108 K0 = 15.0956

Base: Area

Ref.channel: chl

ISTD:

Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	11.07	362.3	3	20	24.73		
3	21.95	715.9	6	20	24.73		
4	27.77	898.9	7.5	20	24.73		
5	57.89	1847	15	20	24.73		
6	124.1	3935	30	20	24.73		
7	158.5	4998	37.5	20	24.73		

Report date: 8/16/2021 2:41:00 PM
Printed by: wet


Ident: STD1
Analysis from: 8/16/2021 10:41:20 AM
File: _2021-08-16_

Last save: 8/16/2021 2:19:03 PM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 27902

Last save: 8/16/2021 1:34:

SAMPLE:
: AM/AP
Vial number: 2
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

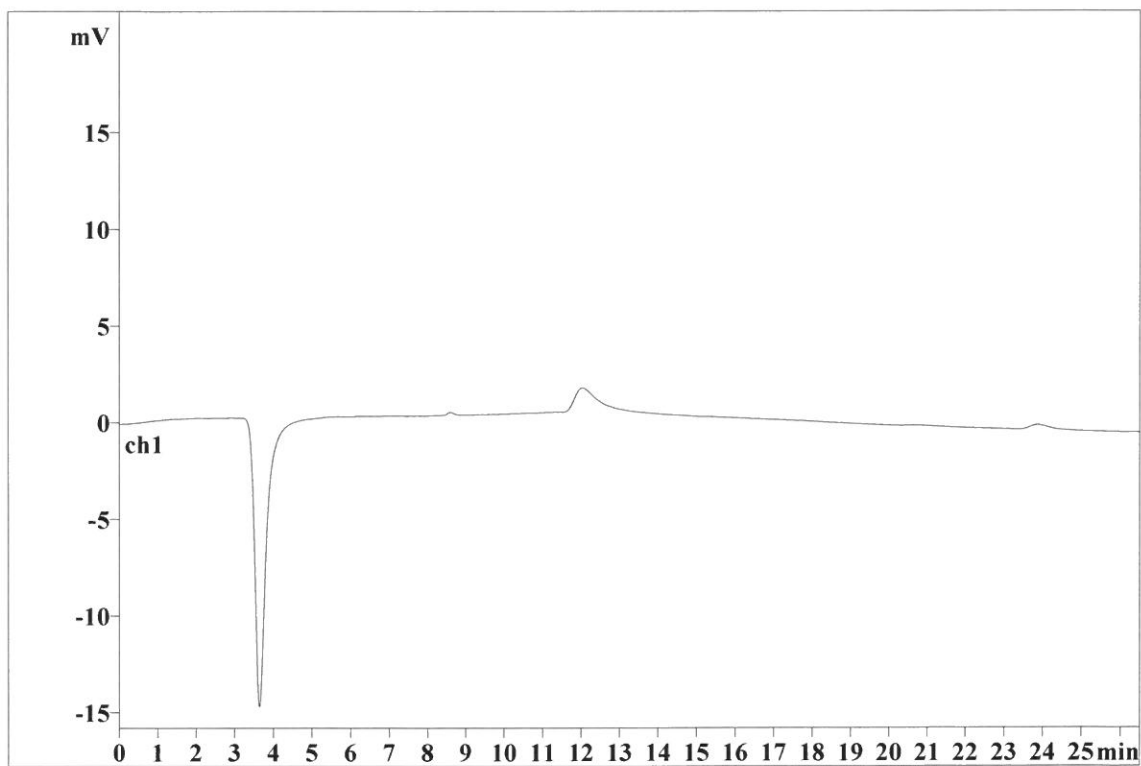

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 8/16/2021 2:41:09 PM
Printed by: wet


Ident: STD2
Analysis from: 8/16/2021 11:10:29 AM
File: _2021-08-16_

Last save: 8/16/2021 2:19:03 PM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 27903

Last save: 8/16/2021 1:34:

SAMPLE:
: AM/AP
Vial number: 3
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

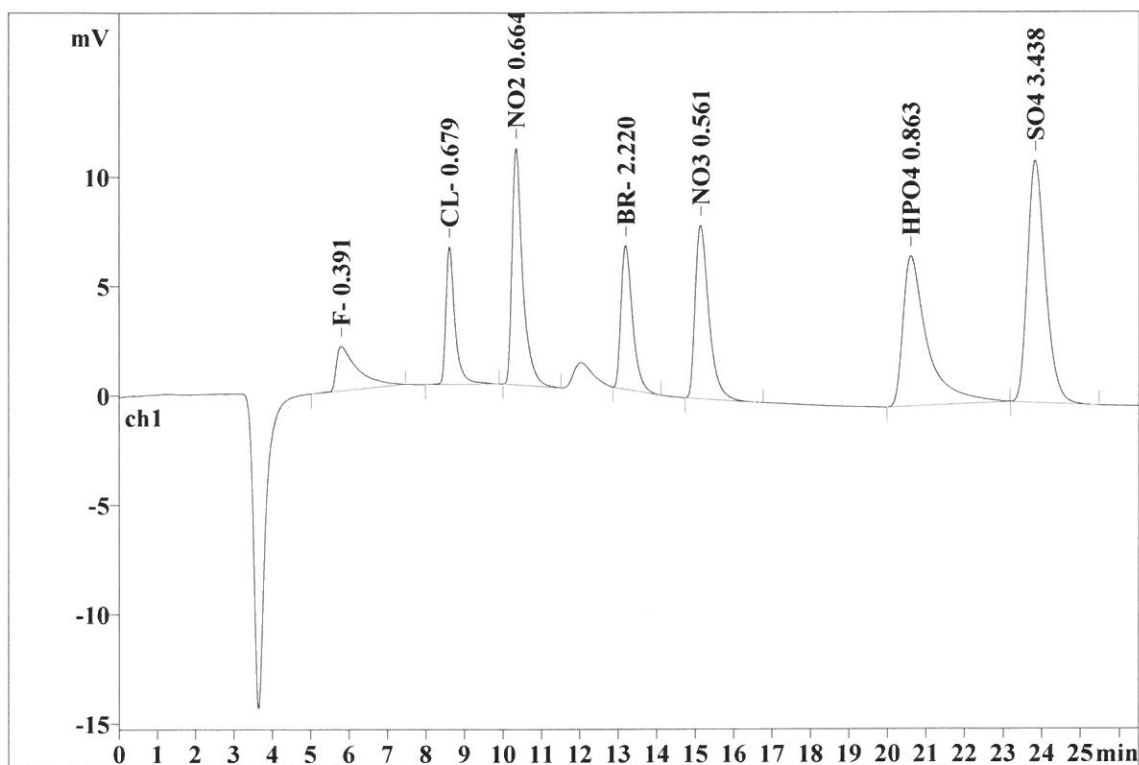

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.79	0.528	2.04	3.95	78.638	5.66
2	8.59	0.227	6.28	12.19	102.434	7.37
3	10.31	0.280	10.82	20.97	212.618	15.30
4	13.18	0.310	6.57	12.74	135.403	9.74
5	15.12	0.370	7.93	15.38	197.114	14.19
6	20.60	0.581	6.86	13.31	300.994	21.66
7	23.82	0.498	11.07	21.46	362.315	26.07
7	26.50	0.399	51.57	99.99	1389.516	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/16/2021 2:41:15 PM
Printed by: wet


Ident: STD3
Analysis from: 8/16/2021 11:40:29 AM
File: _2021-08-16_

Last save: 8/16/2021 2:19:03 PM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 27904

Last save: 8/16/2021 1:34:

SAMPLE:
: AM/AP
Vial number: 4
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

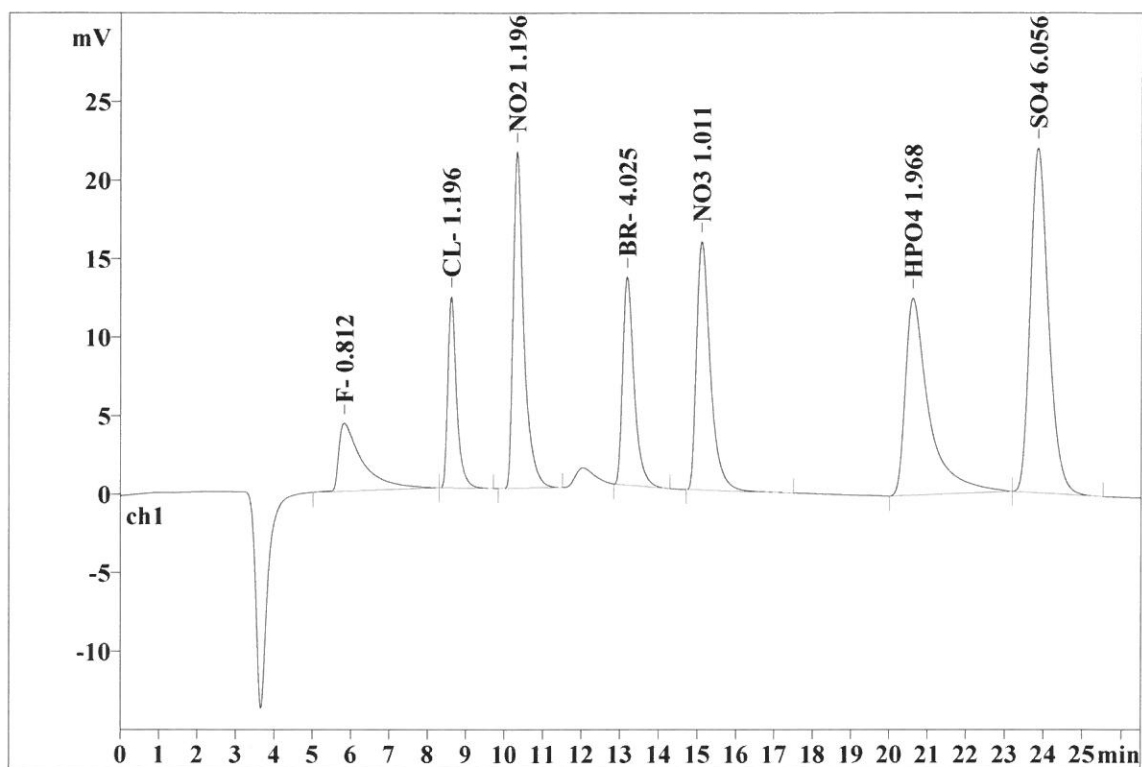

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.82	0.561	4.33	4.27	185.440	6.82
2	8.60	0.224	12.17	11.99	190.565	7.01
3	10.31	0.278	21.42	21.10	418.497	15.40
4	13.17	0.308	13.25	13.06	274.248	10.09
5	15.10	0.369	15.82	15.59	395.751	14.56
6	20.62	0.570	12.55	12.36	536.946	19.76
7	23.85	0.496	21.95	21.62	715.856	26.34
7	26.50	0.401	101.49	99.99	2717.303	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/16/2021 2:41:22 PM
Printed by: wet


Ident: STD4
Analysis from: 8/16/2021 12:09:38 PM
File: _2021-08-16_

Last save: 8/16/2021 2:19:03 PM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 27905

Last save: 8/16/2021 1:34:

SAMPLE:
: AM/AP
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

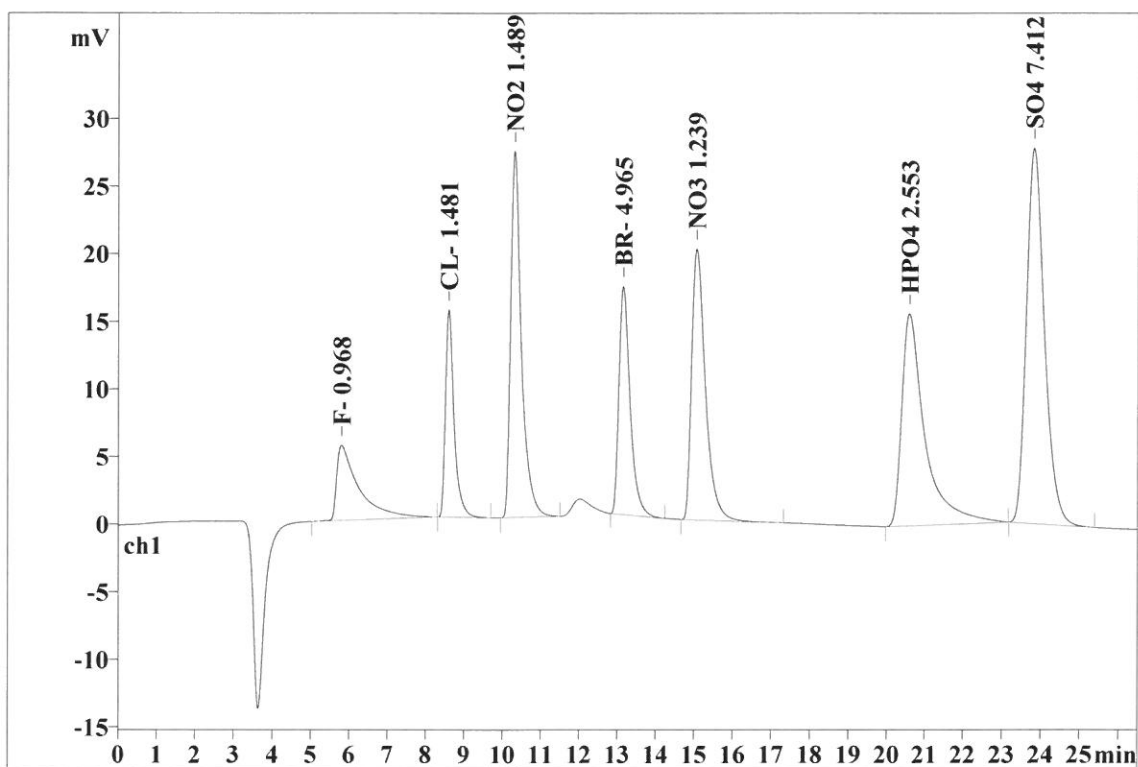

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.80	0.516	5.55	4.32	225.116	6.62
2	8.58	0.224	15.33	11.94	239.230	7.04
3	10.29	0.279	27.07	21.09	531.854	15.64
4	13.14	0.306	16.89	13.16	346.535	10.19
5	15.06	0.366	20.05	15.62	496.499	14.60
6	20.58	0.561	15.70	12.23	661.773	19.46
7	23.82	0.492	27.77	21.63	898.941	26.44
7	26.50	0.392	128.37	100.00	3399.949	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/16/2021 2:41:29 PM

Printed by: wet

Ident: STD5

Analysis from: 8/16/2021 12:38:45 PM

File: _2021-08-16_

Last save: 8/16/2021 2:19:03 PM

Method: AnionsIC2-081621.mtw

Last save: 8/16/2021 1:34:

Run operator: wet

Analysis number: 27906

SAMPLE:

: AM/AP

Vial number:

6

Volume:


20.0 µL

Dilution:

1.00

Amount:

1.0000

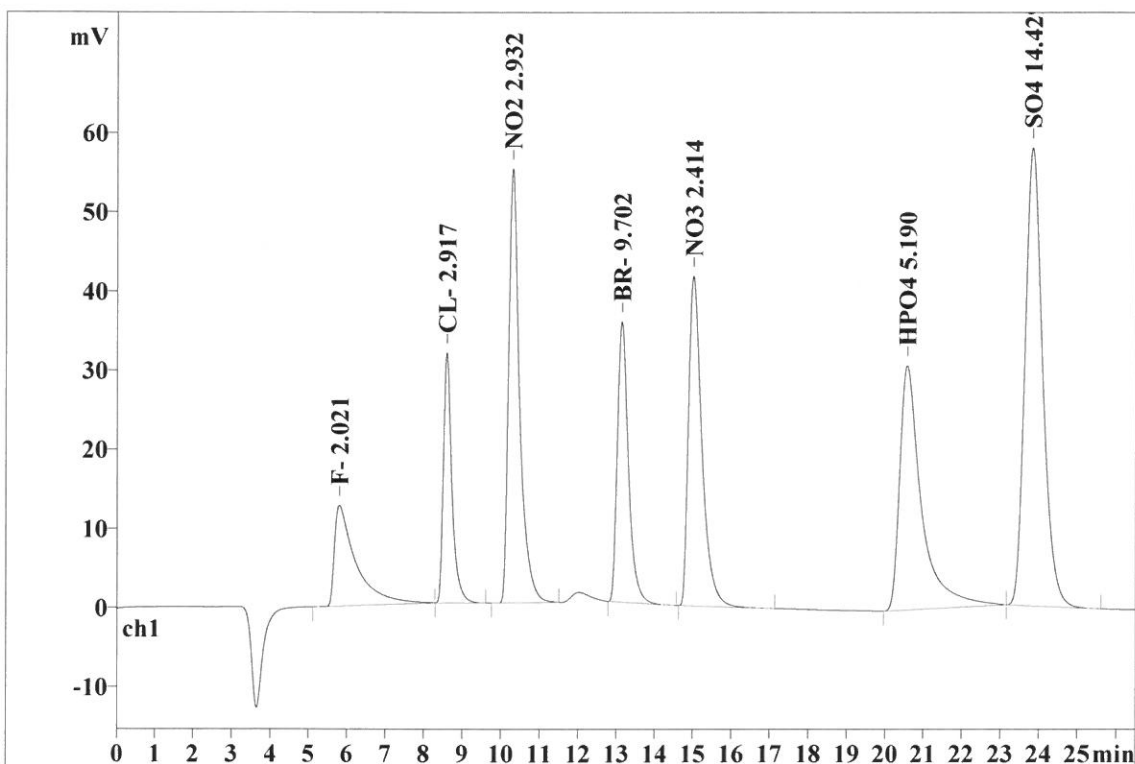

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.80	0.504	12.72	4.80	492.593	7.18
2	8.58	0.220	31.62	11.93	484.207	7.05
3	10.28	0.284	54.81	20.68	1090.559	15.89
4	13.12	0.298	35.45	13.38	710.881	10.36
5	15.01	0.360	41.66	15.72	1014.578	14.78
6	20.56	0.532	30.87	11.65	1224.844	17.84
7	23.81	0.484	57.89	21.84	1846.544	26.90
7	26.50	0.383	265.03	100.00	6864.205	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/16/2021 2:41:36 PM
Printed by: wet


Ident: STD6
Analysis from: 8/16/2021 1:07:53 PM
File: _2021-08-16_

Last save: 8/16/2021 2:19:03 PM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 27907

Last save: 8/16/2021 1:34:

SAMPLE:
: AM/AP
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

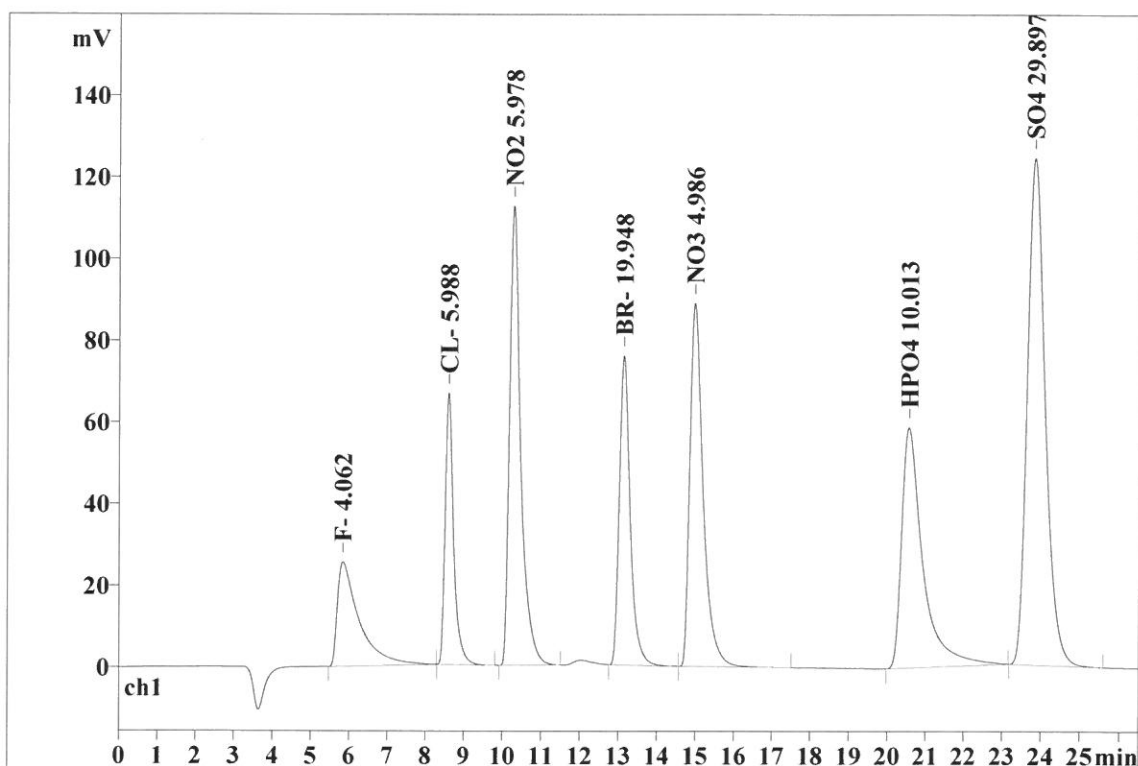

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.84	0.534	25.53	4.62	1010.837	7.16
2	8.59	0.216	66.52	12.05	1008.142	7.14
3	10.27	0.286	112.49	20.37	2269.338	16.06
4	13.13	0.292	75.70	13.71	1498.913	10.61
5	14.97	0.354	88.92	16.10	2149.238	15.21
6	20.56	0.519	58.85	10.66	2254.471	15.96
7	23.83	0.480	124.14	22.48	3935.287	27.86
7	26.50	0.383	552.16	100.00	14126.227	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/16/2021 2:41:42 PM
Printed by: wet


Ident: STD7
Analysis from: 8/16/2021 1:37:00 PM
File: _2021-08-16_

Last save: 8/16/2021 2:19:03 PM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 27908

Last save: 8/16/2021 1:34:

SAMPLE:
: AM/AP
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

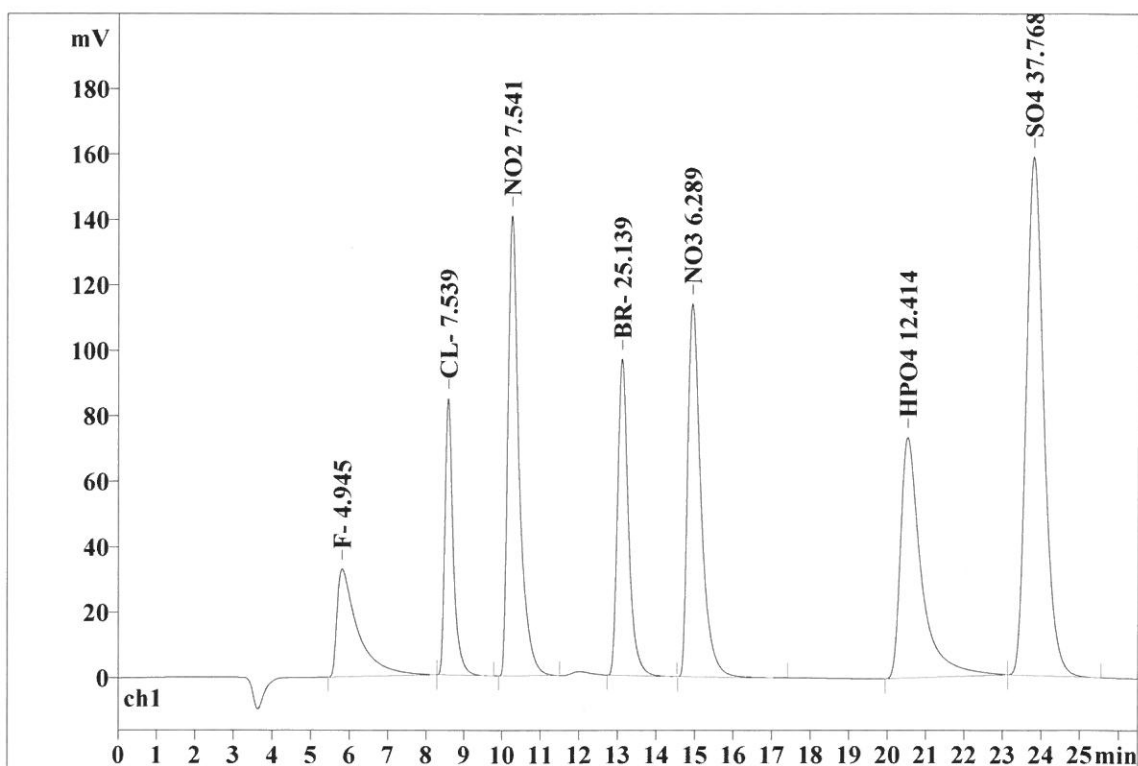

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.81	0.494	32.96	4.70	1235.210	6.95
2	8.57	0.214	84.64	12.07	1272.799	7.16
3	10.24	0.290	140.66	20.06	2873.891	16.17
4	13.11	0.290	96.71	13.79	1898.166	10.68
5	14.93	0.350	114.00	16.26	2724.121	15.33
6	20.52	0.512	73.57	10.49	2766.841	15.57
7	23.79	0.478	158.53	22.61	4998.116	28.13
7	26.50	0.375	701.07	100.00	17769.143	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/17/2021 4:31:35 PM
Printed by: wet


Ident: ICV
Analysis from: 8/16/2021 2:22:07 PM
File: _2021-08-16_

Last save: 8/16/2021 2:48:38 PM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 27909

Last save: 8/16/2021 2:03:

SAMPLE:
: AM/AP
Vial number: 9
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

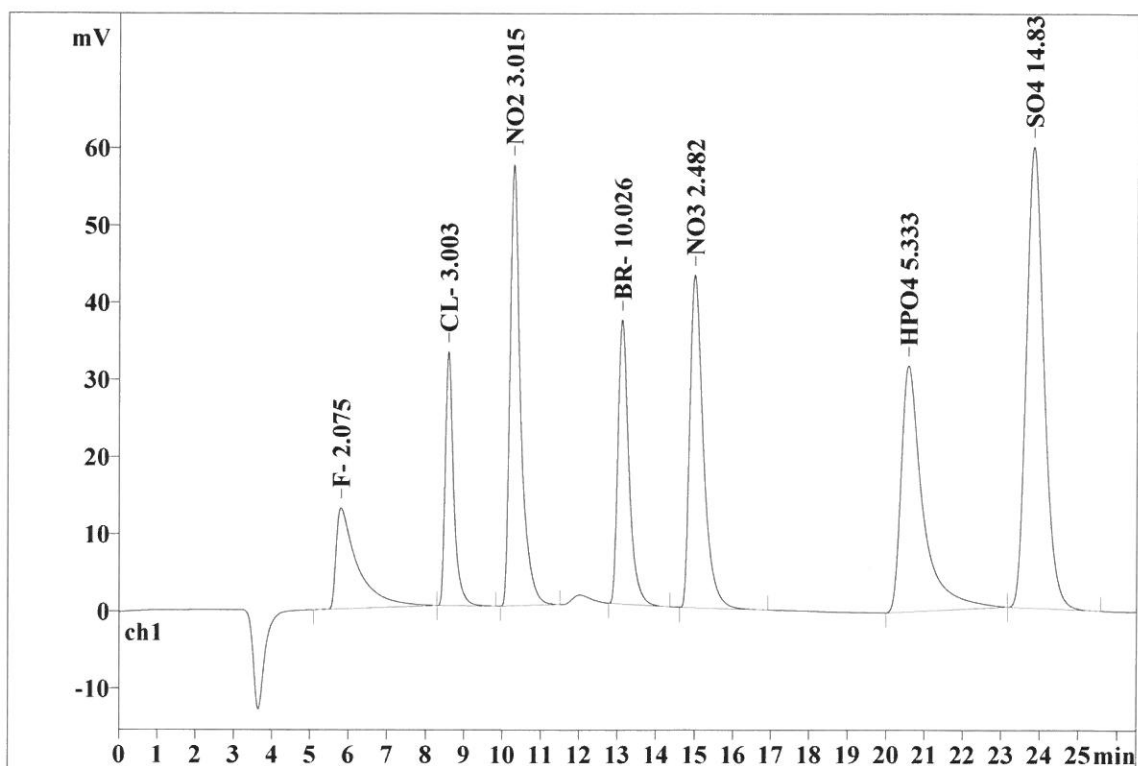

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.80	0.504	13.08	4.76	506.270	7.17
2	8.58	0.217	32.89	11.98	498.972	7.06
3	10.27	0.279	57.10	20.79	1122.328	15.89
4	13.11	0.296	36.82	13.41	735.757	10.41
5	14.99	0.358	43.10	15.69	1044.695	14.79
6	20.57	0.528	31.89	11.61	1255.288	17.77
7	23.82	0.482	59.76	21.76	1901.107	26.91
7	26.50	0.381	274.65	100.00	7064.419	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/17/2021 4:31:44 PM
Printed by: wet


Ident: ICB
Analysis from: 8/16/2021 2:51:40 PM
File: _2021-08-16_

Last save: 8/16/2021 3:22:33 PM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 27910

Last save: 8/16/2021 2:03:

SAMPLE:
: AP/MA
Vial number: 10
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

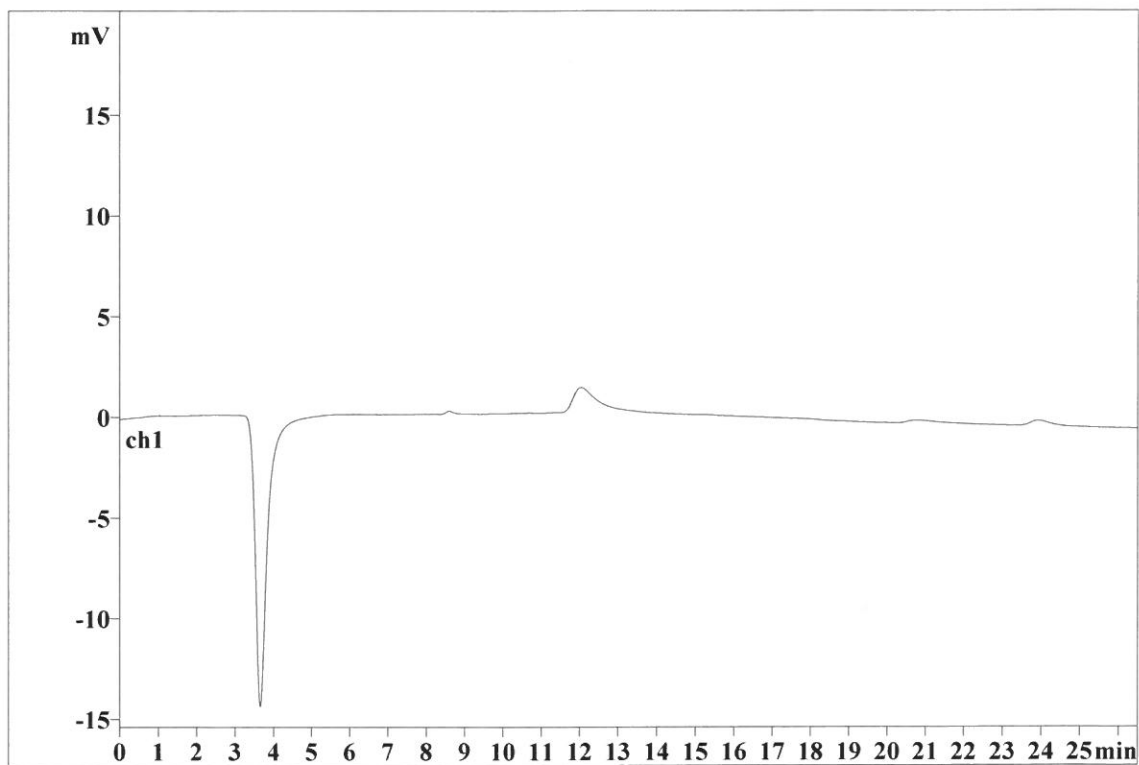

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 8/31/2021 3:14:52 PM
Printed by: wet


Ident: CCV
Analysis from: 8/31/2021 8:49:20 AM
File: _2021-08-31_

Last save: 8/31/2021 9:16:19 AM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 28036

Last save: 8/23/2021 10:23

SAMPLE:
: AP/MA
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

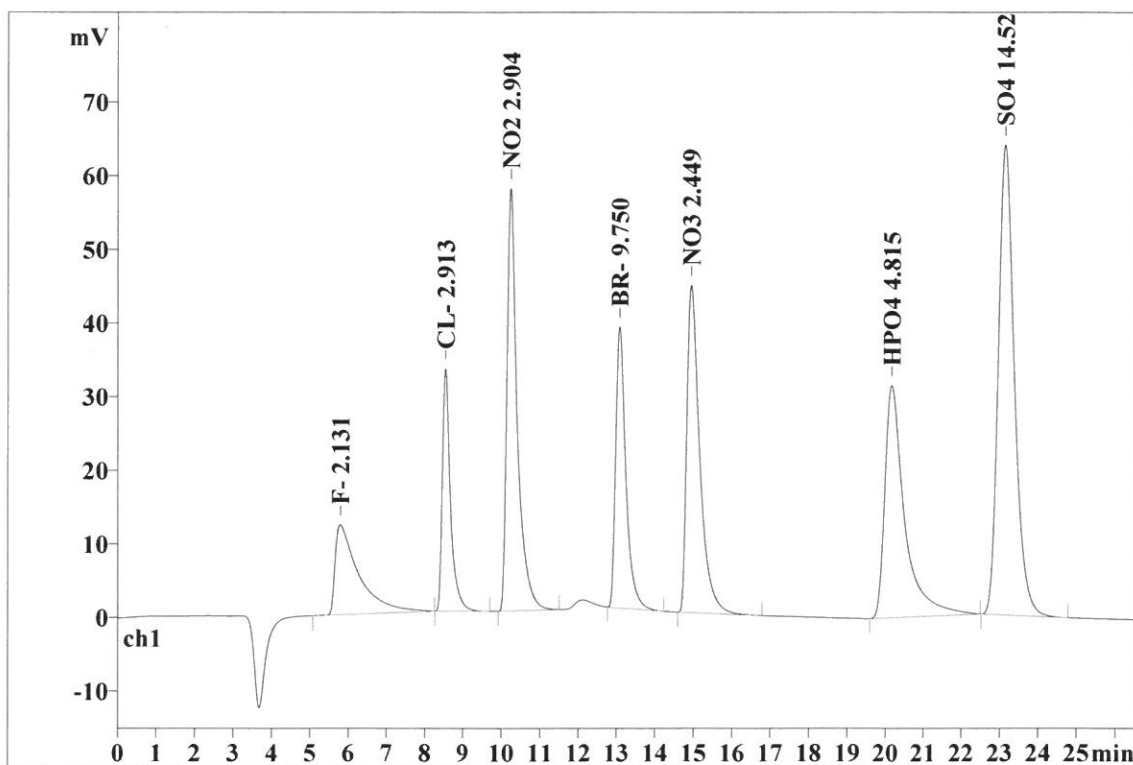

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.79	0.567	12.22	4.35	520.509	7.62
2	8.53	0.203	32.98	11.75	483.512	7.08
3	10.23	0.260	57.41	20.46	1079.704	15.80
4	13.08	0.273	38.21	13.61	714.566	10.46
5	14.94	0.336	44.45	15.84	1030.129	15.08
6	20.16	0.488	31.52	11.23	1144.747	16.76
7	23.13	0.438	63.86	22.75	1858.829	27.21
7	26.50	0.367	280.64	100.00	6831.996	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/31/2021 3:15:00 PM
Printed by: wet


Ident: CCB
Analysis from: 8/31/2021 9:19:12 AM
File: _2021-08-31_

Last save: 8/31/2021 9:45:12 AM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 28037

Last save: 8/31/2021 9:16:

SAMPLE:
: AP/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

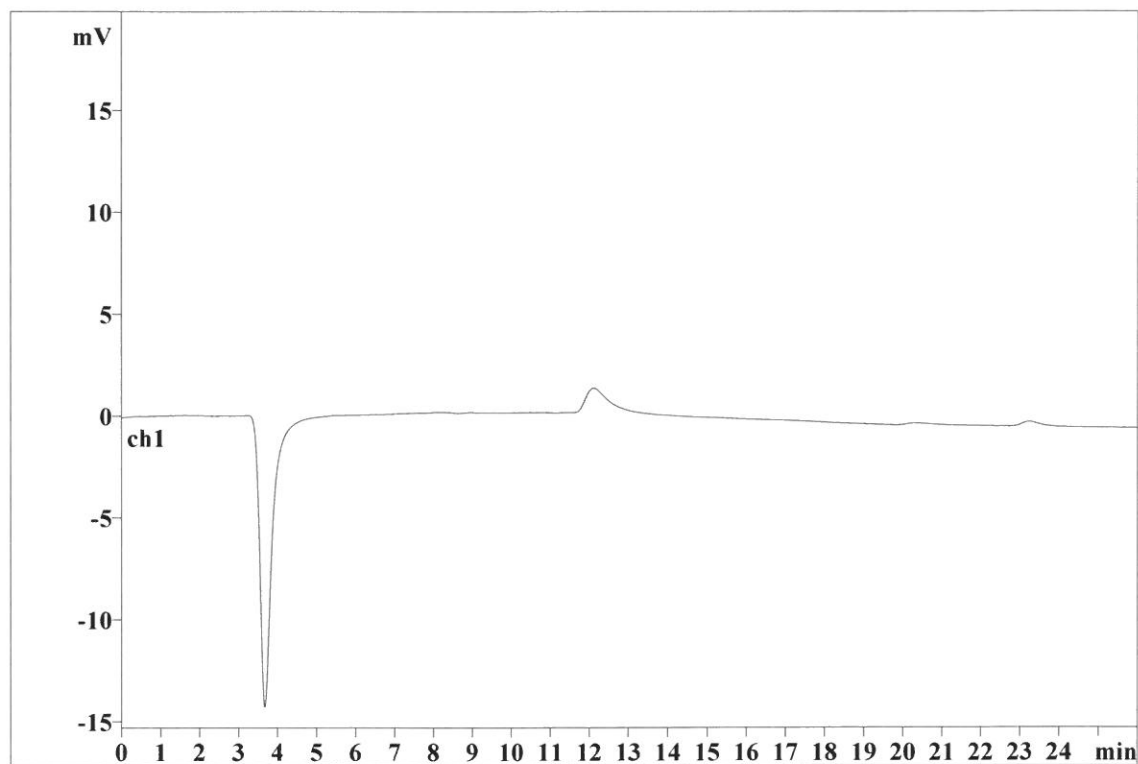

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 8/31/2021 3:15:07 PM
Printed by: wet


Ident: LB116093BLW
Analysis from: 8/31/2021 9:47:48 AM
File: _2021-08-31_

Last save: 8/31/2021 3:14:45 PM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 28038

Last save: 8/31/2021 9:16:

SAMPLE:
: AP/MA
Vial number: 13
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

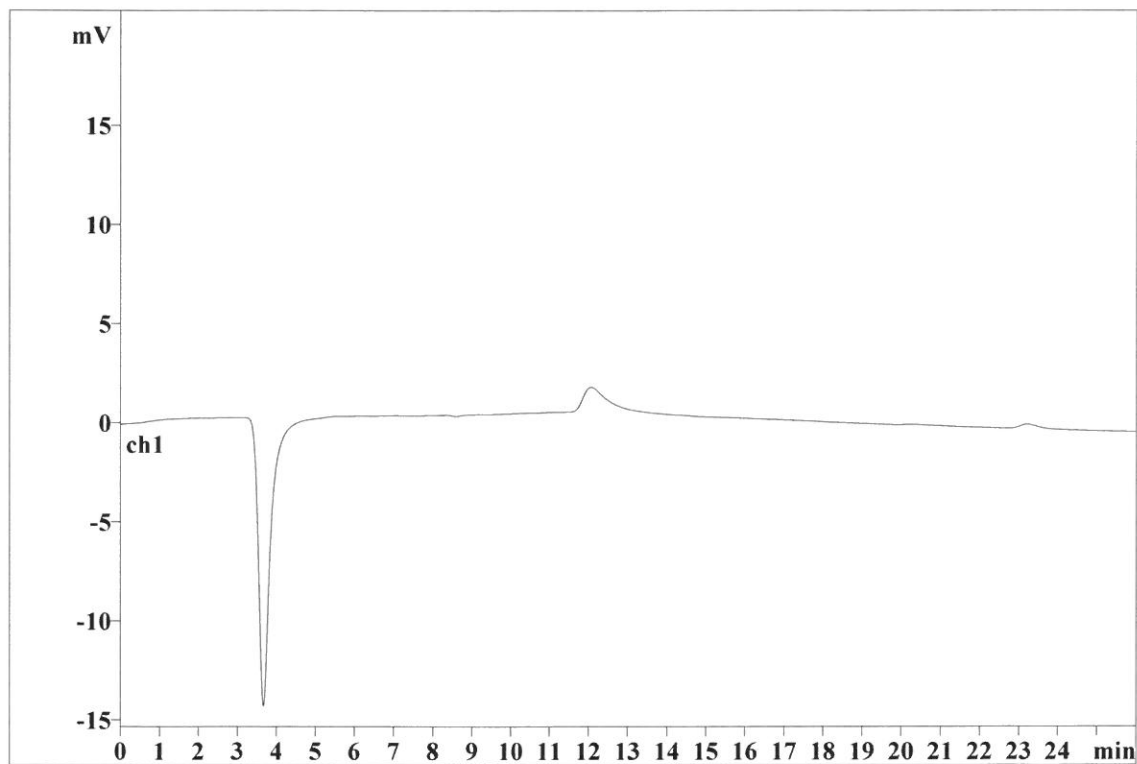

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 8/31/2021 3:15:15 PM
Printed by: wet


Ident: LB116093BSW
Analysis from: 8/31/2021 10:16:23 AM
File: _2021-08-31_

Last save: 8/31/2021 3:14:45 PM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 28039

Last save: 8/31/2021 9:16:

SAMPLE:
: AP/MA
Vial number: 14
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

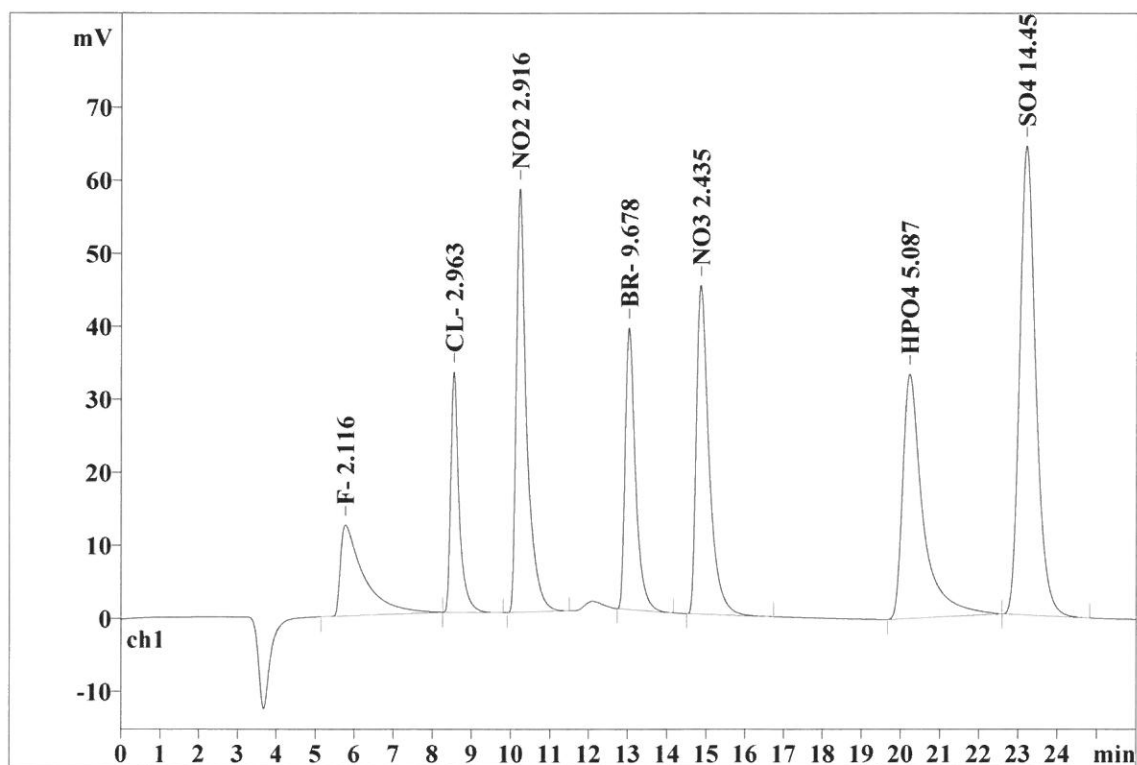

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.77	0.545	12.46	4.38	516.671	7.51
2	8.54	0.207	32.95	11.57	492.004	7.15
3	10.22	0.258	57.98	20.36	1084.296	15.76
4	13.03	0.269	38.59	13.55	708.995	10.31
5	14.85	0.330	45.04	15.82	1023.811	14.89
6	20.23	0.479	33.46	11.75	1202.858	17.49
7	23.20	0.433	64.27	22.57	1849.331	26.89
7	26.00	0.360	284.76	100.00	6877.966	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/31/2021 3:15:47 PM
Printed by: wet


Ident: M3610-01
Analysis from: 8/31/2021 12:00:47 PM
File: _2021-08-31_

Last save: 8/31/2021 3:15:46 PM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 28041

Last save: 8/31/2021 9:16:

SAMPLE:
: AP/MA
Vial number: 15
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

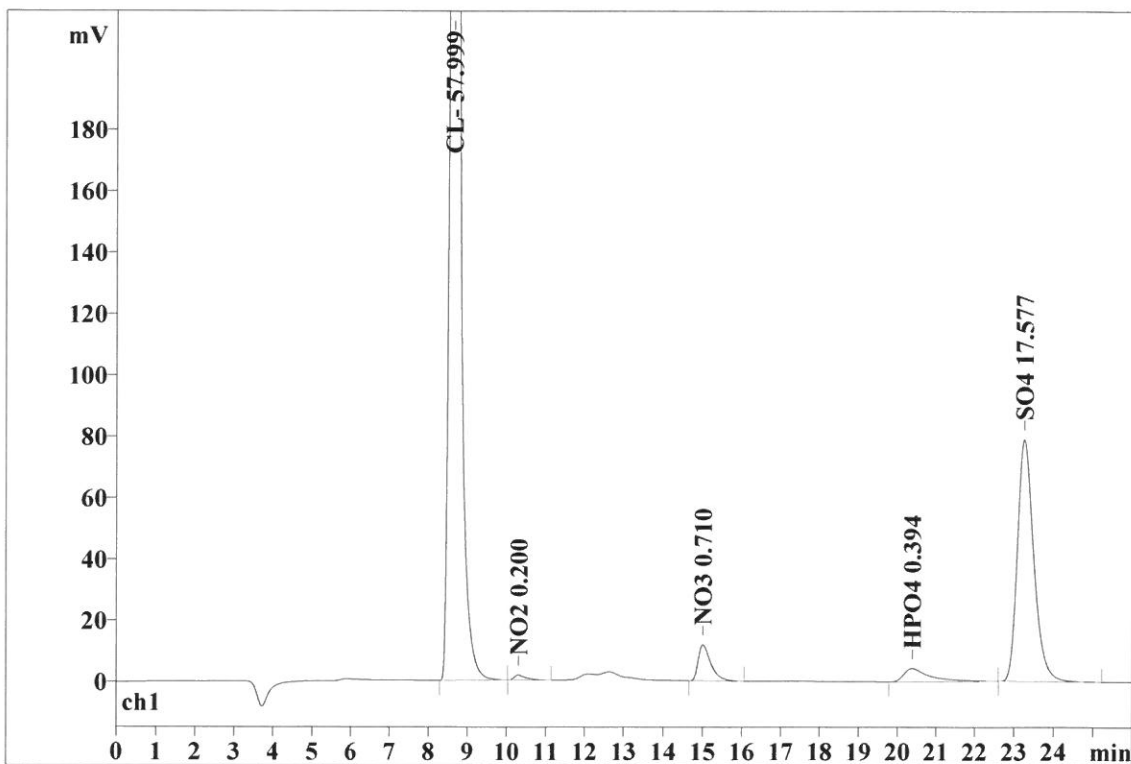

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	8.62	0.192	725.66	88.26	9881.897	78.12
3	10.30	0.297	1.59	0.19	32.925	0.26
4	0.00	0.000	0.00	0.00	0.000	0.00
5	15.01	0.332	11.76	1.43	262.961	2.08
6	20.38	0.614	4.28	0.52	200.962	1.59
7	23.26	0.433	78.84	9.59	2271.548	17.96
7	26.00	0.267	822.13	100.00	12650.293	100.00

This report has been created by IC Net
METROHM LTD


Report date: 8/31/2021 3:16:12 PM
Printed by: wet

Ident: M3610-02
Analysis from: 8/31/2021 12:29:25 PM
File: _2021-08-31_
Modified!
Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 28042

Last save: 8/31/2021 12:59:13 PM

Last save: 8/31/2021 9:16:

SAMPLE:
: AP/MA
Vial number: 18
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

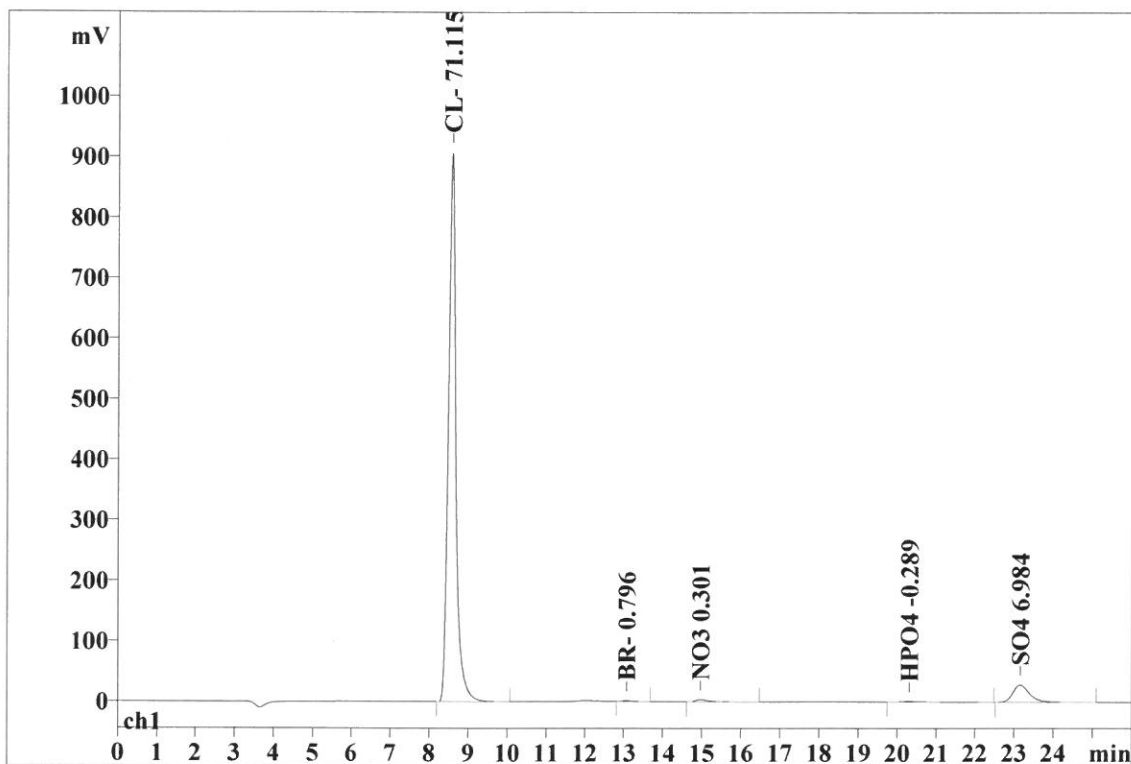

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	8.55	0.189	907.42	96.30	12119.686	92.34
3	0.00	0.000	0.00	0.00	0.000	0.00
4	13.07	0.273	1.44	0.15	25.890	0.20
5	14.97	0.337	3.57	0.38	82.386	0.63
6	20.30	0.644	1.13	0.12	55.223	0.42
7	23.16	0.440	28.63	3.04	841.219	6.41
7	26.00	0.269	942.19	100.00	13124.404	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/31/2021 3:16:21 PM
Printed by: wet


Ident: M3610-02
Analysis from: 8/31/2021 12:29:25 PM
File: _2021-08-31_

Last save: 8/31/2021 3:16:21 PM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 28042

Last save: 8/31/2021 9:16:

SAMPLE:
: AP/MA
Vial number: 18
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

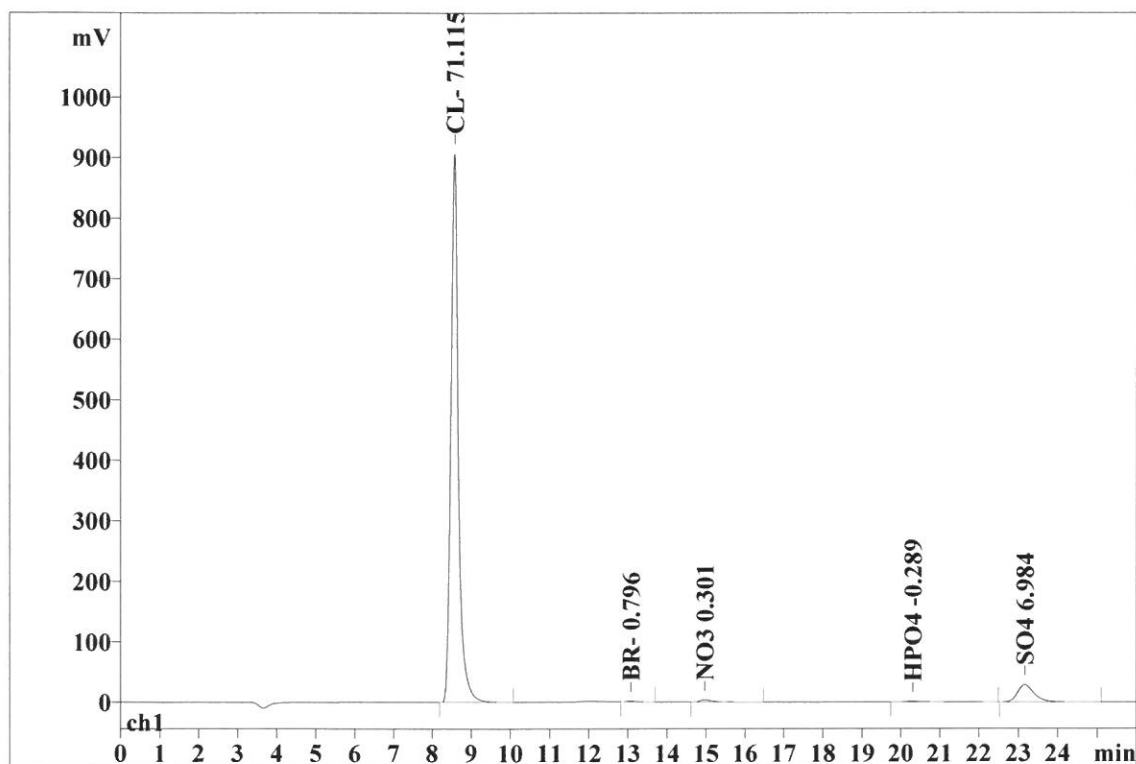

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	8.55	0.189	907.42	96.30	12119.686	92.34
3	0.00	0.000	0.00	0.00	0.000	0.00
4	13.07	0.273	1.44	0.15	25.890	0.20
5	14.97	0.337	3.57	0.38	82.386	0.63
6	20.30	0.644	1.13	0.12	55.223	0.42
7	23.16	0.440	28.63	3.04	841.219	6.41
7	26.00	0.269	942.19	100.00	13124.404	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/31/2021 3:16:28 PM
Printed by: wet


Ident: M3610-01MS
Analysis from: 8/31/2021 12:58:02 PM
File: _2021-08-31_

Last save: 8/31/2021 1:41:23 PM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 28043

Last save: 8/31/2021 9:16:

SAMPLE:
: AP/MA
Vial number: 16
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

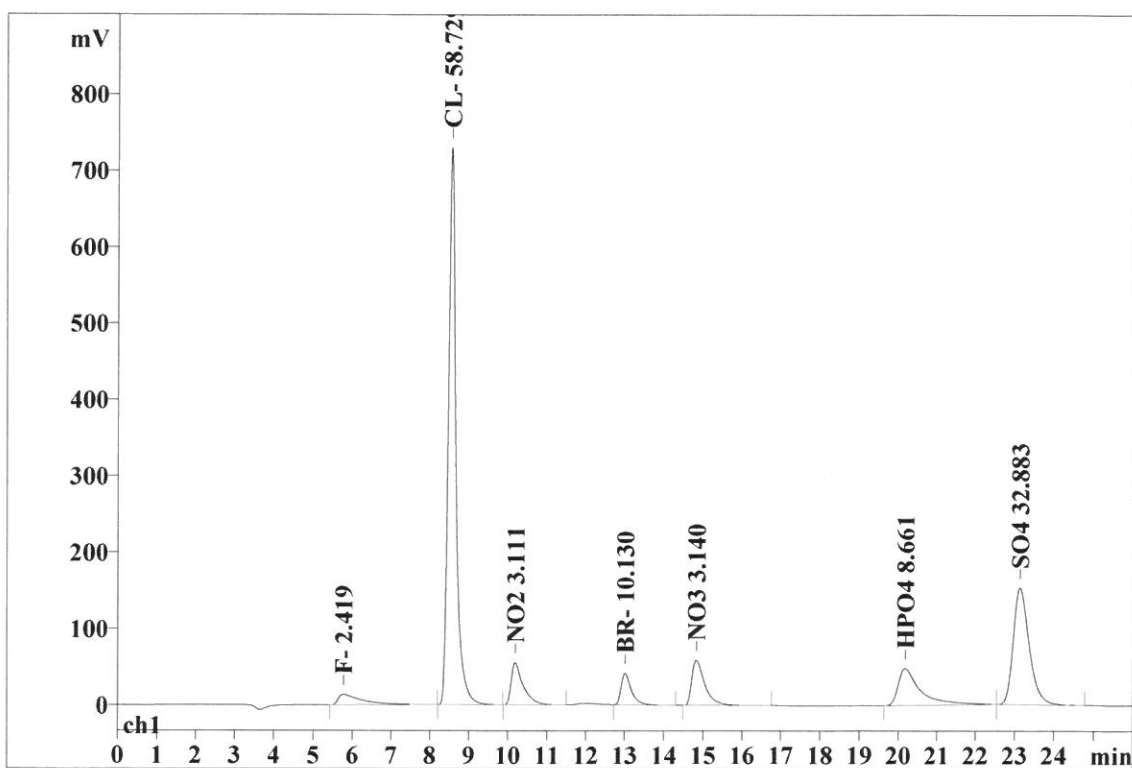

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.77	0.579	13.67	1.24	593.607	2.95
2	8.53	0.192	729.96	66.35	10006.570	49.68
3	10.19	0.295	55.05	5.00	1159.462	5.76
4	13.01	0.264	41.01	3.73	743.768	3.69
5	14.83	0.327	59.05	5.37	1335.068	6.63
6	20.18	0.519	48.64	4.42	1965.690	9.76
7	23.13	0.426	152.78	13.89	4338.514	21.54
7	26.00	0.372	1100.16	100.00	20142.680	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/31/2021 3:16:37 PM
Printed by: wet


Ident: M3610-01MSD
Analysis from: 8/31/2021 1:26:37 PM
File: _2021-08-31_

Last save: 8/31/2021 1:52:49 PM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 28044

Last save: 8/31/2021 9:16:

SAMPLE:
: AP/MA
Vial number: 17
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

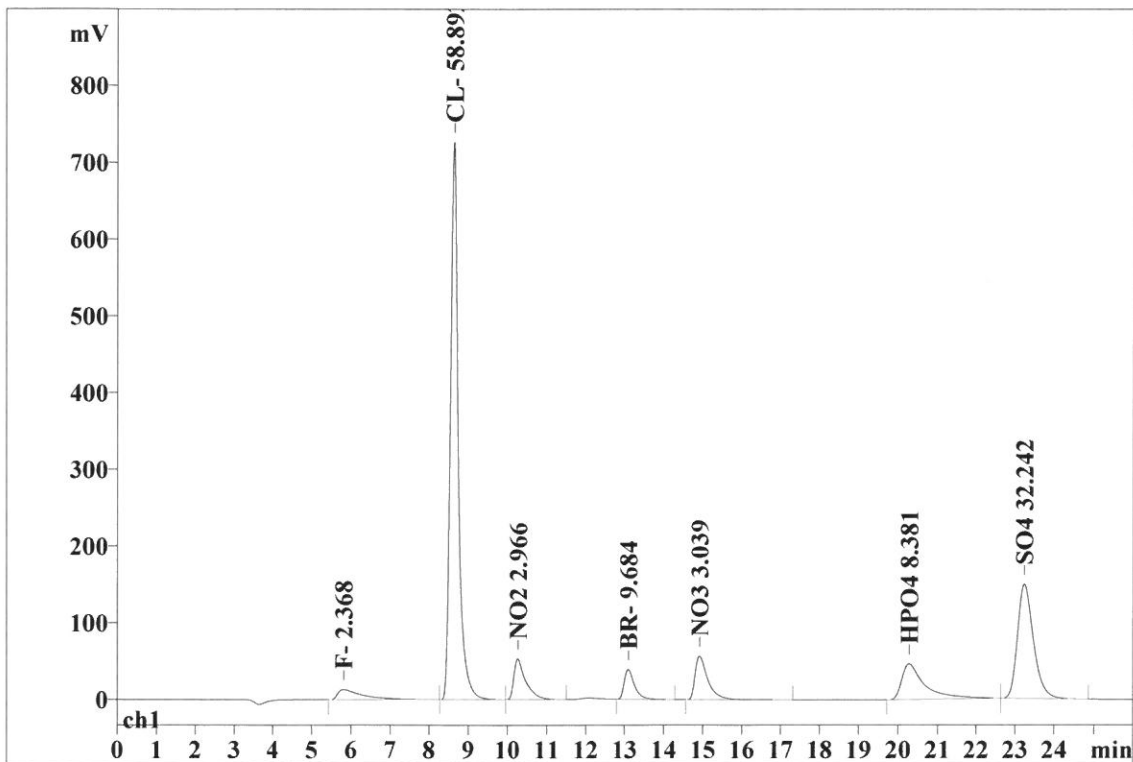

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.81	0.590	13.23	1.22	580.736	2.92
2	8.61	0.194	726.60	67.02	10034.327	50.48
3	10.27	0.292	52.91	4.88	1103.718	5.55
4	13.09	0.267	38.84	3.58	709.470	3.57
5	14.92	0.329	56.64	5.22	1290.157	6.49
6	20.28	0.525	46.60	4.30	1905.955	9.59
7	23.23	0.428	149.27	13.77	4251.906	21.39
7	26.00	0.375	1084.09	100.00	19876.268	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/31/2021 3:16:43 PM
Printed by: wet


Ident: CCV
Analysis from: 8/31/2021 1:56:53 PM
File: _2021-08-31_

Last save: 8/31/2021 2:23:49 PM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 28045

Last save: 8/31/2021 9:16:

SAMPLE:
: AP/MA
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

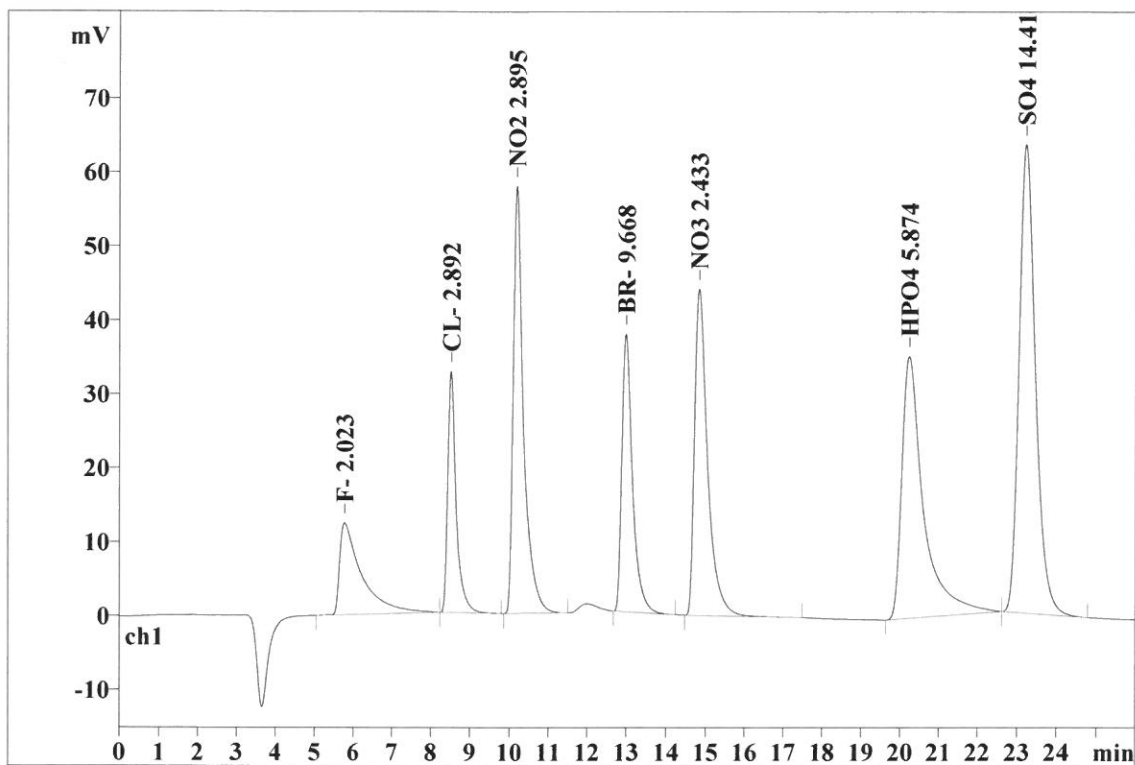

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.77	0.517	12.42	4.38	493.141	7.05
2	8.50	0.203	32.64	11.52	480.020	6.86
3	10.18	0.256	57.75	20.38	1075.941	15.38
4	12.98	0.275	37.58	13.26	708.245	10.12
5	14.83	0.335	44.14	15.58	1022.954	14.62
6	20.23	0.509	35.43	12.50	1370.845	19.59
7	23.22	0.438	63.41	22.38	1845.084	26.37
7	26.00	0.362	283.36	100.00	6996.231	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/31/2021 3:16:50 PM
Printed by: wet


Ident: CCB
Analysis from: 8/31/2021 2:25:29 PM
File: _2021-08-31_

Last save: 8/31/2021 2:51:29 PM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 28046

Last save: 8/31/2021 9:16:

SAMPLE:
: AP/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

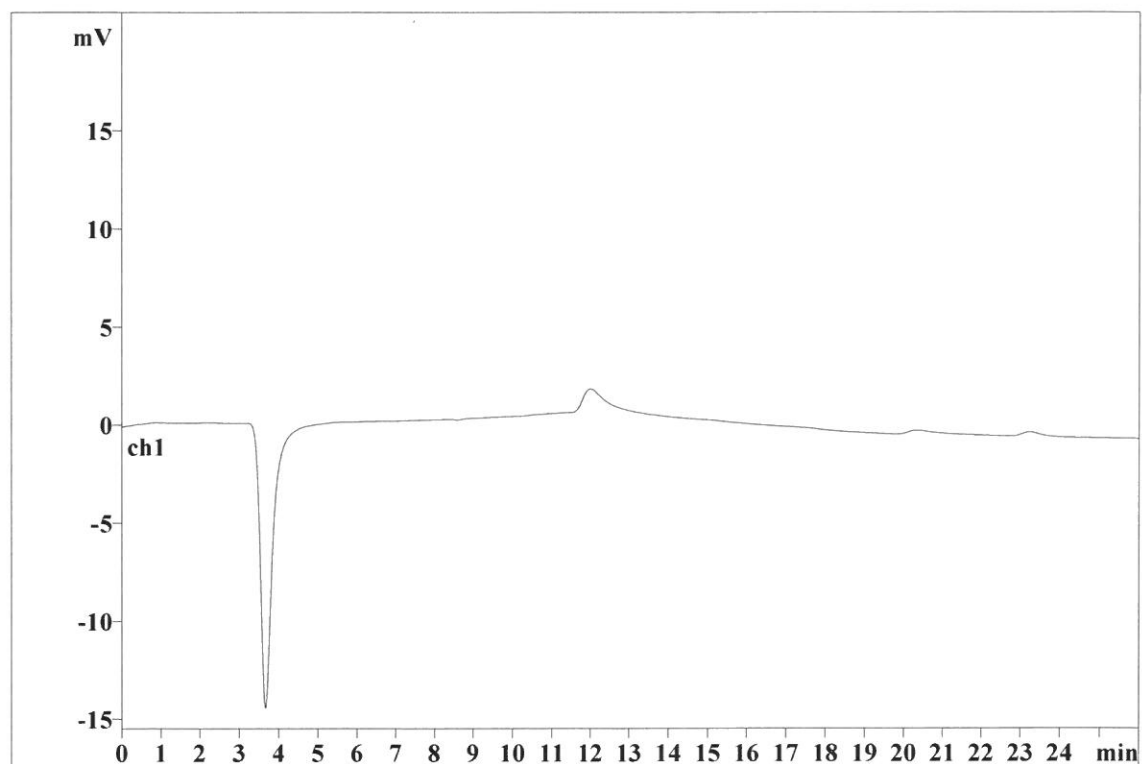

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD