


LB116099

7470A

INSTRUMENT ID: CV1

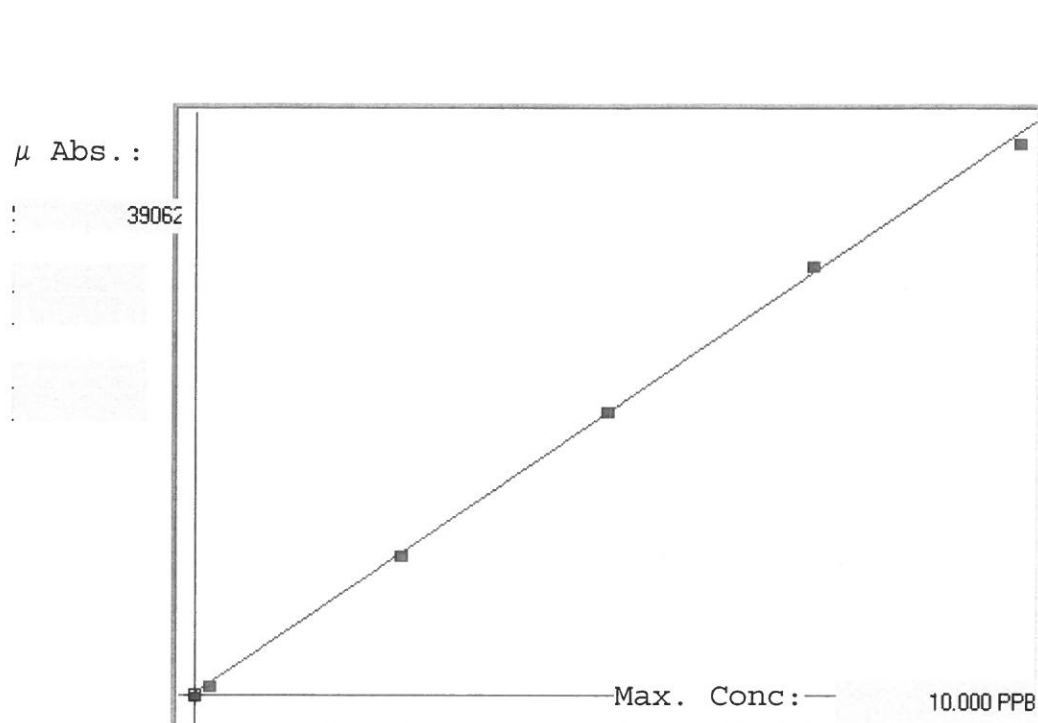

A= 0.0000e+000

B= 2.5287e-004

C= -2.2087e-002

Rho= 0.9996894

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	0/0/0
0.0	0.000	-0.023	-0.023	-4	0.000	-4					-11
0.2	0.200	0.179	-0.021	794	0.0 %	794					-1
2.5	2.500	2.482	-0.018	9903	0.0 %	9903					1
5.0	5.000	5.043	0.043	20031	0.0 %	20031					2
7.5	7.500	7.663	0.163	30393	0.0 %	30393					-1
10.0	10.000	9.856	-0.144	39062	0.0 %	39062					

LB116099 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 01 Sep 2021 09:19:41

Sample ID	Extended ID	μ Abs.	Conc.	Std Cond	Method	Units	Date	Type	Type
0.0 - 1	50	-4	-	0.0000	7470A	PPB	01 Sep 2021 09:28:30	S	Std
0.2 - 1	50.2	794	-	0.2000	7470A	PPB	01 Sep 2021 09:34:10	S	Std
2.5 - 1	52.5	9903	-	2.5000	7470A	PPB	01 Sep 2021 09:36:27	S	Std
5.0 - 1	55	20031	-	5.0000	7470A	PPB	01 Sep 2021 09:38:44	S	Std
7.5 - 1	57.5	30393	-	7.5000	7470A	PPB	01 Sep 2021 09:41:01	S	Std
10.0 - 1	510	39062	-	10.0000	7470A	PPB	01 Sep 2021 09:45:56	S	Std
ICV76 - 1	ICV76	14996	3.7700	-	7470A	PPB	01 Sep 2021 09:48:39	U	SMPL
ICB76 - 1	ICB76	-19	-0.0269	-	7470A	PPB	01 Sep 2021 09:50:53	U	SMPL
CCV70 - 1	CCV70	19672	4.9524	-	7470A	PPB	01 Sep 2021 09:53:08	U	SMPL
CCB70 - 1	CCB70	-33	-0.0304	-	7470A	PPB	01 Sep 2021 09:55:22	U	SMPL
CRA - 1	CRA	778	0.1746	-	7470A	PPB	01 Sep 2021 09:57:38	U	SMPL
HighStd - 1	HighStd	39465	9.9575	-	7470A	PPB	01 Sep 2021 09:59:52	U	SMPL
ChkStd - 1	ChkStd	28516	7.1888	-	7470A	PPB	01 Sep 2021 10:02:07	U	SMPL
PB138851BL - 1	PBW	-83	-0.0431	-	7470A	PPB	01 Sep 2021 10:04:24	U	SMPL
PB138851BS - 1	LCSW	16161	4.0646	-	7470A	PPB	01 Sep 2021 10:06:40	U	SMPL
M3571-02 - 1	BL-1	-19	-0.0269	-	7470A	PPB	01 Sep 2021 10:08:57	U	SMPL
M3578-01 - 1	CULVER-AVE-PAINT-CHIPS	61	-0.0067	-	7470A	PPB	01 Sep 2021 10:11:13	U	SMPL
M3593-02 - 1	ETGI-280	40	-0.0120	-	7470A	PPB	01 Sep 2021 10:13:30	U	SMPL
M3597-02 - 1	RO-124030	52	-0.0089	-	7470A	PPB	01 Sep 2021 10:15:47	U	SMPL
M3597-04 - 1	RO-PSC124042	36	-0.0130	-	7470A	PPB	01 Sep 2021 10:18:02	U	SMPL
CCV71 - 1	CCV71	19869	5.0022	-	7470A	PPB	01 Sep 2021 10:20:17	U	SMPL
CCB71 - 1	CCB71	-26	-0.0287	-	7470A	PPB	01 Sep 2021 10:22:33	U	SMPL
M3602-10 - 1	TP-1COMP	47	-0.0102	-	7470A	PPB	01 Sep 2021 10:24:48	U	SMPL
M3602-10DUP - 1	TP-1COMPDUP	25	-0.0158	-	7470A	PPB	01 Sep 2021 10:27:04	U	SMPL
M3602-10MS - 1	TP-1COMPMS	14785	3.7166	-	7470A	PPB	01 Sep 2021 10:29:19	U	SMPL
M3602-10MSD - 1	TP-1COMPMSD	15404	3.8732	-	7470A	PPB	01 Sep 2021 10:31:35	U	SMPL
PB138852BL - 1	PBW	-27	-0.0289	-	7470A	PPB	01 Sep 2021 10:33:50	U	SMPL
PB138852BS - 1	LCSW	15649	3.9351	-	7470A	PPB	01 Sep 2021 10:36:06	U	SMPL
M3603-01 - 1	TRE-1242	-22	-0.0276	-	7470A	PPB	01 Sep 2021 10:38:22	U	SMPL
M3603-01DUP - 1	TRE-1242DUP	30	-0.0145	-	7470A	PPB	01 Sep 2021 10:40:39	U	SMPL
M3603-01MS - 1	TRE-1242MS	15996	4.0229	-	7470A	PPB	01 Sep 2021 10:42:56	U	SMPL
M3603-01MSD - 1	TRE-1242MSD	14843	3.7313	-	7470A	PPB	01 Sep 2021 10:45:11	U	SMPL
CCV72 - 1	CCV72	19873	5.0032	-	7470A	PPB	01 Sep 2021 10:47:27	U	SMPL
CCB72 - 1	CCB72	-25	-0.0284	-	7470A	PPB	01 Sep 2021 10:49:42	U	SMPL
M3603-03 - 1	TRE-1243-TRE-1244	28	-0.0150	-	7470A	PPB	01 Sep 2021 10:51:58	U	SMPL
PB138853BL - 1	PBW	30	-0.0145	-	7470A	PPB	01 Sep 2021 10:54:13	U	SMPL
PB138853BS - 1	LCSW	13707	3.4440	-	7470A	PPB	01 Sep 2021 10:56:28	U	SMPL
M3577-03 - 1	FIELD-BLANK	-19	-0.0269	-	7470A	PPB	01 Sep 2021 10:58:44	U	SMPL
M3584-16 - 1	FB02-20210827	51	-0.0092	-	7470A	PPB	01 Sep 2021 11:00:59	U	SMPL
M3606-01 - 1	BPU-1	45	-0.0107	-	7470A	PPB	01 Sep 2021 11:03:15	U	SMPL
M3606-02 - 1	BPU-2	40	-0.0120	-	7470A	PPB	01 Sep 2021 11:05:31	U	SMPL
M3606-02DUP - 1	BPU-2DUP	52	-0.0089	-	7470A	PPB	01 Sep 2021 11:07:48	U	SMPL
M3606-03 - 1	M3606-02MS	16855	4.2401	-	7470A	PPB	01 Sep 2021 11:10:05	U	SMPL
M3606-04 - 1	M3606-02MSD	15451	3.8850	-	7470A	PPB	01 Sep 2021 11:12:21	U	SMPL
CCV73 - 1	CCV73	19862	5.0005	-	7470A	PPB	01 Sep 2021 11:14:36	U	SMPL
CCB73 - 1	CCB73	-36	-0.0312	-	7470A	PPB	01 Sep 2021 11:16:51	U	SMPL
M3606-05 - 1	BPU-BFD	17	-0.0178	-	7470A	PPB	01 Sep 2021 11:19:07	U	SMPL
M3607-01 - 1	20211021-SITE-WATER	106	0.0047	-	7470A	PPB	01 Sep 2021 11:21:24	U	SMPL
M3607-02 - 1	20211022-FIELD-BLANK	50	-0.0094	-	7470A	PPB	01 Sep 2021 11:23:40	U	SMPL
PB138851TB - 1	PB138803TB	36	-0.0130	-	7470A	PPB	01 Sep 2021 11:25:56	U	SMPL
PB138852TB - 1	PB138833TB	43	-0.0112	-	7470A	PPB	01 Sep 2021 11:28:13	U	SMPL
CCV74 - 1	CCV74	20189	5.0832	-	7470A	PPB	01 Sep 2021 11:30:30	U	SMPL
CCB74 - 1	CCB74	-35	-0.0309	-	7470A	PPB	01 Sep 2021 11:32:47	U	SMPL
M3602-10LX5 - 1		4	-0.0211	-	7470A	PPB	01 Sep 2021 11:35:03	U	SMPL
M3602-10A - 1		16459	4.1399	-	7470A	PPB	01 Sep 2021 11:37:20	U	SMPL
M3603-01LX5 - 1		-46	-0.0337	-	7470A	PPB	01 Sep 2021 11:39:35	U	SMPL
M3603-01A - 1		15728	3.9551	-	7470A	PPB	01 Sep 2021 11:41:51	U	SMPL
M3606-02LX5 - 1		-42	-0.0327	-	7470A	PPB	01 Sep 2021 11:44:06	U	SMPL
M3606-02A - 1		16331	4.1076	-	7470A	PPB	01 Sep 2021 11:46:21	U	SMPL
CCV75 - 1	CCV75	19844	4.9959	-	7470A	PPB	01 Sep 2021 11:48:37	U	SMPL
CCB75 - 1	CCB75	-32	-0.0302	-	7470A	PPB	01 Sep 2021 11:50:53	U	SMPL