

LB3116108

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : mb Instrument ID : Konelab

9/1/2021 14:21

Test: Phenolics- mb

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.057	0.0	0.114	
ICB1	0.001	0.0	0.005	
CCV1	1.054	0.0	0.114	
CCB1	0.002	0.0	0.005	
PB138868BL	0.002	0.0	0.005	
PB138868BS	1.072	0.0	0.116	
M3610-01	0.024	0.0	0.007	
M3610-01DUP	0.025	0.0	0.007	
M3610-01MS	1.041	0.0	0.113	
M3610-01MSD	1.057	0.0	0.114	
M3610-02	0.003	0.0	0.005	
CCV2	1.053	0.0	0.114	
CCB2	0.001	0.0	0.005	

N	13
Mean	0.492
SD	0.5434
CV%	110.53

Aquakem v. 7.2AQ1

Results from time period:

Wed Sep 01 13:41:50 2021

Wed Sep 01 14:13:12 2021

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	0.0018	mg/l	9/1/2021 13:41:50	
0.05PPM	A	Phenolics-	P	0.051	mg/l	9/1/2021 13:41:51	
0.1PPM	A	Phenolics-	P	0.1022	mg/l	9/1/2021 13:41:52	
0.25PPM	A	Phenolics-	P	0.2543	mg/l	9/1/2021 13:41:53	
0.50PPM	A	Phenolics-	P	0.4976	mg/l	9/1/2021 13:41:54	
1.0PPM	A	Phenolics-	P	0.9863	mg/l	9/1/2021 13:41:55	
2.0PPM	A	Phenolics-	P	2.0068	mg/l	9/1/2021 13:41:56	
ICV1	S	Phenolics-	P	1.0567	mg/l	9/1/2021 14:07:18	
ICB1	S	Phenolics-	P	0.0008	mg/l	9/1/2021 14:07:19	
CCV1	S	Phenolics-	P	1.0538	mg/l	9/1/2021 14:07:22	
CCB1	S	Phenolics-	P	0.002	mg/l	9/1/2021 14:07:23	
PB138868BL	S	Phenolics-	P	0.002	mg/l	9/1/2021 14:07:25	
PB138868BS	S	Phenolics-	P	1.0723	mg/l	9/1/2021 14:07:27	
M3610-01	S	Phenolics-	P	0.0241	mg/l	9/1/2021 14:07:28	
M3610-01DUP	S	Phenolics-	P	0.0255	mg/l	9/1/2021 14:13:07	
M3610-01MS	S	Phenolics-	P	1.0406	mg/l	9/1/2021 14:13:08	
M3610-01MSD	S	Phenolics-	P	1.0566	mg/l	9/1/2021 14:13:09	
M3610-02	S	Phenolics-	P	0.0028	mg/l	9/1/2021 14:13:10	
CCV2	S	Phenolics-	P	1.053	mg/l	9/1/2021 14:13:11	
CCB2	S	Phenolics-	P	0.0015	mg/l	9/1/2021 14:13:12	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

9/1/2021 13:42

Reviewed by : AS

Instrument ID : Konelab


Test Phenolics-

Accepted 9/1/2021 13:42

Factor 9.656
Bias 0.005

Coeff. of det. 0.999915

Errors

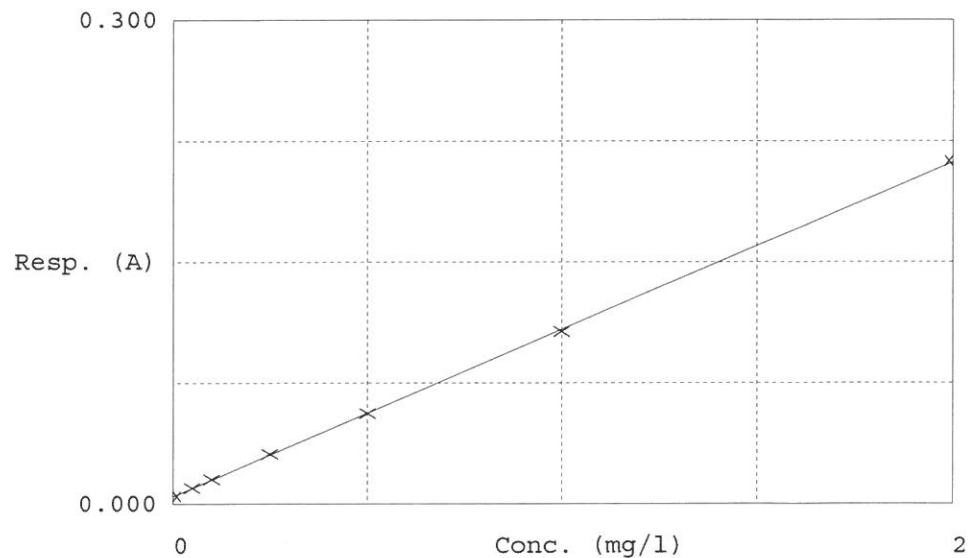

	Calibrator	Response	Calc. con.	Conc.	Del. Errors
1	0.00PPM	0.005	0.0018	0.0000	2.0
2	Phenol-2	0.010	0.0510	0.0500	2.2
3	Phenol-2	0.015	0.1022	0.1000	1.7
4	Phenol-2	0.031	0.2543	0.2500	-0.5
5	Phenol-2	0.056	0.4976	0.5000	-1.4
6	Phenol-2	0.107	0.9863	1.0000	0.3
7	Phenol-2	0.213	2.0068	2.0000	

AS 9/1/21