


LB116109

7470A

INSTRUMENT ID: CV2

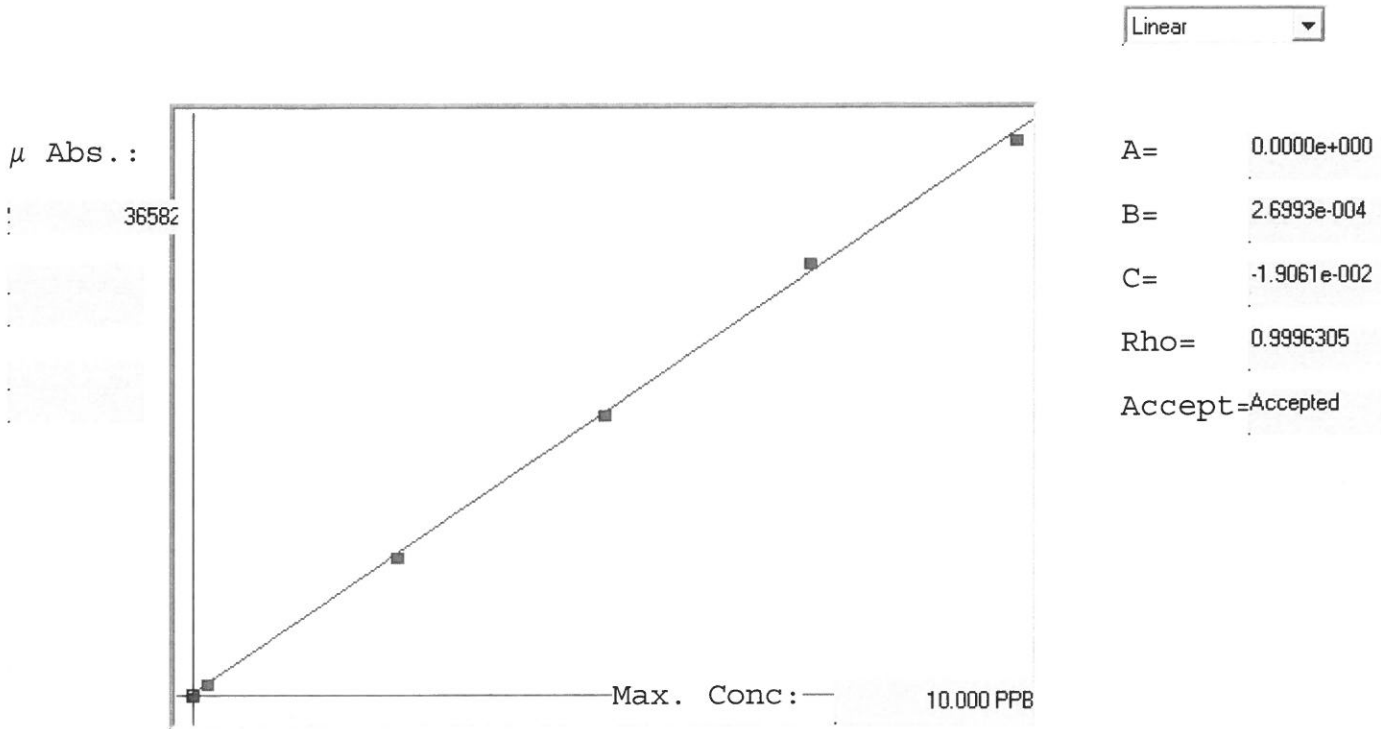

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	0/0/1
0.0	0.000	-0.007	-0.007	46	0.000	46					-6
0.2	0.200	0.189	-0.011	772	0.0 %	772					-1
2.5	2.500	2.464	-0.036	9199	0.0 %	9199					0
5.0	5.000	5.003	0.003	18604	0.0 %	18604					3
7.5	7.500	7.695	0.195	28578	0.0 %	28578					-1
10.0	10.000	9.856	-0.144	36582	0.0 %	36582					

LB116109 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 01 Sep 2021 15:14:09

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	46	-	0.0000	7470A	PPB	01 Sep 2021 15:15:31	S	Std
0.2 - 1	50.2	772	-	0.2000	7470A	PPB	01 Sep 2021 15:17:47	S	Std
2.5 - 1	52.5	9199	-	2.5000	7470A	PPB	01 Sep 2021 15:20:04	S	Std
5.0 - 1	55	18604	-	5.0000	7470A	PPB	01 Sep 2021 15:22:21	S	Std
7.5 - 1	57.5	28578	-	7.5000	7470A	PPB	01 Sep 2021 15:24:37	S	Std
10.0 - 1	510	36582	-	10.0000	7470A	PPB	01 Sep 2021 15:29:23	S	Std
ICV78 - 1	ICV78	15575	4.1851	-	7470A	PPB	01 Sep 2021 15:32:07	U	SMPL
ICB78 - 1	ICB78	-38	-0.0293	-	7470A	PPB	01 Sep 2021 15:34:22	U	SMPL
CCV79 - 1	CCV79	18687	5.0251	-	7470A	PPB	01 Sep 2021 15:36:36	U	SMPL
CCB79 - 1	CCB79	-32	-0.0277	-	7470A	PPB	01 Sep 2021 15:38:52	U	SMPL
CRA - 1	CRA	759	0.1858	-	7470A	PPB	01 Sep 2021 15:41:06	U	SMPL
HighStd - 1	HighStd	36110	9.7281	-	7470A	PPB	01 Sep 2021 15:43:21	U	SMPL
ChkStd - 1	ChkStd	26369	7.0987	-	7470A	PPB	01 Sep 2021 15:45:36	U	SMPL
PB138873BL - 1	PBW	-57	-0.0344	-	7470A	PPB	01 Sep 2021 15:47:53	U	SMPL
PB138873BS - 1	LCSW	15009	4.0323	-	7470A	PPB	01 Sep 2021 15:50:10	U	SMPL
M3611-01 - 1	NWB-1528	80	0.0025	-	7470A	PPB	01 Sep 2021 15:52:27	U	SMPL
M3611-03 - 1	NWB-1601	8	-0.0169	-	7470A	PPB	01 Sep 2021 15:54:43	U	SMPL
M3611-03DUP - 1	NWB-1601DUP	23	-0.0129	-	7470A	PPB	01 Sep 2021 15:57:00	U	SMPL
M3611-03MS - 1	NWB-1601MS	15423	4.1441	-	7470A	PPB	01 Sep 2021 15:59:17	U	SMPL
M3611-03MSD - 1	NWB-1601MSD	14664	3.9392	-	7470A	PPB	01 Sep 2021 16:01:33	U	SMPL
CCV80 - 1	CCV80	18764	5.0459	-	7470A	PPB	01 Sep 2021 16:03:48	U	SMPL
CCB80 - 1	CCB80	-37	-0.0290	-	7470A	PPB	01 Sep 2021 16:06:04	U	SMPL
PB138873TB - 1	PB138803TB	44	-0.0072	-	7470A	PPB	01 Sep 2021 16:08:18	U	SMPL
M3611-03LX5 - 1		48	-0.0061	-	7470A	PPB	01 Sep 2021 16:10:34	U	SMPL
M3611-03A - 1		15139	4.0674	-	7470A	PPB	01 Sep 2021 16:12:49	U	SMPL
CCV81 - 1	CCV81	18383	4.9431	-	7470A	PPB	01 Sep 2021 16:15:04	U	SMPL
CCB81 - 1	CCB81	298	0.0614	-	7470A	PPB	01 Sep 2021 16:17:20	U	SMPL
CCB81 - 1	CCB81	45	-0.0069	-	7470A	PPB	01 Sep 2021 16:21:06	U	SMPL