


LB116119

7471B

INSTRUMENT ID: CV2

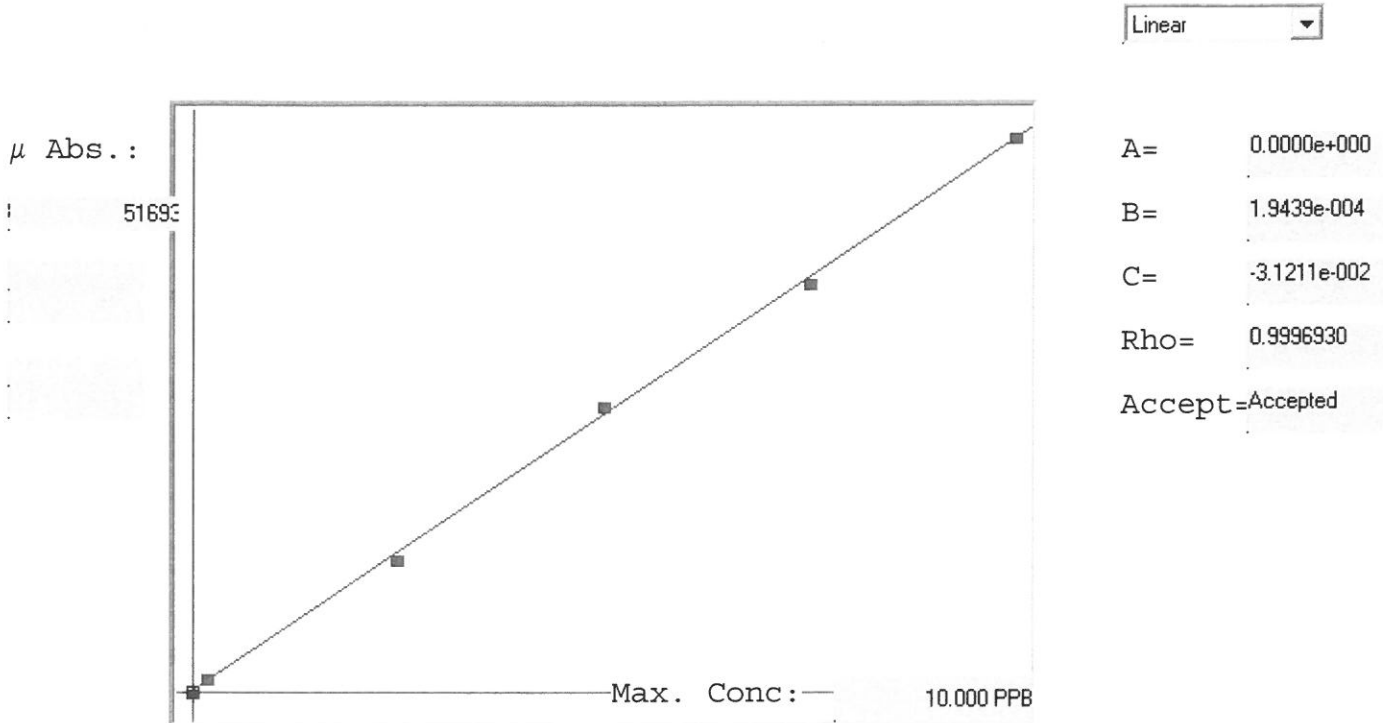

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	-0.009	-0.009	112	0.000	112					-
0.2	0.200	0.238	0.038	1387	0.0 %	1387					19
2.5	2.500	2.396	-0.104	12484	0.0 %	12484					-4
5.0	5.000	5.163	0.163	26718	0.0 %	26718					3
7.5	7.500	7.395	-0.105	38204	0.0 %	38204					-1
10.0	10.000	10.018	0.018	51693	0.0 %	51693					0

LB116119 INSTRUMENT ID : CV1

Method: 7471B		Operator: Admin		Date of Analysis: 02 Sep 2021 11:23:31					
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	112	-	0.0000	7471B	PPB	02 Sep 2021 11:27:45	S	Std
0.2 - 1	50.2	1387	-	0.2000	7471B	PPB	02 Sep 2021 11:30:02	S	Std
2.5 - 1	52.5	12484	-	2.5000	7471B	PPB	02 Sep 2021 11:32:19	S	Std
5.0 - 1	55	26718	-	5.0000	7471B	PPB	02 Sep 2021 11:34:36	S	Std
7.5 - 1	57.5	38204	-	7.5000	7471B	PPB	02 Sep 2021 11:36:52	S	Std
10.0 - 1	511	51693	-	10.0000	7471B	PPB	02 Sep 2021 11:42:09	S	Std
ICV80 - 1	ICV80	20112	3.8784	-	7471B	PPB	02 Sep 2021 11:44:49	U	SMPL
ICB80 - 1	ICB80	41	-0.0232	-	7471B	PPB	02 Sep 2021 11:47:03	U	SMPL
CCV82 - 1	CCV82	26729	5.1647	-	7471B	PPB	02 Sep 2021 11:49:18	U	SMPL
CCB82 - 1	CCB82	42	-0.0230	-	7471B	PPB	02 Sep 2021 11:51:33	U	SMPL
CRA - 1	CRA	1277	0.2170	-	7471B	PPB	02 Sep 2021 11:56:21	U	SMPL
HighStd - 1	HighStd	51435	9.9674	-	7471B	PPB	02 Sep 2021 11:58:36	U	SMPL
ChkStd - 1	ChkStd	36414	7.0474	-	7471B	PPB	02 Sep 2021 12:00:52	U	SMPL
PB138890BL - 1	pbs	41	-0.0232	-	7471B	PPB	02 Sep 2021 12:03:08	U	SMPL
PB138890BS - 1	lcss	22804	4.4017	-	7471B	PPB	02 Sep 2021 12:05:25	U	SMPL
M3609-01 - 1	EO-01-083121	3679	0.6840	-	7471B	PPB	02 Sep 2021 12:07:42	U	SMPL
M3609-01DUP - 1	EO-01-083121DUP	3573	0.6634	-	7471B	PPB	02 Sep 2021 12:09:58	U	SMPL
M3609-01MS - 1	EO-01-083121MS	23716	4.5790	-	7471B	PPB	02 Sep 2021 12:12:15	U	SMPL
M3609-01MSD - 1	EO-01-083121MSD	25378	4.9021	-	7471B	PPB	02 Sep 2021 12:14:32	U	SMPL
M3609-03 - 1	EO-03-083121	5643	1.0657	-	7471B	PPB	02 Sep 2021 12:16:47	U	SMPL
CCV83 - 1	CCV83	26810	5.1805	-	7471B	PPB	02 Sep 2021 12:19:02	U	SMPL
CCB83 - 1	CCB83	40	-0.0234	-	7471B	PPB	02 Sep 2021 12:21:17	U	SMPL
M3612-01 - 1	M-1	1333	0.2279	-	7471B	PPB	02 Sep 2021 12:23:32	U	SMPL
M3614-01 - 1	NB-8-083121	1842	0.3269	-	7471B	PPB	02 Sep 2021 12:25:47	U	SMPL
M3615-01 - 1	TPR-10-COMP	779	0.1202	-	7471B	PPB	02 Sep 2021 12:28:03	U	SMPL
M3616-01 - 1	CL-01-083121	4148	0.7751	-	7471B	PPB	02 Sep 2021 12:30:19	U	SMPL
M3624-01 - 1	HD-01-090121	2319	0.4196	-	7471B	PPB	02 Sep 2021 12:32:34	U	SMPL
M3626-01 - 1	G-1	932	0.1500	-	7471B	PPB	02 Sep 2021 12:34:51	U	SMPL
M3634-01 - 1	OK-01-090121	1268	0.2153	-	7471B	PPB	02 Sep 2021 12:37:08	U	SMPL
M3634-03 - 1	OK-02-090121	1640	0.2876	-	7471B	PPB	02 Sep 2021 12:39:25	U	SMPL
M3636-01 - 1	SA-01-090121	3241	0.5988	-	7471B	PPB	02 Sep 2021 12:41:42	U	SMPL
CCV84 - 1	CCV84	26483	5.1169	-	7471B	PPB	02 Sep 2021 12:43:58	U	SMPL
CCB84 - 1	CCB84	54	-0.0207	-	7471B	PPB	02 Sep 2021 12:46:13	U	SMPL
M3609-01LX5 - 1		759	0.1163	-	7471B	PPB	02 Sep 2021 12:48:29	U	SMPL
M3609-01A - 1		24429	4.7176	-	7471B	PPB	02 Sep 2021 12:50:45	U	SMPL
CCV85 - 1	CCV85	26923	5.2024	-	7471B	PPB	02 Sep 2021 12:53:00	U	SMPL
CCB85 - 1	CCB85	48	-0.0219	-	7471B	PPB	02 Sep 2021 12:55:16	U	SMPL