


LB116141

7470A

INSTRUMENT ID: CV1

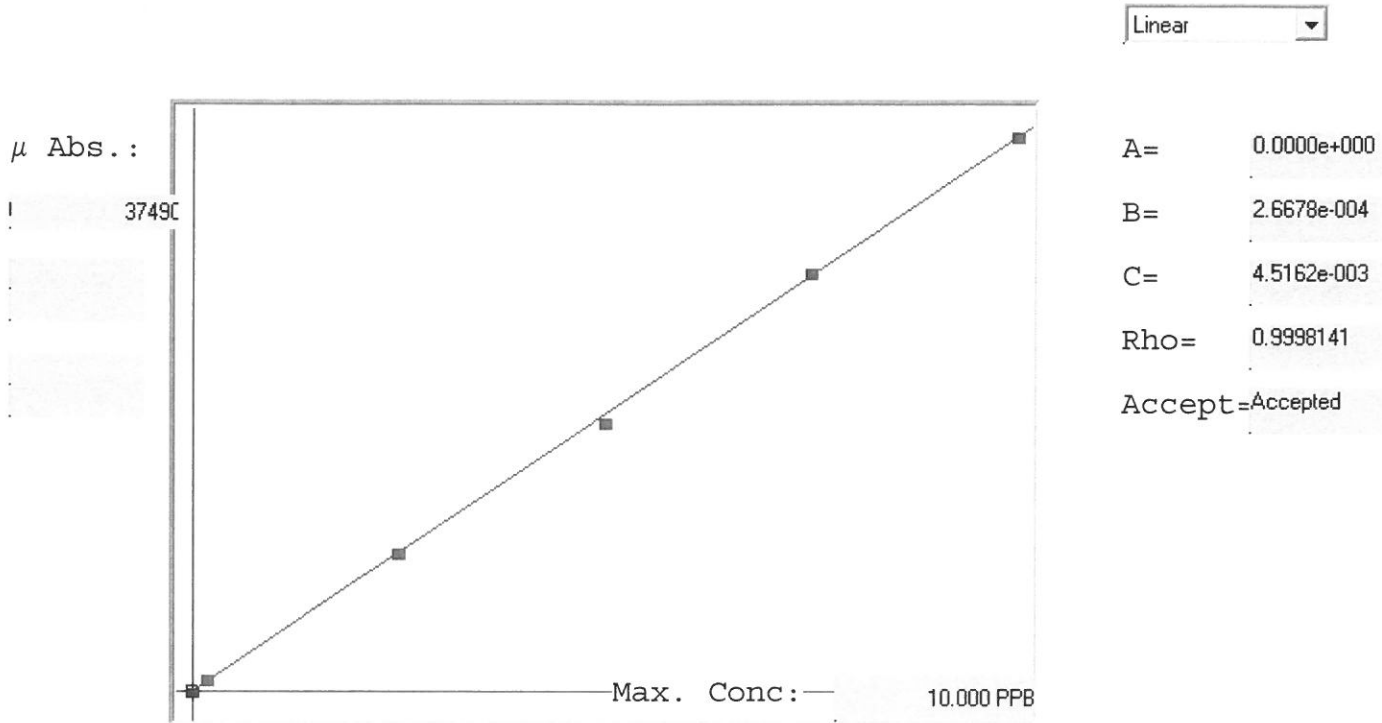

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	0/0D
0.0	0.000	0.026	0.026	82	0.000	82					6
0.2	0.200	0.213	0.013	781	0.0 %	781					1
2.5	2.500	2.526	0.026	9451	0.0 %	9451					-3
5.0	5.000	4.850	-0.150	18162	0.0 %	18162					1
7.5	7.500	7.579	0.079	28392	0.0 %	28392					0
10.0	10.000	10.006	0.006	37490	0.0 %	37490					

LB116141 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 03 Sep 2021 08:57:15

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	82	-	0.0000	7470A	PPB	03 Sep 2021 09:48:35	S	Std
0.2 - 1	50.2	781	-	0.2000	7470A	PPB	03 Sep 2021 09:50:52	S	Std
2.5 - 1	52.5	9451	-	2.5000	7470A	PPB	03 Sep 2021 09:53:09	S	Std
5.0 - 1	55	18162	-	5.0000	7470A	PPB	03 Sep 2021 09:55:26	S	Std
7.5 - 1	57.5	28392	-	7.5000	7470A	PPB	03 Sep 2021 09:57:42	S	Std
10.0 - 1	59.6	37490	-	10.0000	7470A	PPB	03 Sep 2021 10:02:33	S	Std
ICV81 - 1	ICV81	15207	4.0615	-	7470A	PPB	03 Sep 2021 10:05:14	U	SMPL
ICB81 - 1	ICB81	9	0.0069	-	7470A	PPB	03 Sep 2021 10:07:29	U	SMPL
CCV90 - 1	CCV90	18545	4.9520	-	7470A	PPB	03 Sep 2021 10:09:44	U	SMPL
CCB90 - 1	CCB90	18	0.0093	-	7470A	PPB	03 Sep 2021 10:12:00	U	SMPL
CRA - 1	CRA	794	0.2163	-	7470A	PPB	03 Sep 2021 10:14:15	U	SMPL
HighStd - 1	HighStd	37931	10.1238	-	7470A	PPB	03 Sep 2021 10:16:30	U	SMPL
ChkStd - 1	ChkStd	27366	7.3052	-	7470A	PPB	03 Sep 2021 10:18:45	U	SMPL
PB138914BL - 1	PBW	-30	-0.0035	-	7470A	PPB	03 Sep 2021 10:21:02	U	SMPL
PB138914BS - 1	LCSW	15926	4.2533	-	7470A	PPB	03 Sep 2021 10:23:18	U	SMPL
M3545-05 - 1	NCS-COMP-2	10	0.0072	-	7470A	PPB	03 Sep 2021 10:25:34	U	SMPL
M3545-05DUP - 1	NCS-COMP-2DUP	37	0.0144	-	7470A	PPB	03 Sep 2021 10:27:50	U	SMPL
M3545-05MS - 1	NCS-COMP-2MS	16382	4.3749	-	7470A	PPB	03 Sep 2021 10:30:07	U	SMPL
M3545-05MSD - 1	NCS-COMP-2MSD	14978	4.0004	-	7470A	PPB	03 Sep 2021 10:32:23	U	SMPL
PB138915BL - 1	PBW	-3	0.0037	-	7470A	PPB	03 Sep 2021 10:34:39	U	SMPL
CCV91 - 1	CCV91	18541	4.9509	-	7470A	PPB	03 Sep 2021 10:36:54	U	SMPL
CCB91 - 1	CCB91	9	0.0069	-	7470A	PPB	03 Sep 2021 10:39:10	U	SMPL
PB138915BS - 1	LCSW	14187	3.7893	-	7470A	PPB	03 Sep 2021 10:41:25	U	SMPL
M3646-11 - 1	2105	281	0.0795	-	7470A	PPB	03 Sep 2021 10:43:40	U	SMPL
M3646-13 - 1	1992	201	0.0581	-	7470A	PPB	03 Sep 2021 10:45:56	U	SMPL
M3646-14 - 1	06-07-24	212	0.0611	-	7470A	PPB	03 Sep 2021 10:48:12	U	SMPL
M3646-15 - 1	99-01	160	0.0472	-	7470A	PPB	03 Sep 2021 10:50:28	U	SMPL
M3646-16 - 1	93-94	179	0.0523	-	7470A	PPB	03 Sep 2021 10:52:44	U	SMPL
M3646-16DUP - 1	93-94DUP	196	0.0568	-	7470A	PPB	03 Sep 2021 10:55:01	U	SMPL
M3646-16MS - 1	93-94MS	14641	3.9105	-	7470A	PPB	03 Sep 2021 10:57:18	U	SMPL
M3646-16MSD - 1	93-94MSD	14800	3.9529	-	7470A	PPB	03 Sep 2021 10:59:35	U	SMPL
CCV92 - 1	CCV92	18023	4.8127	-	7470A	PPB	03 Sep 2021 11:01:50	U	SMPL
CCB92 - 1	CCB92	-3	0.0037	-	7470A	PPB	03 Sep 2021 11:04:05	U	SMPL
PB138914TB - 1	PB138859TB	34	0.0136	-	7470A	PPB	03 Sep 2021 11:06:21	U	SMPL
PB138915TB - 1	PB138913TB	49	0.0176	-	7470A	PPB	03 Sep 2021 11:08:37	U	SMPL
M3545-05LX5 - 1		12	0.0077	-	7470A	PPB	03 Sep 2021 11:10:53	U	SMPL
M3545-05A - 1		15318	4.0911	-	7470A	PPB	03 Sep 2021 11:13:08	U	SMPL
M3646-16LX5 - 1		3	0.0053	-	7470A	PPB	03 Sep 2021 11:15:24	U	SMPL
M3646-16A - 1		14195	3.7915	-	7470A	PPB	03 Sep 2021 11:17:40	U	SMPL
CCV93 - 1	CCV93	18202	4.8605	-	7470A	PPB	03 Sep 2021 11:19:56	U	SMPL
CCB93 - 1	CCB93	9	0.0069	-	7470A	PPB	03 Sep 2021 11:22:12	U	SMPL