


LB 116156

7470A

INSTRUMENT ID: CV1

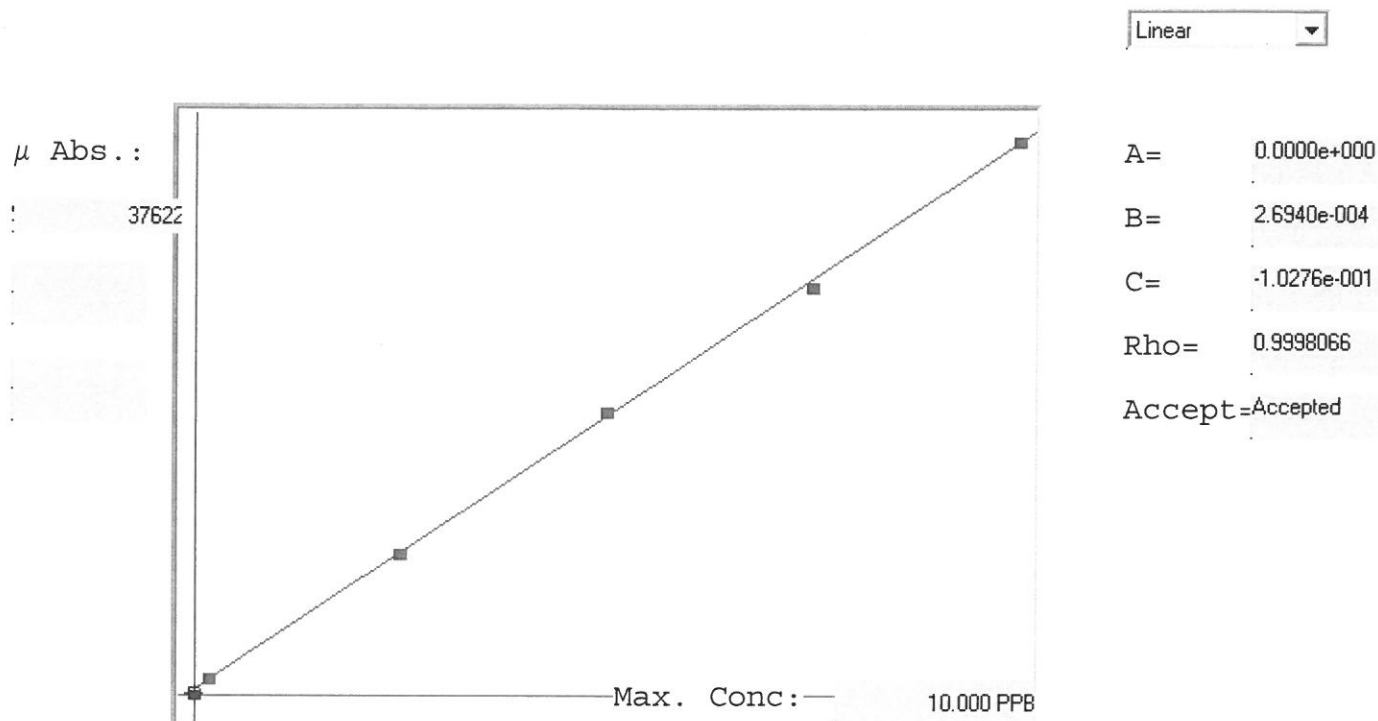

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	-0.041	-0.041	229	0.000	229					11
0.2	0.200	0.222	0.022	1206	0.0 %	1206					0
2.5	2.500	2.495	-0.005	9641	0.0 %	9641					2
5.0	5.000	5.115	0.115	19367	0.0 %	19367					-2
7.5	7.500	7.377	-0.123	27764	0.0 %	27764					0
10.0	10.000	10.033	0.033	37622	0.0 %	37622					

LB116156 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 03 Sep 2021 15:38:50

Sample ID	Extended ID	μ Abs	Conc	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	229	-	0.0007470A	PPB		03 Sep 2021 15:43:31	S	Std
0.2 - 1	50.2	1206	-	0.2007470A	PPB		03 Sep 2021 15:45:49	S	Std
2.5 - 1	52.5	9641	-	2.5007470A	PPB		03 Sep 2021 15:48:06	S	Std
5.0 - 1	55	19367	-	5.0007470A	PPB		03 Sep 2021 15:50:22	S	Std
7.5 - 1	57.5	27764	-	7.5007470A	PPB		03 Sep 2021 15:52:38	S	Std
10.0 - 1	50	37622	-	10.0007470A	PPB		03 Sep 2021 15:54:54	S	Std
ICV82 - 1	ICV82	13845	3.6271	-7470A	PPB		03 Sep 2021 15:58:08	U	SMPL
ICB82 - 1	ICB82	112	-0.0726	-7470A	PPB		03 Sep 2021 16:00:24	U	SMPL
CCV01 - 1	CCV01	17951	4.7333	-7470A	PPB		03 Sep 2021 16:02:38	U	SMPL
CCB01 - 1	CCB01	106	-0.0737	-7470A	PPB		03 Sep 2021 16:04:53	U	SMPL
CRA - 1	CRA	1221	0.2262	-7470A	PPB		03 Sep 2021 16:07:09	U	SMPL
HighStd - 1	HighStd	35998	9.5952	-7470A	PPB		03 Sep 2021 16:09:24	U	SMPL
ChkStd - 1	ChkStd	25193	6.6843	-7470A	PPB		03 Sep 2021 16:11:39	U	SMPL
PB138935BL - 1	PBW	99	-0.0761	-7470A	PPB		03 Sep 2021 16:13:58	U	SMPL
PB138935BS - 1	LCSW	14823	3.8906	-7470A	PPB		03 Sep 2021 16:16:14	U	SMPL
M3629-01 - 1	LPA-02	1115	0.1976	-7470A	PPB		03 Sep 2021 16:18:30	U	SMPL
M3629-01DUP - 1	LPA-02DUP	1149	0.2068	-7470A	PPB		03 Sep 2021 16:20:49	U	SMPL
M3629-01MS - 1	LPA-02MS	15595	4.0986	-7470A	PPB		03 Sep 2021 16:23:06	U	SMPL
M3629-01MSD - 1	LPA-02MSD	14954	3.9259	-7470A	PPB		03 Sep 2021 16:25:23	U	SMPL
M3648-05 - 1	20211056-SI-COMP-1-MODIFIED-ELUTRIATE	305	-0.0206	-7470A	PPB		03 Sep 2021 16:27:38	U	SMPL
CCV02 - 1	CCV02	18538	4.8914	-7470A	PPB		03 Sep 2021 16:29:53	U	SMPL
CCB02 - 1	CCB02	102	-0.0753	-7470A	PPB		03 Sep 2021 16:32:08	U	SMPL
M3648-06 - 1	20211056-SI-COMP-1-MODIFIED-ELUTRIATE	292	-0.0241	-7470A	PPB		03 Sep 2021 16:34:24	U	SMPL
M3648-07 - 1	20211057-SI-COMP-2-MODIFIED-ELUTRIATE	327	-0.0147	-7470A	PPB		03 Sep 2021 16:36:40	U	SMPL
M3648-08 - 1	20211057-SI-COMP-2-MODIFIED-ELUTRIATE	346	-0.0095	-7470A	PPB		03 Sep 2021 16:38:55	U	SMPL
M3648-09 - 1	20211058-SI-COMP-3-MODIFIED-ELUTRIATE	351	-0.0082	-7470A	PPB		03 Sep 2021 16:41:11	U	SMPL
M3648-10 - 1	20211058-SI-COMP-3-MODIFIED-ELUTRIATE	315	-0.0179	-7470A	PPB		03 Sep 2021 16:43:27	U	SMPL
M3648-11 - 1	20211059-SI-COMP-4-MODIFIED-ELUTRIATE	260	-0.0327	-7470A	PPB		03 Sep 2021 16:45:43	U	SMPL
M3648-12 - 1	20211059-SI-COMP-4-MODIFIED-ELUTRIATE	266	-0.0311	-7470A	PPB		03 Sep 2021 16:48:00	U	SMPL
M3629-01LX5 - 1		203	-0.0481	-7470A	PPB		03 Sep 2021 16:50:17	U	SMPL
M3629-01A - 1		15410	4.0487	-7470A	PPB		03 Sep 2021 16:52:34	U	SMPL
CCV03 - 1	CCV03	18975	5.0091	-7470A	PPB		03 Sep 2021 16:54:52	U	SMPL
CCB03 - 1	CCB03	45	-0.0906	-7470A	PPB		03 Sep 2021 16:57:07	U	SMPL