


LB116165

7471B

INSTRUMENT ID: CV2

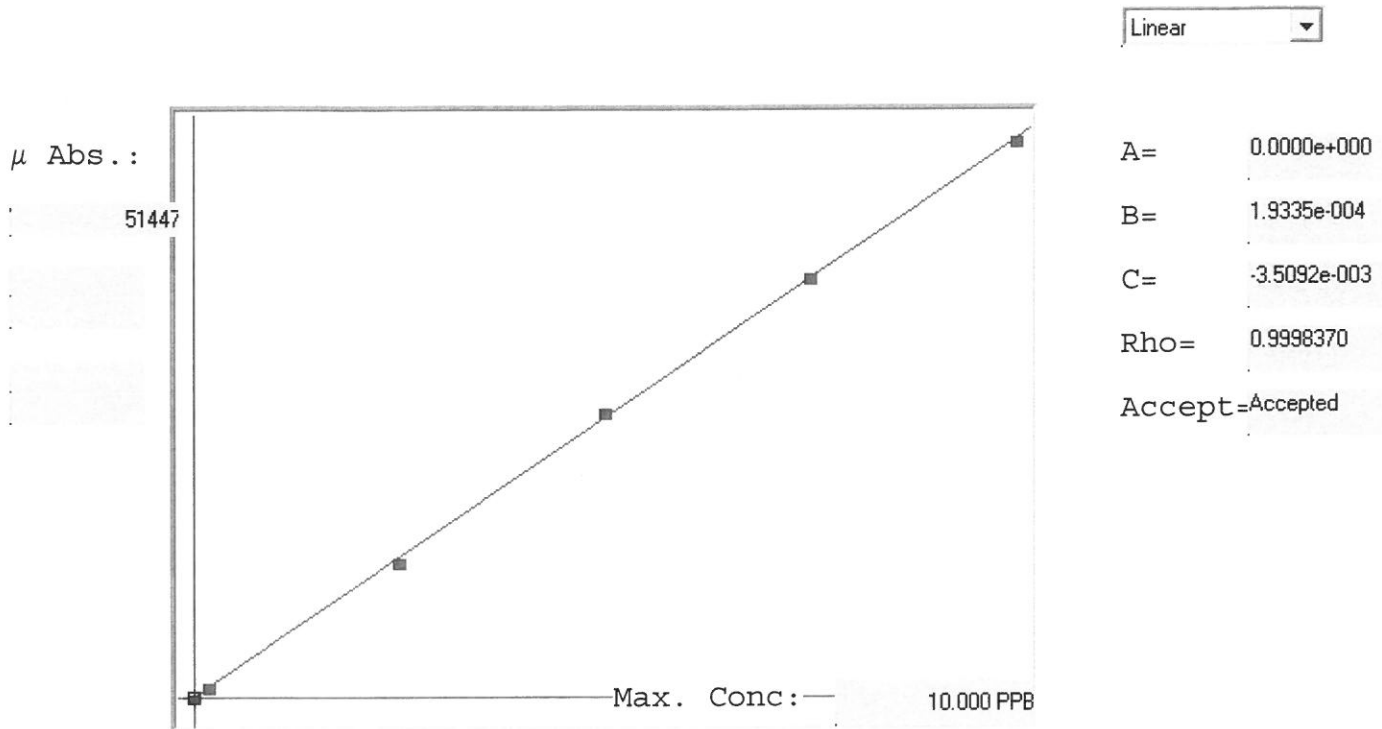

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.027	0.027	159	0.000	159					
0.2	0.200	0.170	-0.030	896	0.0 %	896					-15
2.5	2.500	2.419	-0.081	12531	0.0 %	12531					-3
5.0	5.000	5.122	0.122	26511	0.0 %	26511					2
7.5	7.500	7.518	0.018	38901	0.0 %	38901					0
10.0	10.000	9.944	-0.056	51447	0.0 %	51447					-1

LB116165 INSTRUMENT ID : CV1

Method: 7471B		Operator: Admin		Date of Analysis: 07 Sep 2021 12:12:40					
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	159	-	0.0000	7471B	PPB	07 Sep 2021 12:21:20	S	Std
0.2 - 1	50.2	896	-	0.2000	7471B	PPB	07 Sep 2021 12:23:37	S	Std
2.5 - 1	52.5	12531	-	2.5000	7471B	PPB	07 Sep 2021 12:25:53	S	Std
5.0 - 1	55	26511	-	5.0000	7471B	PPB	07 Sep 2021 12:28:10	S	Std
7.5 - 1	57.5	38901	-	7.5000	7471B	PPB	07 Sep 2021 12:30:27	S	Std
10.0 - 1	51V	51447	-	10.0000	7471B	PPB	07 Sep 2021 12:38:05	S	Std
ICV83 - 1	ICV83	20645	3.9881	-	7471B	PPB	07 Sep 2021 12:40:57	U	SMPL
ICB83 - 1	ICB83	-19	-0.0072	-	7471B	PPB	07 Sep 2021 12:43:12	U	SMPL
CCV04 - 1	CCV04	26038	5.0308	-	7471B	PPB	07 Sep 2021 12:45:27	U	SMPL
CCB04 - 1	CCB04	-34	-0.0101	-	7471B	PPB	07 Sep 2021 12:47:43	U	SMPL
CRA - 1	CRA	887	0.1680	-	7471B	PPB	07 Sep 2021 12:49:59	U	SMPL
HighStd - 1	HighStd	51326	9.9202	-	7471B	PPB	07 Sep 2021 12:52:14	U	SMPL
ChkStd - 1	ChkStd	35644	6.8881	-	7471B	PPB	07 Sep 2021 12:54:29	U	SMPL
PB138957BL - 1	PB138957BL	195	0.0342	-	7471B	PPB	07 Sep 2021 12:56:46	U	SMPL
PB138957BS - 1	PB138957BS	19712	3.8077	-	7471B	PPB	07 Sep 2021 12:59:03	U	SMPL
M3648-01 - 1	20211052-SI-COMPOSITE-1	4940	0.9516	-	7471B	PPB	07 Sep 2021 13:01:19	U	SMPL
M3648-02 - 1	20211053-SI-COMPOSITE-2	7485	1.4437	-	7471B	PPB	07 Sep 2021 13:03:35	U	SMPL
M3648-03 - 1	20211054-SI-COMPOSITE-3	9671	1.8663	-	7471B	PPB	07 Sep 2021 13:05:52	U	SMPL
M3648-04 - 1	20211055-SI-COMPOSITE-4	8248	1.5912	-	7471B	PPB	07 Sep 2021 13:08:09	U	SMPL
M3657-01 - 1	TFI-358	2846	0.5468	-	7471B	PPB	07 Sep 2021 13:10:24	U	SMPL
CCV05 - 1	CCV05	25305	4.8891	-	7471B	PPB	07 Sep 2021 13:12:39	U	SMPL
CCB05 - 1	CCB05	-38	-0.0109	-	7471B	PPB	07 Sep 2021 13:14:55	U	SMPL
M3657-03 - 1	RO-72-11944	1199	0.2283	-	7471B	PPB	07 Sep 2021 13:17:10	U	SMPL
M3658-01 - 1	CHRT-24029	6737	1.2991	-	7471B	PPB	07 Sep 2021 13:19:26	U	SMPL
M3658-03 - 1	RBR-251607	8935	1.7240	-	7471B	PPB	07 Sep 2021 13:21:41	U	SMPL
M3658-05 - 1	RBR-400027	7731	1.4913	-	7471B	PPB	07 Sep 2021 13:23:57	U	SMPL
M3660-01 - 1	ETGI-332	2933	0.5636	-	7471B	PPB	07 Sep 2021 13:26:12	U	SMPL
M3660-01DUP - 1	ETGI-332DUP	2943	0.5655	-	7471B	PPB	07 Sep 2021 13:28:29	U	SMPL
M3660-01MS - 1	ETGI-332MS	22297	4.3075	-	7471B	PPB	07 Sep 2021 13:30:45	U	SMPL
M3660-01MSD - 1	ETGI-332MSD	22064	4.2625	-	7471B	PPB	07 Sep 2021 13:33:02	U	SMPL
M3660-01LX5 - 1		473	0.0879	-	7471B	PPB	07 Sep 2021 13:35:19	U	SMPL
M3660-01A - 1		22462	4.3394	-	7471B	PPB	07 Sep 2021 13:37:35	U	SMPL
CCV06 - 1	CCV06	25405	4.9085	-	7471B	PPB	07 Sep 2021 13:39:50	U	SMPL
CCB06 - 1	CCB06	-75	-0.0180	-	7471B	PPB	07 Sep 2021 13:42:06	U	SMPL