


LB116182

245.1

INSTRUMENT ID: CV2

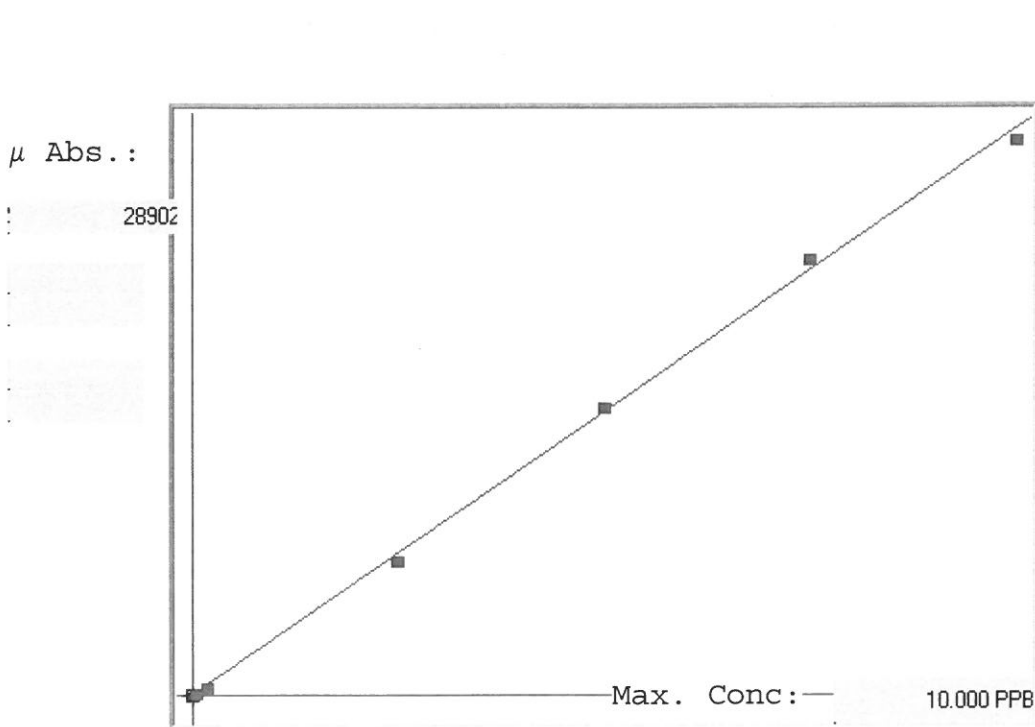

Linear

A= 0.0000e+000

B= 3.3915e-004

C= 7.6570e-004

Rho= 0.9994361

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	7/06
0.0	0.000	0.008	0.008	20	0.000	20					20
0.05	0.050	0.060	0.010	175	0.0 %	175	0				-16
0.2	0.200	0.168	-0.032	494	0.0 %	494					-4
2.5	2.500	2.395	-0.105	7061	0.0 %	7061					2
5.0	5.000	5.095	0.095	15021	0.0 %	15021					3
7.5	7.500	7.721	0.221	22763	0.0 %	22763					-2
10.0	10.000	9.803	-0.197	28902	0.0 %	28902					

LB116182 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 08 Sep 2021 11:52:45

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	20	-	0.0000	245.1	PPB	08 Sep 2021 13:13:18	S	Std
0.05 - 1	50.05	175	-	0.0500	245.1	PPB	08 Sep 2021 13:15:35	S	Std
0.2 - 1	50.2	494	-	0.2000	245.1	PPB	08 Sep 2021 13:17:52	S	Std
2.5 - 1	52.5	7061	-	2.5000	245.1	PPB	08 Sep 2021 13:20:09	S	Std
5.0 - 1	55	15021	-	5.0000	245.1	PPB	08 Sep 2021 13:22:25	S	Std
7.5 - 1	57.5	22763	-	7.5000	245.1	PPB	08 Sep 2021 13:24:41	S	Std
10.0 - 1	510	28902	-	10.0000	245.1	PPB	08 Sep 2021 13:26:57	S	Std
ICV85 - 1	ICV85	11711	3.9725	-245.1		PPB	08 Sep 2021 13:34:50	U	SMPL
ICB85 - 1	ICB85	17	0.0065	-245.1		PPB	08 Sep 2021 13:37:04	U	SMPL
CCV10 - 1	CCV10	14031	4.7593	-245.1		PPB	08 Sep 2021 13:39:19	U	SMPL
CCB10 - 1	CCB10	25	0.0092	-245.1		PPB	08 Sep 2021 13:41:34	U	SMPL
CRA - 1	CRA	167	0.0574	-245.1		PPB	08 Sep 2021 13:43:50	U	SMPL
HighStd - 1	HighStd	30435	10.3227	-245.1		PPB	08 Sep 2021 13:46:05	U	SMPL
ChkStd - 1	ChkStd	21997	7.4610	-245.1		PPB	08 Sep 2021 13:48:20	U	SMPL
PB138971BL - 1	PBW	48	0.0170	-245.1		PPB	08 Sep 2021 13:50:38	U	SMPL
PB138971BS - 1	LCSW	12238	4.1512	-245.1		PPB	08 Sep 2021 13:55:30	U	SMPL
M3625-02 - 1	COMP	626	0.2131	-245.1		PPB	08 Sep 2021 14:03:23	U	SMPL
M3625-02DUP - 1	COMPDUP	607	0.2066	-245.1		PPB	08 Sep 2021 14:05:39	U	SMPL
M3625-02MS - 1	COMPMS	14152	4.8004	-245.1		PPB	08 Sep 2021 14:10:29	U	SMPL
M3625-02MSD - 1	COMPMSD	13974	4.7400	-245.1		PPB	08 Sep 2021 14:12:46	U	SMPL
M3640-01 - 1	HP-627-EB	298	0.1018	-245.1		PPB	08 Sep 2021 14:15:01	U	SMPL
CCV11 - 1	CCV11	15221	5.1629	-245.1		PPB	08 Sep 2021 14:21:42	U	SMPL
CCB11 - 1	CCB11	52	0.0184	-245.1		PPB	08 Sep 2021 14:23:57	U	SMPL
M3640-03 - 1	HP-627	478	0.1629	-245.1		PPB	08 Sep 2021 14:26:12	U	SMPL
M3640-04 - 1	HP-627-X	442	0.1507	-245.1		PPB	08 Sep 2021 14:28:28	U	SMPL
M3641-03 - 1	HP-640	340	0.1161	-245.1		PPB	08 Sep 2021 14:30:43	U	SMPL
M3644-02 - 1	191-0902-W	345	0.1178	-245.1		PPB	08 Sep 2021 14:32:59	U	SMPL
M3644-04 - 1	191-0902-DUP	395	0.1347	-245.1		PPB	08 Sep 2021 14:35:15	U	SMPL
M3625-02LX5 - 1		95	0.0330	-245.1		PPB	08 Sep 2021 14:37:32	U	SMPL
M3625-02A - 1		13866	4.7034	-245.1		PPB	08 Sep 2021 14:39:47	U	SMPL
CCV12 - 1	CCV12	14789	5.0164	-245.1		PPB	08 Sep 2021 14:42:04	U	SMPL
CCB12 - 1	CCB12	56	0.0198	-245.1		PPB	08 Sep 2021 14:44:21	U	SMPL