

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : AK Instrument ID : Konelab

9/8/2021 15:56

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	0.985	0.0	0.097	
ICB1	0.006	0.0	0.005	
CCV1	0.986	0.0	0.097	
CCB1	0.004	0.0	0.005	
PB138949BL	0.004	0.0	0.005	
PB138949BS	0.976	0.0	0.096	
M3644-02	0.003	0.0	0.005	
M3644-02DUP	0.002	0.0	0.005	
M3644-02MS	0.973	0.0	0.096	
M3644-02MSD	0.982	0.0	0.096	
M3644-04	0.003	0.0	0.005	
CCV2	0.972	0.0	0.096	
CCB2	-0.001	0.0	0.005	

N	13
Mean	0.454
SD	0.5064
CV%	111.64

Aquakem v. 7.2AQ1

Results from time period:

Wed Sep 08 14:14:30 2021

Wed Sep 08 15:50:18 2021

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	0.0023	mg/l	9/8/2021 14:14:30	
0.05PPM	A	Phenolics-	P	0.05	mg/l	9/8/2021 14:14:31	
0.1PPM	A	Phenolics-	P	0.1018	mg/l	9/8/2021 14:14:32	
0.25PPM	A	Phenolics-	P	0.2507	mg/l	9/8/2021 14:14:33	
0.50PPM	A	Phenolics-	P	0.4982	mg/l	9/8/2021 14:14:34	
1.0PPM	A	Phenolics-	P	0.9935	mg/l	9/8/2021 14:14:35	
2.0PPM	A	Phenolics-	P	2.0035	mg/l	9/8/2021 14:14:36	
ICV1	S	Phenolics-	P	0.9849	mg/l	9/8/2021 15:47:30	
ICB1	S	Phenolics-	P	0.0061	mg/l	9/8/2021 15:47:31	
CCV1	S	Phenolics-	P	0.9861	mg/l	9/8/2021 15:47:32	
CCB1	S	Phenolics-	P	0.0045	mg/l	9/8/2021 15:47:33	
PB138949BL	S	Phenolics-	P	0.0043	mg/l	9/8/2021 15:47:34	
PB138949BS	S	Phenolics-	P	0.9761	mg/l	9/8/2021 15:47:35	
M3644-02	S	Phenolics-	P	0.0034	mg/l	9/8/2021 15:47:36	
M3644-02DUP	S	Phenolics-	P	0.0018	mg/l	9/8/2021 15:47:37	
M3644-02MS	S	Phenolics-	P	0.9728	mg/l	9/8/2021 15:47:38	
M3644-02MSD	S	Phenolics-	P	0.9818	mg/l	9/8/2021 15:47:39	
M3644-04	S	Phenolics-	P	0.0031	mg/l	9/8/2021 15:47:40	
CCV2	S	Phenolics-	P	0.9725	mg/l	9/8/2021 15:47:41	
CCB2	S	Phenolics-	P	-0.001	mg/l	9/8/2021 15:50:18	

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : PS

Instrument ID : Konelab

9/8/2021 14:15

Test Phenolics-


Accepted 9/8/2021 14:15

Factor 10.73

Bias 0.005

Coeff. of det. 0.999979

Errors

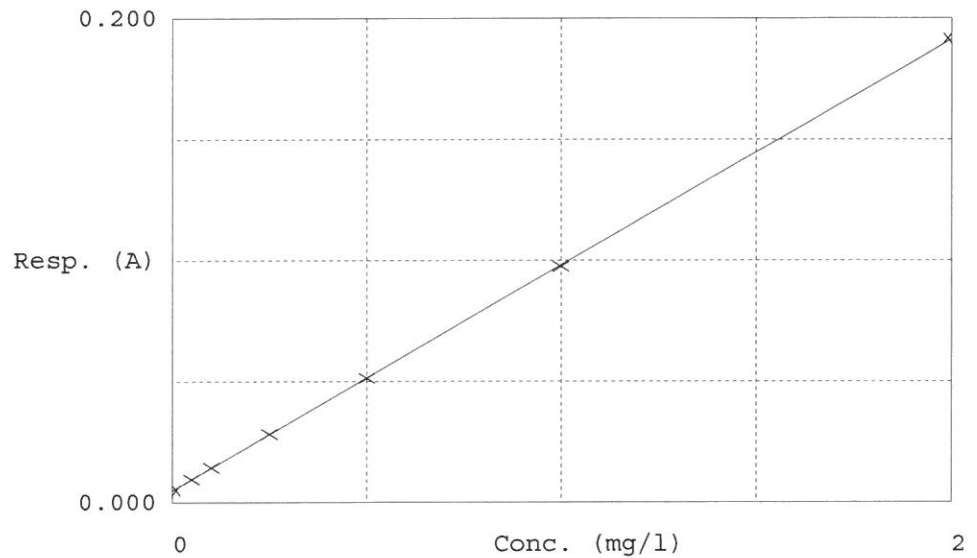

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.00PPM	0.005	0.0023	0.0000	0.0
2	Phenol-2	0.010	0.0500	0.0500	1.8
3	Phenol-2	0.014	0.1018	0.1000	0.2
4	Phenol-2	0.028	0.2507	0.2500	-0.4
5	Phenol-2	0.051	0.4982	0.5000	-0.6
6	Phenol-2	0.098	0.9935	1.0000	0.2
7	Phenol-2	0.192	2.0035	2.0000	

9/19/21