

Clear table

Instrument ID: IC-2										Analyst :		AP		Method:		300.0	
ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time	Initial wt/ Final Vol	Analyst						
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2021-08-16_	8/16/21 10:41		AP/MA						
STD2	0.3910	0.6790	0.6640	2.2200	0.5610	0.8630	3.4380	_2021-08-16_	8/16/21 11:10		AP/MA						
STD3	0.8120	1.1960	1.1960	4.0250	1.0110	1.9680	6.0560	_2021-08-16_	8/16/21 11:40		AP/MA						
STD4	0.9680	1.4810	1.4890	4.9650	1.2390	2.5530	7.4120	_2021-08-16_	8/16/21 12:09		AP/MA						
STD5	2.0210	2.9170	2.9320	9.7020	2.4140	5.1900	14.4290	_2021-08-16_	8/16/21 12:38		AP/MA						
STD6	4.0620	5.9880	5.9780	19.9480	4.9860	10.0130	29.8970	_2021-08-16_	8/16/21 13:07		AP/MA						
STD7	4.9450	7.5390	7.5410	25.1390	6.2890	12.4140	37.7680	_2021-08-16_	8/16/21 13:37		AP/MA						
ICV	2.0750	3.0030	3.0150	10.0260	2.4820	5.3330	14.8330	_2021-08-16_	8/16/21 14:22		AP/MA						
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2021-08-16_	8/16/21 14:51		AP/MA						
CCV	2.0490	2.9440	2.8850	9.7490	2.4480	4.9590	14.5870	_2021-09-10_	9/10/21 11:08		AP/MA						
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2021-09-10_	9/10/21 11:47		AP/MA						
LB116261BLW	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2021-09-10_	9/10/21 12:16		AP/MA						
LB116261BSW	2.0340	2.9370	2.8880	9.7340	2.4320	5.1640	14.5700	_2021-09-10_	9/10/21 12:45		AP/MA						
M3688-01	1.1780	195.6430	0.1620	0.0000	6.1090	0.0000	25.3220	_2021-09-10_	9/10/21 13:14		AP/MA						
M3681-04RE	0.4300	54.5750	1.0840	0.0000	0.2640	0.0000	16.9930	_2021-09-10_	9/10/21 15:16		AP/MA						
M3688-01MS	3.4280	190.2620	2.9670	9.9790	8.5360	8.4750	40.6250	_2021-09-10_	9/10/21 15:45		AP/MA						
M3688-01MSD	3.2660	190.6880	2.9430	9.8040	8.5500	8.1880	40.3370	_2021-09-10_	9/10/21 16:13		AP/MA						
CCV	1.9410	2.8930	2.8050	9.5550	2.3940	5.3700	14.3900	_2021-09-10_	9/10/21 17:39		AP/MA						
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2021-09-10_	9/10/21 18:08		AP/MA						


AP 9/16/21

Clear table

Instrument ID: IC-2									
Analyst : AP				Method: 300 / 9056A					
ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time
ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4		Initial wt/ Final Vol
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-08-16_	8/16/21 10:41
STD2	0.3910	0.6790	0.6640	2.2200	0.5610	0.8630	3.4380	2021-08-16_	8/16/21 11:10
STD3	0.8120	1.1960	1.1960	4.0250	1.0110	1.9680	6.0560	2021-08-16_	8/16/21 11:40
STD4	0.9680	1.4810	1.4890	4.9650	1.2390	2.5530	7.4120	2021-08-16_	8/16/21 12:09
STD5	2.0210	2.9170	2.9320	9.7020	2.4140	5.1900	14.4290	2021-08-16_	8/16/21 12:38
STD6	4.0620	5.9880	5.9780	19.9480	4.9860	10.0130	29.8970	2021-08-16_	8/16/21 13:07
STD7	4.9450	7.5390	7.5410	25.1390	6.2890	12.4140	37.7680	2021-08-16_	8/16/21 13:37
ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4		Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000		AP/MA
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000		AP/MA
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000		AP/MA
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000		AP/MA
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000		AP/MA
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000		AP/MA
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.5000		AP/MA
ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4		
STD1									
STD2	-2.2500	13.1667	10.6667	11.0000	12.2000	-13.7000	14.6000		
STD3	1.5000	-0.3333	-0.3333	0.6250	1.1000	-1.6000	0.9333		
STD4	-3.2000	-1.2667	-0.7333	-0.7000	-0.8800	2.1200	-1.1733		
STD5	1.0500	-2.7667	-2.2667	-2.9800	-3.4400	3.8000	-3.8067		
STD6	1.5500	-0.2000	-0.3667	-0.2600	-0.2800	0.1300	-0.3433		
STD7	-1.1000	0.5200	0.5467	0.5560	0.6240	-0.6880	0.7147		

CALIBRATION OF COMPONENT F-

Method: AnionsIC2-081621.mtw
 Equation: $Q = 0.0787508 \cdot A + 1.63425$
 RSD: 2.096 %
 Correlation coefficient: 0.999761

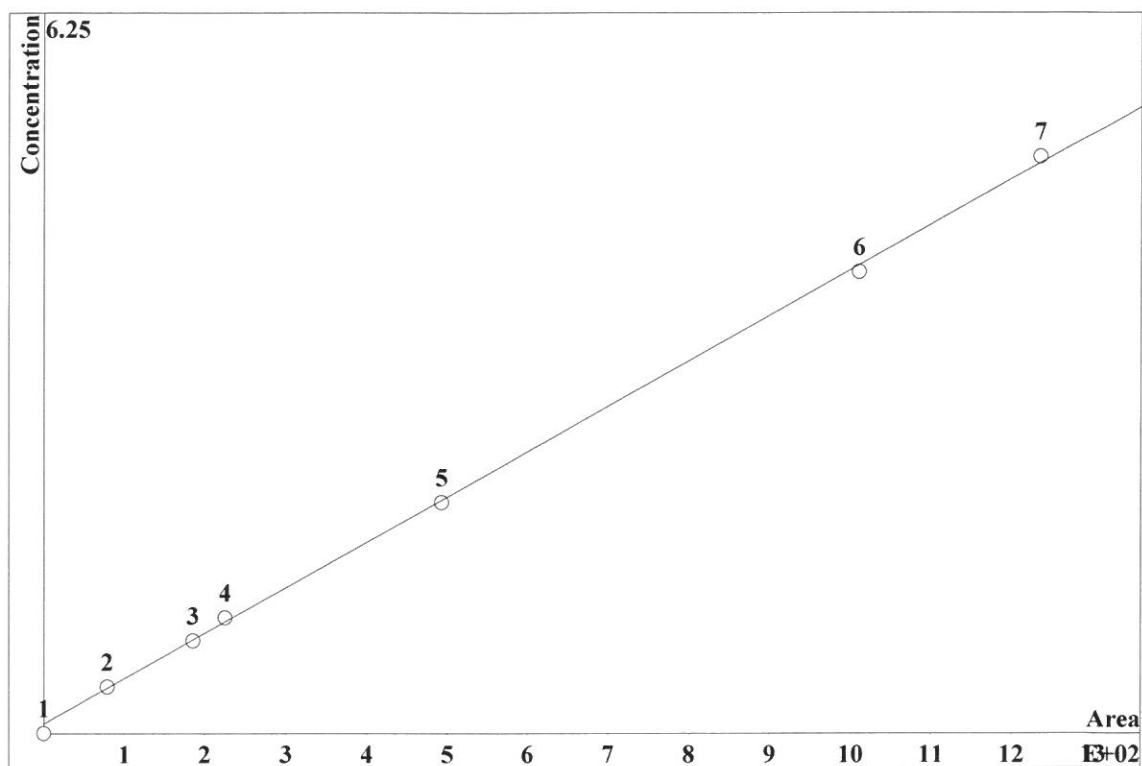

K3 = 0 K2 = 0 K1 = 0.0787508 K0 = 1.63425

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	2.039	78.64	0.4	20	5.75		
3	4.335	185.4	0.8	20	5.75		
4	5.553	225.1	1	20	5.75		
5	12.72	492.6	2	20	5.75		
6	25.53	1011	4	20	5.75		
7	32.96	1235	5	20	5.75		

CALIBRATION OF COMPONENT CL-

Method: AnionsIC2-081621.mtw
 Equation: $Q = 0.117224 \cdot A + 1.57793$
 RSD: 1.870 %
 Correlation coefficient: 0.999809

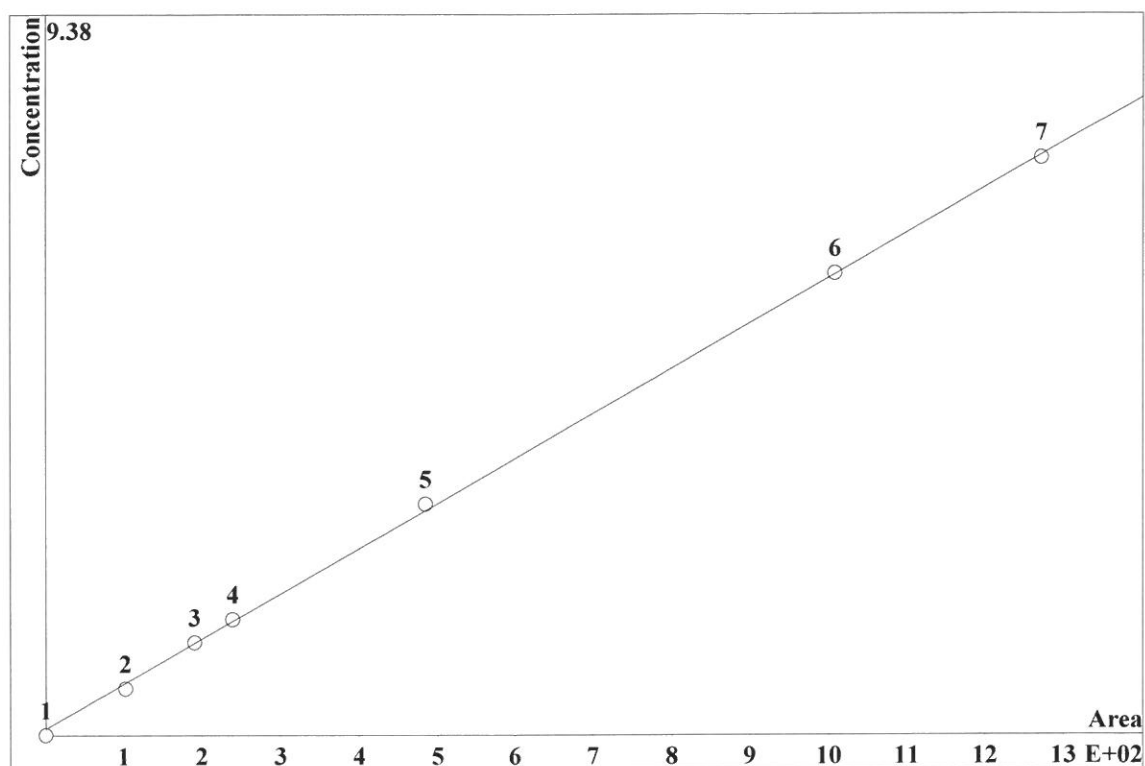

K3 = 0 K2 = 0 K1 = 0.117224 K0 = 1.57793

Base: Area

Ref.channel: chl

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	6.284	102.4	0.6	20	8.834		
3	12.17	190.6	1.2	20	8.834		
4	15.33	239.2	1.5	20	8.834		
5	31.62	484.2	3	20	8.834		
6	66.52	1008	6	20	8.834		
7	84.64	1273	7.5	20	8.834		

CALIBRATION OF COMPONENT NO2

Method: AnionsIC2-081621.mtw
 Equation: $Q = 0.0516801 \cdot A + 2.2891$
 RSD: 1.582 %
 Correlation coefficient: 0.999864

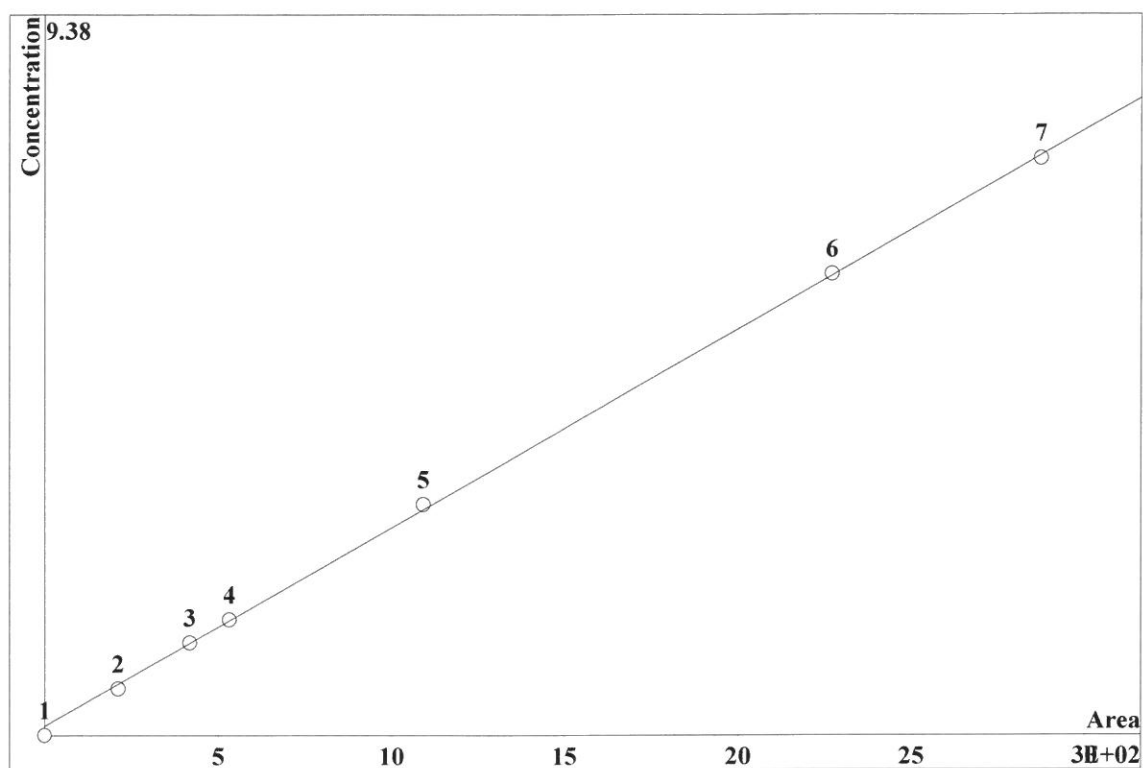

K3 = 0 K2 = 0 K1 = 0.0516801 K0 = 2.2891

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	10.82	212.6	0.6	20	10.64		
3	21.42	418.5	1.2	20	10.64		
4	27.07	531.9	1.5	20	10.64		
5	54.81	1091	3	20	10.64		
6	112.5	2269	6	20	10.64		
7	140.7	2874	7.5	20	10.64		

CALIBRATION OF COMPONENT BR-

Method: AnionsIC2-081621.mtw
 Equation: $Q = 0.260041 \cdot A + 9.18714$
 RSD: 1.824 %
 Correlation coefficient: 0.999819

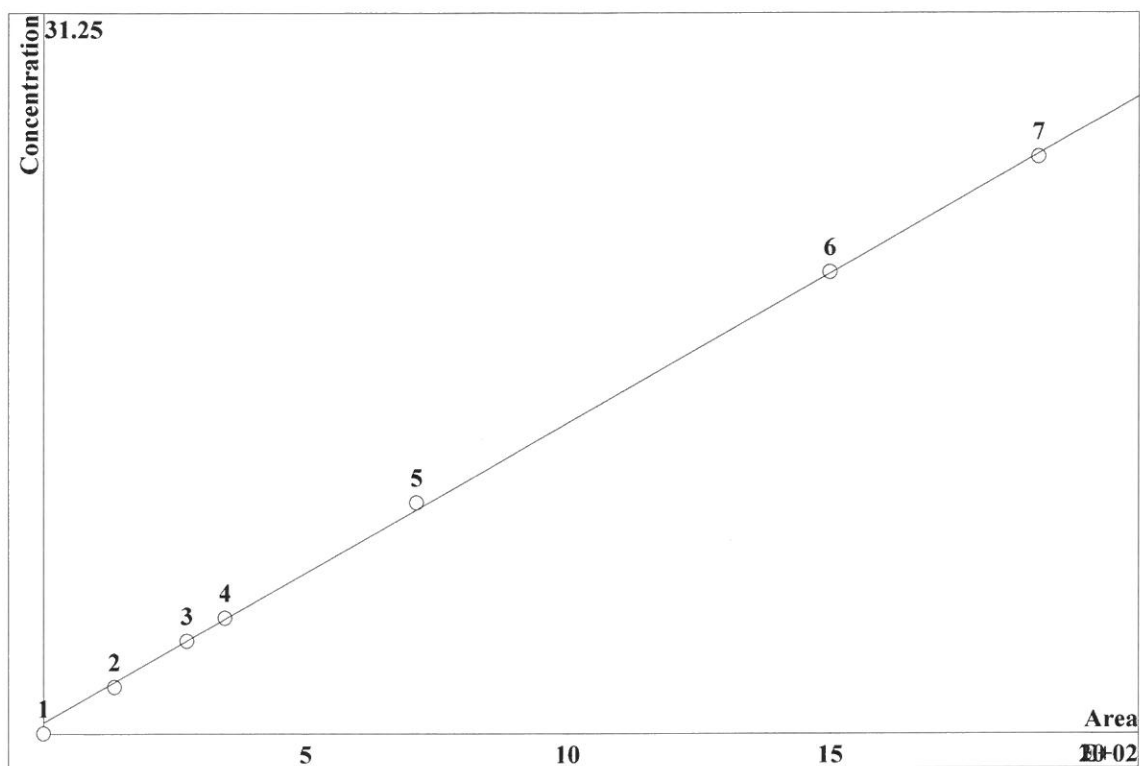

K3 = 0 K2 = 0 K1 = 0.260041 K0 = 9.18714

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	6.57	135.4	2	20			14
3	13.26	274.2	4	20			14
4	16.89	346.5	5	20			14
5	35.45	710.9	10	20			14
6	75.7	1499	20	20			14
7	96.72	1898	25	20			14

CALIBRATION OF COMPONENT NO3

Method: AnionsIC2-081621.mtw
 Equation: $Q = 0.0453375 \cdot A + 2.27775$
 RSD: 2.079 %
 Correlation coefficient: 0.999764

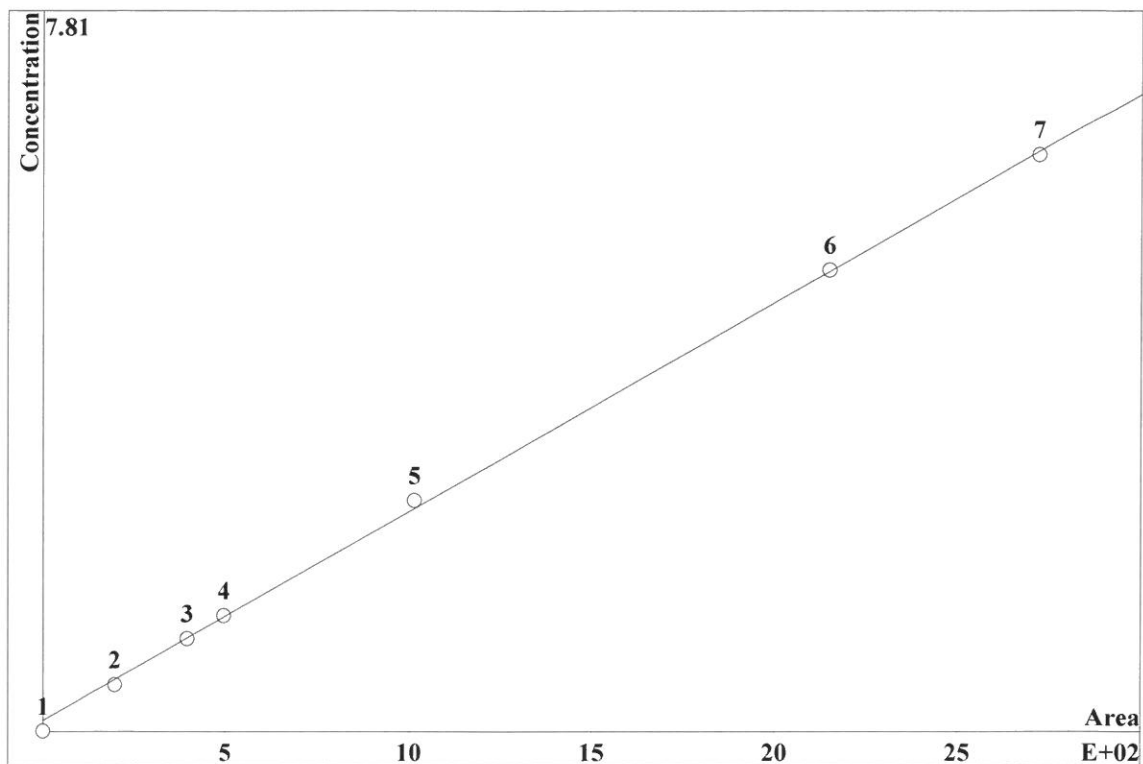

K3 = 0 K2 = 0 K1 = 0.0453375 K0 = 2.27775

Base: Area

Ref.channel: chl

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	7.929	197.1	0.5	20	16.28		
3	15.82	395.8	1	20	16.28		
4	20.05	496.5	1.25	20	16.28		
5	41.67	1015	2.5	20	16.28		
6	88.92	2149	5	20	16.28		
7	114	2724	6.25	20	16.28		

CALIBRATION OF COMPONENT HPO4

Method: AnionsIC2-081621.mtw
 Equation: $Q = 0.093688 \cdot A - 10.9491$
 RSD: 2.345 %
 Correlation coefficient: 0.999700

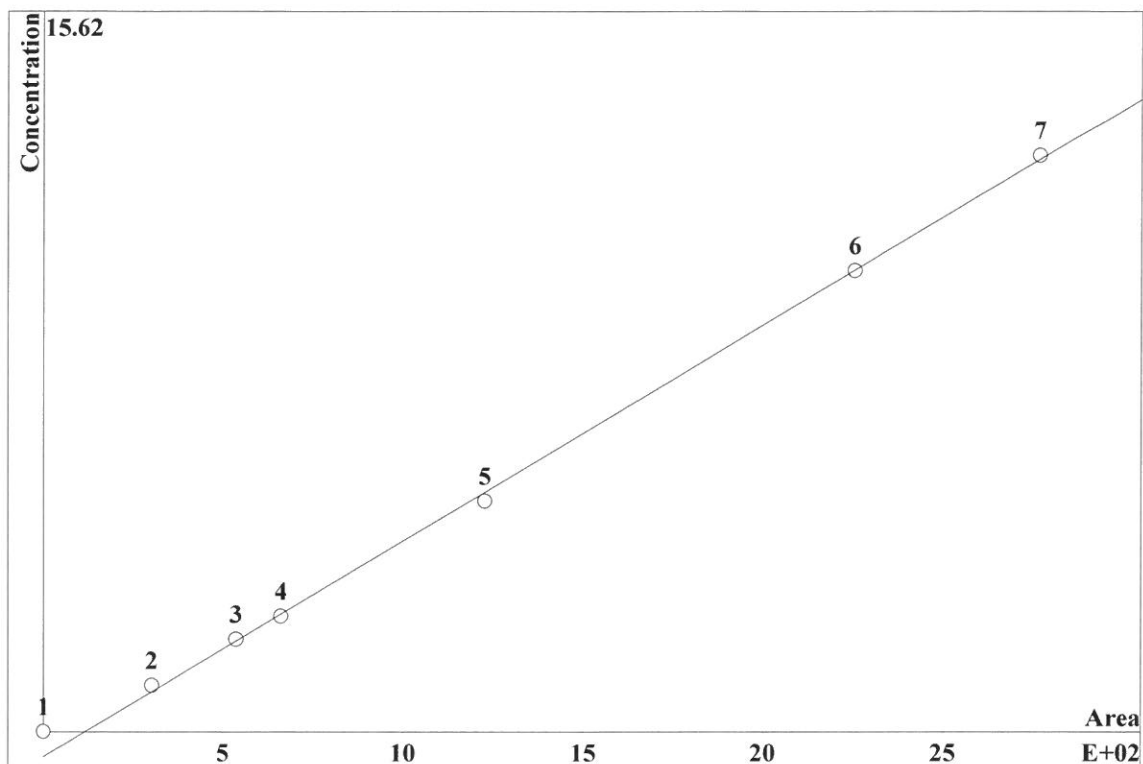

K3 = 0 K2 = 0 K1 = 0.093688 K0 = -10.9491

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	6.866	301	1	20	21.2		
3	12.55	536.9	2	20	21.2		
4	15.7	661.8	2.5	20	21.2		
5	30.88	1225	5	20	21.2		
6	58.85	2254	10	20	21.2		
7	73.57	2767	12.5	20	21.2		

CALIBRATION OF COMPONENT SO4

Method: AnionsIC2-081621.mtw
 Equation: $Q = 0.148108 \cdot A + 15.0956$
 RSD: 2.368 %
 Correlation coefficient: 0.999694

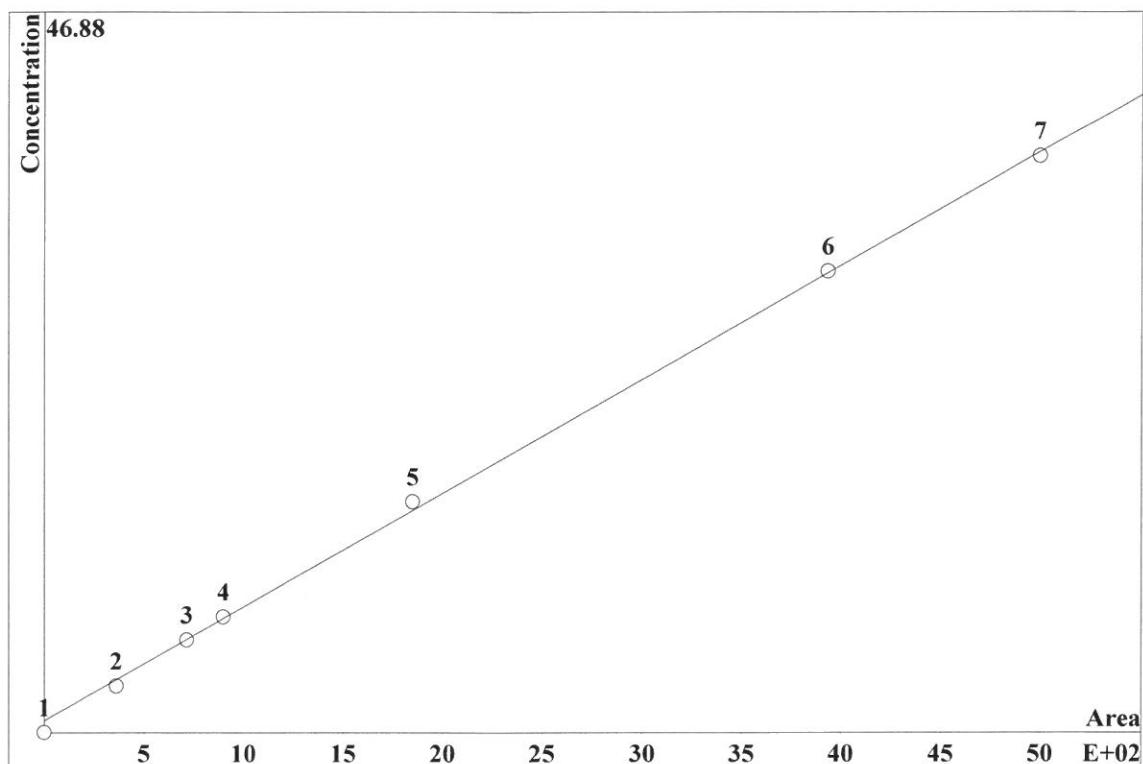

K3 = 0 K2 = 0 K1 = 0.148108 K0 = 15.0956

Base: Area

Ref.channel: ch1

ISTD:

Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	11.07	362.3	3	20	24.73		
3	21.95	715.9	6	20	24.73		
4	27.77	898.9	7.5	20	24.73		
5	57.89	1847	15	20	24.73		
6	124.1	3935	30	20	24.73		
7	158.5	4998	37.5	20	24.73		

Report date: 8/16/2021 2:41:00 PM
Printed by: wet


Ident: STD1
Analysis from: 8/16/2021 10:41:20 AM
File: _2021-08-16_

Last save: 8/16/2021 2:19:03 PM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 27902

Last save: 8/16/2021 1:34:

SAMPLE:
: AM/AP
Vial number: 2
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

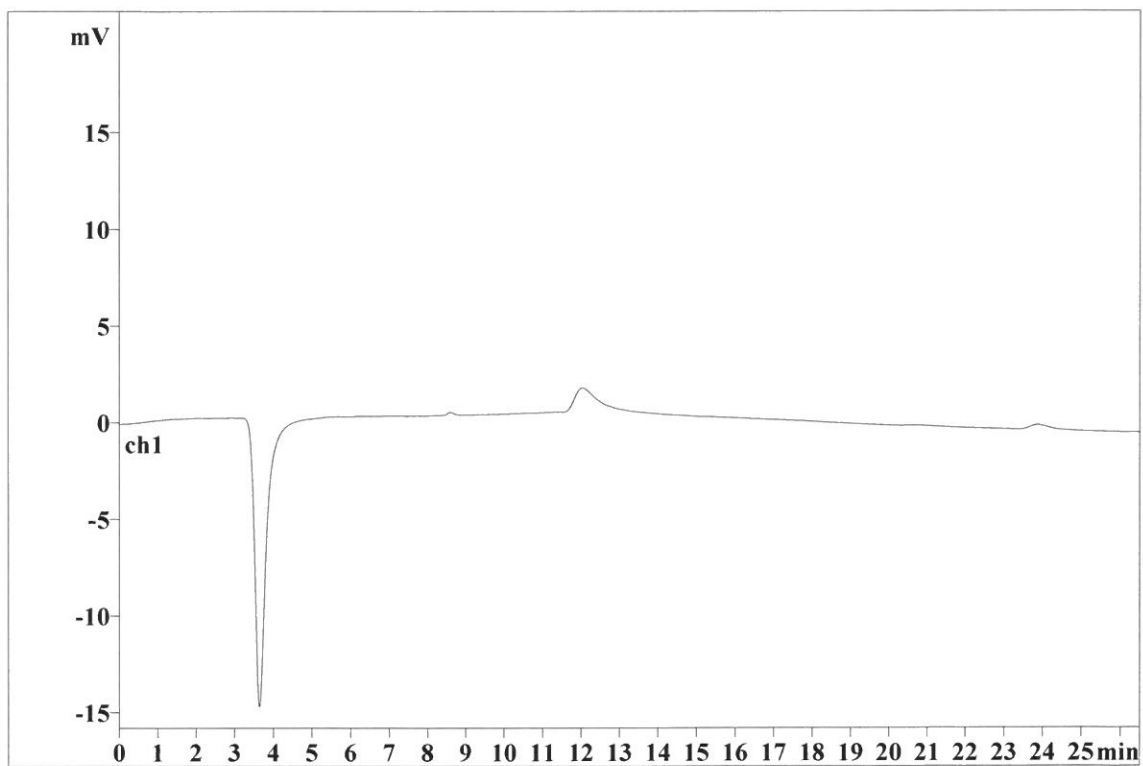

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 8/16/2021 2:41:09 PM
Printed by: wet


Ident: STD2
Analysis from: 8/16/2021 11:10:29 AM
File: _2021-08-16_

Last save: 8/16/2021 2:19:03 PM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 27903

Last save: 8/16/2021 1:34:

SAMPLE:
: AM/AP
Vial number: 3
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

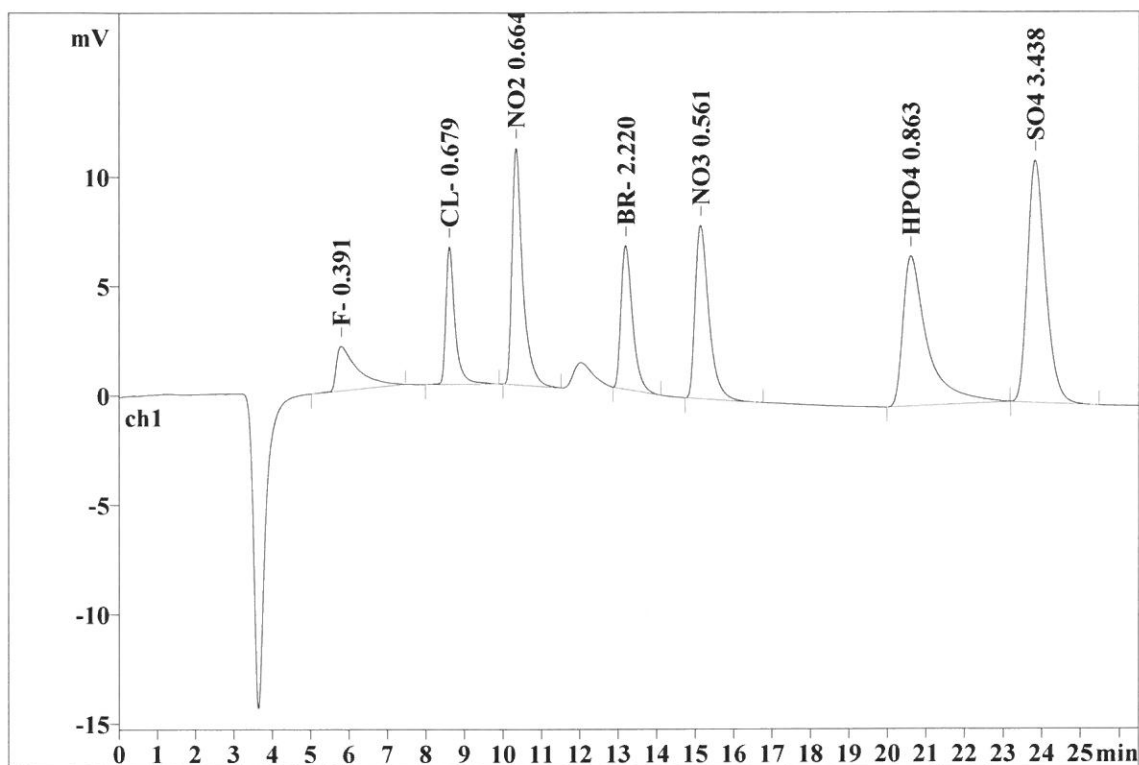

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.79	0.528	2.04	3.95	78.638	5.66
2	8.59	0.227	6.28	12.19	102.434	7.37
3	10.31	0.280	10.82	20.97	212.618	15.30
4	13.18	0.310	6.57	12.74	135.403	9.74
5	15.12	0.370	7.93	15.38	197.114	14.19
6	20.60	0.581	6.86	13.31	300.994	21.66
7	23.82	0.498	11.07	21.46	362.315	26.07
7	26.50	0.399	51.57	99.99	1389.516	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/16/2021 2:41:15 PM
Printed by: wet


Ident: STD3
Analysis from: 8/16/2021 11:40:29 AM
File: _2021-08-16_

Last save: 8/16/2021 2:19:03 PM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 27904

Last save: 8/16/2021 1:34:

SAMPLE:
: AM/AP
Vial number: 4
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

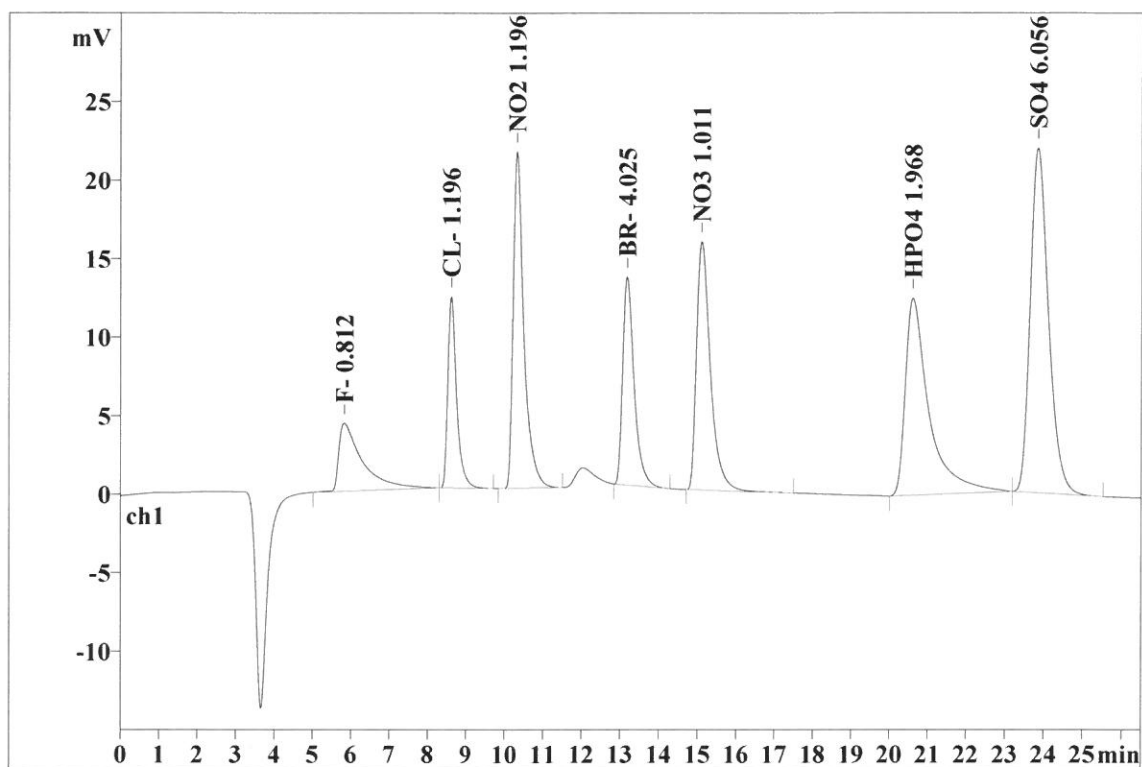

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.82	0.561	4.33	4.27	185.440	6.82
2	8.60	0.224	12.17	11.99	190.565	7.01
3	10.31	0.278	21.42	21.10	418.497	15.40
4	13.17	0.308	13.25	13.06	274.248	10.09
5	15.10	0.369	15.82	15.59	395.751	14.56
6	20.62	0.570	12.55	12.36	536.946	19.76
7	23.85	0.496	21.95	21.62	715.856	26.34
7	26.50	0.401	101.49	99.99	2717.303	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/16/2021 2:41:22 PM
Printed by: wet


Ident: STD4
Analysis from: 8/16/2021 12:09:38 PM
File: _2021-08-16_

Last save: 8/16/2021 2:19:03 PM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 27905

Last save: 8/16/2021 1:34:

SAMPLE:
: AM/AP
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

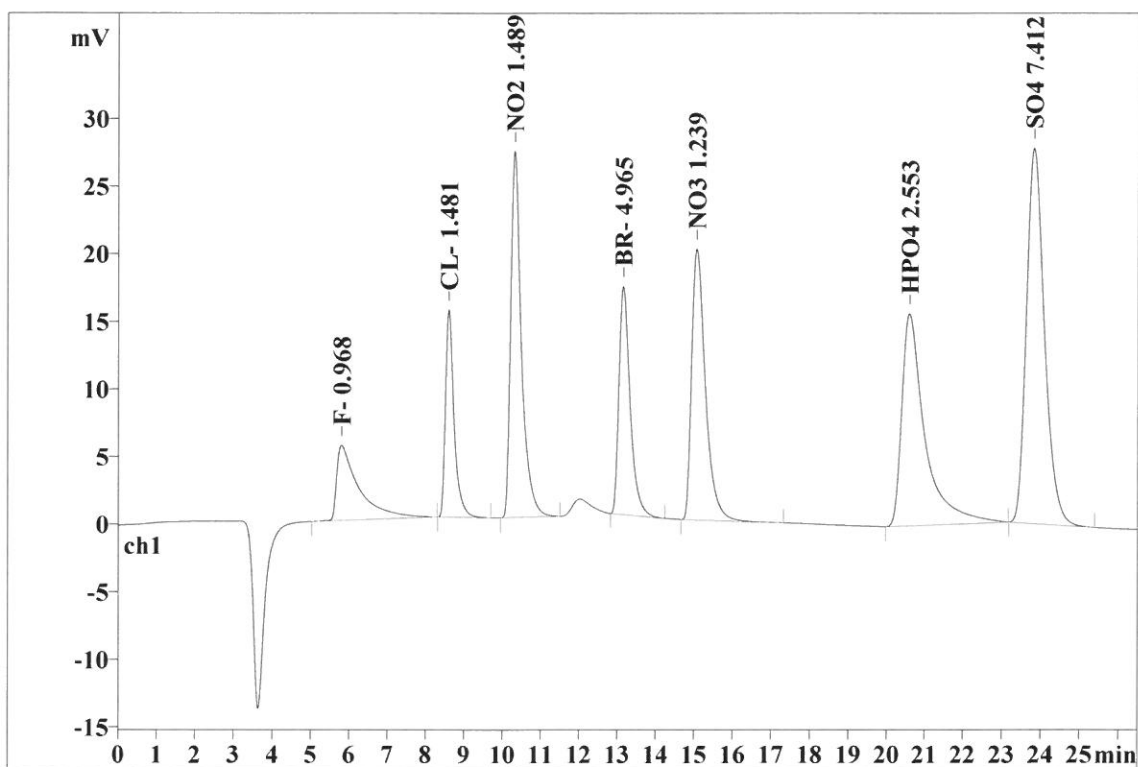

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.80	0.516	5.55	4.32	225.116	6.62
2	8.58	0.224	15.33	11.94	239.230	7.04
3	10.29	0.279	27.07	21.09	531.854	15.64
4	13.14	0.306	16.89	13.16	346.535	10.19
5	15.06	0.366	20.05	15.62	496.499	14.60
6	20.58	0.561	15.70	12.23	661.773	19.46
7	23.82	0.492	27.77	21.63	898.941	26.44
7	26.50	0.392	128.37	100.00	3399.949	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/16/2021 2:41:29 PM

Printed by: wet

Ident: STD5

Analysis from: 8/16/2021 12:38:45 PM

File: _2021-08-16_

Last save: 8/16/2021 2:19:03 PM

Method: AnionsIC2-081621.mtw

Last save: 8/16/2021 1:34:

Run operator: wet

Analysis number: 27906

SAMPLE:

: AM/AP

Vial number:

6

Volume:


20.0 µL

Dilution:

1.00

Amount:

1.0000

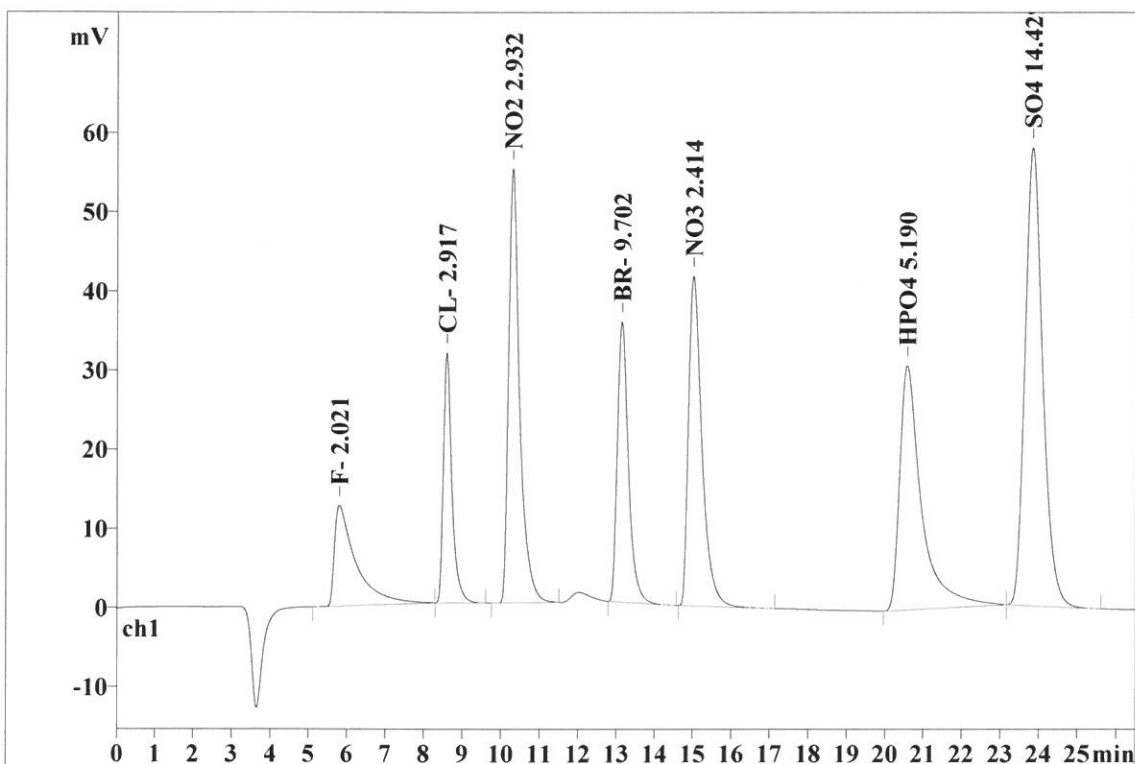

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.80	0.504	12.72	4.80	492.593	7.18
2	8.58	0.220	31.62	11.93	484.207	7.05
3	10.28	0.284	54.81	20.68	1090.559	15.89
4	13.12	0.298	35.45	13.38	710.881	10.36
5	15.01	0.360	41.66	15.72	1014.578	14.78
6	20.56	0.532	30.87	11.65	1224.844	17.84
7	23.81	0.484	57.89	21.84	1846.544	26.90
7	26.50	0.383	265.03	100.00	6864.205	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/16/2021 2:41:36 PM
Printed by: wet


Ident: STD6
Analysis from: 8/16/2021 1:07:53 PM
File: _2021-08-16_

Last save: 8/16/2021 2:19:03 PM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 27907

Last save: 8/16/2021 1:34:

SAMPLE:
: AM/AP
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

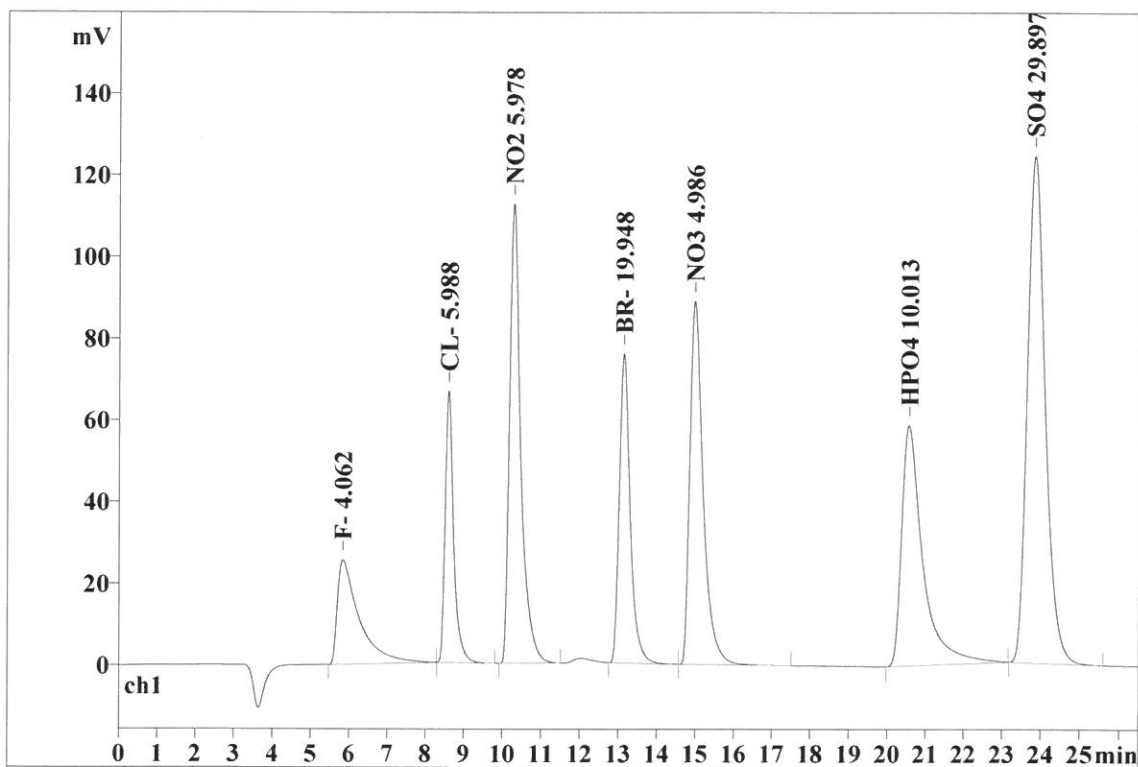

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.84	0.534	25.53	4.62	1010.837	7.16
2	8.59	0.216	66.52	12.05	1008.142	7.14
3	10.27	0.286	112.49	20.37	2269.338	16.06
4	13.13	0.292	75.70	13.71	1498.913	10.61
5	14.97	0.354	88.92	16.10	2149.238	15.21
6	20.56	0.519	58.85	10.66	2254.471	15.96
7	23.83	0.480	124.14	22.48	3935.287	27.86
7	26.50	0.383	552.16	100.00	14126.227	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/16/2021 2:41:42 PM
Printed by: wet


Ident: STD7
Analysis from: 8/16/2021 1:37:00 PM
File: _2021-08-16_

Last save: 8/16/2021 2:19:03 PM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 27908

Last save: 8/16/2021 1:34:

SAMPLE:
: AM/AP
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

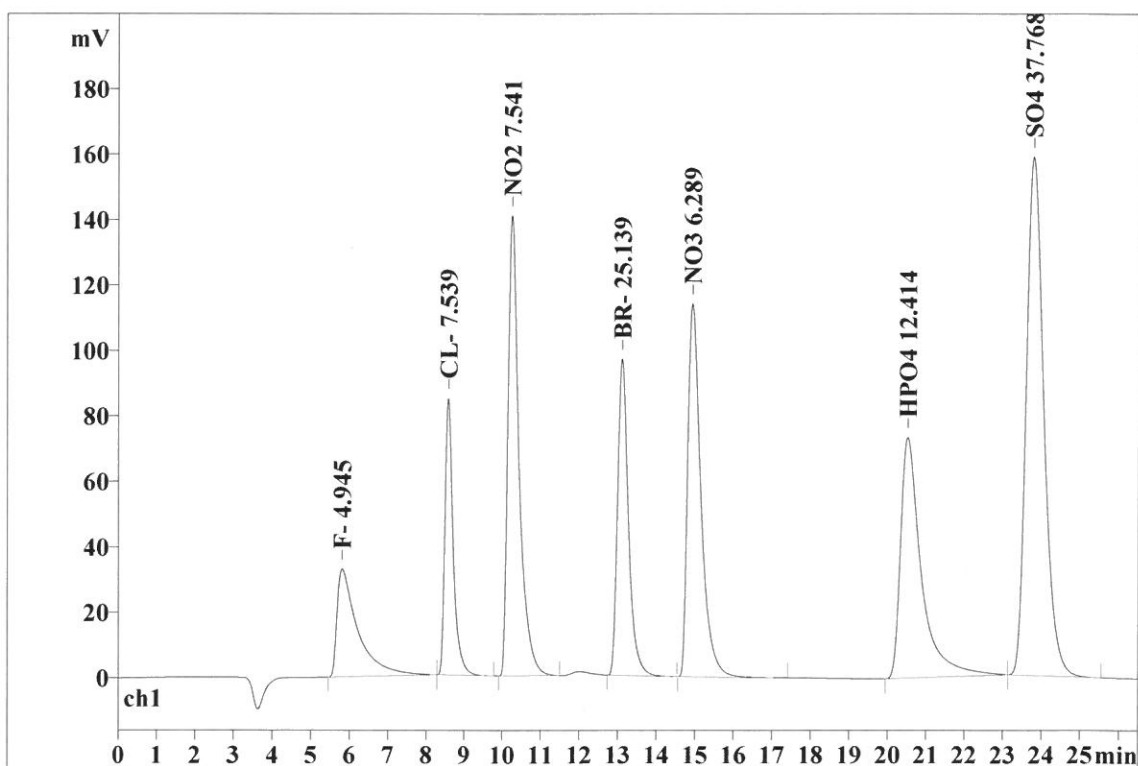

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.81	0.494	32.96	4.70	1235.210	6.95
2	8.57	0.214	84.64	12.07	1272.799	7.16
3	10.24	0.290	140.66	20.06	2873.891	16.17
4	13.11	0.290	96.71	13.79	1898.166	10.68
5	14.93	0.350	114.00	16.26	2724.121	15.33
6	20.52	0.512	73.57	10.49	2766.841	15.57
7	23.79	0.478	158.53	22.61	4998.116	28.13
7	26.50	0.375	701.07	100.00	17769.143	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/17/2021 4:31:35 PM
Printed by: wet


Ident: ICV
Analysis from: 8/16/2021 2:22:07 PM
File: _2021-08-16_

Last save: 8/16/2021 2:48:38 PM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 27909

Last save: 8/16/2021 2:03:

SAMPLE:
: AM/AP
Vial number: 9
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

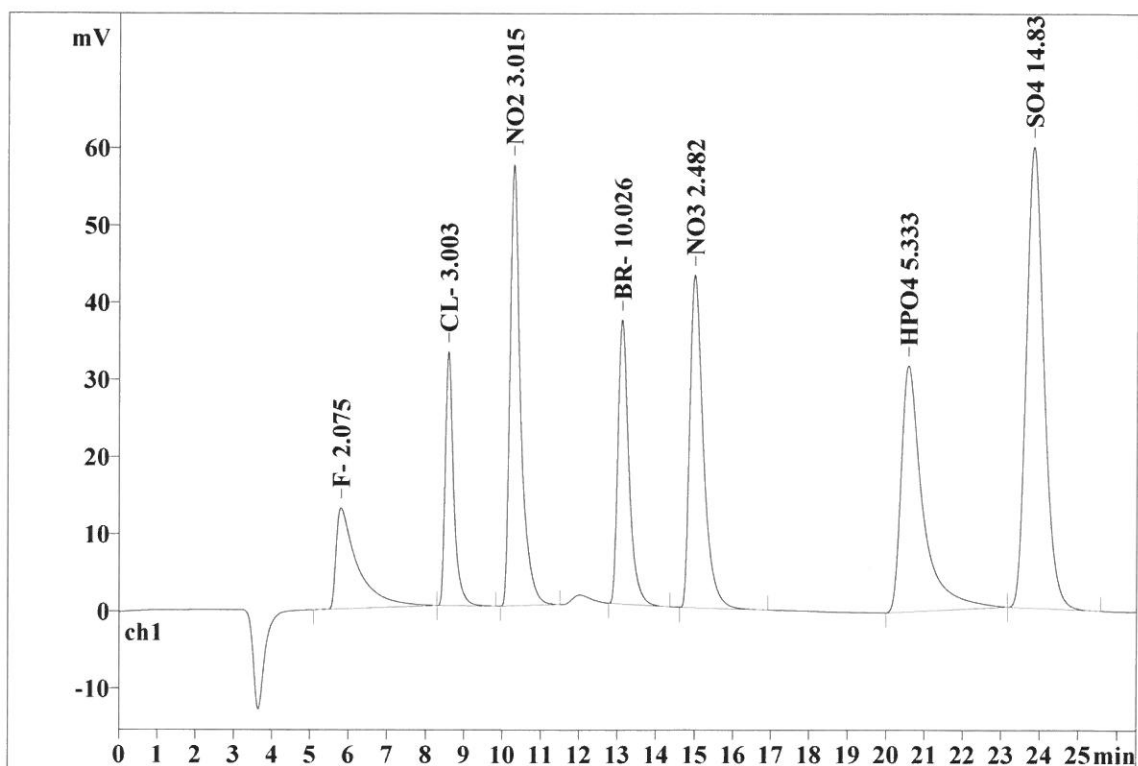

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.80	0.504	13.08	4.76	506.270	7.17
2	8.58	0.217	32.89	11.98	498.972	7.06
3	10.27	0.279	57.10	20.79	1122.328	15.89
4	13.11	0.296	36.82	13.41	735.757	10.41
5	14.99	0.358	43.10	15.69	1044.695	14.79
6	20.57	0.528	31.89	11.61	1255.288	17.77
7	23.82	0.482	59.76	21.76	1901.107	26.91
7	26.50	0.381	274.65	100.00	7064.419	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/17/2021 4:31:44 PM
Printed by: wet


Ident: ICB
Analysis from: 8/16/2021 2:51:40 PM
File: _2021-08-16_

Last save: 8/16/2021 3:22:33 PM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 27910

Last save: 8/16/2021 2:03:

SAMPLE:
: AP/MA
Vial number: 10
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

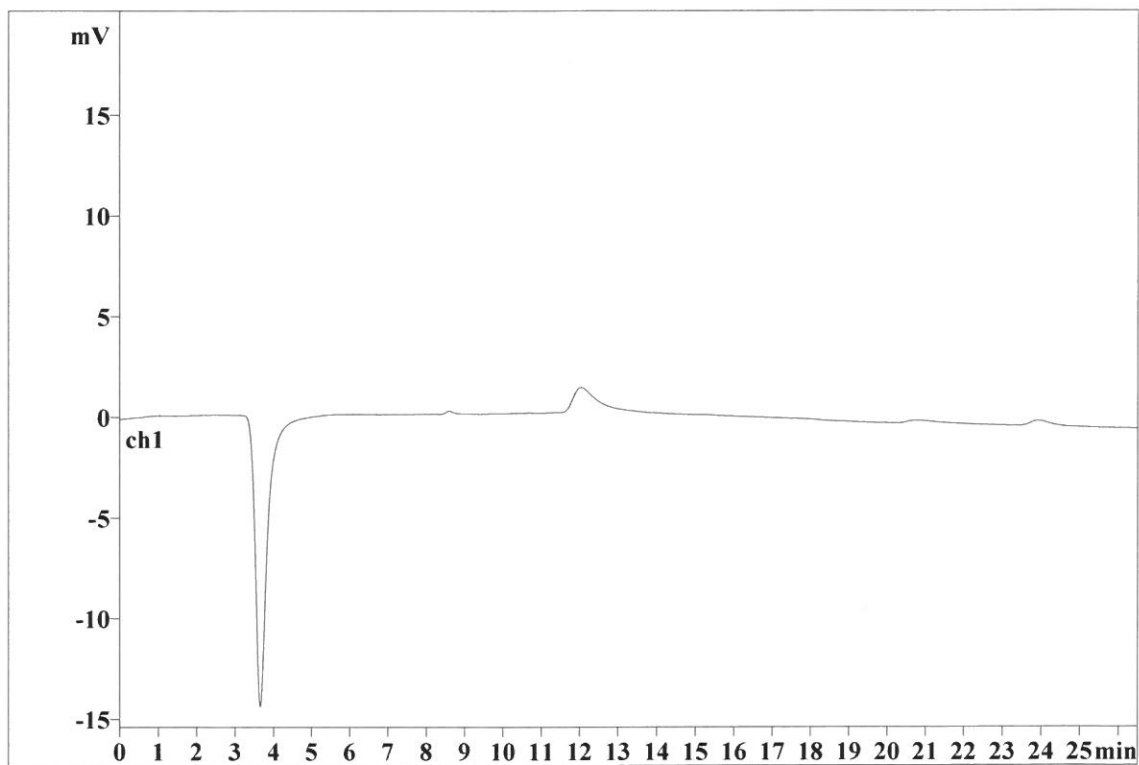

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 9/13/2021 10:55:01 AM
Printed by: wet


Ident: CCV
Analysis from: 9/10/2021 11:08:27 AM
File: _2021-09-10_

Last save: 9/10/2021 11:45:06 AM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 28154

Last save: 8/31/2021 9:16:

SAMPLE:
: AP/MA
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

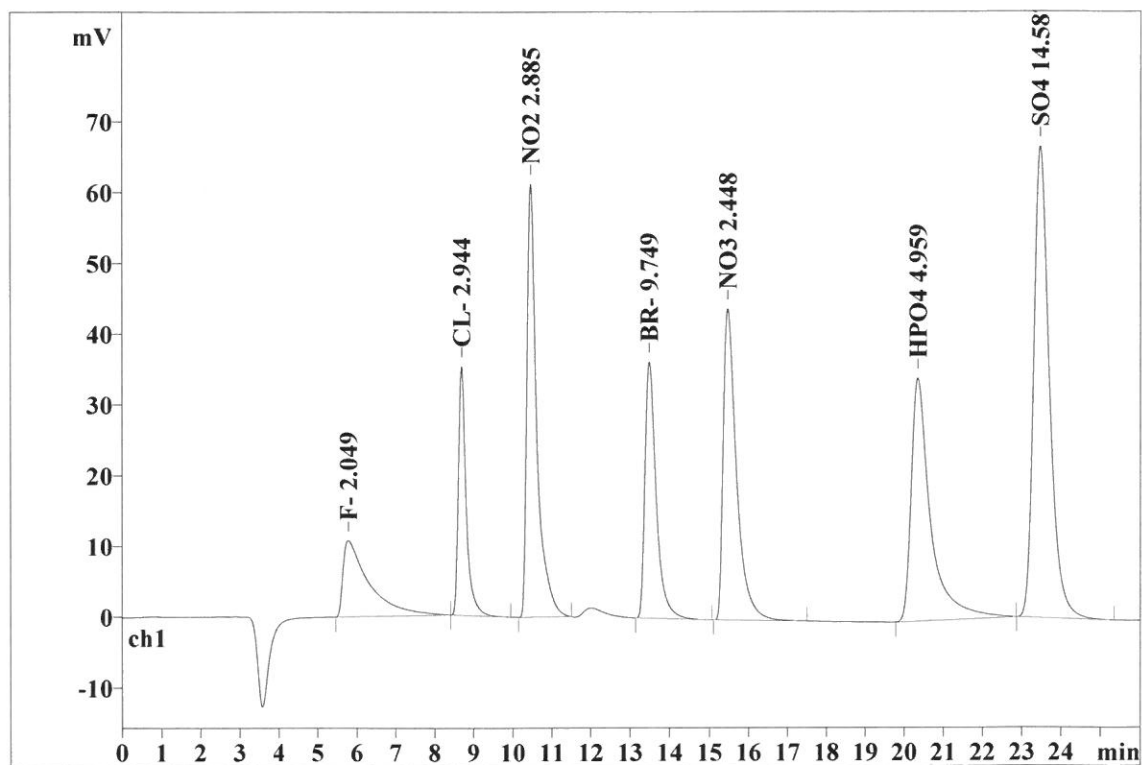

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.78	0.608	10.79	3.74	499.611	7.30
2	8.68	0.194	35.14	12.18	488.758	7.14
3	10.45	0.238	61.23	21.23	1072.223	15.66
4	13.48	0.285	36.27	12.57	714.509	10.43
5	15.47	0.336	43.98	15.25	1029.571	15.03
6	20.35	0.447	34.35	11.91	1175.405	17.16
7	23.48	0.416	66.65	23.11	1867.843	27.28
7	26.00	0.361	288.41	100.00	6847.921	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/13/2021 10:56:03 AM
Printed by: wet


Ident: CCB
Analysis from: 9/10/2021 11:47:53 AM
File: _2021-09-10_

Last save: 9/10/2021 12:13:53 PM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 28155

Last save: 8/31/2021 9:16:

SAMPLE:
: AP/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

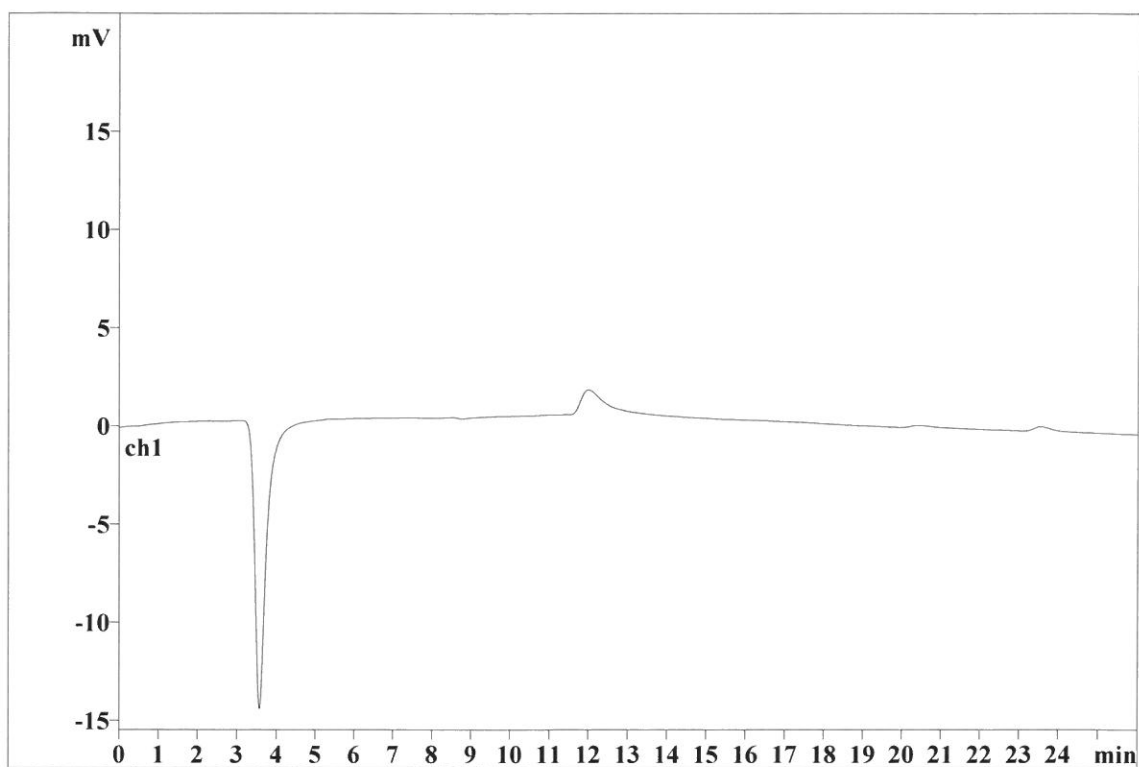

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 9/13/2021 10:56:10 AM
Printed by: wet


Ident: LB116261BLW
Analysis from: 9/10/2021 12:16:31 PM
File: _2021-09-10_

Last save: 9/13/2021 10:54:46 AM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 28156

Last save: 8/31/2021 9:16:

SAMPLE:
: AP/MA
Vial number: 13
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

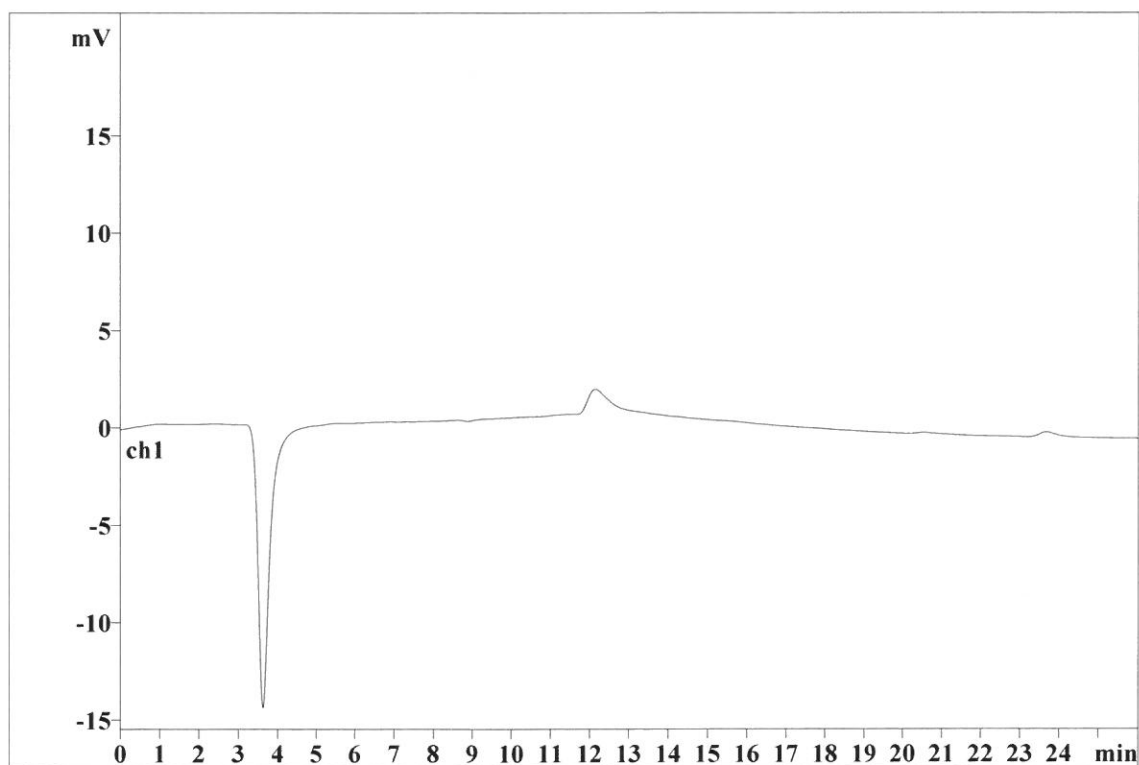

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 9/13/2021 10:56:17 AM
Printed by: wet


Ident: LB116261BSW
Analysis from: 9/10/2021 12:45:08 PM
File: _2021-09-10_

Last save: 9/13/2021 10:54:46 AM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 28157

Last save: 8/31/2021 9:16:

SAMPLE:
: AP/MA
Vial number: 14
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

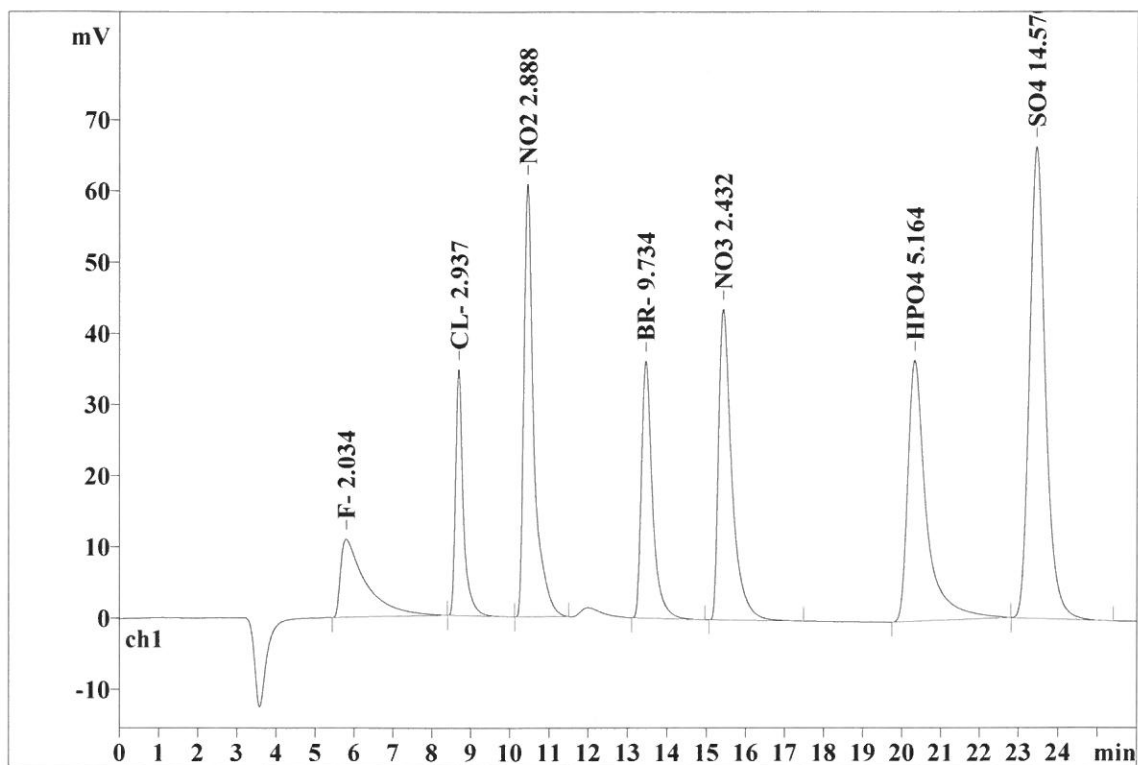

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.78	0.599	10.98	3.80	495.787	7.21
2	8.67	0.194	34.59	11.96	487.607	7.09
3	10.43	0.237	60.82	21.03	1073.223	15.61
4	13.44	0.285	36.14	12.50	713.325	10.37
5	15.42	0.336	43.66	15.10	1022.520	14.87
6	20.31	0.440	36.70	12.69	1219.343	17.73
7	23.43	0.418	66.29	22.92	1865.526	27.13
7	26.00	0.358	289.18	100.00	6877.331	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/13/2021 10:56:43 AM
Printed by: wet


Ident: M3688-01
Analysis from: 9/10/2021 1:14:21 PM
File: _2021-09-10_

Last save: 9/10/2021 1:42:07 PM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 28158

Last save: 8/31/2021 9:16:

SAMPLE:
: AP/MA
Vial number: 19
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

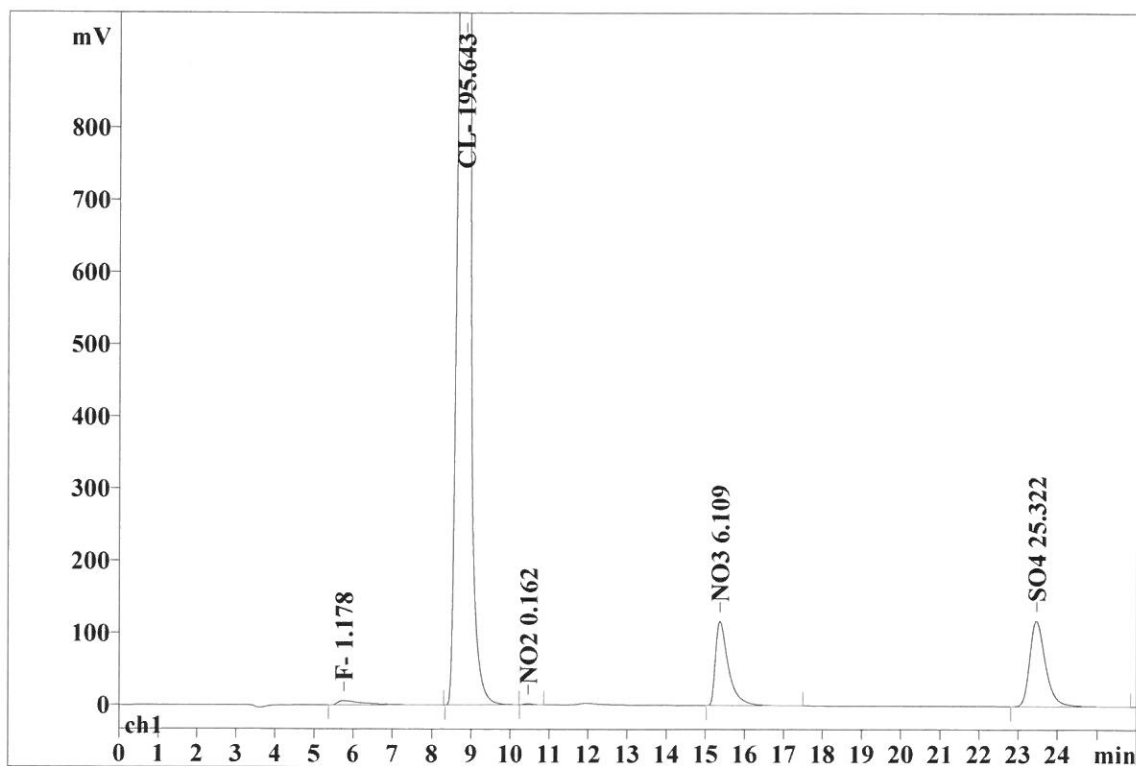

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.76	0.622	5.85	0.33	278.315	0.70
2	8.81	0.340	1526.05	86.29	33365.789	84.20
3	10.47	0.216	1.33	0.08	18.340	0.05
4	0.00	0.000	0.00	0.00	0.000	0.00
5	15.37	0.322	116.55	6.59	2644.637	6.67
6	0.00	0.000	0.00	0.00	0.000	0.00
7	23.46	0.413	118.68	6.71	3317.413	8.37
7	26.00	0.273	1768.46	99.99	39624.494	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/13/2021 10:57:06 AM
 Printed by: wet


Ident: M3681-04RE
 Analysis from: 9/10/2021 3:16:32 PM
 File: _2021-09-10_

Last save: 9/13/2021 10:57:01 AM

Method: AnionsIC2-081621.mtw
 Run operator: wet
 Analysis number: 28162

Last save: 8/31/2021 9:16:

SAMPLE:
 : AP/MA
 Vial number: 18
 Volume: 20.0 µL
 Dilution: 1.00
 Amount: 1.0000

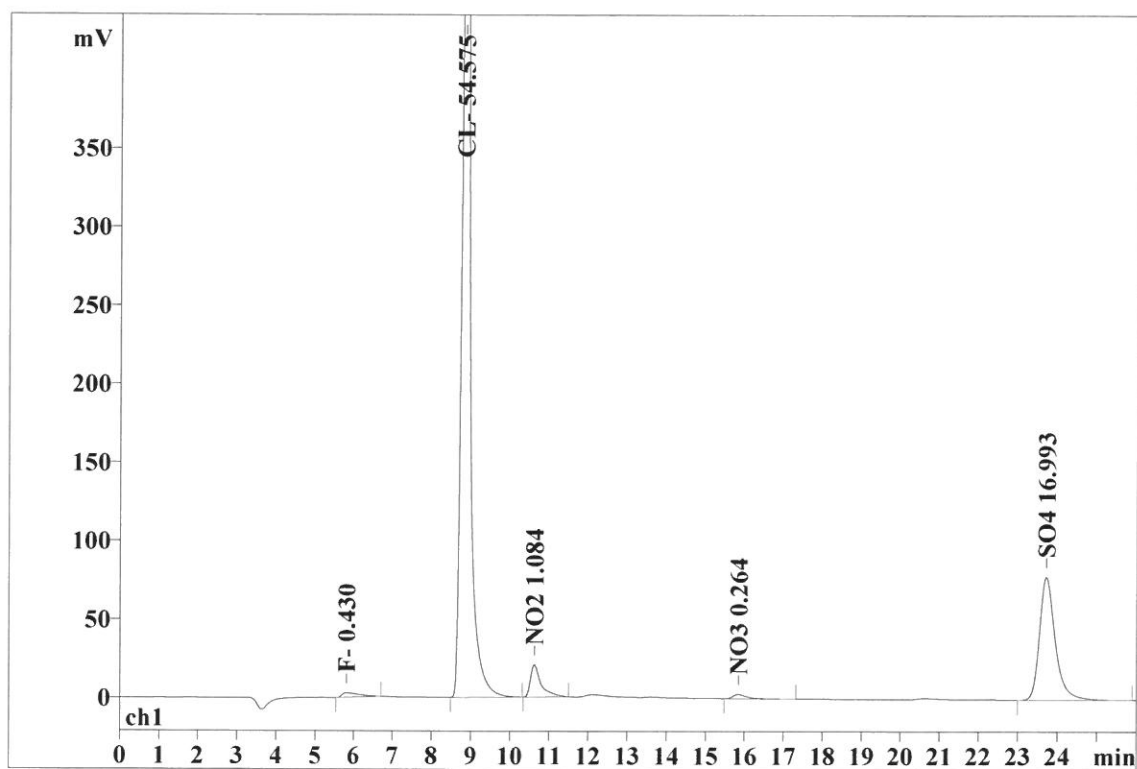

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.82	0.479	2.88	0.36	88.409	0.74
2	8.81	0.181	705.47	87.10	9297.740	77.35
3	10.62	0.238	20.47	2.53	375.156	3.12
4	0.00	0.000	0.00	0.00	0.000	0.00
5	15.85	0.338	2.77	0.34	66.013	0.55
6	0.00	0.000	0.00	0.00	0.000	0.00
7	23.71	0.406	78.32	9.67	2192.691	18.24
7	26.00	0.235	809.91	100.00	12020.009	100.00

This report has been created by IC Net
 METROHM LTD

Report date: 9/13/2021 10:58:16 AM
Printed by: wet


Ident: M3688-01MS
Analysis from: 9/10/2021 3:45:12 PM
File: _2021-09-10_

Last save: 9/13/2021 10:58:14 AM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 28163

Last save: 8/31/2021 9:16:

SAMPLE:
: AP/MA
Vial number: 20
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

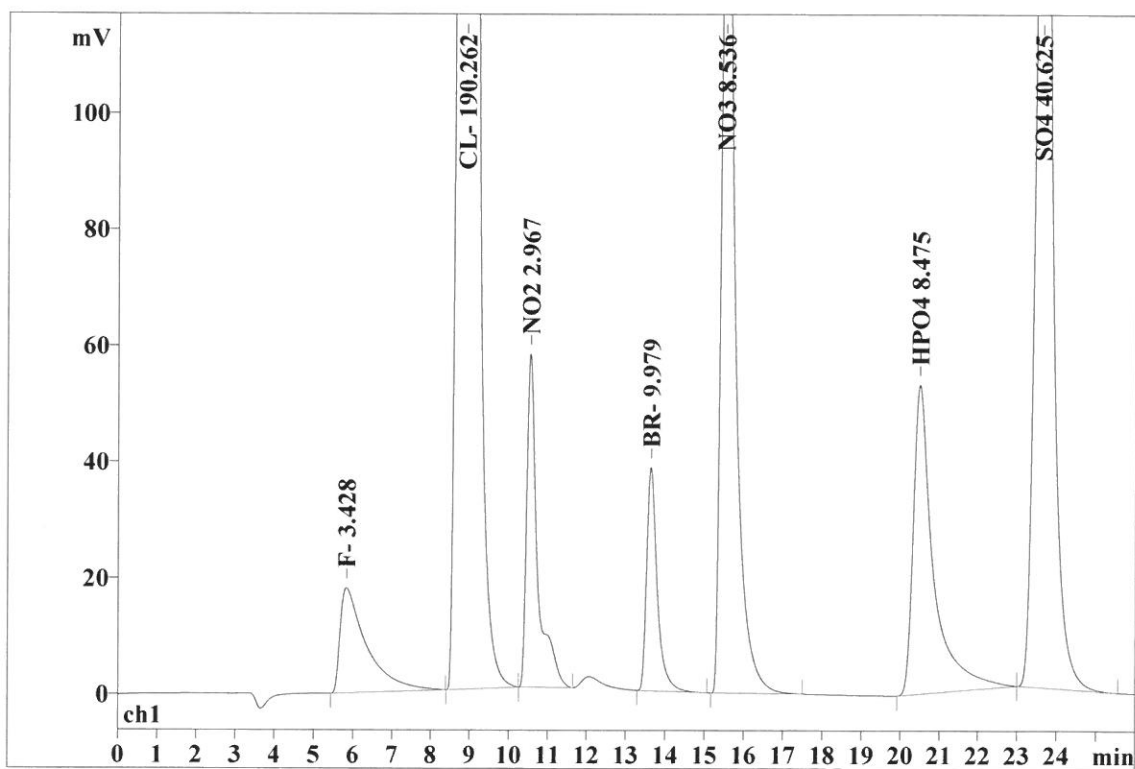

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.82	0.635	18.07	0.88	849.791	1.84
2	8.88	0.329	1516.81	74.08	32447.748	70.30
3	10.54	0.237	57.36	2.80	1103.927	2.39
4	13.62	0.274	38.42	1.88	732.191	1.59
5	15.51	0.318	164.72	8.05	3715.423	8.05
6	20.49	0.452	53.22	2.60	1926.113	4.17
7	23.61	0.400	198.76	9.71	5383.992	11.66
7	26.00	0.378	2047.37	100.00	46159.185	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/13/2021 10:58:54 AM
Printed by: wet


Ident: M3688-01MSD
Analysis from: 9/10/2021 4:13:50 PM
File: _2021-09-10_

Last save: 9/13/2021 10:58:54 AM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 28164

Last save: 8/31/2021 9:16:

SAMPLE:
: AP/MA
Vial number: 21
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

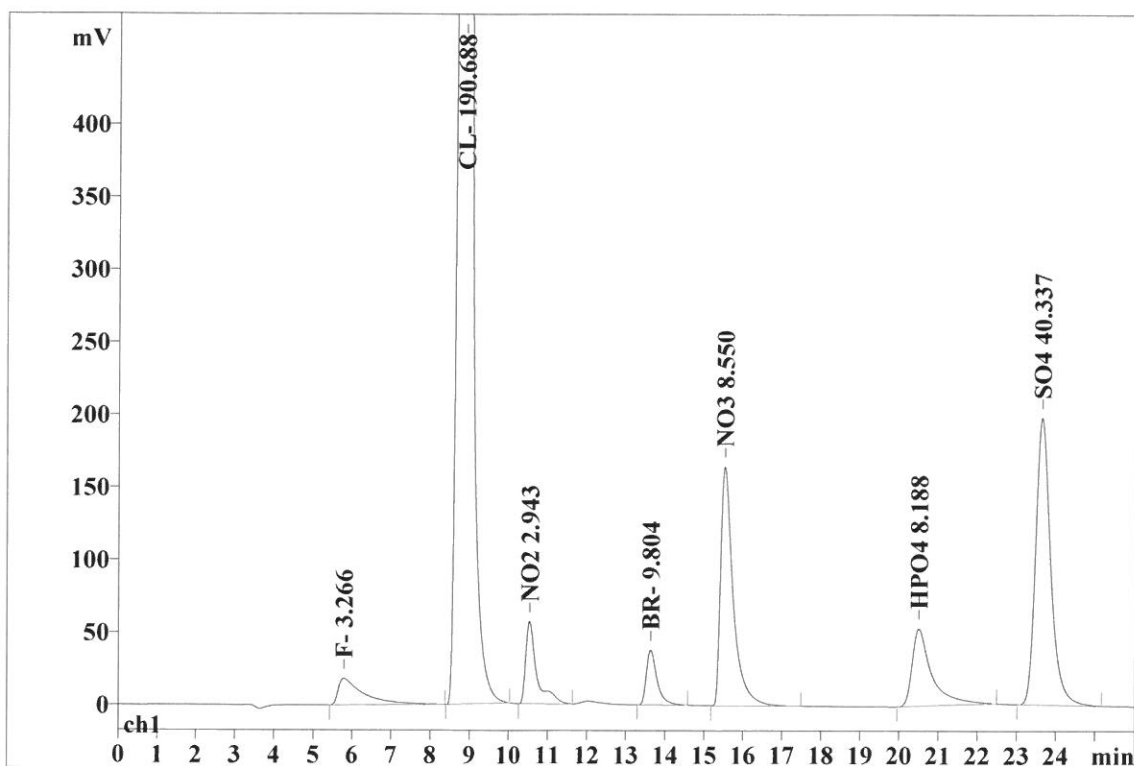

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.79	0.585	18.15	0.89	808.776	1.76
2	8.87	0.330	1517.98	74.17	32520.390	70.58
3	10.54	0.238	56.72	2.77	1094.614	2.38
4	13.63	0.275	37.87	1.85	718.712	1.56
5	15.52	0.318	164.68	8.05	3721.290	8.08
6	20.50	0.452	53.27	2.60	1864.743	4.05
7	23.63	0.399	197.77	9.66	5345.010	11.60
7	26.00	0.371	2046.44	100.00	46073.536	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/13/2021 10:59:25 AM
Printed by: wet


Ident: CCV
Analysis from: 9/10/2021 5:39:54 PM
File: _2021-09-10_

Last save: 9/10/2021 6:05:55 PM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 28167

Last save: 8/31/2021 9:16:

SAMPLE:
: AP/MA
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

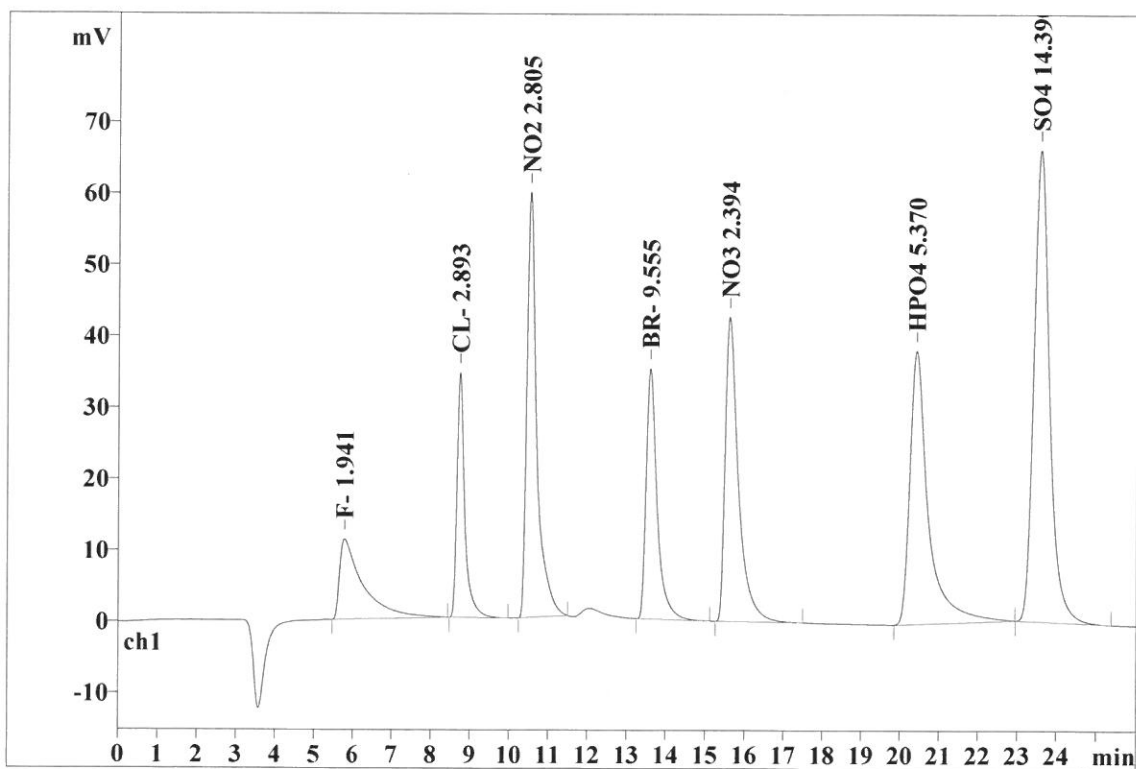

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.78	0.538	11.25	3.92	472.207	6.94
2	8.73	0.192	34.34	11.95	480.112	7.06
3	10.53	0.236	59.56	20.73	1041.312	15.31
4	13.59	0.285	35.10	12.22	699.538	10.28
5	15.61	0.335	42.63	14.84	1005.951	14.79
6	20.41	0.430	38.31	13.34	1263.309	18.57
7	23.57	0.410	66.11	23.01	1841.261	27.06
7	26.00	0.346	287.29	100.00	6803.691	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/13/2021 10:59:34 AM
Printed by: wet


Ident: CCB
Analysis from: 9/10/2021 6:08:33 PM
File: _2021-09-10_

Last save: 9/10/2021 6:34:33 PM

Method: AnionsIC2-081621.mtw
Run operator: wet
Analysis number: 28168

Last save: 8/31/2021 9:16:

SAMPLE:
: AP/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

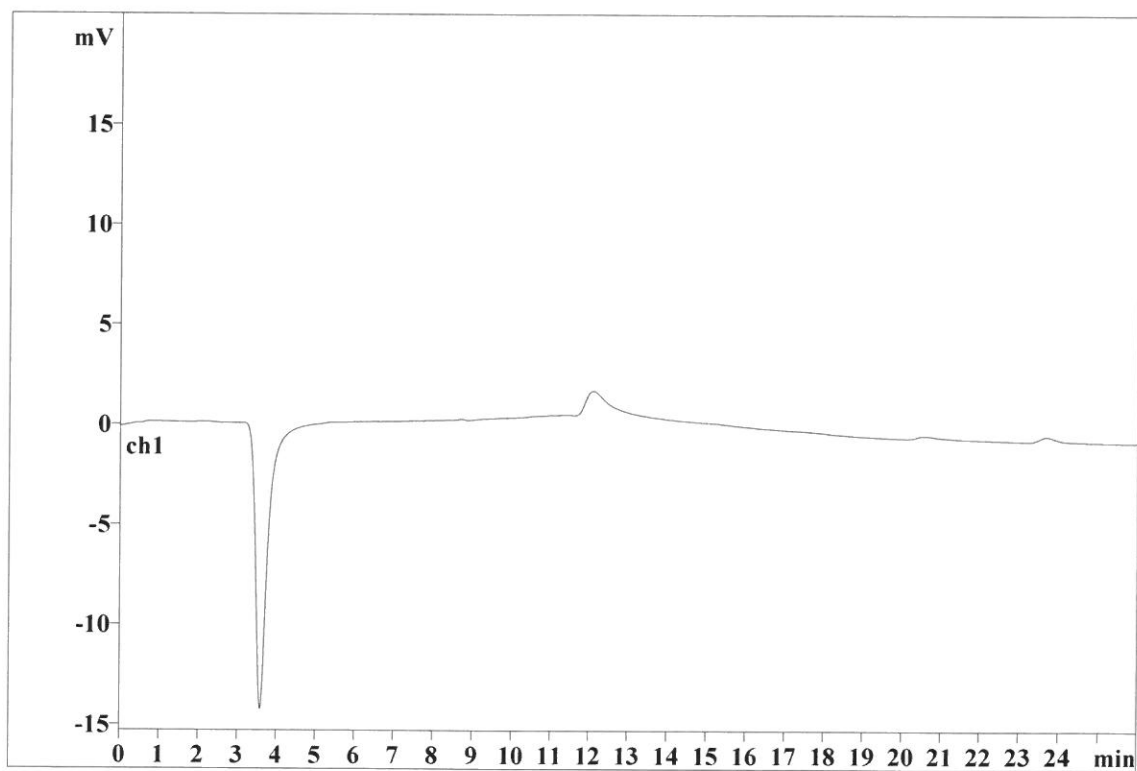

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD