

LB116265

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092Reviewed by : PS Instrument ID : Konelab

9/13/2021 11:15

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.228	0.0	0.073	
ICB1	1.891	0.0	0.001	
CCV1	235.373	0.0	0.180	
CCB1	1.610	0.0	0.001	
PB139048BL	1.741	0.0	0.001	
M3686-02	1.401	0.0	0.000	
M3686-02DUP	1.899	0.0	0.001	
M3709-02	1.670	0.0	0.001	
M3709-05	1.815	0.0	0.001	
PB139049BL	1.656	0.0	0.001	
M3688-01	1.764	0.0	0.001	
M3688-01DUP	1.775	0.0	0.001	
CCV2	253.180	0.0	0.194	
CCB2	1.882	0.0	0.001	

N	14
Mean	43.063
SD	88.8560
CV%	206.34

Aquakem v. 7.2AQ1

Results from time period:

Mon Sep 13 10:15:01 2021

Mon Sep 13 11:10:08 2021

Sample Id	Sam/Ctr/c/	Test short narr	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	-0.9606	µg/l	9/13/2021 10:32:10	
5.OPPBCN	A	Reactive CN	P	5.6913	µg/l	9/13/2021 10:32:11	
10PPBCN	A	Reactive CN	P	10.5393	µg/l	9/13/2021 10:32:12	
50PPBCN	A	Reactive CN	P	52.4711	µg/l	9/13/2021 10:32:13	
100PPBCN	A	Reactive CN	P	98.6147	µg/l	9/13/2021 10:32:14	
250PPBCN	A	Reactive CN	P	247.2641	µg/l	9/13/2021 10:32:15	
500PPBCN	A	Reactive CN	P	501.3802	µg/l	9/13/2021 10:32:16	
ICV1	S	Reactive CN	P	95.228	µg/l	9/13/2021 11:06:15	
ICB1	S	Reactive CN	P	1.8914	µg/l	9/13/2021 11:06:16	
CCV1	S	Reactive CN	P	235.3728	µg/l	9/13/2021 11:06:17	
CCB1	S	Reactive CN	P	1.6095	µg/l	9/13/2021 11:06:18	
PB139048BL	S	Reactive CN	P	1.7406	µg/l	9/13/2021 11:06:19	
M3686-02	S	Reactive CN	P	1.4006	µg/l	9/13/2021 11:06:20	
M3686-02DUP	S	Reactive CN	P	1.899	µg/l	9/13/2021 11:06:21	
M3709-02	S	Reactive CN	P	1.6704	µg/l	9/13/2021 11:06:22	
M3709-05	S	Reactive CN	P	1.8152	µg/l	9/13/2021 11:06:23	
PB139049BL	S	Reactive CN	P	1.656	µg/l	9/13/2021 11:06:24	
M3688-01	S	Reactive CN	P	1.7636	µg/l	9/13/2021 11:06:25	
M3688-01DUP	S	Reactive CN	P	1.7748	µg/l	9/13/2021 11:10:06	
CCV2	S	Reactive CN	P	253.1801	µg/l	9/13/2021 11:10:07	
CCB2	S	Reactive CN	P	1.8823	µg/l	9/13/2021 11:10:08	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : ph Instrument ID : Konelab

9/13/2021 10:33


Test Total CN

Accepted 9/13/2021 10:33

Factor 1300
Bias -0.001

Coeff. of det. 0.999907

Errors

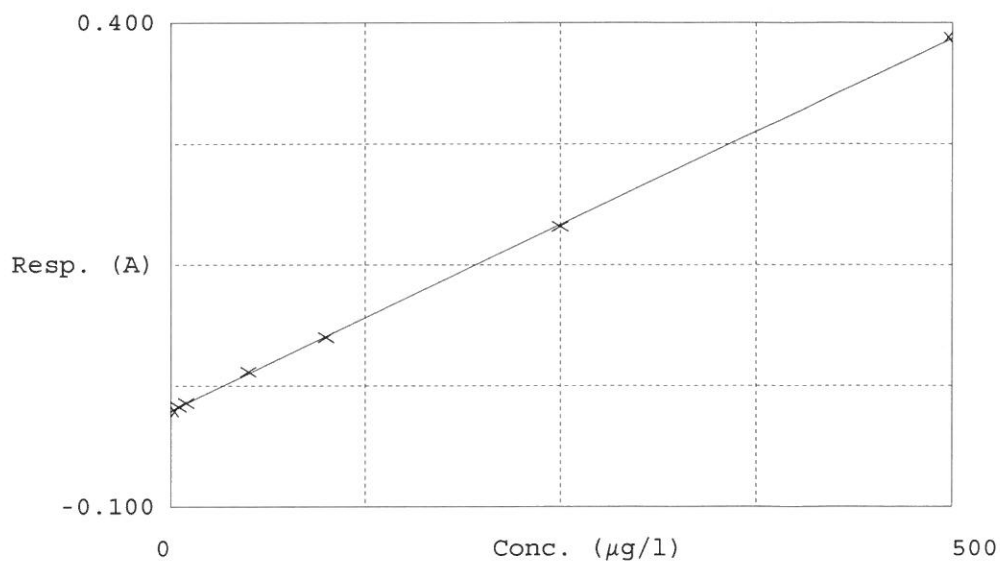

	Calibrator	Response	Calc. con.	Conc.	Rel. Errors
1	0.0PPBCN	-0.001	-0.9606	0.0000	
2	5.0PPBCN	0.004	5.6913	5.0000	13.8
3	10PPBCN	0.007	10.5393	10.0000	5.4
4	50PPBCN	0.040	52.4711	50.0000	4.9
5	100PPBCN	0.075	98.6147	100.0000	-1.4
6	250PPBCN	0.190	247.2641	250.0000	-1.1
7	500PPBCN	0.385	501.3802	500.0000	0.3

9/13/21