

=====

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : *ph*

Instrument ID : Konelab

9/16/2021 12:33

Test: Total CN

ml

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	93.667	0.0	0.071	
ICB1	1.457	0.0	0.001	
CCV1	240.116	0.0	0.182	
CCB1	1.794	0.0	0.001	
PB139140BL	1.764	0.0	0.001	
PB139140BS	99.980	0.0	0.076	
LOWPB139140	11.100	0.0	0.008	
HIGHPB139140	546.683	0.0	0.416	Test limit high
M3720-02	1.834	0.0	0.001	
M3720-02DUP	2.001	0.0	0.001	
M3720-02MS	40.631	0.0	0.031	
M3720-02MSD	41.386	0.0	0.031	
CCV2	246.967	0.0	0.188	
CCB2	1.963	0.0	0.001	

N	14
Mean	95.096
SD	155.2124
CV%	163.22

Aquakem v. 7.2AQ1

Results from time period:

Thu Sep 16 11:43:44 2021

Thu Sep 16 12:13:57 2021

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	0.9354	µg/l	9/16/2021 8:44:03	
5.0PPBCN	A	Total CN	P	5.7854	µg/l	9/16/2021 8:44:04	
10PPBCN	A	Total CN	P	10.4836	µg/l	9/16/2021 8:44:05	
50PPBCN	A	Total CN	P	52.2694	µg/l	9/16/2021 8:44:06	
100PPBCN	A	Total CN	P	97.8746	µg/l	9/16/2021 8:44:07	
250PPBCN	A	Total CN	P	244.9418	µg/l	9/16/2021 8:44:08	
500PPBCN	A	Total CN	P	502.7097	µg/l	9/16/2021 8:44:09	
ICV1	S	Total CN	P	93.6666	µg/l	9/16/2021 11:43:44	
ICB1	S	Total CN	P	1.4568	µg/l	9/16/2021 11:43:46	
CCV1	S	Total CN	P	240.1156	µg/l	9/16/2021 11:43:48	
CCB1	S	Total CN	P	1.7935	µg/l	9/16/2021 11:43:51	
PB139140BL	S	Total CN	P	1.7643	µg/l	9/16/2021 11:43:52	
PB139140BS	S	Total CN	P	99.9796	µg/l	9/16/2021 11:43:54	
LOWPB139140	S	Total CN	P	11.1001	µg/l	9/16/2021 12:07:40	
HIGHPB139140	S	Total CN	P	546.6832	µg/l	9/16/2021 12:07:41	
M3720-02	S	Total CN	P	1.8344	µg/l	9/16/2021 12:13:50	
M3720-02DUP	S	Total CN	P	2.0009	µg/l	9/16/2021 12:13:51	
M3720-02MS	S	Total CN	P	40.6305	µg/l	9/16/2021 12:13:52	
M3720-02MSD	S	Total CN	P	41.3856	µg/l	9/16/2021 12:13:53	
CCV2	S	Total CN	P	246.9671	µg/l	9/16/2021 12:13:55	
CCB2	S	Total CN	P	1.9631	µg/l	9/16/2021 12:13:57	

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : *ad*

Instrument ID : Konelab

9/16/2021 8:47


Test Total CN

Accepted 9/16/2021 8:47

Factor 1313
Bias 0

Coeff. of det. 0.999784

Errors

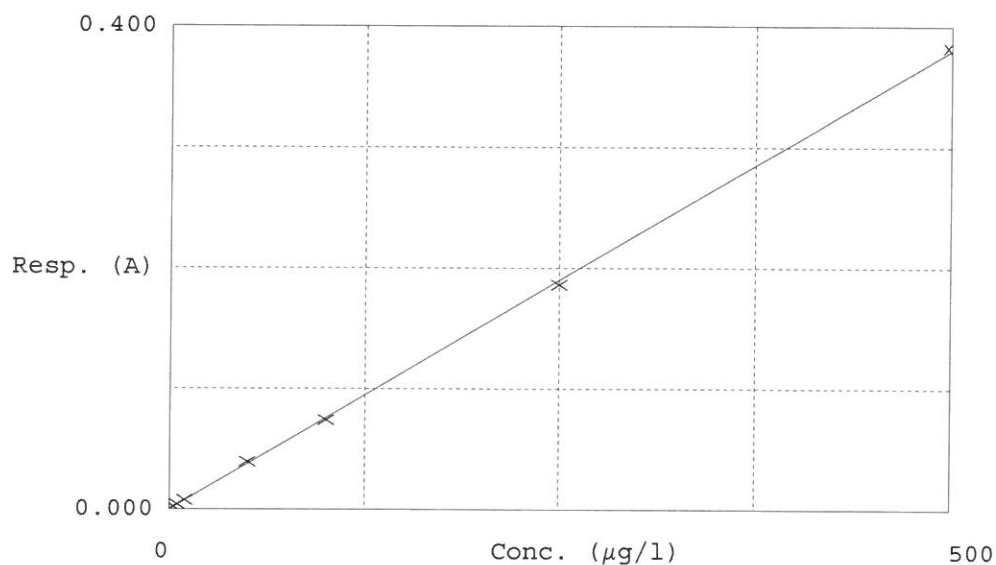

	Calibrator	Response	Calc. con.	Conc.
1	0.0PPBCN	0.000	0.9354	0.0000
2	5.0PPBCN	0.004	5.7854	5.0000
3	10PPBCN	0.008	10.4836	10.0000
4	50PPBCN	0.039	52.2694	50.0000
5	100PPBCN	0.074	97.8746	100.0000
6	250PPBCN	0.186	244.9418	250.0000
7	500PPBCN	0.382	502.7097	500.0000

Del.
Errors

Handwritten notes:
15.7
4.5
2.1
2.0
0.5
ad 9/16/21