

Clear table

Instrument ID: IC-2											Analyst : AP		Method: 300.0	
ident	concentra tion F-	concentratio n CL-	concentratio on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time	Initial wt/ Final Vol	Analyst			
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2021-09-13_	9/13/21 9:28		AP/MA			
STD2	0.4530	0.6660	0.6610	2.2230	0.5600	0.9030	3.4950	_2021-09-13_	9/13/21 9:56		AP/MA			
STD3	0.7810	1.2120	1.2070	4.0240	1.0050	2.0220	6.0720	_2021-09-13_	9/13/21 10:25		AP/MA			
STD4	0.9790	1.4690	1.4720	4.9020	1.2130	2.5760	7.3160	_2021-09-13_	9/13/21 10:53		AP/MA			
STD5	1.9870	2.9190	2.9230	9.7380	2.4490	5.0000	14.4070	_2021-09-13_	9/13/21 11:22		AP/MA			
STD6	3.9650	6.0220	6.0400	20.0810	5.0120	10.0590	30.0300	_2021-09-13_	9/13/21 11:51		AP/MA			
STD7	5.0350	7.5120	7.4970	25.0320	6.2620	12.4400	37.6810	_2021-09-13_	9/13/21 12:19		AP/MA			
ICV	1.9020	2.7850	2.8100	9.2990	2.3050	4.8630	13.7840	_2021-09-13_	9/13/21 12:53		AP/MA			
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2021-09-13_	9/13/21 13:24		AP/MA			
CCV	2.0420	2.8510	2.8470	9.5100	2.3640	5.4240	14.0850	_2021-09-14_	9/14/21 8:26		AP/MA			
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2021-09-14_	9/14/21 8:54		AP/MA			
LB116348BLW	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2021-09-14_	9/14/21 9:22		AP/MA			
LB116348BSW	2.0170	2.8470	2.8440	9.4970	2.3550	5.4230	14.0390	_2021-09-14_	9/14/21 9:50		AP/MA			
M3728-01	0.5780	108.1710	2.2740	0.0000	0.0000	0.1190	23.2800	_2021-09-14_	9/14/21 14:27		AP/MA			
M3728-01MS	2.3320	106.8240	5.1920	9.8640	2.4250	6.2880	38.2010	_2021-09-14_	9/14/21 15:01		AP/MA			
M3728-01MSD	2.2990	107.8890	5.2020	9.9500	2.4430	6.6090	38.0040	_2021-09-14_	9/14/21 15:29		AP/MA			
CCV	1.9480	2.8530	2.8650	9.5090	2.3690	5.8000	14.0720	_2021-09-14_	9/14/21 16:33		AP/MA			
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2021-09-14_	9/14/21 17:01		AP/MA			

21/12/21

Clear table

Instrument ID: IC-2 Analyst: AP Method: 300 / 9056A


ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time	Initial wt/ Final Vol	Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-09-13_	9/13/21 9:28		AP/MA
STD2	0.4530	0.6660	0.6610	2.2230	0.5600	0.9030	3.4950	2021-09-13_	9/13/21 9:56		AP/MA
STD3	0.7810	1.2120	1.2070	4.0240	1.0050	2.0220	6.0720	2021-09-13_	9/13/21 10:25		AP/MA
STD4	0.9790	1.4690	1.4720	4.9020	1.2130	2.5760	7.3160	2021-09-13_	9/13/21 10:53		AP/MA
STD5	1.9870	2.9190	2.9230	9.7380	2.4490	5.0000	14.4070	2021-09-13_	9/13/21 11:22		AP/MA
STD6	3.9650	6.0220	6.0400	20.0810	5.0120	10.0590	30.0300	2021-09-13_	9/13/21 11:51		AP/MA
STD7	5.0350	7.5120	7.4970	25.0320	6.2620	12.4400	37.6810	2021-09-13_	9/13/21 12:19		AP/MA

ident	True Value	True Value	True Value	True Value	True Value	True Value	True Value
	CL-	NO2	BR-	NO3	HPO4	SO4	SO4
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000
STD2	0.4000	0.6000	2.0000	0.5000	1.0000	3.0000	3.0000
STD3	0.8000	1.2000	4.0000	1.0000	2.0000	6.0000	6.0000
STD4	1.0000	1.5000	5.0000	1.2500	2.5000	7.5000	7.5000
STD5	2.0000	3.0000	10.0000	2.5000	5.0000	15.0000	15.0000
STD6	4.0000	6.0000	20.0000	5.0000	10.0000	30.0000	30.0000
STD7	5.0000	7.5000	25.0000	6.2500	12.5000	37.5000	37.5000

ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4
STD1							
STD2	13.2500	11.0000	10.1667	11.1500	12.0000	-9.7000	16.5000
STD3	-2.3750	1.0000	0.5833	0.6000	0.5000	1.1000	1.2000
STD4	-2.1000	-2.0667	-1.8667	-1.9600	-2.9600	3.0400	-2.4533
STD5	-0.6500	-2.7000	-2.5667	-2.6200	-2.0400	0.0000	-3.9533
STD6	-0.8750	0.3667	0.6667	0.4050	0.2400	0.5900	0.1000
STD7	0.7000	0.1600	-0.0400	0.1280	0.1920	-0.4800	0.4827

CALIBRATION OF COMPONENT F-

Method: AnionsIC2-091321.mtw
 Equation: $Q = 0.0749559 \cdot A + 2.23179$
 RSD: 1.789 %
 Correlation coefficient: 0.999825

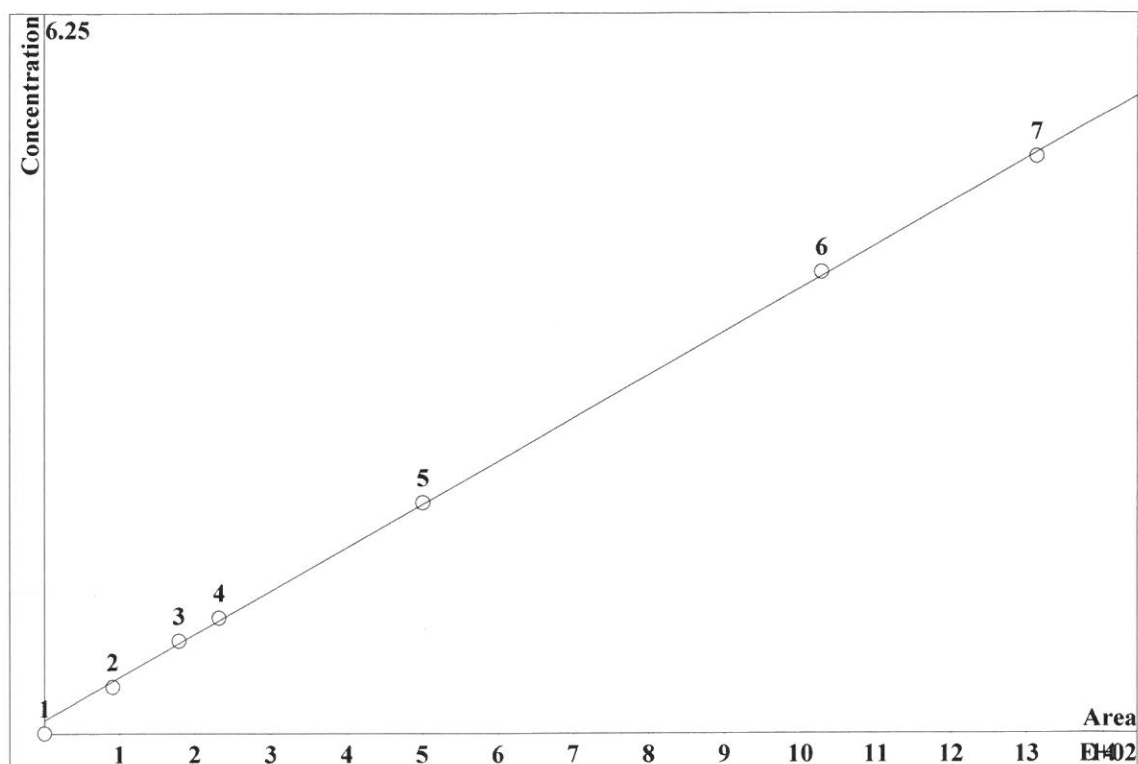

K3 = 0 K2 = 0 K1 = 0.0749559 K0 = 2.23179

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used File
1	0	0	0	0	0	
2	1.941	90.97	0.4	20	5.75	
3	4.144	178.7	0.8	20	5.681	
4	5.603	231.5	1	20	5.681	
5	11.65	500.5	2	20	5.681	
6	26.23	1028	4	20	5.681	
7	34.59	1314	5	20	5.681	

CALIBRATION OF COMPONENT CL-

Method: AnionsIC2-091321.mtw
 Equation: $Q = 0.113181 \cdot A + 2.59138$
 RSD: 1.710 %
 Correlation coefficient: 0.999841

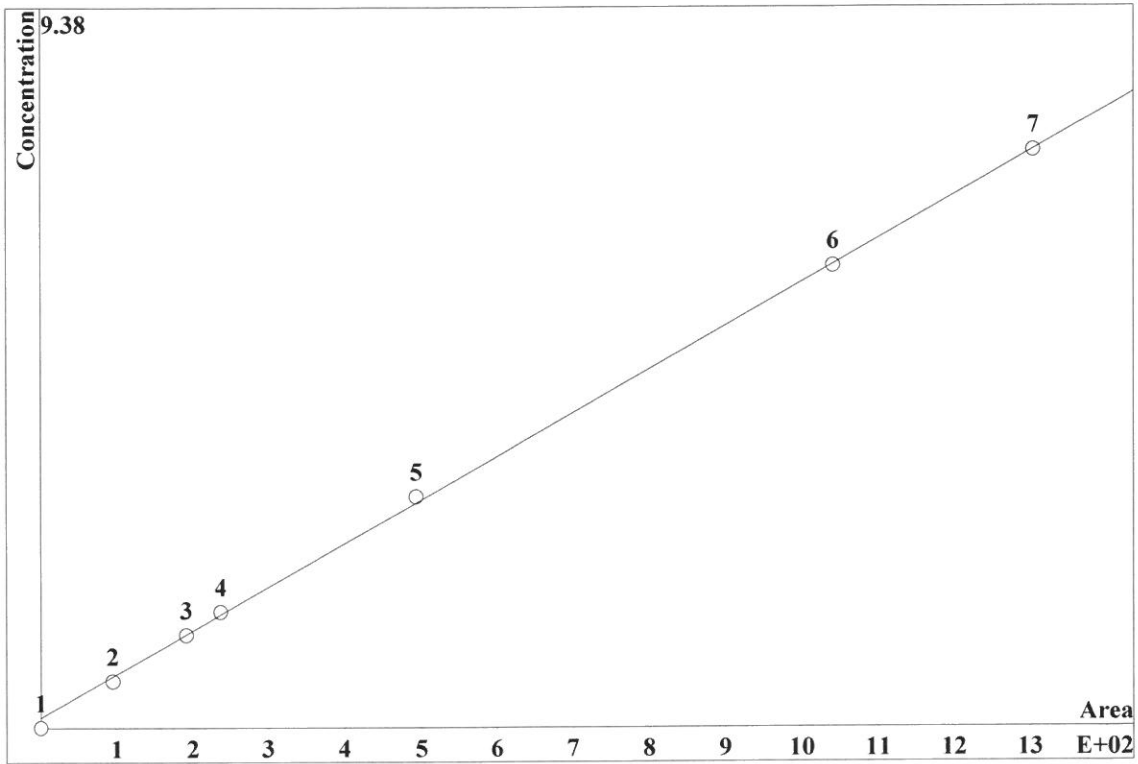


K3 = 0 K2 = 0 K1 = 0.113181 K0 = 2.59138
 Base: Area
 Ref.channel: chl
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used File
1	0	0	0	0	0	
2	6.714	94.84	0.6	20	8.834	
3	13.67	191.2	1.2	20	8.597	
4	16.95	236.7	1.5	20	8.597	
5	35.52	492.9	3	20	8.597	
6	77.36	1041	6	20	8.597	
7	97.01	1305	7.5	20	8.597	

CALIBRATION OF COMPONENT NO2

Method: AnionsIC2-091321.mtw
 Equation: $Q = 0.0503187 \cdot A + 2.6077$
 RSD: 1.668 %
 Correlation coefficient: 0.999848

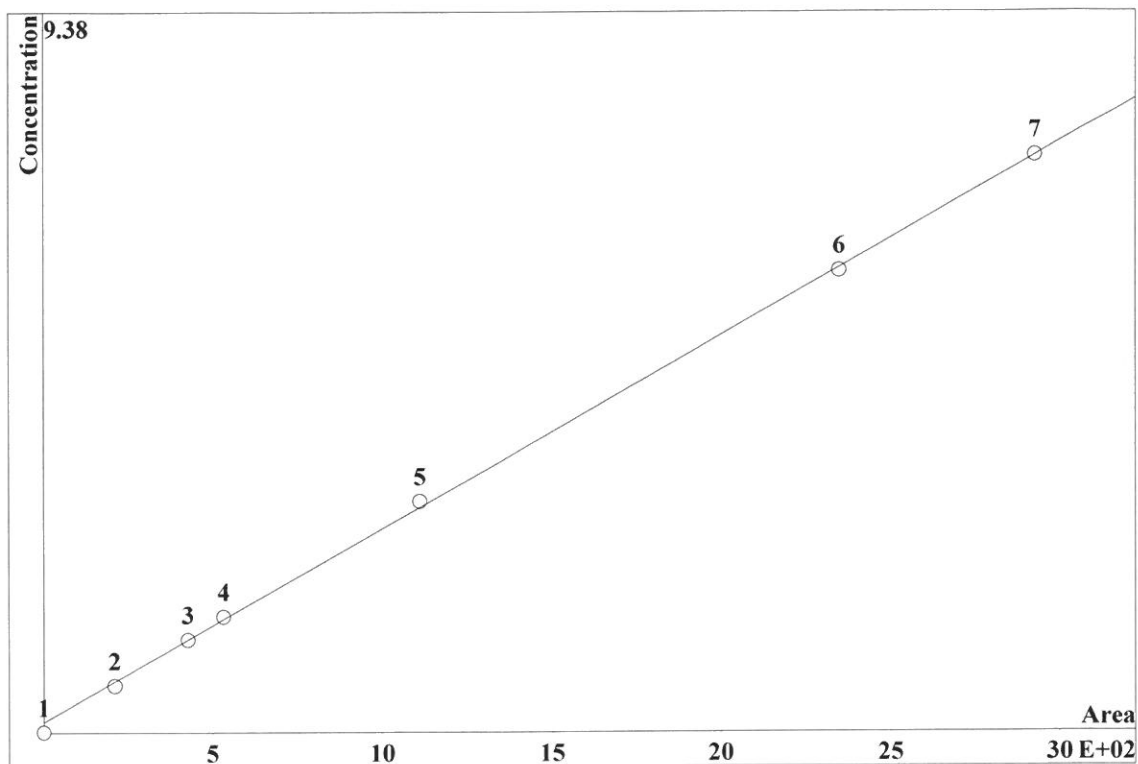

K3 = 0 K2 = 0 K1 = 0.0503187 K0 = 2.6077

Base: Area

Ref.channel: chl

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	12.42	211	0.6	20	10.64		
3	25.18	427.8	1.2	20	10.39		
4	30.84	533.3	1.5	20	10.39		
5	64.62	1110	3	20	10.39		
6	134	2349	6	20	10.39		
7	160.7	2928	7.5	20	10.39		

CALIBRATION OF COMPONENT BR-

Method: AnionsIC2-091321.mtw
 Equation: $Q = 0.253715 \cdot A + 9.42786$
 RSD: 1.675 %
 Correlation coefficient: 0.999847

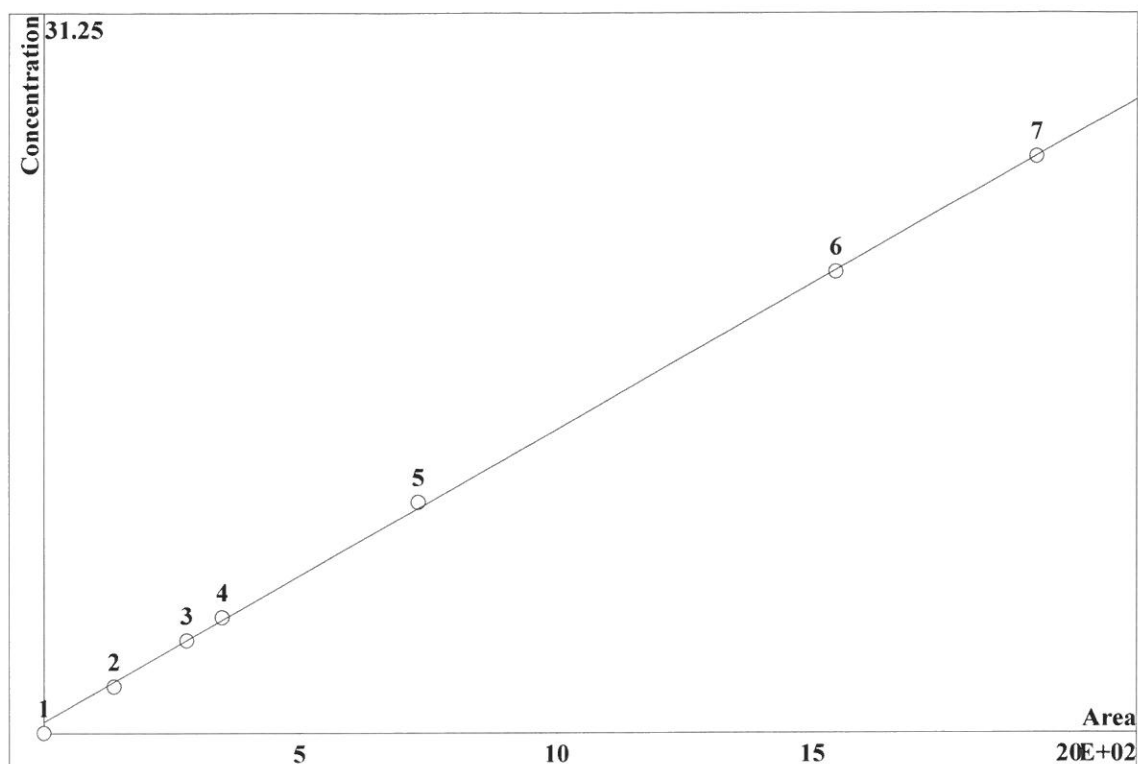

K3 = 0 K2 = 0 K1 = 0.253715 K0 = 9.42786

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	6.833	138	138	2	20		14
3	13.96	280	280	4	20		13.42
4	17.55	349.2	349.2	5	20		13.42
5	37.21	730.5	730.5	10	20		13.42
6	80.38	1546	1546	20	20		13.42
7	101.2	1936	1936	25	20		13.42

CALIBRATION OF COMPONENT NO3

Method: AnionsIC2-091321.mtw
 Equation: $Q = 0.0441836 \cdot A + 2.32995$
 RSD: 1.615 %
 Correlation coefficient: 0.999858

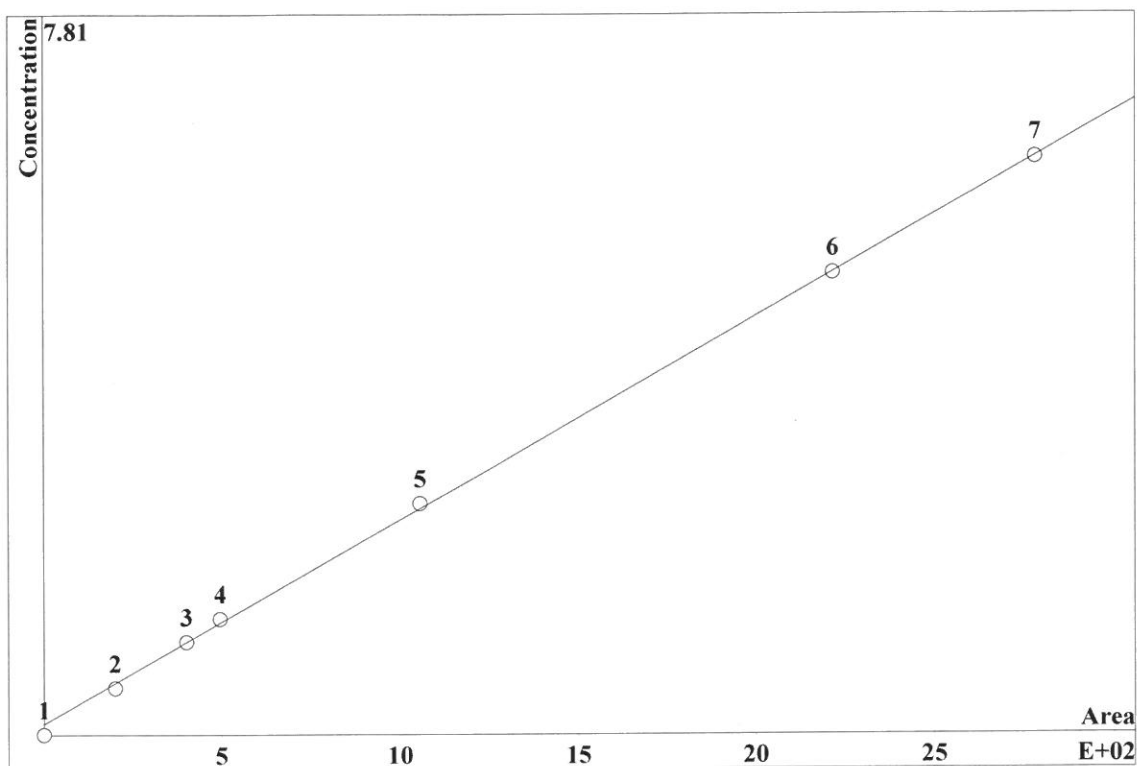

K3 = 0 K2 = 0 K1 = 0.0441836 K0 = 2.32995

Base: Area

Ref.channel: chl

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	8.385	200.7	0.5	20	16.28		
3	16.94	402.2	1	20	15.44		
4	21.23	496.4	1.25	20	15.44		
5	44.76	1056	2.5	20	15.44		
6	97.12	2216	5	20	15.44		
7	123.1	2782	6.25	20	15.44		

CALIBRATION OF COMPONENT HPO4

Method: AnionsIC2-091321.mtw
 Equation: $Q = 0.0871518 \cdot A - 5.87665$
 RSD: 1.374 %
 Correlation coefficient: 0.999897

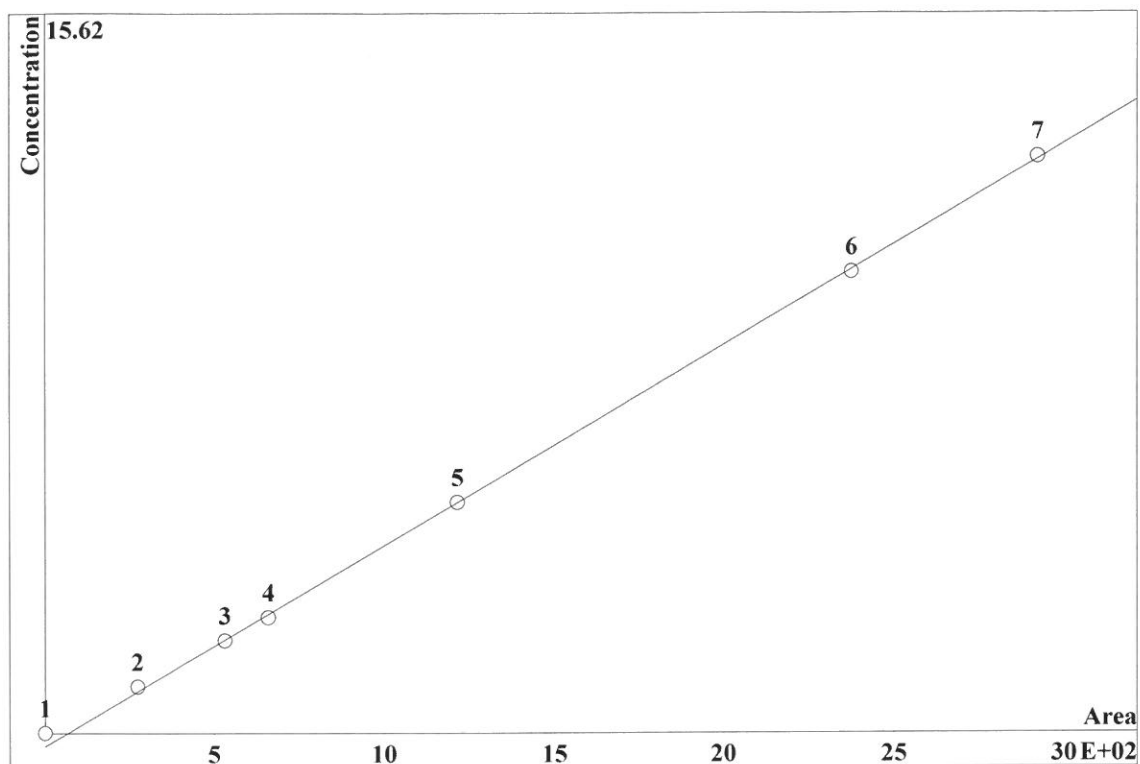

K3 = 0 K2 = 0 K1 = 0.0871518 K0 = -5.87665

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used File
1	0	0	0	0	0	0
2	7.585	274.6	1	20	21.2	
3	15.21	531.5	2	20	20.23	
4	19.46	658.7	2.5	20	20.23	
5	36.61	1215	5	20	20.23	
6	75.64	2376	10	20	20.23	
7	94.35	2922	12.5	20	20.23	

CALIBRATION OF COMPONENT SO4

Method: AnionsIC2-091321.mtw
 Equation: $Q = 0.142086 \cdot A + 17.996$
 RSD: 2.479 %
 Correlation coefficient: 0.999665

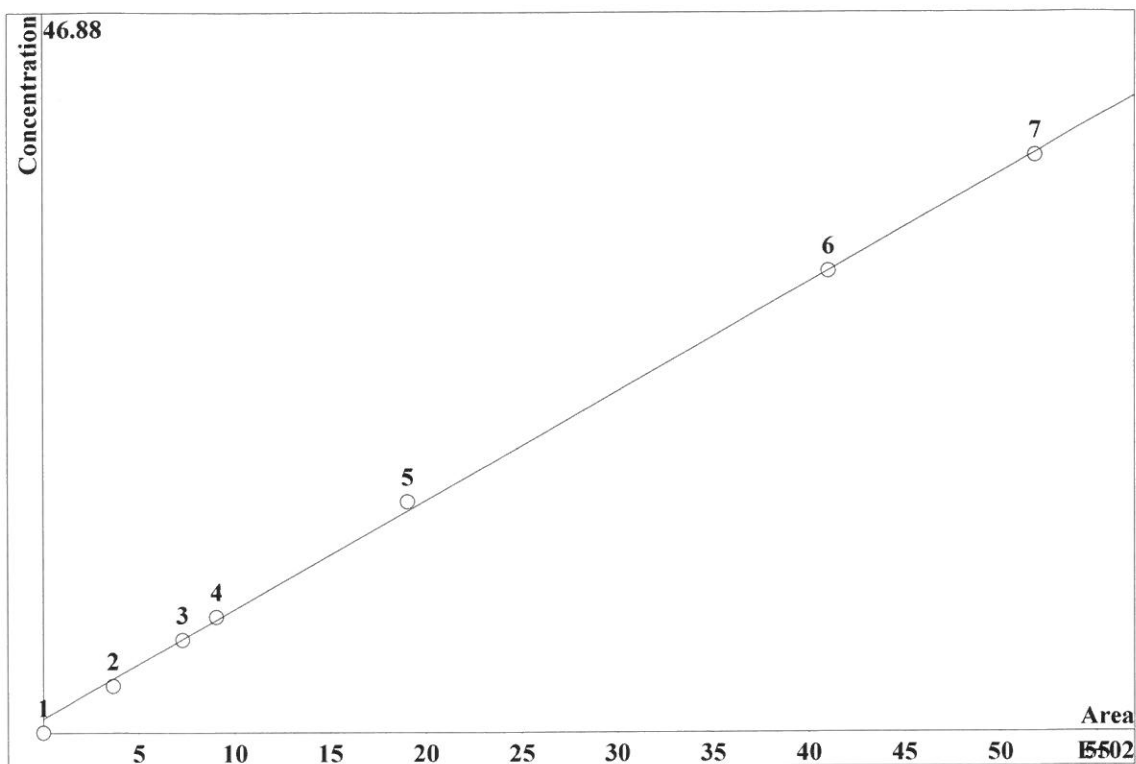

K3 = 0 K2 = 0 K1 = 0.142086 K0 = 17.996

Base: Area

Ref.channel: chl

ISTD:

Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used File
1	0	0	0	0	0	0
2	12.87	365.2	3	20	23.16	
3	25.71	728	6	20	23.11	
4	32.15	903.1	7.5	20	23.11	
5	68.6	1901	15	20	23.11	
6	151.4	4100	30	20	23.11	
7	191.6	5177	37.5	20	23.11	

Report date: 9/14/2021 11:39:52 AM
Printed by: wet


Ident: STD1
Analysis from: 9/13/2021 9:28:12 AM
File: _2021-09-13_

Last save: 9/13/2021 12:47:10 PM

Method: AnionsIC2-091321.mtw
Run operator: wet
Analysis number: 28174

Last save: 9/13/2021 8:25:

SAMPLE:
: AP/MA
Vial number: 2
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

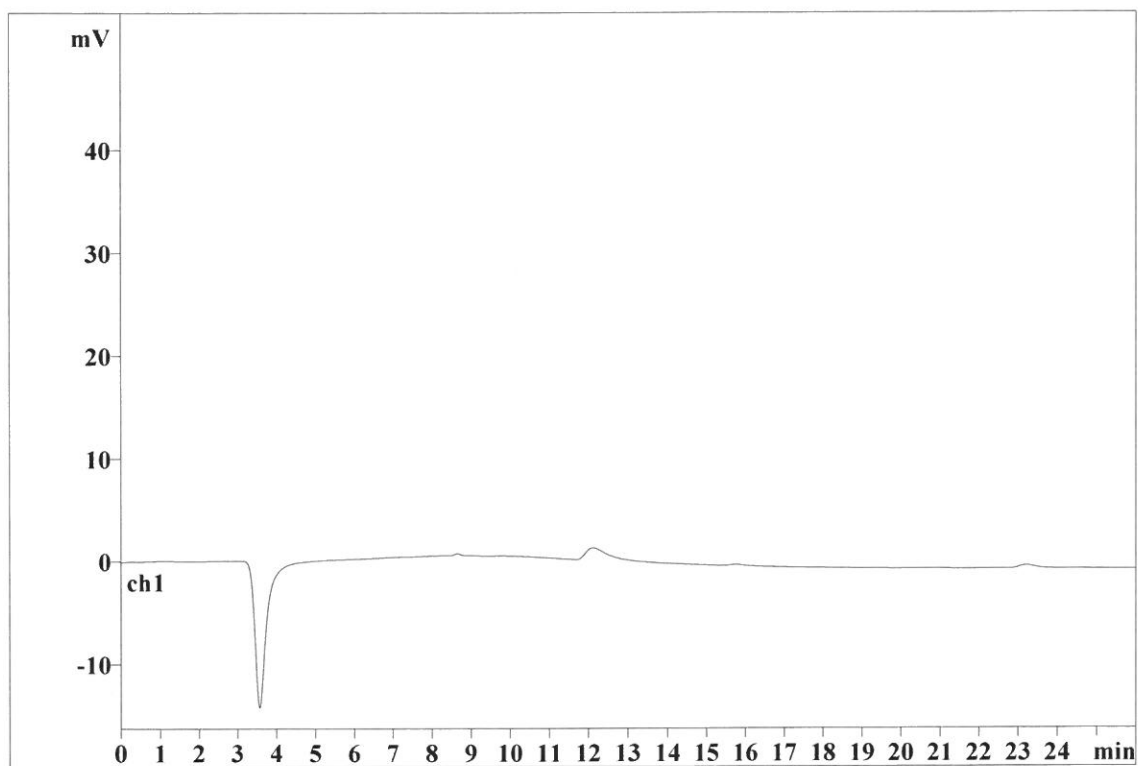

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 9/14/2021 11:39:59 AM
Printed by: wet


Ident: STD2
Analysis from: 9/13/2021 9:56:47 AM
File: _2021-09-13_

Last save: 9/13/2021 12:47:10 PM

Method: AnionsIC2-091321.mtw
Run operator: wet
Analysis number: 28175

Last save: 9/13/2021 8:25:

SAMPLE:
: AP/MA
Vial number: 3
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

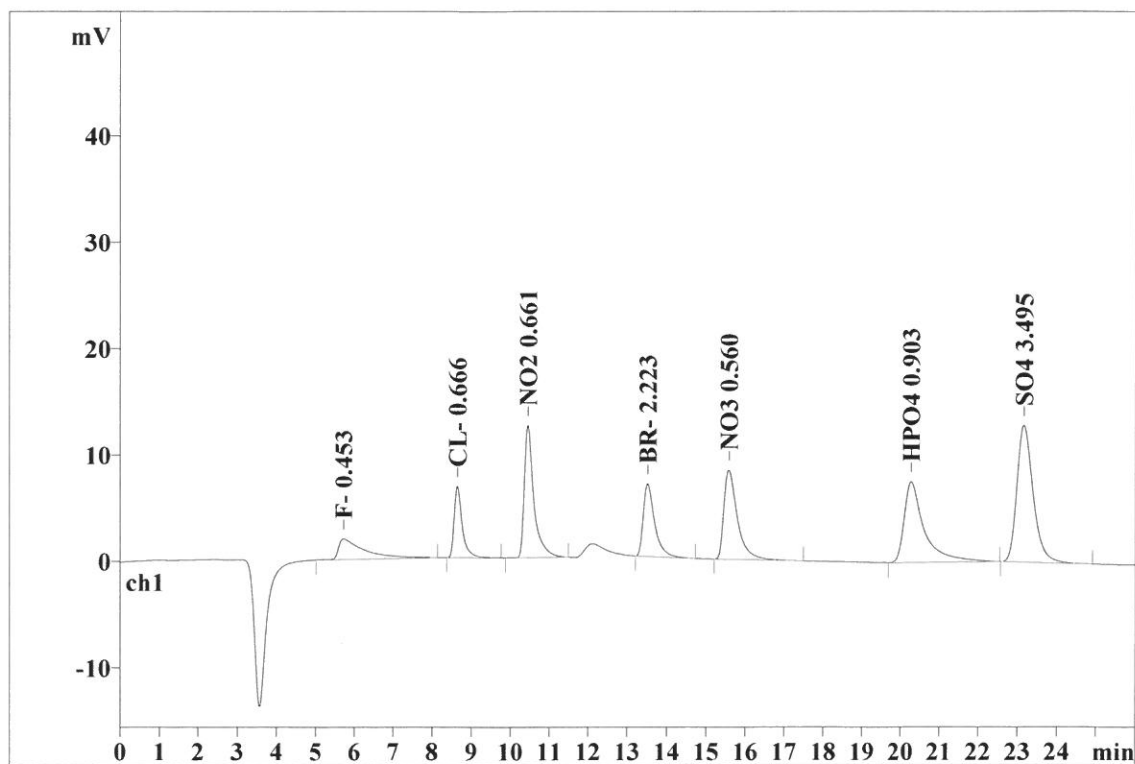

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.72	0.616	1.94	3.42	90.973	6.61
2	8.64	0.196	6.71	11.83	94.836	6.90
3	10.45	0.231	12.42	21.88	211.033	15.34
4	13.52	0.292	6.83	12.04	138.039	10.04
5	15.58	0.341	8.38	14.77	200.693	14.59
6	20.28	0.471	7.58	13.36	274.554	19.96
7	23.16	0.420	12.87	22.68	365.241	26.56
7	26.00	0.367	56.74	99.99	1375.368	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/14/2021 11:40:07 AM
Printed by: wet


Ident: STD3
Analysis from: 9/13/2021 10:25:23 AM
File: _2021-09-13_

Last save: 9/13/2021 12:47:11 PM

Method: AnionsIC2-091321.mtw
Run operator: wet
Analysis number: 28176

Last save: 9/13/2021 8:25:

SAMPLE:
: AP/MA
Vial number: 4
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

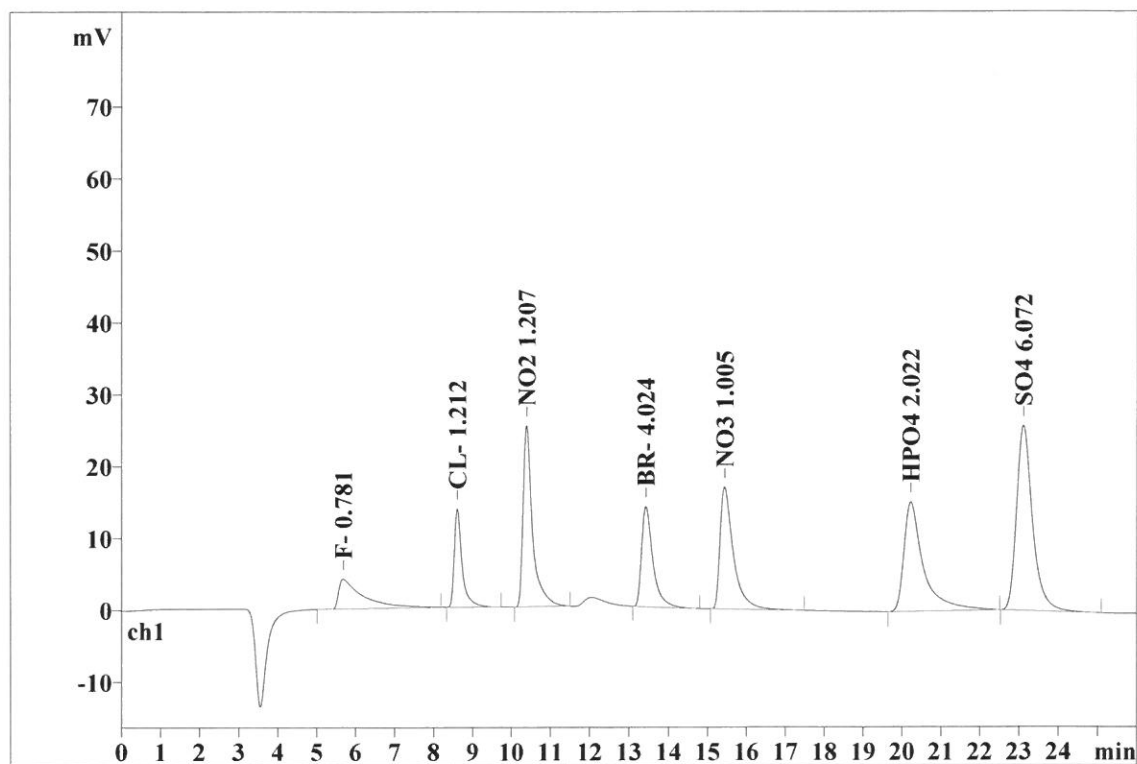

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.68	0.549	4.14	3.61	178.711	6.52
2	8.60	0.192	13.67	11.91	191.242	6.98
3	10.39	0.228	25.18	21.93	427.785	15.62
4	13.42	0.287	13.96	12.16	280.045	10.22
5	15.44	0.335	16.94	14.76	402.155	14.68
6	20.23	0.456	15.21	13.25	531.527	19.40
7	23.11	0.416	25.71	22.39	727.995	26.57
7	26.00	0.352	114.81	99.99	2739.460	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/14/2021 11:40:15 AM
Printed by: wet


Ident: STD4
Analysis from: 9/13/2021 10:53:59 AM
File: _2021-09-13_

Last save: 9/13/2021 12:47:11 PM

Method: AnionsIC2-091321.mtw
Run operator: wet
Analysis number: 28177

Last save: 9/13/2021 8:25:

SAMPLE:
: AP/MA
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

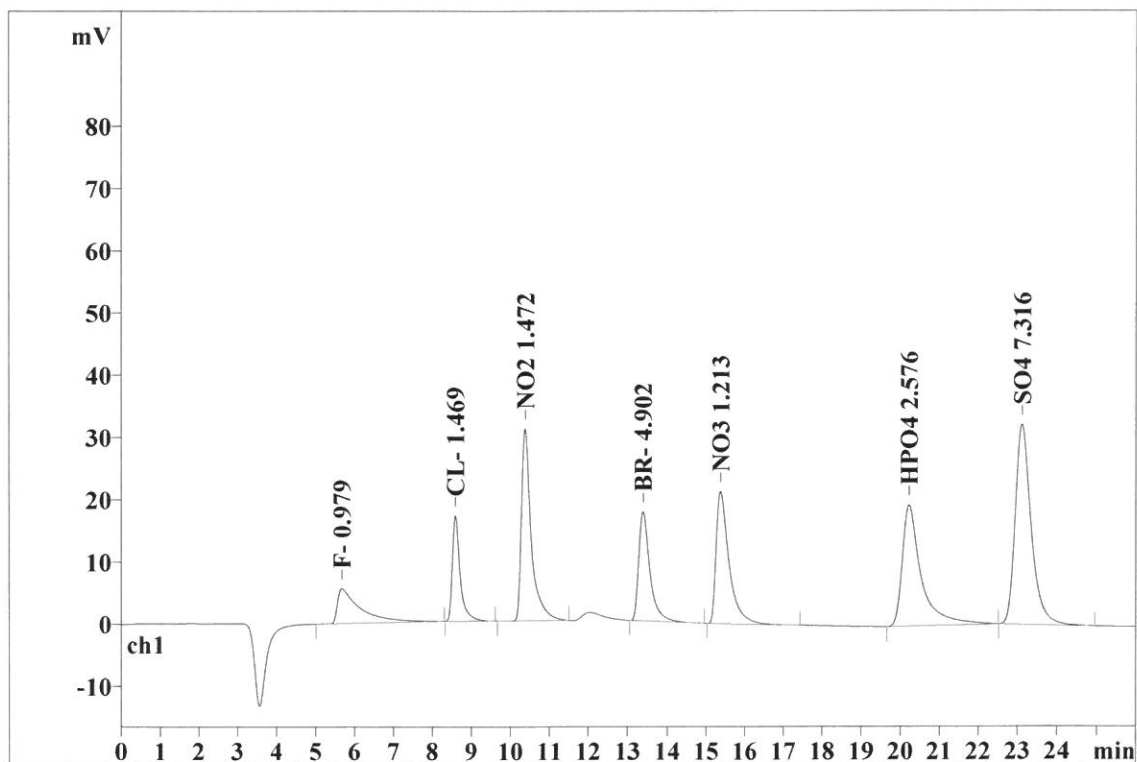

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.67	0.522	5.60	3.90	231.469	6.79
2	8.58	0.192	16.95	11.79	236.674	6.94
3	10.37	0.232	30.83	21.45	533.339	15.65
4	13.38	0.285	17.55	12.21	349.226	10.24
5	15.38	0.332	21.23	14.77	496.435	14.56
6	20.22	0.444	19.46	13.53	658.673	19.32
7	23.12	0.413	32.15	22.36	903.114	26.49
7	26.00	0.346	143.77	100.00	3408.930	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/14/2021 11:40:21 AM
Printed by: wet


Ident: STD5
Analysis from: 9/13/2021 11:22:36 AM
File: _2021-09-13_

Last save: 9/13/2021 12:47:11 PM

Method: AnionsIC2-091321.mtw
Run operator: wet
Analysis number: 28178

Last save: 9/13/2021 8:25:

SAMPLE:
: AP/MA
Vial number: 6
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

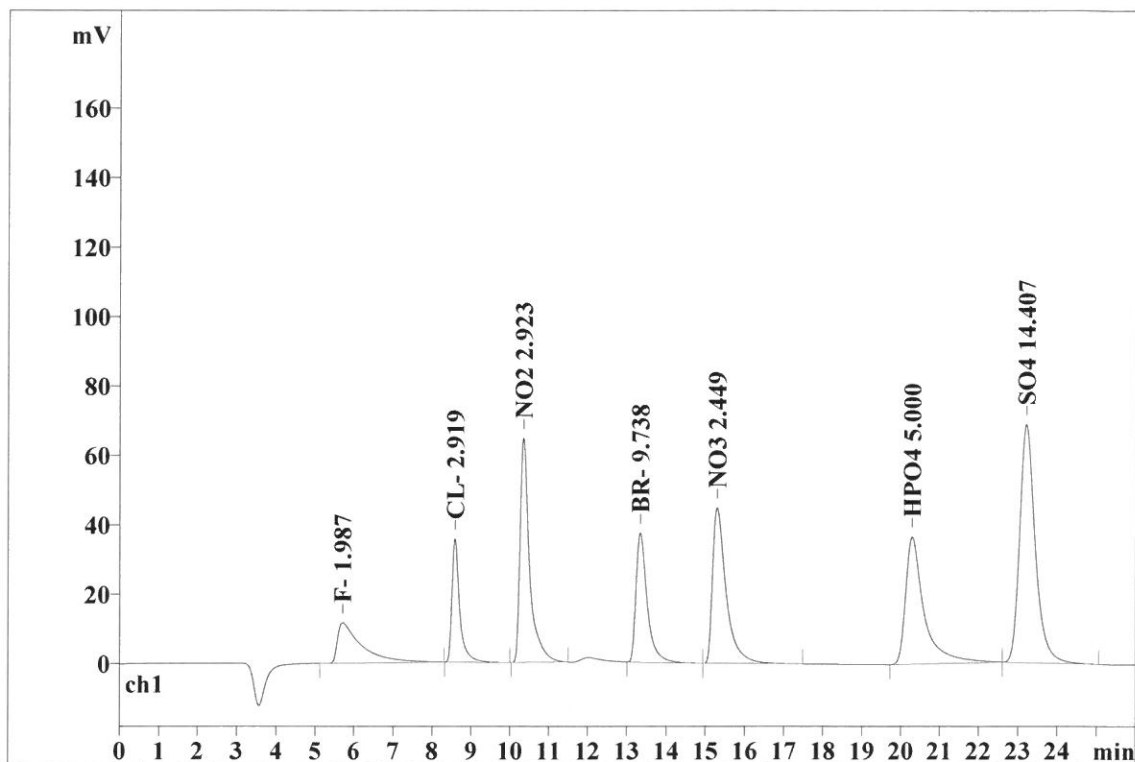

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.71	0.569	11.65	3.90	500.483	7.14
2	8.58	0.190	35.52	11.88	492.871	7.04
3	10.35	0.231	64.61	21.61	1109.973	15.84
4	13.34	0.281	37.21	12.45	730.510	10.43
5	15.30	0.333	44.76	14.97	1055.611	15.07
6	20.29	0.436	36.61	12.24	1214.792	17.34
7	23.21	0.407	68.60	22.94	1901.230	27.14
7	26.00	0.350	298.97	100.00	7005.470	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/14/2021 11:40:28 AM
Printed by: wet


Ident: STD6
Analysis from: 9/13/2021 11:51:11 AM
File: _2021-09-13_

Last save: 9/13/2021 12:47:11 PM

Method: AnionsIC2-091321.mtw
Run operator: wet
Analysis number: 28179

Last save: 9/13/2021 8:25:

SAMPLE:
: AP/MA
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

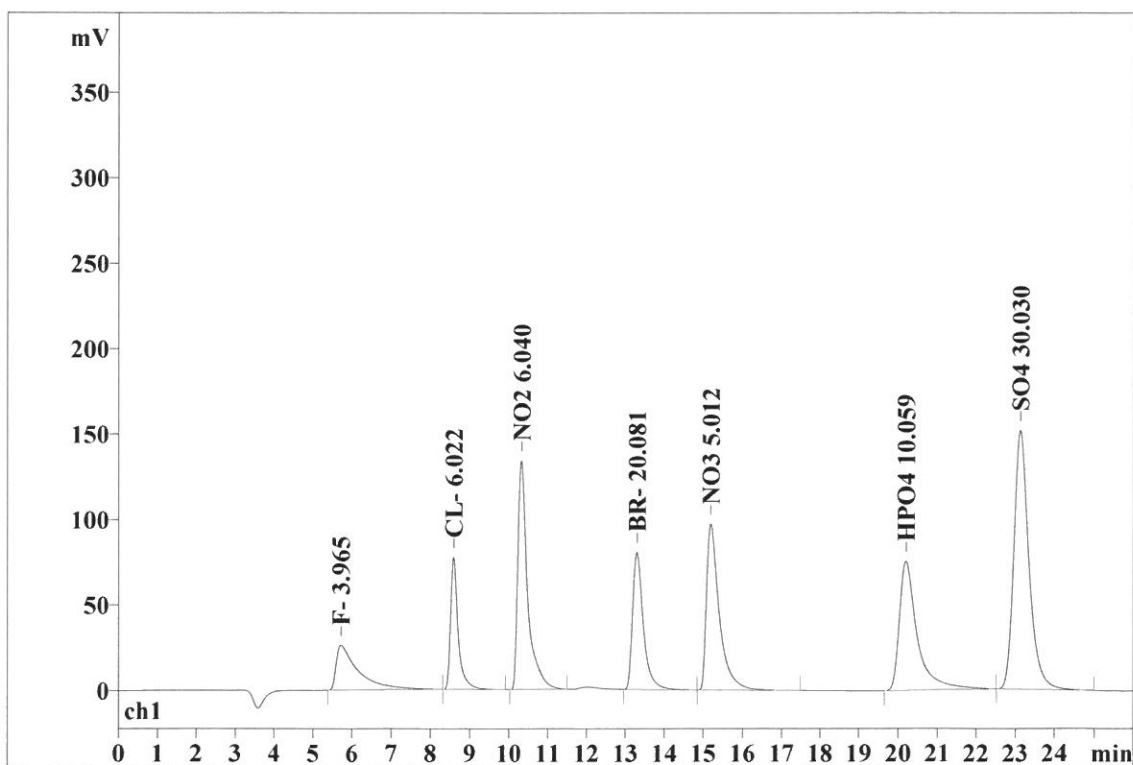

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.72	0.510	26.23	4.08	1028.060	7.01
2	8.58	0.184	77.36	12.05	1041.275	7.10
3	10.32	0.235	133.98	20.86	2348.881	16.03
4	13.29	0.276	80.37	12.52	1545.803	10.55
5	15.20	0.323	97.12	15.12	2215.871	15.12
6	20.19	0.419	75.64	11.78	2375.757	16.21
7	23.12	0.400	151.44	23.58	4100.375	27.98
7	26.00	0.335	642.13	100.00	14656.022	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/14/2021 11:40:34 AM
Printed by: wet


Ident: STD7
Analysis from: 9/13/2021 12:19:47 PM
File: _2021-09-13_

Last save: 9/13/2021 12:47:11 PM

Method: AnionsIC2-091321.mtw
Run operator: wet
Analysis number: 28180

Last save: 9/13/2021 8:25:

SAMPLE:
: AP/MA
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

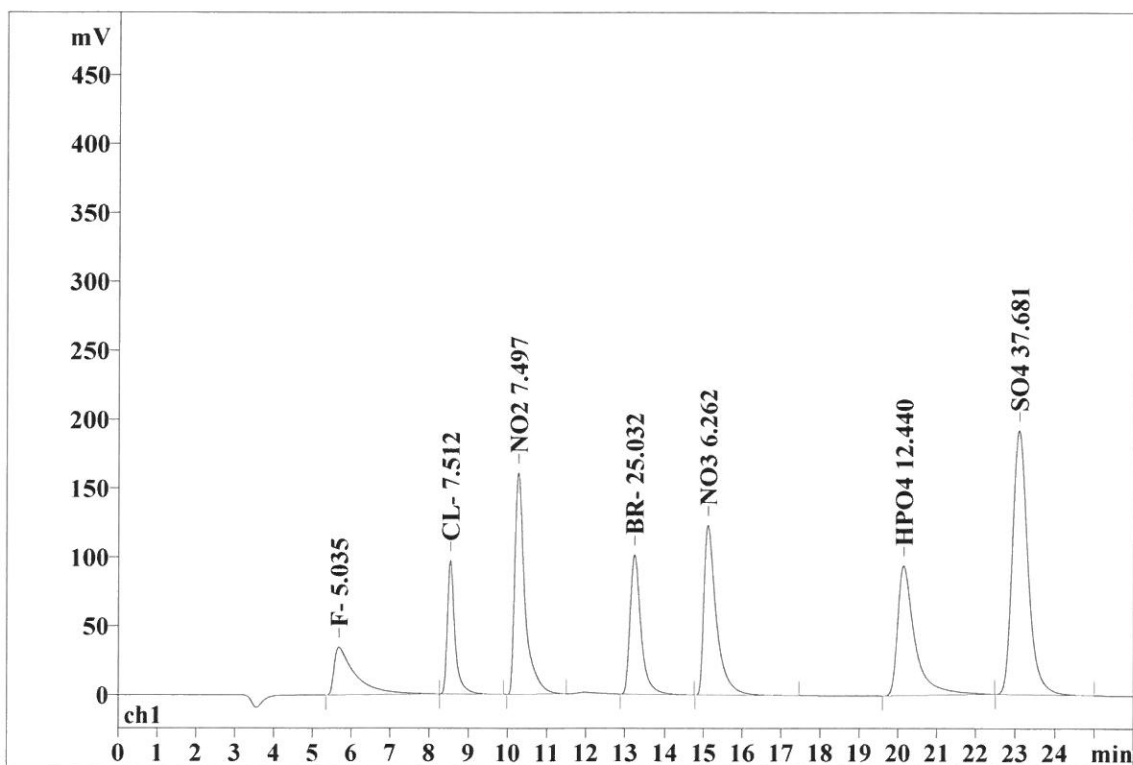

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.68	0.495	34.59	4.31	1313.724	7.15
2	8.54	0.185	97.01	12.09	1304.548	7.10
3	10.27	0.248	160.68	20.02	2927.879	15.94
4	13.23	0.276	101.16	12.60	1936.105	10.54
5	15.11	0.320	123.14	15.34	2781.661	15.15
6	20.14	0.415	94.35	11.76	2922.270	15.91
7	23.08	0.399	191.56	23.87	5177.368	28.19
7	26.00	0.334	802.49	100.00	18363.557	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/14/2021 11:41:12 AM
Printed by: wet


Ident: ICV
Analysis from: 9/13/2021 12:53:47 PM
File: _2021-09-13_

Last save: 9/13/2021 1:19:47 PM

Method: AnionsIC2-091321.mtw
Run operator: wet
Analysis number: 28181

Last save: 9/13/2021 12:47

SAMPLE:
: AP/MA
Vial number: 9
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

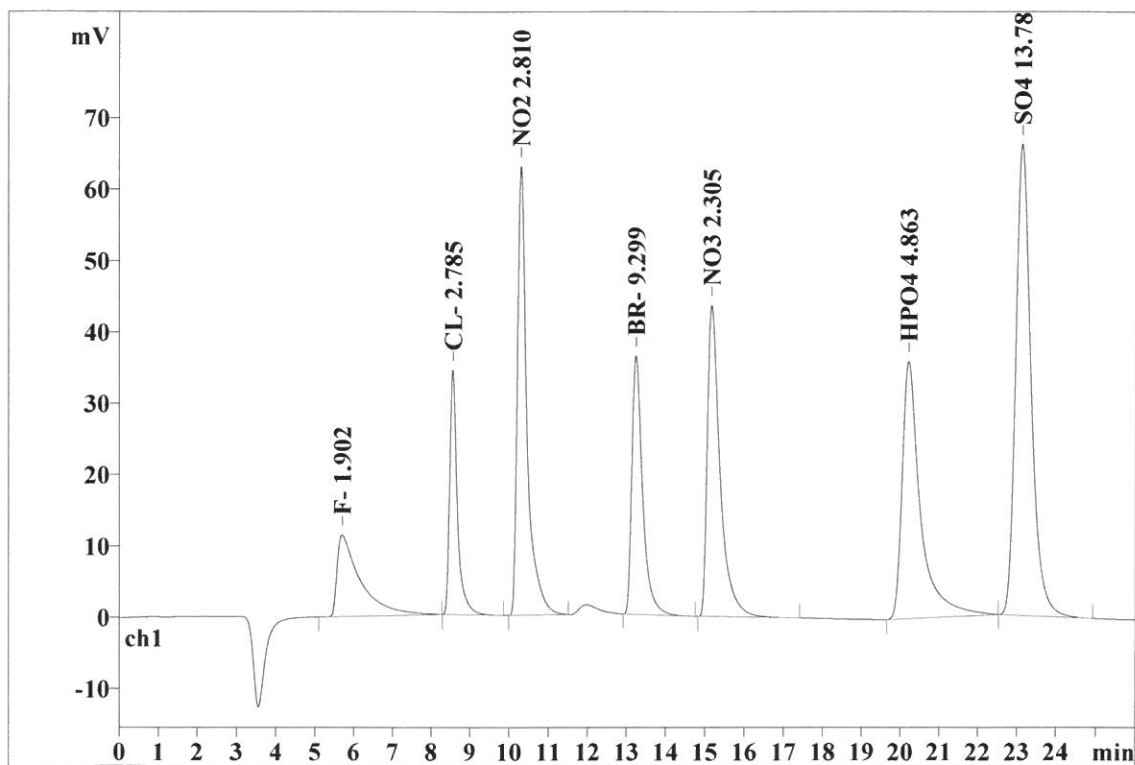

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.70	0.552	11.41	3.92	477.593	7.13
2	8.54	0.189	34.29	11.80	469.231	7.01
3	10.29	0.228	62.91	21.65	1065.183	15.91
4	13.24	0.276	36.25	12.47	695.906	10.39
5	15.17	0.323	43.62	15.01	990.801	14.80
6	20.22	0.432	36.06	12.41	1183.405	17.67
7	23.13	0.406	66.08	22.74	1813.643	27.09
7	26.00	0.344	290.63	100.00	6695.761	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/14/2021 11:41:23 AM
Printed by: wet


Ident: ICB
Analysis from: 9/13/2021 1:24:18 PM
File: _2021-09-13_

Last save: 9/13/2021 1:50:18 PM

Method: AnionsIC2-091321.mtw
Run operator: wet
Analysis number: 28182

Last save: 9/13/2021 12:47

SAMPLE:
: AP/MA
Vial number: 10
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

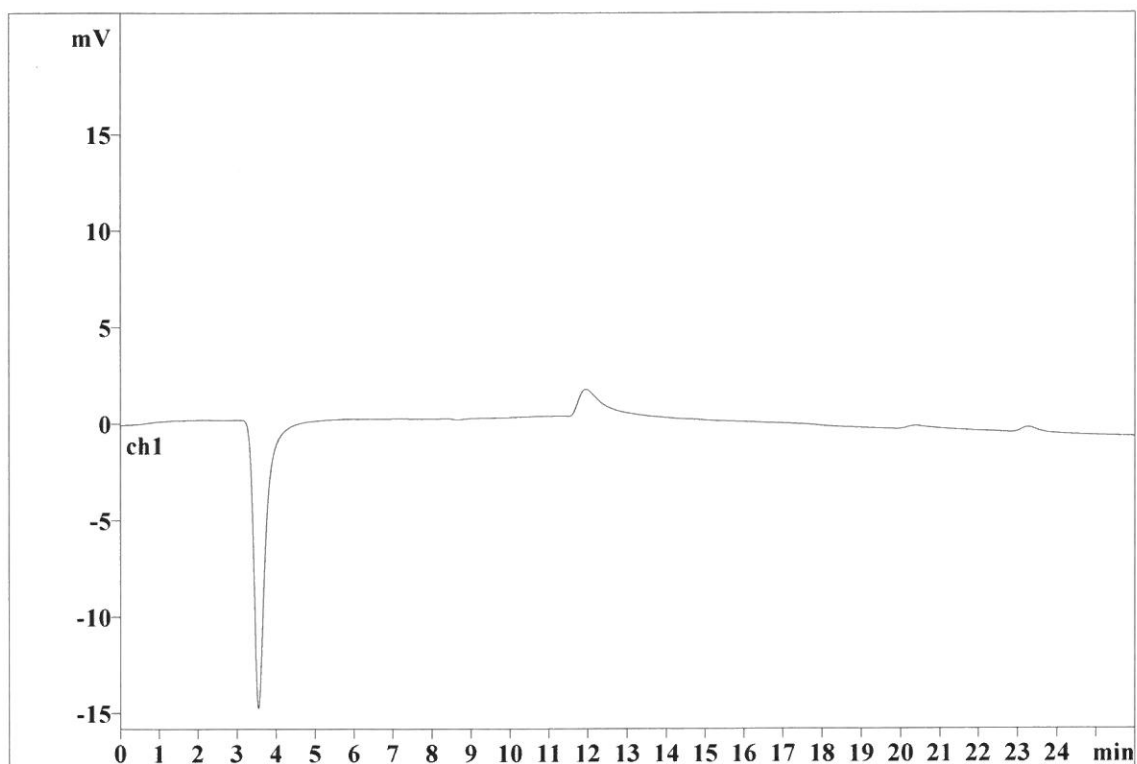

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 9/16/2021 1:42:44 PM
Printed by: wet


Ident: CCV
Analysis from: 9/14/2021 8:26:00 AM
File: _2021-09-14_

Last save: 9/14/2021 8:51:30 AM

Method: AnionsIC2-091321.mtw
Run operator: wet
Analysis number: 28218

Last save: 9/13/2021 3:44:

SAMPLE:
: AP/MA
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

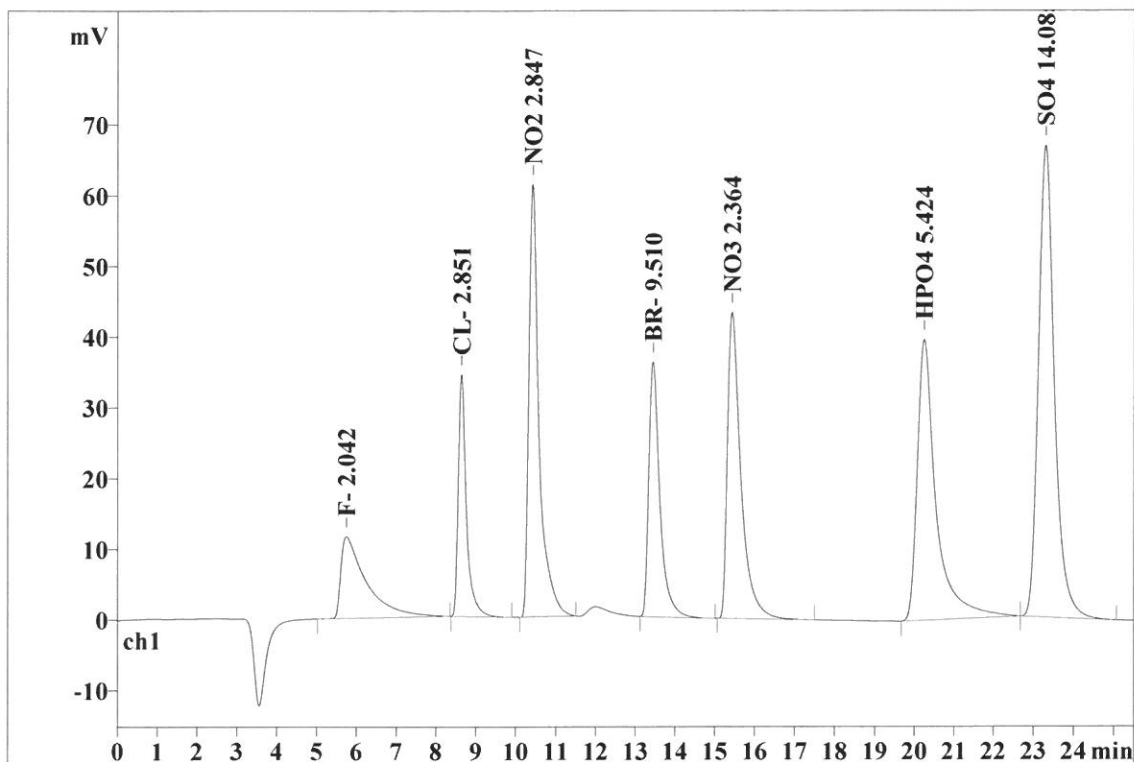

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.74	0.593	11.58	3.96	515.107	7.39
2	8.63	0.194	34.19	11.68	480.948	6.90
3	10.40	0.236	61.17	20.89	1079.773	15.48
4	13.44	0.284	36.06	12.32	712.475	10.22
5	15.42	0.334	43.35	14.81	1017.538	14.59
6	20.23	0.434	39.71	13.56	1312.181	18.82
7	23.29	0.411	66.70	22.78	1855.959	26.61
7	25.50	0.355	292.77	100.00	6973.982	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/16/2021 1:42:52 PM
Printed by: wet


Ident: CCB
Analysis from: 9/14/2021 8:54:27 AM
File: _2021-09-14_

Last save: 9/14/2021 9:19:58 AM

Method: AnionsIC2-091321.mtw
Run operator: wet
Analysis number: 28219

Last save: 9/13/2021 3:44:

SAMPLE:
: AP/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

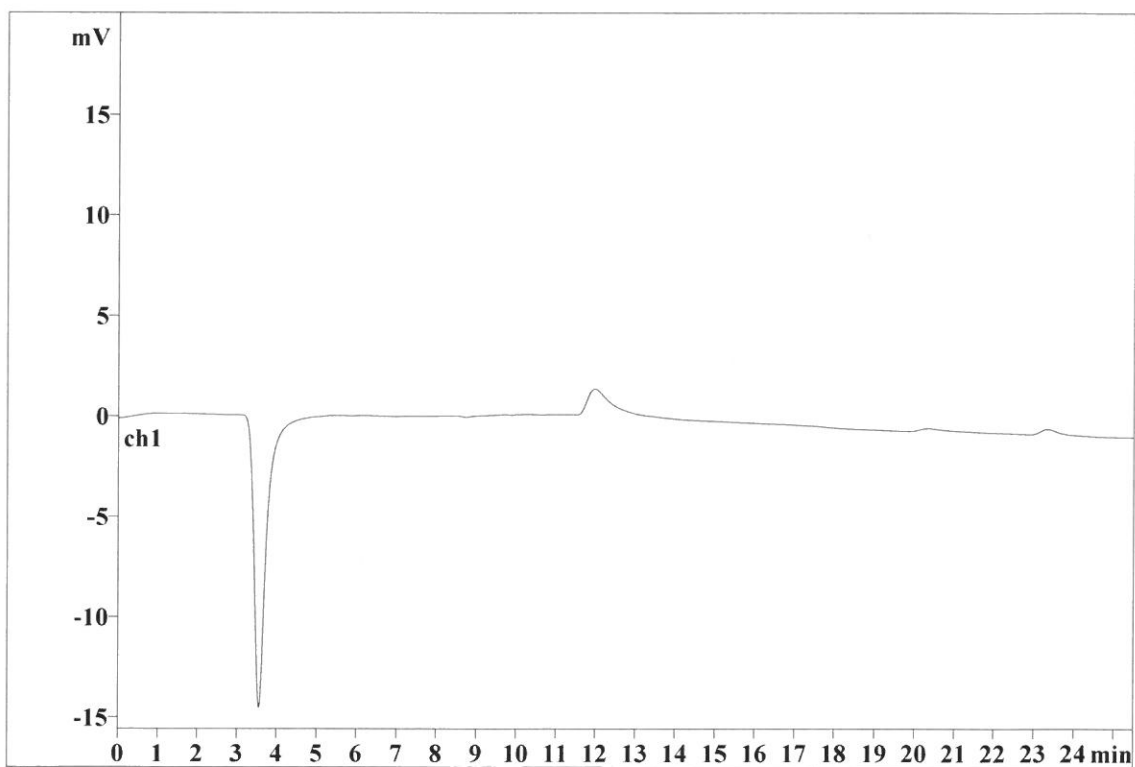

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 9/16/2021 1:42:59 PM
Printed by: wet


Ident: LB116348BLW
Analysis from: 9/14/2021 9:22:36 AM
File: _2021-09-14_

Last save: 9/16/2021 1:42:36 PM

Method: AnionsIC2-091321.mtw
Run operator: wet
Analysis number: 28220

Last save: 9/13/2021 3:44:

SAMPLE:
: AP/MA
Vial number: 13
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

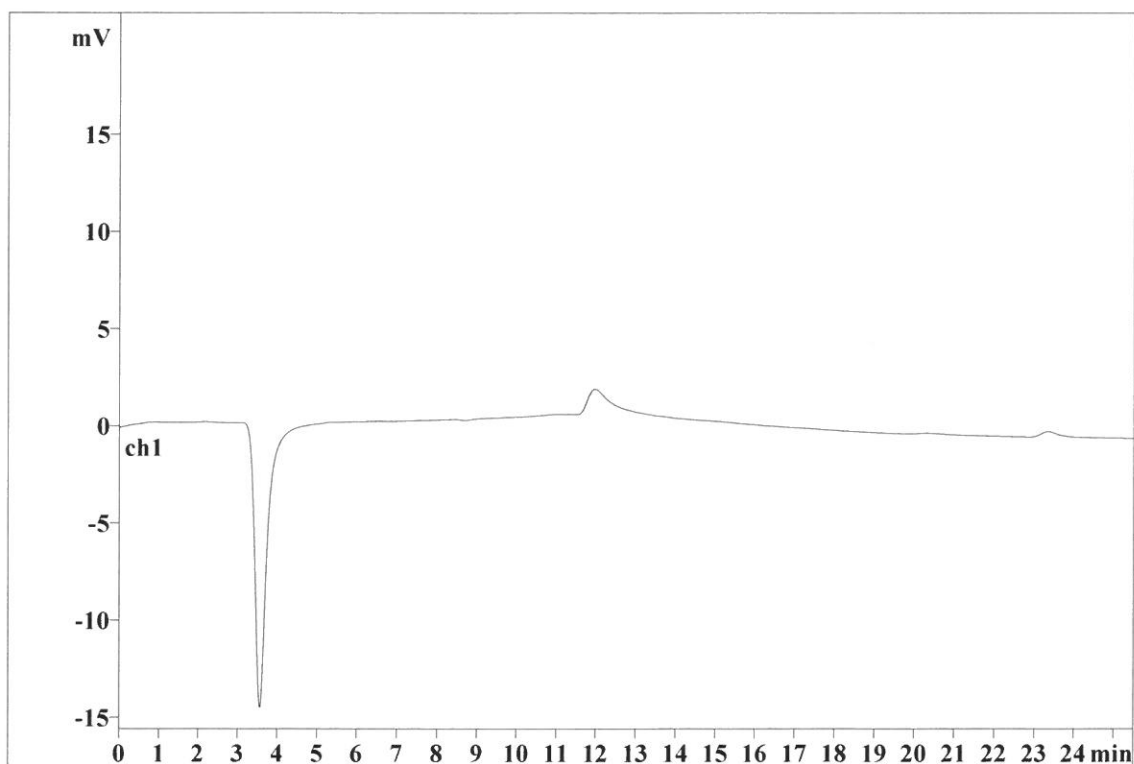

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 9/16/2021 1:43:07 PM
Printed by: wet


Ident: LB116348BSW
Analysis from: 9/14/2021 9:50:44 AM
File: _2021-09-14_

Last save: 9/16/2021 1:42:37 PM

Method: AnionsIC2-091321.mtw
Run operator: wet
Analysis number: 28221

Last save: 9/13/2021 3:44:

SAMPLE:
: AP/MA
Vial number: 14
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

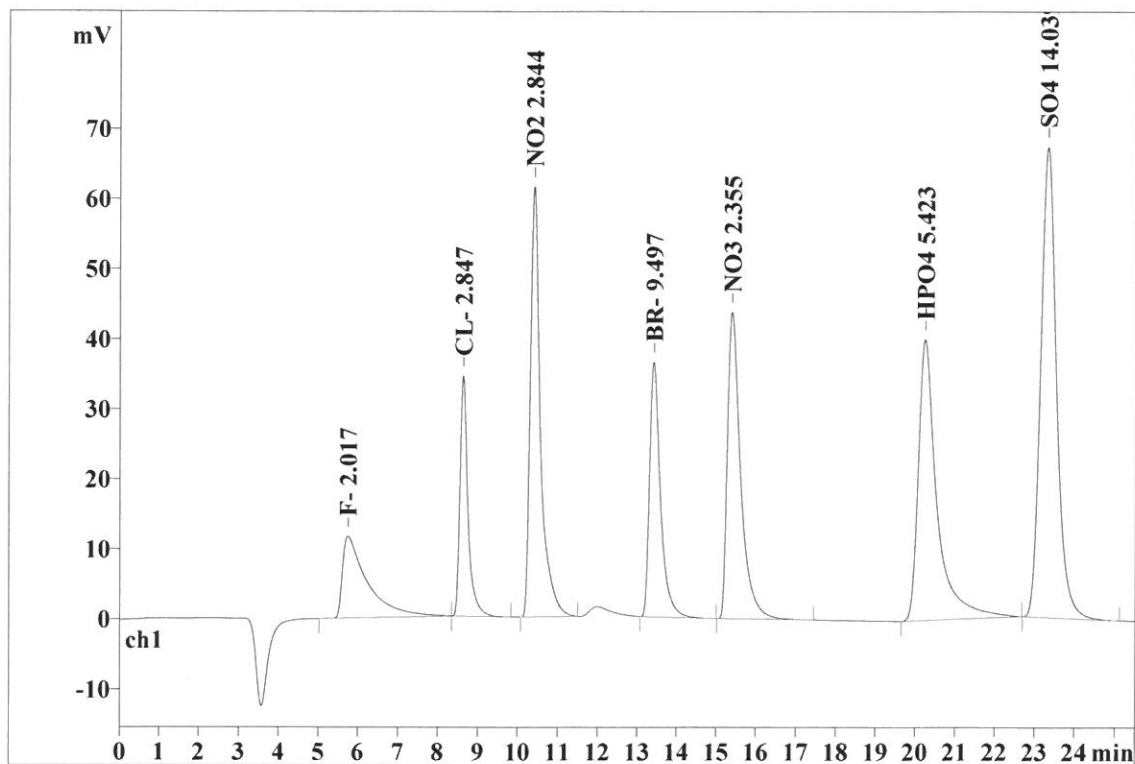

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.74	0.576	11.67	3.96	508.379	7.31
2	8.61	0.195	34.37	11.65	480.116	6.90
3	10.39	0.238	61.42	20.83	1078.507	15.51
4	13.41	0.283	36.38	12.33	711.449	10.23
5	15.39	0.332	43.77	14.84	1013.461	14.58
6	20.24	0.431	40.09	13.60	1311.885	18.87
7	23.30	0.409	67.19	22.79	1849.531	26.60
7	25.50	0.352	294.89	100.00	6953.328	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/16/2021 1:43:22 PM
Printed by: wet


Ident: M3728-01
Analysis from: 9/14/2021 2:27:39 PM
File: _2021-09-14_

Last save: 9/14/2021 2:53:09 PM

Method: AnionsIC2-091321.mtw
Run operator: wet
Analysis number: 28230

Last save: 9/13/2021 3:44:

SAMPLE:
: AP/MA
Vial number: 33
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

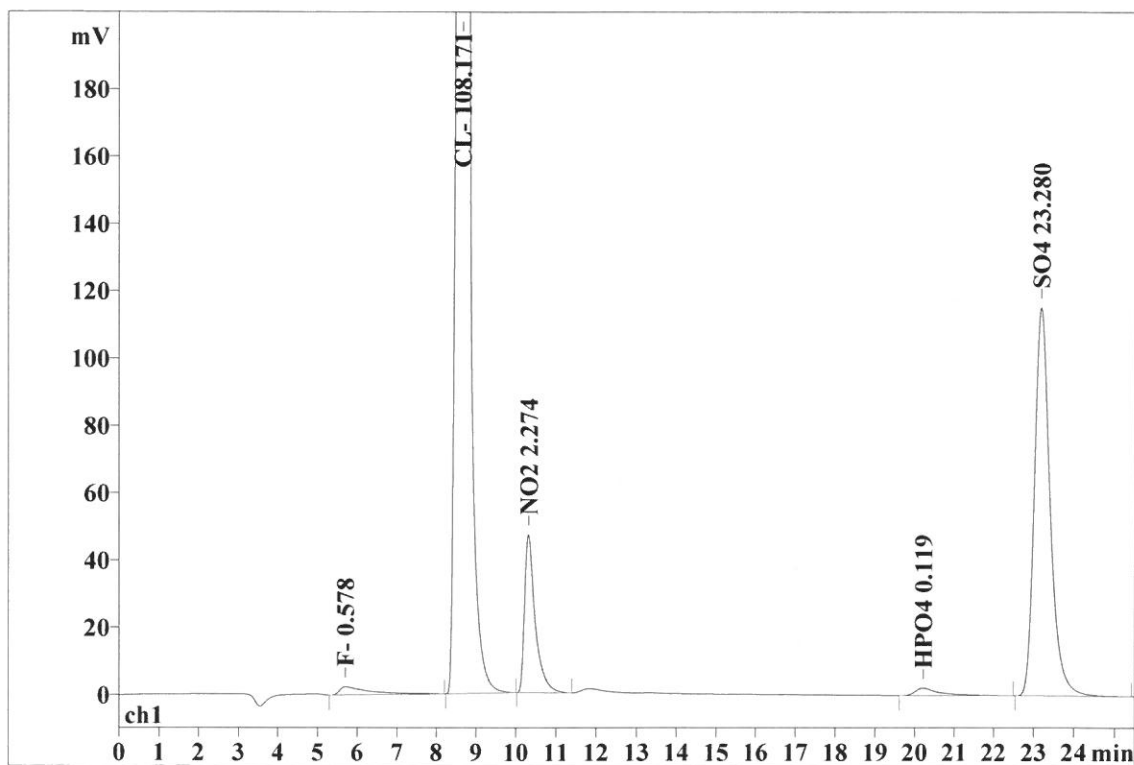

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.70	0.660	2.41	0.16	124.511	0.53
2	8.62	0.214	1308.18	88.68	19091.730	81.89
3	10.31	0.253	46.98	3.18	852.199	3.66
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	20.21	0.541	2.22	0.15	94.837	0.41
7	23.18	0.403	115.39	7.82	3150.173	13.51
7	25.50	0.296	1475.16	100.00	23313.450	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/16/2021 1:43:30 PM
Printed by: wet


Ident: M3728-01MS
Analysis from: 9/14/2021 3:01:08 PM
File: _2021-09-14_

Last save: 9/14/2021 3:26:39 PM

Method: AnionsIC2-091321.mtw
Run operator: wet
Analysis number: 28231

Last save: 9/13/2021 3:44:

SAMPLE:
: AP/MA
Vial number: 34
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

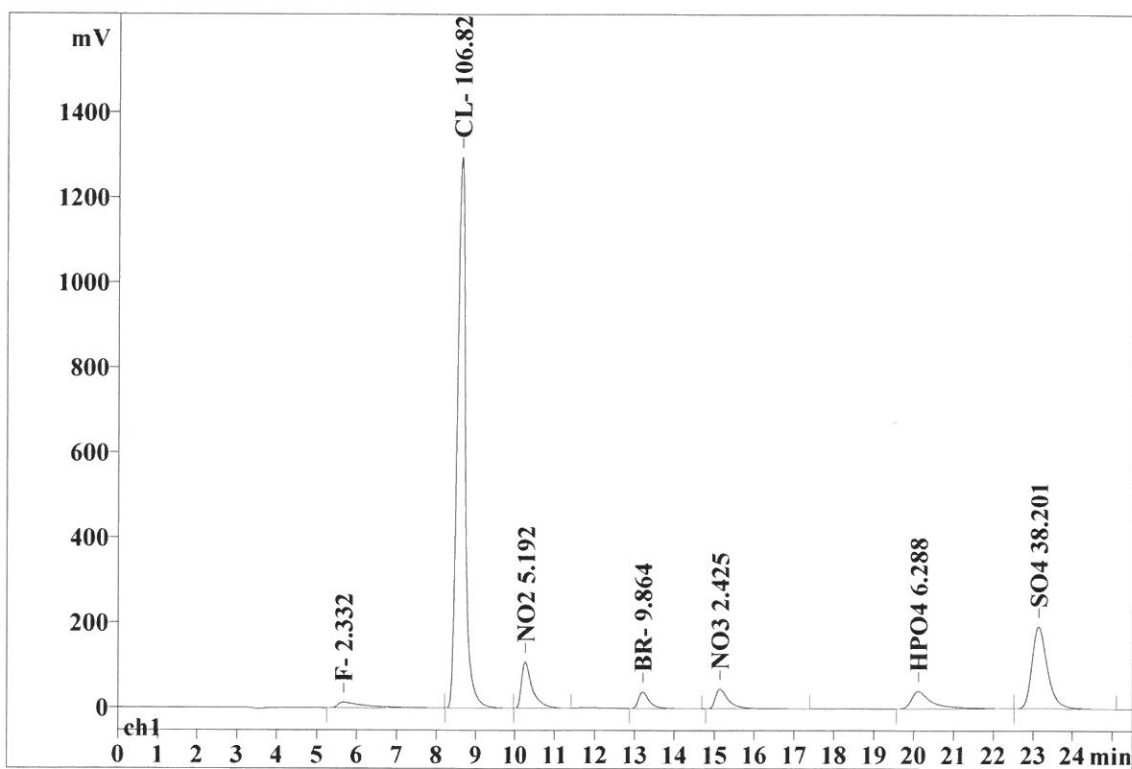

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.67	0.585	12.94	0.75	592.530	1.97
2	8.60	0.211	1295.77	74.63	18853.685	62.84
3	10.26	0.254	108.26	6.24	2011.975	6.71
4	13.20	0.272	39.09	2.25	740.398	2.47
5	15.14	0.323	46.07	2.65	1044.975	3.48
6	20.12	0.464	41.39	2.38	1510.347	5.03
7	23.13	0.403	192.81	11.10	5250.510	17.50
7	25.50	0.359	1736.34	100.00	30004.420	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/16/2021 1:43:38 PM
Printed by: wet


Ident: M3728-01MSD
Analysis from: 9/14/2021 3:29:17 PM
File: _2021-09-14_

Last save: 9/14/2021 3:54:47 PM

Method: AnionsIC2-091321.mtw
Run operator: wet
Analysis number: 28232

Last save: 9/13/2021 3:44:

SAMPLE:
: AP/MA
Vial number: 35
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

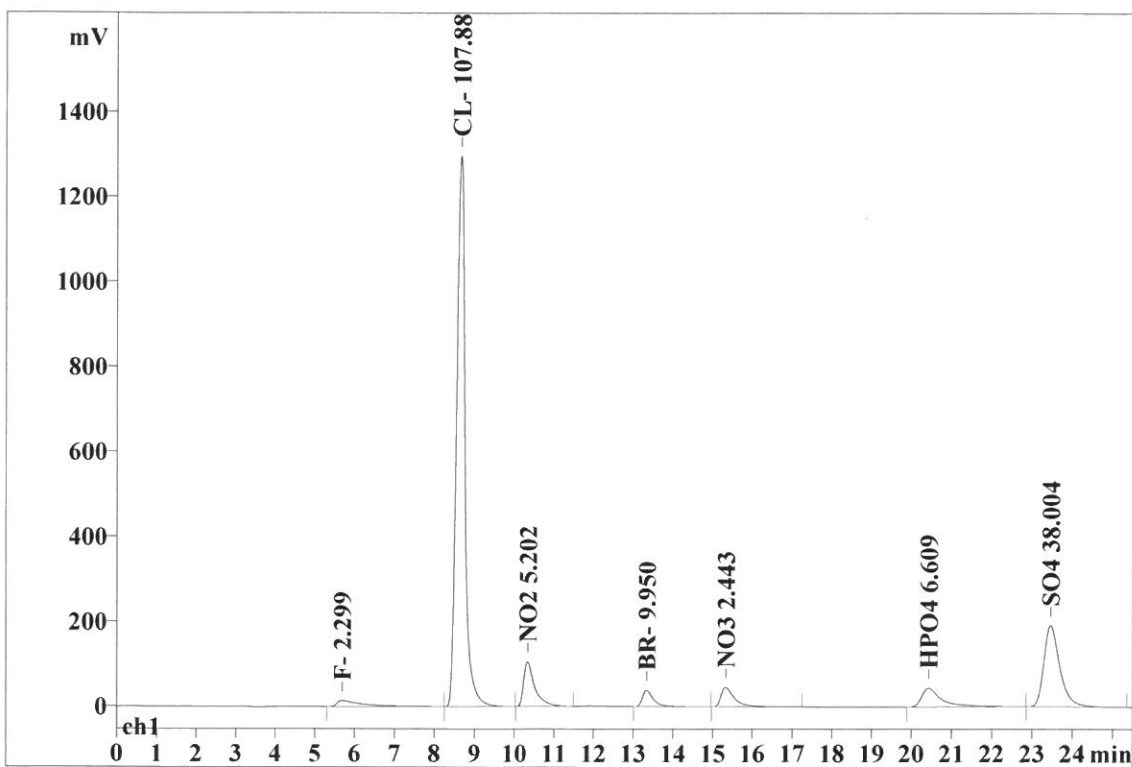

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.69	0.548	13.76	0.79	583.634	1.93
2	8.63	0.212	1296.19	74.77	19041.941	62.95
3	10.33	0.263	104.57	6.03	2015.731	6.66
4	13.34	0.278	38.29	2.21	747.196	2.47
5	15.33	0.331	45.13	2.60	1053.255	3.48
6	20.43	0.453	44.42	2.56	1584.190	5.24
7	23.46	0.403	191.17	11.03	5222.813	17.27
7	25.50	0.356	1733.52	100.00	30248.758	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/16/2021 1:43:45 PM
Printed by: wet


Ident: CCV
Analysis from: 9/14/2021 4:33:06 PM
File: _2021-09-14_

Last save: 9/14/2021 4:58:36 PM

Method: AnionsIC2-091321.mtw
Run operator: wet
Analysis number: 28234

Last save: 9/13/2021 3:44:

SAMPLE:
: AP/MA
Vial number: 40
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

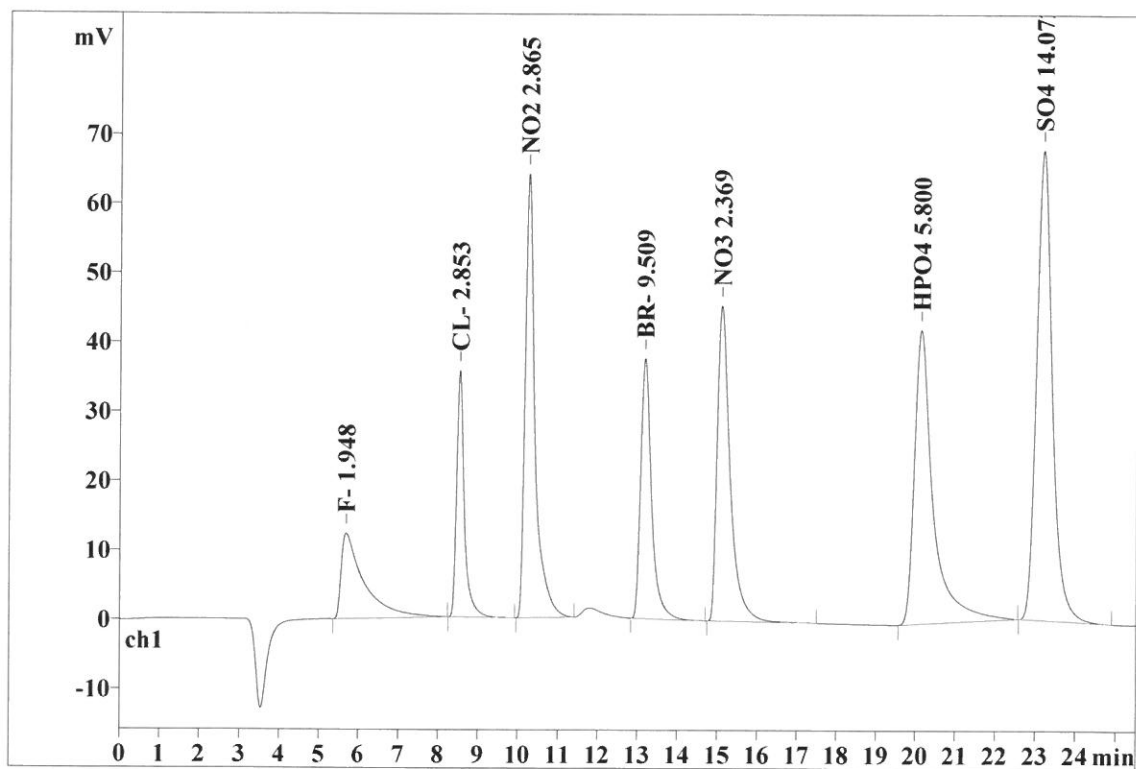

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.68	0.509	12.34	4.05	489.895	6.96
2	8.52	0.188	35.55	11.65	481.332	6.83
3	10.24	0.229	64.05	20.99	1087.088	15.43
4	13.17	0.274	37.53	12.30	712.421	10.12
5	15.09	0.320	45.47	14.90	1019.575	14.48
6	20.12	0.429	42.38	13.89	1398.534	19.86
7	23.17	0.404	67.80	22.22	1854.170	26.33
7	25.50	0.336	305.12	100.00	7043.015	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/16/2021 1:43:54 PM
Printed by: wet


Ident: CCB
Analysis from: 9/14/2021 5:01:22 PM
File: _2021-09-14_

Last save: 9/14/2021 5:26:53 PM

Method: AnionsIC2-091321.mtw
Run operator: wet
Analysis number: 28235

Last save: 9/13/2021 3:44:

SAMPLE:
: AP/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

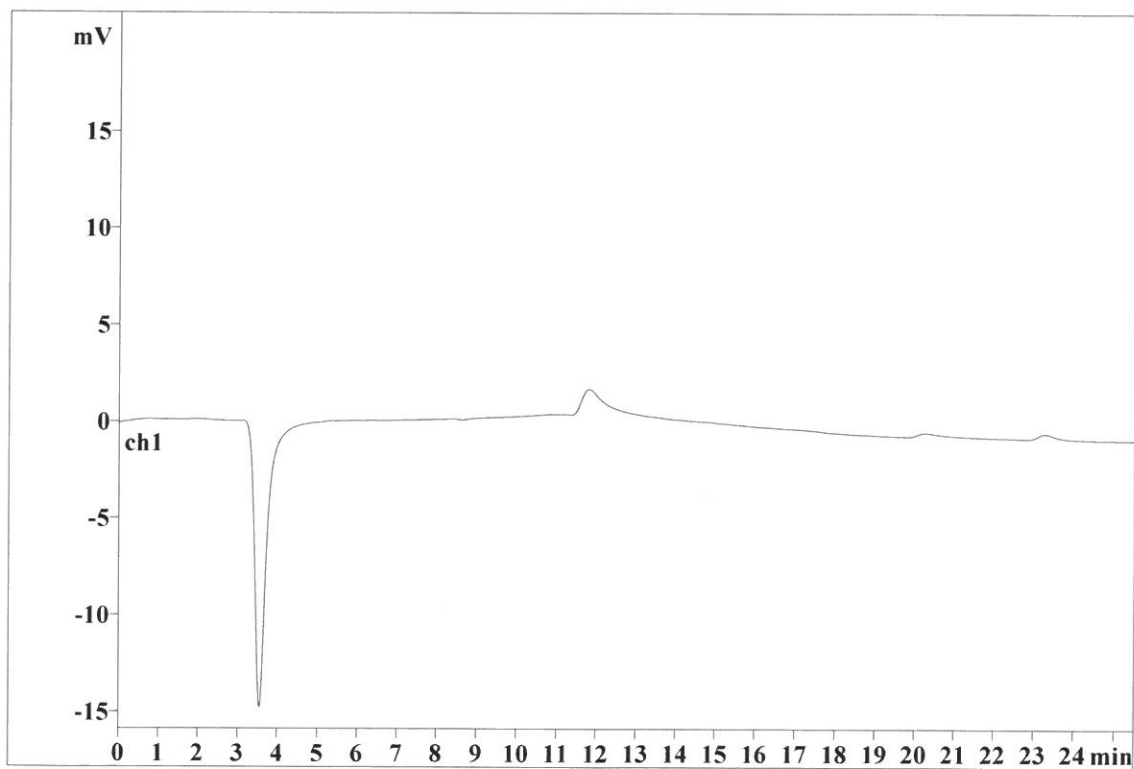

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD