

UB116371


7470A

INSTRUMENT ID: KV2

Linear

μ Abs.:

39512

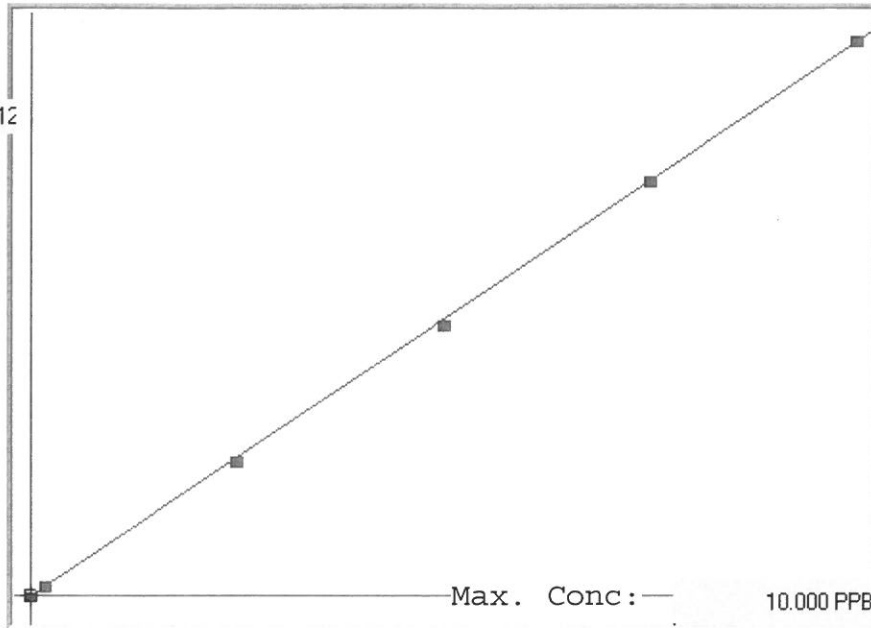

A= 0.0000e+000

B= 2.5308e-004

C= 2.8494e-002

Rho= 0.9999216

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	% (1)
0.0	0.000	0.037	0.037	33	0.000	33					-
0.2	0.200	0.234	0.034	811	0.0 %	811					17
2.5	2.500	2.452	-0.048	9576	0.0 %	9576					-2
5.0	5.000	4.920	-0.080	19329	0.0 %	19329					-2
7.5	7.500	7.529	0.029	29638	0.0 %	29638					0
10.0	10.000	10.028	0.028	39512	0.0 %	39512					0

LB116371 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 17 Sep 2021 15:06:50

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	SO	33	-	0.0000	7470A	PPB	17 Sep 2021 15:07:24	S	Std
0.2 - 1	SO-2	811	-	0.2000	7470A	PPB	17 Sep 2021 15:09:41	S	Std
2.5 - 1	SO-5	9576	-	2.5000	7470A	PPB	17 Sep 2021 15:11:58	S	Std
5.0 - 1	SO-5	19329	-	5.0000	7470A	PPB	17 Sep 2021 15:14:15	S	Std
7.5 - 1	SO-5	29638	-	7.5000	7470A	PPB	17 Sep 2021 15:16:31	S	Std
10.0 - 1	SIV	39512	-	10.0000	7470A	PPB	17 Sep 2021 15:18:46	S	Std
ICV97 - 1	ICV97	14430	3.6804	-	7470A	PPB	17 Sep 2021 15:21:27	U	SMPL
ICB97 - 1	ICB97	-80	0.0082	-	7470A	PPB	17 Sep 2021 15:23:42	U	SMPL
CCV63 - 1	CCV63	19494	4.9620	-	7470A	PPB	17 Sep 2021 15:25:56	U	SMPL
CCB63 - 1	CCB63	-19	0.0237	-	7470A	PPB	17 Sep 2021 15:28:12	U	SMPL
CRA - 1	CRA	793	0.2292	-	7470A	PPB	17 Sep 2021 15:30:26	U	SMPL
HighStd - 1	HighStd	39421	10.0050	-	7470A	PPB	17 Sep 2021 15:32:42	U	SMPL
ChkStd - 1	ChkStd	28016	7.1187	-	7470A	PPB	17 Sep 2021 15:34:57	U	SMPL
PB139181BL - 1	PBW	16	0.0325	-	7470A	PPB	17 Sep 2021 15:37:12	U	SMPL
PB139181BS - 1	LCSW	14527	3.7049	-	7470A	PPB	17 Sep 2021 15:39:28	U	SMPL
M3704-07 - 1	PT-HG-WP	21772	5.5385	-	7470A	PPB	17 Sep 2021 15:41:44	U	SMPL
CCV64 - 1	CCV64	19567	4.9804	-	7470A	PPB	17 Sep 2021 15:50:50	U	SMPL
CCB64 - 1	CCB64	-28	0.0214	-	7470A	PPB	17 Sep 2021 15:53:05	U	SMPL