


LB116385

7470A

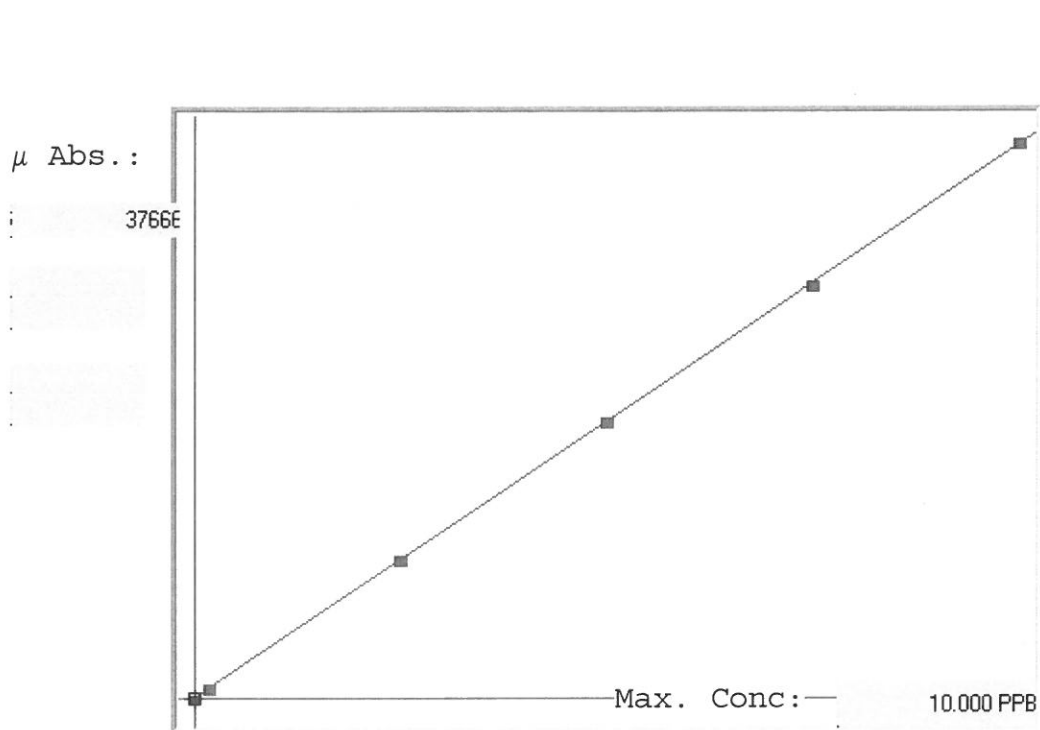

Linear

A= 0.0000e+000

B= 2.6620e-004

C= -5.5884e-003

Rho= 0.9999840

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	-0.003	-0.003	11	0.000	11					
0.2	0.200	0.194	-0.006	749	0.0 %	749					-3
2.5	2.500	2.519	0.019	9485	0.0 %	9485					1
5.0	5.000	5.010	0.010	18840	0.0 %	18840					0
7.5	7.500	7.459	-0.041	28042	0.0 %	28042					-1
10.0	10.000	10.021	0.021	37666	0.0 %	37666					0

LB116385 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 20 Sep 2021 10:51:14

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	57	11	-	0.0000	7470A	PPB	20 Sep 2021 10:51:29	S	Std
0.2 - 1	50.2	749	-	0.2000	7470A	PPB	20 Sep 2021 10:53:46	S	Std
2.5 - 1	52.5	9485	-	2.5000	7470A	PPB	20 Sep 2021 10:56:03	S	Std
5.0 - 1	55	18840	-	5.0000	7470A	PPB	20 Sep 2021 10:58:20	S	Std
7.5 - 1	57.5	28042	-	7.5000	7470A	PPB	20 Sep 2021 11:00:37	S	Std
10.0 - 1	57.5	37666	-	10.0000	7470A	PPB	20 Sep 2021 11:02:52	S	Std
ICV99 - 1	ICV99	13698	3.6408	-	7470A	PPB	20 Sep 2021 11:05:33	U	SMPL
ICB99 - 1	ICB99	-28	-0.0130	-	7470A	PPB	20 Sep 2021 11:07:48	U	SMPL
CCV68 - 1	CCV68	19181	5.1003	-	7470A	PPB	20 Sep 2021 11:10:03	U	SMPL
CCB68 - 1	CCB68	-28	-0.0130	-	7470A	PPB	20 Sep 2021 11:12:18	U	SMPL
CRA - 1	CRA	732	0.1893	-	7470A	PPB	20 Sep 2021 11:14:33	U	SMPL
HighStd - 1	HighStd	37087	9.8668	-	7470A	PPB	20 Sep 2021 11:16:48	U	SMPL
ChkStd - 1	ChkStd	25726	6.8426	-	7470A	PPB	20 Sep 2021 11:19:04	U	SMPL
PB139189BL - 1	PBW	-41	-0.0165	-	7470A	PPB	20 Sep 2021 11:21:19	U	SMPL
PB139189BS - 1	LCSW	13644	3.6264	-	7470A	PPB	20 Sep 2021 11:23:35	U	SMPL
M3786-07 - 1		127	0.0282	-	7470A	PPB	20 Sep 2021 11:25:51	U	SMPL
M3786-07DUP - 1	N71924DUP	190	0.0450	-	7470A	PPB	20 Sep 2021 11:28:07	U	SMPL
M3786-07MS - 1	N71924MS	13277	3.5287	-	7470A	PPB	20 Sep 2021 11:30:24	U	SMPL
M3786-07MSD - 1	N71924MSD	14546	3.8665	-	7470A	PPB	20 Sep 2021 11:32:41	U	SMPL
M3791-07 - 1	SW-RR-02-(1.0)	-12	-0.0088	-	7470A	PPB	20 Sep 2021 11:34:56	U	SMPL
CCV69 - 1	CCV69	18986	5.0484	-	7470A	PPB	20 Sep 2021 11:37:12	U	SMPL
CCB69 - 1	CCB69	-32	-0.0141	-	7470A	PPB	20 Sep 2021 11:39:27	U	SMPL
M3791-08 - 1	SW-CB-03-(1.0)	21	0.0000	-	7470A	PPB	20 Sep 2021 11:41:42	U	SMPL
M3791-09 - 1	SW-CB-02-(0.3)	28	0.0019	-	7470A	PPB	20 Sep 2021 11:43:57	U	SMPL
M3791-10 - 1	SW-RR-01-(2.0)	19	-0.0005	-	7470A	PPB	20 Sep 2021 11:46:13	U	SMPL
M3792-05 - 1	FM782	2350	0.6200	-	7470A	PPB	20 Sep 2021 11:48:28	U	SMPL
M3786-07A - 1		14305	3.8023	-	7470A	PPB	20 Sep 2021 11:53:00	U	SMPL
M3759-15DLX100 - 1	41264	-53	-0.0197	-	7470A	PPB	20 Sep 2021 11:55:16	U	SMPL
M3759-17 - 1	31185	94	0.0194	-	7470A	PPB	20 Sep 2021 12:03:53	U	SMPL
M3786-07LX5 - 1		17	-0.0011	-	7470A	PPB	20 Sep 2021 12:50:48	U	SMPL
CCV70 - 1	CCV70	18753	4.9864	-	7470A	PPB	20 Sep 2021 12:53:05	U	SMPL
CCB70 - 1	CCB70	-48	-0.0184	-	7470A	PPB	20 Sep 2021 12:55:20	U	SMPL