


L3116388

7471B

INSTRUMENT ID: CV2

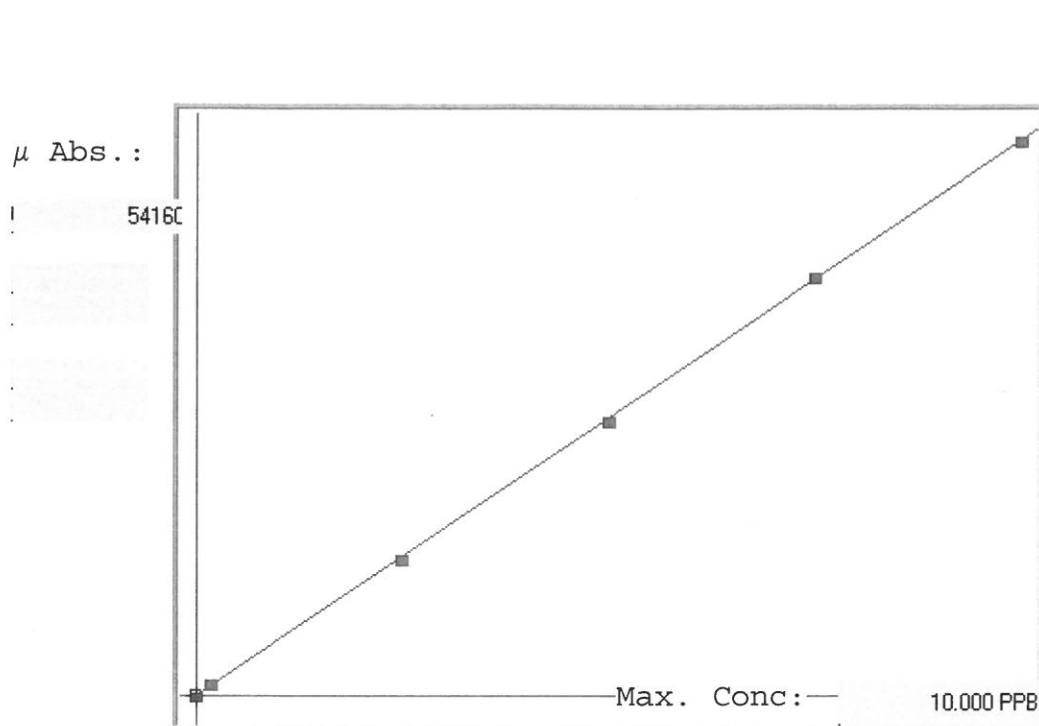

Linear

A= 0.0000e+000

B= 1.8426e-004

C= 5.0722e-003

Rho= 0.9999509

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.010	0.010	26	0.000	26					14
0.2	0.200	0.227	0.027	1202	0.0 %	1202					-2
2.5	2.500	2.462	-0.038	13334	0.0 %	13334					-1
5.0	5.000	4.957	-0.043	26873	0.0 %	26873					1
7.5	7.500	7.560	0.060	41004	0.0 %	41004					0
10.0	10.000	9.985	-0.015	54160	0.0 %	54160					

LB116388

INSTRUMENT ID: CV1

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0	26	-		0 7471B	PPB	09/20/2021 15:04	Std
	0.2 S0.2	1202	-		0.2 7471B	PPB	09/20/2021 15:07	Std
	2.5 S2.5	13334	-		2.5 7471B	PPB	09/20/2021 15:09	Std
	5 S5.0	26873	-		5 7471B	PPB	09/20/2021 15:11	Std
	7.5 S7.5	41004	-		7.5 7471B	PPB	09/20/2021 15:13	Std
	10 S10.0	54160	-		10 7471B	PPB	09/20/2021 15:16	Std
ICV01	ICV01	21412	3.9504	-	7471B	PPB	09/20/2021 15:19	SMPL
ICB01	ICB01	-19	0.0016	-	7471B	PPB	09/20/2021 15:21	SMPL
CCV71	CCV71	26751	4.9342	-	7471B	PPB	09/20/2021 15:23	SMPL
CCB71	CCB71	-34	-0.0012	-	7471B	PPB	09/20/2021 15:25	SMPL
CRA	CRA	1195	0.2253	-	7471B	PPB	09/20/2021 15:27	SMPL
HighStd	HighStd	53869	9.9309	-	7471B	PPB	09/20/2021 15:30	SMPL
ChkStd	ChkStd	37711	6.9537	-	7471B	PPB	09/20/2021 15:35	SMPL
PB139201BL	PBS	-20	0.0014	-	7471B	PPB	09/20/2021 15:37	SMPL
PB139201BS	LCSS	19509	3.5998	-	7471B	PPB	09/20/2021 15:39	SMPL
M3733-09	NAPL-01-(8-10)-END-POINT	396	0.078	-	7471B	PPB	09/20/2021 15:41	SMPL
M3733-10	NAPL-02-(8-10)-END-POINT	316	0.0633	-	7471B	PPB	09/20/2021 15:44	SMPL
M3750-05	NAPL-AREA-03-(10-12)-END-POINT	305	0.0613	-	7471B	PPB	09/20/2021 15:46	SMPL
M3750-06	NAPL-AREA-04-(8-10)-END-POINT	260	0.053	-	7471B	PPB	09/20/2021 15:48	SMPL
M3757-01	AU-06-091521	1442	0.2708	-	7471B	PPB	09/20/2021 15:50	SMPL
CCV72	CCV72	26648	4.9152	-	7471B	PPB	09/20/2021 15:53	SMPL
CCB72	CCB72	-23	0.0008	-	7471B	PPB	09/20/2021 15:55	SMPL
M3757-01DUP	AU-06-091521DUP	1388	0.2608	-	7471B	PPB	09/20/2021 15:57	SMPL
M3757-01MS	AU-06-091521MS	21627	3.99	-	7471B	PPB	09/20/2021 15:59	SMPL
M3757-01MSD	AU-06-091521MSD	21397	3.9477	-	7471B	PPB	09/20/2021 16:02	SMPL
M3762-01	11934	1982	0.3703	-	7471B	PPB	09/20/2021 16:04	SMPL
PB139202BL	PBS	23	0.0093	-	7471B	PPB	09/20/2021 16:06	SMPL
PB139202BS	LCSS	19664	3.6283	-	7471B	PPB	09/20/2021 16:11	SMPL
M3804-01	CL-01-091721	2807	0.5223	-	7471B	PPB	09/20/2021 16:13	SMPL
M3804-01DUP	CL-01-091721DUP	3290	0.6113	-	7471B	PPB	09/20/2021 16:16	SMPL
M3804-01MS	CL-01-091721MS	22414	4.135	-	7471B	PPB	09/20/2021 16:31	SMPL
M3804-01MSD	CL-01-091721MSD	25350	4.676	-	7471B	PPB	09/20/2021 16:33	SMPL
CCV73	CCV73	27090	4.9966	-	7471B	PPB	09/20/2021 16:35	SMPL
CCB73	CCB73	-21	0.0012	-	7471B	PPB	09/20/2021 16:37	SMPL
M3770-05	NAPL-5-SIDEWALL-END-POINT-(10-12)	428	0.0839	-	7471B	PPB	09/20/2021 16:40	SMPL
M3772-01	PRE-CLASS-WASTE-1	1422	0.2671	-	7471B	PPB	09/20/2021 16:42	SMPL
M3772-03	WASTE-PRE-CLASS	550	0.1064	-	7471B	PPB	09/20/2021 16:44	SMPL
M3786-01	CHRT-26878	9437	1.7439	-	7471B	PPB	09/20/2021 16:46	SMPL
M3786-03	CHRT-25949	23886	4.4063	-	7471B	PPB	09/20/2021 16:49	SMPL
M3786-05	CHRT-26414	1708	0.3198	-	7471B	PPB	09/20/2021 16:51	SMPL
M3792-01	20416	8525	1.5759	-	7471B	PPB	09/20/2021 16:53	SMPL
M3792-03	RT4213	58418	10.7691	-	7471B	PPB	09/20/2021 16:56	SMPL
M3797-01	VB16193	354	0.0703	-	7471B	PPB	09/20/2021 16:58	SMPL
M3797-03	20430	4001	0.7423	-	7471B	PPB	09/20/2021 17:00	SMPL
CCV74	CCV74	26677	4.9205	-	7471B	PPB	09/20/2021 17:02	SMPL
CCB74	CCB74	-17	0.0019	-	7471B	PPB	09/20/2021 17:05	SMPL
M3797-05	26598	83	0.0204	-	7471B	PPB	09/20/2021 17:07	SMPL
M3797-07	26240	6193	1.1462	-	7471B	PPB	09/20/2021 17:09	SMPL
M3798-05	SUB-SLAB-01-(5-8)	566	0.1094	-	7471B	PPB	09/20/2021 17:11	SMPL
M3798-06	SUB-SLAB-01-(15-17)	5962	1.1036	-	7471B	PPB	09/20/2021 17:14	SMPL
M3798-07	DUPLICATE-2	586	0.113	-	7471B	PPB	09/20/2021 17:16	SMPL
M3798-08	NAPL-06-(8-10)-END-POINT	815	0.1552	-	7471B	PPB	09/20/2021 17:18	SMPL
M3798-09	NAPL-07-(8-10)-END-POINT	589	0.1136	-	7471B	PPB	09/20/2021 17:20	SMPL
M3803-01	212	162130	29.879	-	7471B	PPB	09/20/2021 17:23	SMPL
M3803-04	26160	2058	0.3843	-	7471B	PPB	09/20/2021 17:27	SMPL
CCV75	CCV75	26504	4.8887	-	7471B	PPB	09/20/2021 17:47	SMPL
CCB75	CCB75	-13	0.0027	-	7471B	PPB	09/20/2021 17:49	SMPL