

===== LB112411 =====
Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092Reviewed by : AL

Instrument ID : Konelab

9/21/2021 14:10

Test: Total CN

male

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.867	0.0	0.083	
ICB1	0.030	0.0	0.001	
CCV1	239.966	0.0	0.204	
CCB1	0.039	0.0	0.001	
PB139204BL	-0.006	0.0	0.001	
M3762-02	0.166	0.0	0.001	
M3762-02DUP	0.045	0.0	0.001	
M3772-04	-0.241	0.0	0.001	
M3786-04	0.075	0.0	0.001	
M3822-01	0.133	0.0	0.001	
M3822-03	0.234	0.0	0.001	
M3822-05	0.581	0.0	0.001	
M3822-07	-0.105	0.0	0.001	
M3822-09	0.023	0.0	0.001	
CCV2	257.021	0.0	0.218	
CCB2	0.383	0.0	0.001	
M3822-11	0.117	0.0	0.001	
M3823-02	-0.169	0.0	0.001	
M3824-02	0.001	0.0	0.001	
M3824-05	-0.163	0.0	0.001	
M3832-02	0.130	0.0	0.001	
PB139205BL	-0.069	0.0	0.001	
M3786-07	-0.313	0.0	0.001	
M3786-07DUP	-0.253	0.0	0.001	
M3823-04	-0.380	0.0	0.001	
CCV3	267.041	0.0	0.227	
CCB3	-0.226	0.0	0.001	

N	27
Mean	31.886
SD	82.4825
CV%	258.68

Aquakem v. 7.2AQ1

Results from time period:

Tue Sep 21 12:58:04 2021

Tue Sep 21 14:09:29 2021

Sample Id	Sam/Ctr/c/	Test short nam	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	-0.4238	µg/l	9/21/2021 12:58:04	
5.OPPBCN	A	Reactive CN	P	4.4366	µg/l	9/21/2021 12:58:05	
10PPBCN	A	Reactive CN	P	9.4827	µg/l	9/21/2021 12:58:06	
50PPBCN	A	Reactive CN	P	49.7862	µg/l	9/21/2021 12:58:07	
100PPBCN	A	Reactive CN	P	100.0379	µg/l	9/21/2021 12:58:08	
250PPBCN	A	Reactive CN	P	253.3009	µg/l	9/21/2021 12:58:09	
500PPBCN	A	Reactive CN	P	498.3793	µg/l	9/21/2021 12:58:10	
ICV1	S	Reactive CN	P	96.8665	µg/l	9/21/2021 13:29:15	
ICB1	S	Reactive CN	P	0.0296	µg/l	9/21/2021 13:29:16	
CCV1	S	Reactive CN	P	239.9664	µg/l	9/21/2021 13:29:18	
CCB1	S	Reactive CN	P	0.0393	µg/l	9/21/2021 13:29:20	
PB139204BL	S	Reactive CN	P	-0.0063	µg/l	9/21/2021 13:29:22	
M3762-02	S	Reactive CN	P	0.1658	µg/l	9/21/2021 13:29:23	
M3762-02DUP	S	Reactive CN	P	0.0452	µg/l	9/21/2021 13:29:24	
M3772-04	S	Reactive CN	P	-0.2415	µg/l	9/21/2021 13:34:04	
M3786-04	S	Reactive CN	P	0.0746	µg/l	9/21/2021 13:34:05	
M3822-01	S	Reactive CN	P	0.1325	µg/l	9/21/2021 13:34:06	
M3822-03	S	Reactive CN	P	0.2344	µg/l	9/21/2021 13:34:07	
M3822-05	S	Reactive CN	P	0.5808	µg/l	9/21/2021 13:34:08	
M3822-07	S	Reactive CN	P	-0.1052	µg/l	9/21/2021 13:40:05	
M3822-09	S	Reactive CN	P	0.0229	µg/l	9/21/2021 13:40:06	
CCV2	S	Reactive CN	P	257.0211	µg/l	9/21/2021 13:40:07	
CCB2	S	Reactive CN	P	0.3826	µg/l	9/21/2021 13:40:08	
M3822-11	S	Reactive CN	P	0.1169	µg/l	9/21/2021 13:40:09	
M3823-02	S	Reactive CN	P	-0.1692	µg/l	9/21/2021 13:44:52	
M3824-02	S	Reactive CN	P	0.0009	µg/l	9/21/2021 13:44:54	
M3824-05	S	Reactive CN	P	-0.163	µg/l	9/21/2021 13:44:55	
M3832-02	S	Reactive CN	P	0.13	µg/l	9/21/2021 13:44:56	
PB139205BL	S	Reactive CN	P	-0.0689	µg/l	9/21/2021 13:53:51	
M3786-07	S	Reactive CN	P	-0.3135	µg/l	9/21/2021 13:53:52	
M3786-07DUP	S	Reactive CN	P	-0.2534	µg/l	9/21/2021 13:53:53	
M3823-04	S	Reactive CN	P	-0.3803	µg/l	9/21/2021 13:58:52	
CCV3	S	Reactive CN	P	267.0406	µg/l	9/21/2021 14:07:30	
CCB3	S	Reactive CN	P	-0.2255	µg/l	9/21/2021 14:09:29	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : AB Instrument ID : Konelab

9/21/2021 12:59


Test Total CN

Accepted 9/21/2021 12:58

Factor 1181
Bias 0.001

Coeff. of det. 0.999930

Errors

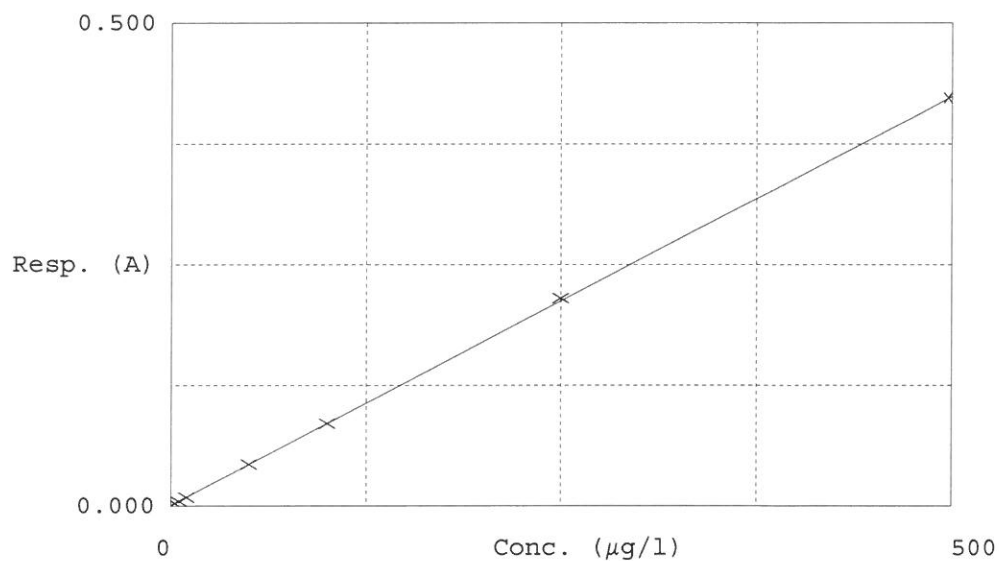

	Calibrator	Response	Calc. con.	Conc.	Rel. Errors
1	0.0PPBCN	0.001	-0.4238	0.0000	-11.3
2	5.0PPBCN	0.005	4.4366	5.0000	-5.2
3	10PPBCN	0.009	9.4827	10.0000	-0.4
4	50PPBCN	0.043	49.7862	50.0000	0.0
5	100PPBCN	0.086	100.0379	100.0000	1.3
6	250PPBCN	0.215	253.3009	250.0000	-0.3
7	500PPBCN	0.423	498.3793	500.0000	

AB 9/21/21