


LB 116412

7471B

INSTRUMENT ID: CV1

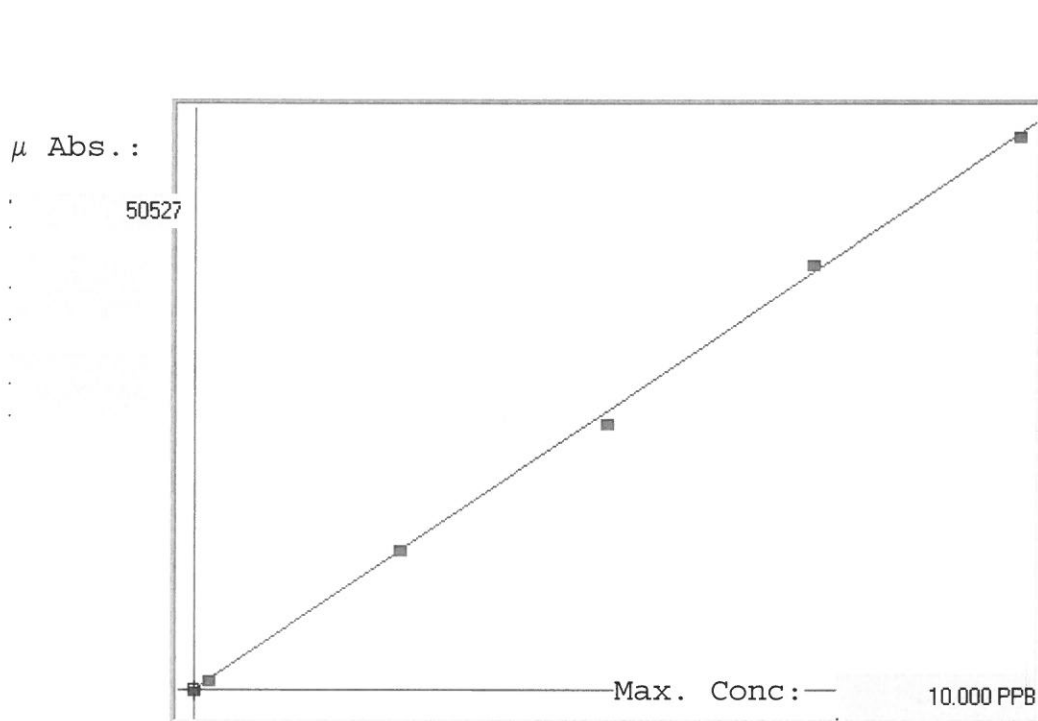

Linear

A= 0.0000e+000

B= 1.9695e-004

C= 9.3300e-003

Rho= 0.9995766

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.018	0.018	45	0.000	45					6
0.2	0.200	0.212	0.012	1031	0.0 %	1031					2
2.5	2.500	2.548	0.048	12890	0.0 %	12890					-4
5.0	5.000	4.801	-0.199	24332	0.0 %	24332					2
7.5	7.500	7.659	0.159	38843	0.0 %	38843					0
10.0	10.000	9.961	-0.039	50527	0.0 %	50527					

LB116412 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 21 Sep 2021 13:47:28

Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	45	-	0.0000	7471B	PPB	21 Sep 2021 13:55:55	S	Std
0.2 - 1	50.2	1031	-	0.2000	7471B	PPB	21 Sep 2021 13:58:12	S	Std
2.5 - 1	52.5	12890	-	2.5000	7471B	PPB	21 Sep 2021 14:00:29	S	Std
5.0 - 1	55	24332	-	5.0000	7471B	PPB	21 Sep 2021 14:02:46	S	Std
7.5 - 1	57.5	38843	-	7.5000	7471B	PPB	21 Sep 2021 14:07:43	S	Std
10.0 - 1	50	50527	-	10.0000	7471B	PPB	21 Sep 2021 14:12:35	S	Std
ICV03 - 1	ICV03	18552	3.6631	-	7471B	PPB	21 Sep 2021 14:15:29	U	SMPL
ICB03 - 1	ICB03	-39	0.0016	-	7471B	PPB	21 Sep 2021 14:17:43	U	SMPL
CCV84 - 1	CCV84	24379	4.8107	-	7471B	PPB	21 Sep 2021 14:19:58	U	SMPL
CCB84 - 1	CCB84	-44	0.0007	-	7471B	PPB	21 Sep 2021 14:22:13	U	SMPL
CRA - 1	CRA	1030	0.2122	-	7471B	PPB	21 Sep 2021 14:24:29	U	SMPL
HighStd - 1	HighStd	50964	10.0466	-	7471B	PPB	21 Sep 2021 14:26:44	U	SMPL
ChkStd - 1	ChkStd	36350	7.1684	-	7471B	PPB	21 Sep 2021 14:28:59	U	SMPL
PB139249BL - 1	PBS	-53	-0.0011	-	7471B	PPB	21 Sep 2021 14:31:16	U	SMPL
PB139249BS - 1	LCSS	21641	4.2715	-	7471B	PPB	21 Sep 2021 14:33:32	U	SMPL
M3821-01 - 1	TEST-PIT-9	94446	18.6103	-	7471B	PPB	21 Sep 2021 14:35:48	U	SMPL
M3823-01 - 1	DKM-ENV-IG-COMP	254	0.0594	-	7471B	PPB	21 Sep 2021 14:38:04	U	SMPL
M3823-03 - 1	DKM-ENV-IG-GRAB	195	0.0477	-	7471B	PPB	21 Sep 2021 14:40:23	U	SMPL
M3824-01 - 1	TP-B	3043	0.6086	-	7471B	PPB	21 Sep 2021 14:42:40	U	SMPL
M3824-01DUP - 1	TP-BDUP	3135	0.6268	-	7471B	PPB	21 Sep 2021 14:44:55	U	SMPL
CCV85 - 1	CCV85	24325	4.8001	-	7471B	PPB	21 Sep 2021 14:47:10	U	SMPL
CCB85 - 1	CCB85	-32	0.0030	-	7471B	PPB	21 Sep 2021 14:49:25	U	SMPL
M3824-01MS - 1	TP-BMS	23880	4.7125	-	7471B	PPB	21 Sep 2021 14:51:40	U	SMPL
M3824-01MSD - 1	TP-BMSD	23978	4.7318	-	7471B	PPB	21 Sep 2021 14:53:55	U	SMPL
M3824-04 - 1	TP-C	698	0.1468	-	7471B	PPB	21 Sep 2021 14:56:11	U	SMPL
M3832-01 - 1	TP-B	5511	1.0947	-	7471B	PPB	21 Sep 2021 14:58:26	U	SMPL
M3824-01LX5 - 1		451	0.0982	-	7471B	PPB	21 Sep 2021 15:00:42	U	SMPL
M3824-01A - 1		24081	4.7520	-	7471B	PPB	21 Sep 2021 15:02:58	U	SMPL
PB3757-01 - 1	AU-06-091521	1414	0.2878	-	7471B	PPB	21 Sep 2021 15:05:14	U	SMPL
PB3757-01DUP - 1	AU-06-091521DUP	1346	0.2744	-	7471B	PPB	21 Sep 2021 15:07:31	U	SMPL
PB3757-01MS - 1	AU-06-091521MS	18877	3.7271	-	7471B	PPB	21 Sep 2021 15:09:49	U	SMPL
PB3757-01MSD - 1	AU-06-091521MSD	21323	4.2089	-	7471B	PPB	21 Sep 2021 15:12:05	U	SMPL
CCV86 - 1	CCV86	24586	4.8515	-	7471B	PPB	21 Sep 2021 15:14:21	U	SMPL
CCB86 - 1	CCB86	-27	0.0040	-	7471B	PPB	21 Sep 2021 15:16:36	U	SMPL
PB3757-01LX5 - 1		260	0.0605	-	7471B	PPB	21 Sep 2021 15:18:52	U	SMPL
PB3757-01A - 1		20593	4.0651	-	7471B	PPB	21 Sep 2021 15:21:07	U	SMPL
M3804-01 - 1	CL-01-091721	2780	0.5568	-	7471B	PPB	21 Sep 2021 15:23:23	U	SMPL
M3804-01DUP - 1	CL-01-091721DUP	3022	0.6045	-	7471B	PPB	21 Sep 2021 15:28:34	U	SMPL
M3804-01MS - 1	CL-01-091721MS	25701	5.0711	-	7471B	PPB	21 Sep 2021 15:30:49	U	SMPL
M3804-01MSD - 1	CL-01-091721MSD	26082	5.1461	-	7471B	PPB	21 Sep 2021 15:33:06	U	SMPL
M3804-01LX5 - 1		543	0.1163	-	7471B	PPB	21 Sep 2021 15:35:22	U	SMPL
M3804-01A - 1		24128	4.7613	-	7471B	PPB	21 Sep 2021 15:37:39	U	SMPL
M3792-03DLX2 - 1		26796	5.2868	-	7471B	PPB	21 Sep 2021 15:42:25	U	SMPL
M3803-01DLX5 - 1		30266	5.9702	-	7471B	PPB	21 Sep 2021 15:44:40	U	SMPL
CCV87 - 1	CCV87	24024	4.7408	-	7471B	PPB	21 Sep 2021 15:46:56	U	SMPL
CCB87 - 1	CCB87	-94	-0.0092	-	7471B	PPB	21 Sep 2021 15:49:13	U	SMPL
M3821-01DLX5 - 1		18414	3.6359	-	7471B	PPB	21 Sep 2021 15:57:17	U	SMPL
CCV88 - 1	CCV88	26859	5.2992	-	7471B	PPB	21 Sep 2021 15:59:32	U	SMPL
CCB88 - 1	CCB88	-37	0.0020	-	7471B	PPB	21 Sep 2021 16:01:48	U	SMPL