

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : AB Instrument ID : Konelab

9/21/2021 15:02

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	94.843	0.0	0.081	
ICB1	0.206	0.0	0.001	
CCV1	250.278	0.0	0.213	
CCB1	0.200	0.0	0.001	
PB139208BL	0.254	0.0	0.001	
PB139208BS	101.303	0.0	0.087	
LOWPB139208	10.269	0.0	0.010	
HIGHPB139208	494.931	0.0	0.420	
M3772-01	0.023	0.0	0.001	
M3772-01DUP	-0.137	0.0	0.001	
M3772-01MS	30.923	0.0	0.027	
M3772-01MSD	31.067	0.0	0.027	
M3772-03	0.228	0.0	0.001	
M3823-01	0.438	0.0	0.001	
CCV2	252.079	0.0	0.214	
CCB2	-0.342	0.0	0.001	
M3823-03	-0.312	0.0	0.001	
M3824-01	1.125	0.0	0.002	
M3824-04	-0.142	0.0	0.001	
M3832-01	1.210	0.0	0.002	
CCV3	253.749	0.0	0.216	
CCB3	0.431	0.0	0.001	

N	22
Mean	69.210
SD	129.3637
CV%	186.91

- 103 % (90-110)
- 99 %

AB
9/21/21

Aquakem v. 7.2AQ1

Results from time period:

Tue Sep 21 14:41:58 2021

Tue Sep 21 14:59:53 2021

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	-0.4238	µg/l	9/21/2021 12:58:04	
5.OPPBCN	A	Total CN	P	4.4366	µg/l	9/21/2021 12:58:05	
10PPBCN	A	Total CN	P	9.4827	µg/l	9/21/2021 12:58:06	
50PPBCN	A	Total CN	P	49.7862	µg/l	9/21/2021 12:58:07	
100PPBCN	A	Total CN	P	100.0379	µg/l	9/21/2021 12:58:08	
250PPBCN	A	Total CN	P	253.3009	µg/l	9/21/2021 12:58:09	
500PPBCN	A	Total CN	P	498.3793	µg/l	9/21/2021 12:58:10	
ICV1	S	Total CN	P	94.8433	µg/l	9/21/2021 14:41:58	
ICB1	S	Total CN	P	0.206	µg/l	9/21/2021 14:42:00	
CCV1	S	Total CN	P	250.278	µg/l	9/21/2021 14:42:02	
CCB1	S	Total CN	P	0.2003	µg/l	9/21/2021 14:42:05	
PB139208BL	S	Total CN	P	0.2538	µg/l	9/21/2021 14:42:06	
PB139208BS	S	Total CN	P	101.3035	µg/l	9/21/2021 14:42:08	
LOWPB139208	S	Total CN	P	10.2687	µg/l	9/21/2021 14:49:30	
HIGHPB139208	S	Total CN	P	494.9307	µg/l	9/21/2021 14:49:31	
M3772-01	S	Total CN	P	0.0229	µg/l	9/21/2021 14:49:32	
M3772-01DUP	S	Total CN	P	-0.137	µg/l	9/21/2021 14:49:33	
M3772-01MS	S	Total CN	P	30.9226	µg/l	9/21/2021 14:49:34	
M3772-01MSD	S	Total CN	P	31.0673	µg/l	9/21/2021 14:49:35	
M3772-03	S	Total CN	P	0.2284	µg/l	9/21/2021 14:49:38	
M3823-01	S	Total CN	P	0.438	µg/l	9/21/2021 14:49:39	
CCV2	S	Total CN	P	252.0786	µg/l	9/21/2021 14:49:40	
CCB2	S	Total CN	P	-0.3415	µg/l	9/21/2021 14:57:05	
M3823-03	S	Total CN	P	-0.3119	µg/l	9/21/2021 14:57:06	
M3824-01	S	Total CN	P	1.1246	µg/l	9/21/2021 14:57:07	
M3824-04	S	Total CN	P	-0.1417	µg/l	9/21/2021 14:57:08	
M3832-01	S	Total CN	P	1.2098	µg/l	9/21/2021 14:57:09	
CCV3	S	Total CN	P	253.7491	µg/l	9/21/2021 14:57:10	
CCB3	S	Total CN	P	0.4312	µg/l	9/21/2021 14:57:11	

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : AB

Instrument ID : Konelab

9/21/2021 12:59


Test Total CN

Accepted 9/21/2021 12:58

Factor 1181
Bias 0.001

Coeff. of det. 0.999930

Errors

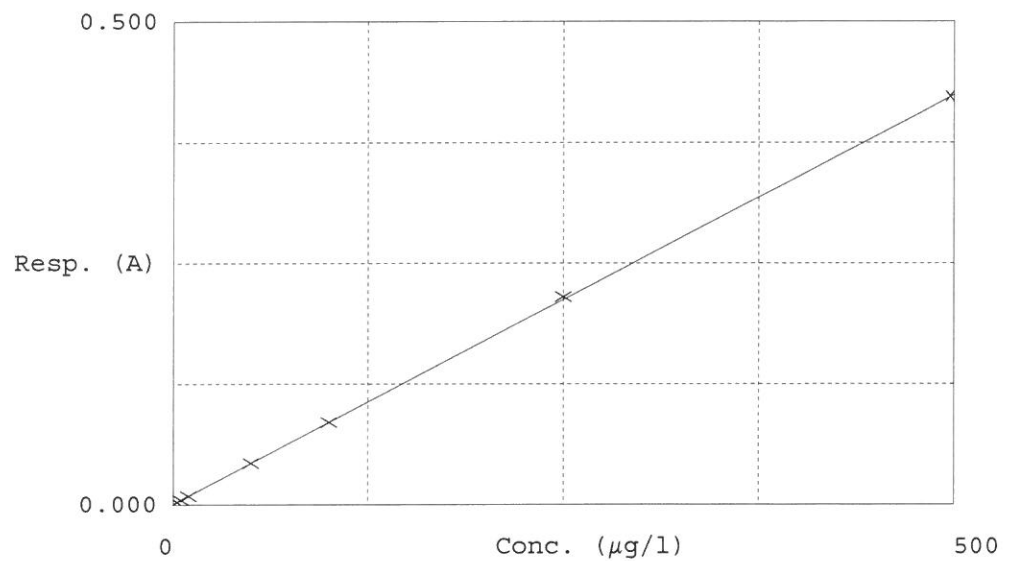

	Calibrator	Response	Calc. con.	Conc.	Rel. Errors
1	0.0PPBCN	0.001	-0.4238	0.0000	-11.3
2	5.0PPBCN	0.005	4.4366	5.0000	-5.2
3	10PPBCN	0.009	9.4827	10.0000	-0.4
4	50PPBCN	0.043	49.7862	50.0000	0.0
5	100PPBCN	0.086	100.0379	100.0000	1.3
6	250PPBCN	0.215	253.3009	250.0000	-0.3
7	500PPBCN	0.423	498.3793	500.0000	

AB

9/21/21